

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110521\
 Data File : PL070818.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2021 19:44
 Operator : AR\AJ
 Sample : M4540-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 03:20:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.567	5.501	8947166	23677881	18.267	18.779
28)	SA Decachlor...	10.329	11.390	6643905	13195220	9.723	9.867
Target Compounds							
9)	A Endosulfan I	7.431f	0.000	688213	0	1.123	N.D. #
12)	B 4,4'-DDE	7.564	8.499	1704857	2961292	2.926	2.007 #
16)	A 4,4'-DDD	0.000	9.037	0	1551162	N.D.	1.289 #
27)	Chlordane-5	0.000	9.226f	0	290423	N.D.	7.010 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110521\
Data File : PL070818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2021 19:44
Operator : AR\AJ
Sample : M4540-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 03:20:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

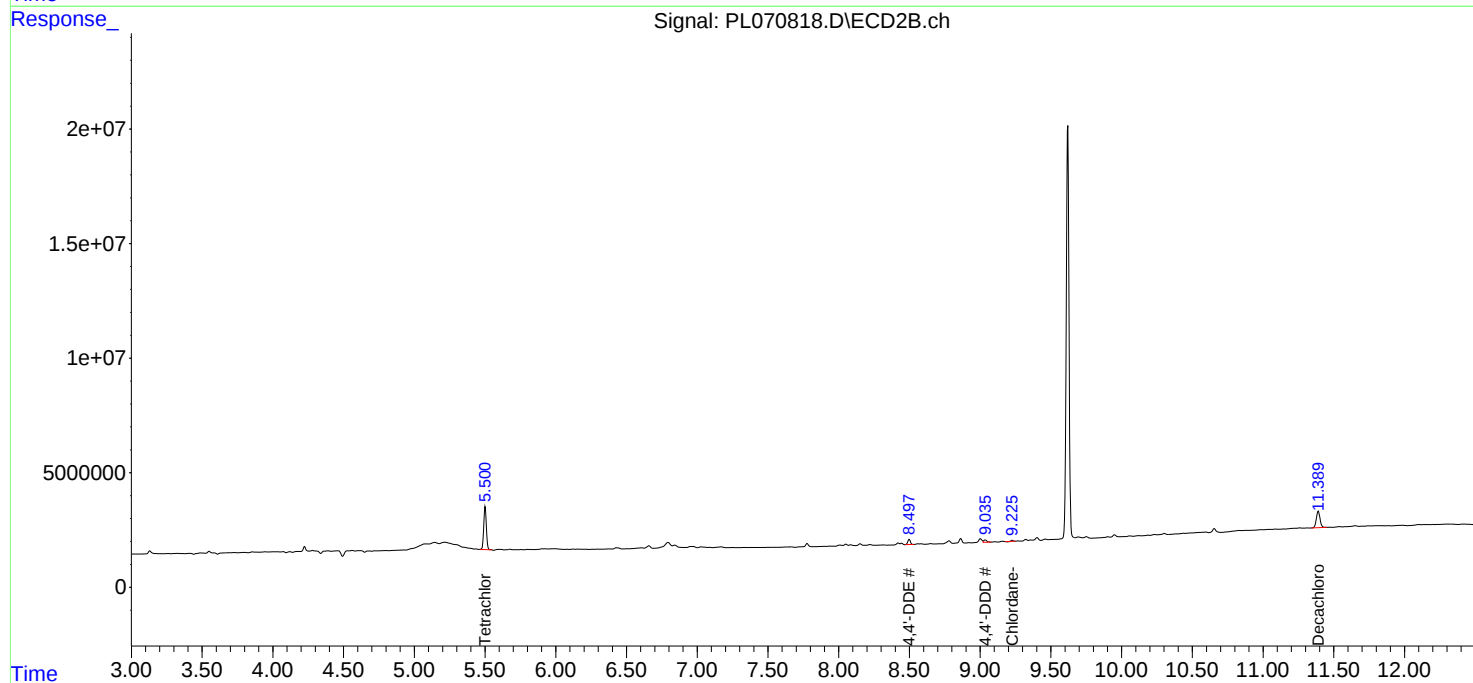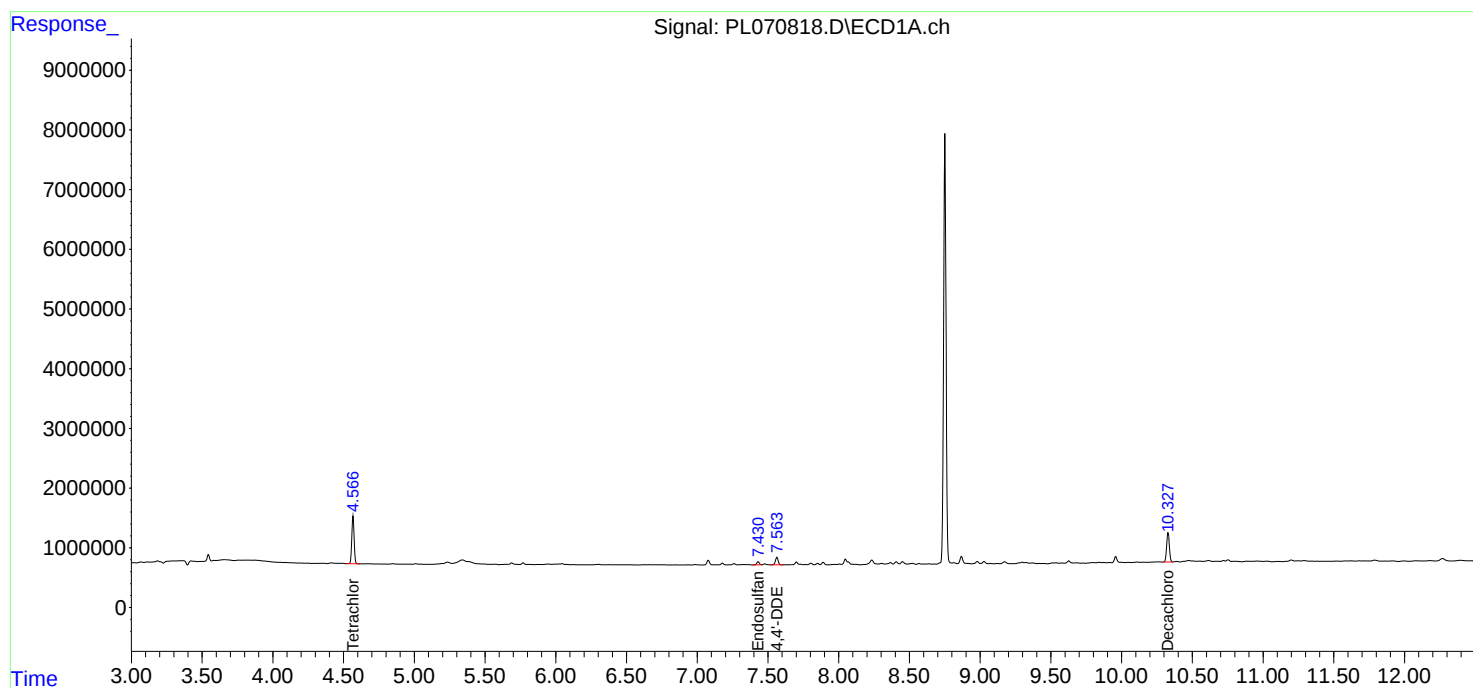


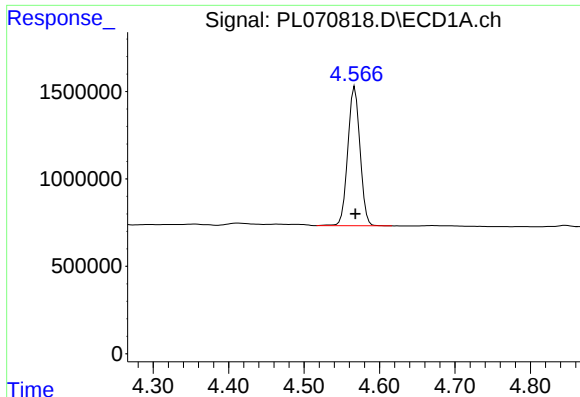

#1 Tetrachloro-m-xylene


R.T.: 4.567 min
Delta R.T.: 0.000 min
Response: 8947166
Conc: 18.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

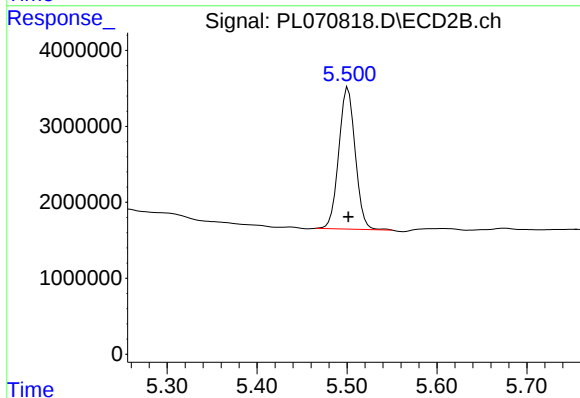


#1 Tetrachloro-m-xylene

R.T.: 5.501 min
Delta R.T.: 0.000 min
Response: 23677881
Conc: 18.78 ng/ml

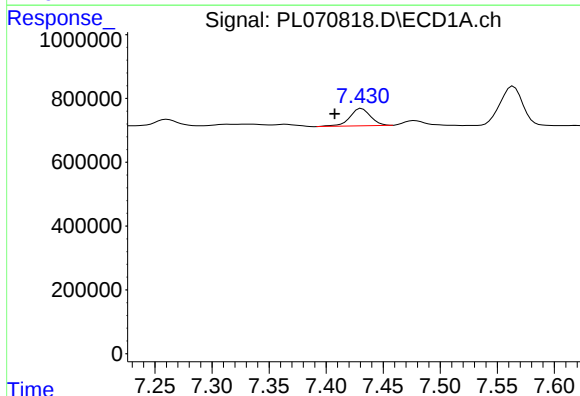


#9 Endosulfan I

R.T.: 7.431 min
Delta R.T.: 0.024 min
Response: 688213
Conc: 1.12 ng/ml

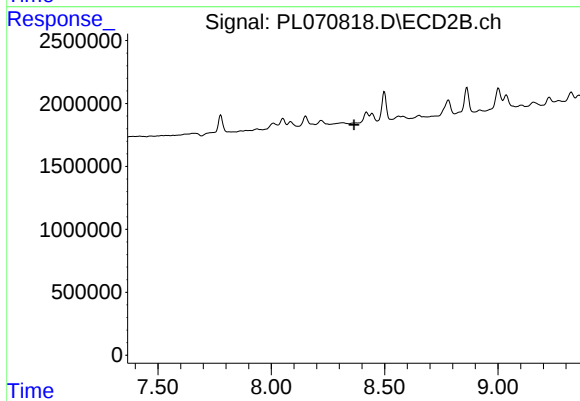

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 8.365 min
Response: 0
Conc: N.D.

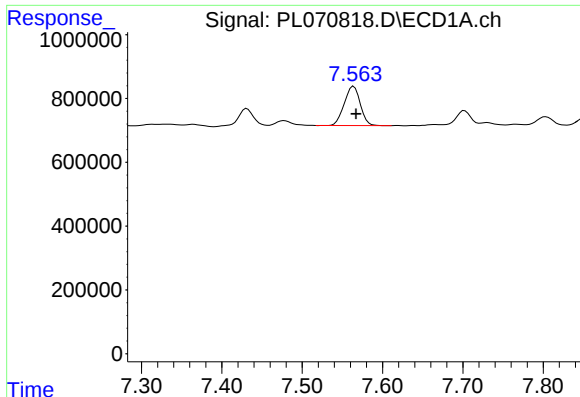

#12 4,4'-DDE


R.T.: 7.564 min
Delta R.T.: -0.003 min
Response: 1704857
Conc: 2.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

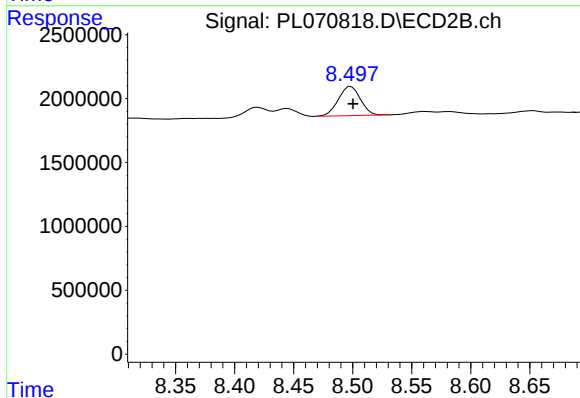


#12 4,4'-DDE

R.T.: 8.499 min
Delta R.T.: -0.002 min
Response: 2961292
Conc: 2.01 ng/ml

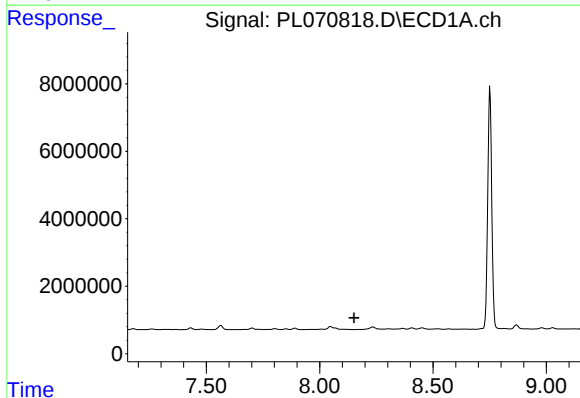


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.152 min
Response: 0
Conc: N.D.

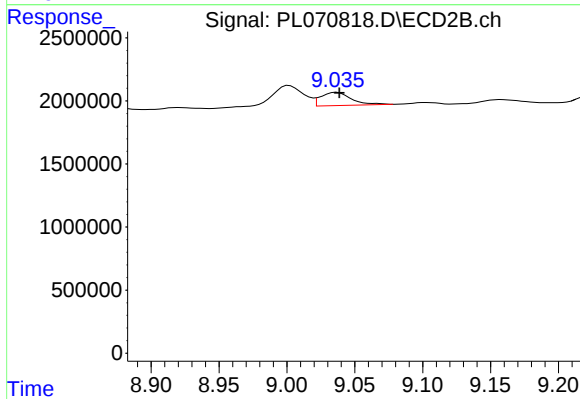

#16 4,4'-DDD


R.T.: 9.037 min
Delta R.T.: -0.002 min
Response: 1551162
Conc: 1.29 ng/ml

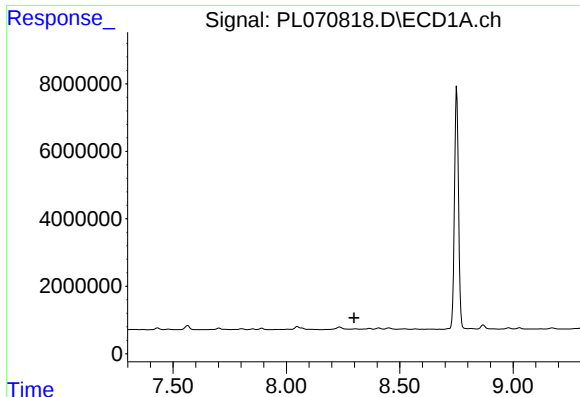

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

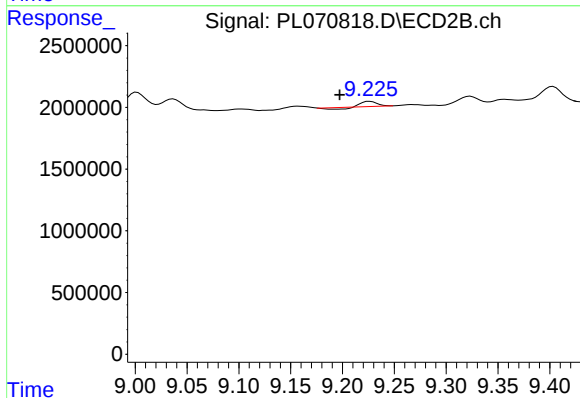


#27 Chlordane-5

R.T.: 9.226 min
Delta R.T.: 0.029 min
Response: 290423
Conc: 7.01 ng/ml

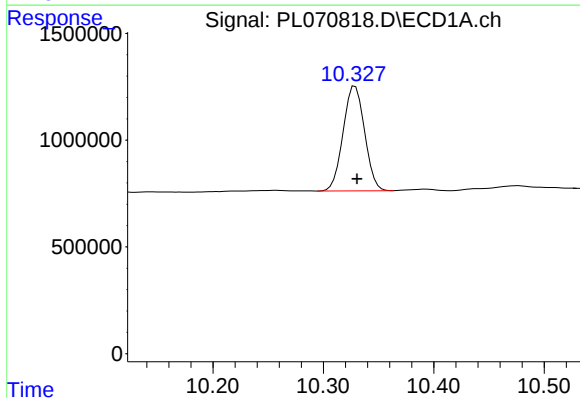

#28 Decachlorobiphenyl

R.T.: 10.329 min
Delta R.T.: -0.001 min
Response: 6643905
Conc: 9.72 ng/ml

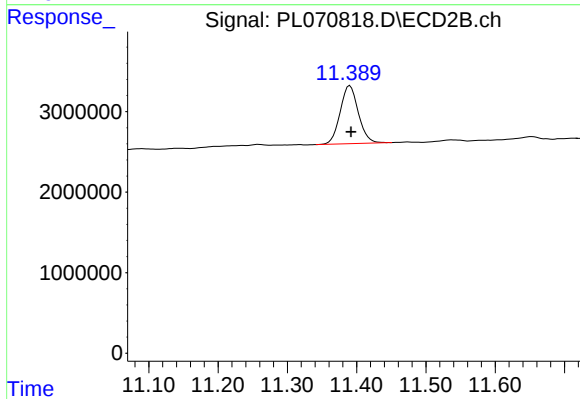

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: -0.002 min
Response: 13195220
Conc: 9.87 ng/ml