

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110524\
 Data File : PL092849.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 15:06
 Operator : AR\AJ
 Sample : P4693-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BP-G4-WC

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/06/2024
 Supervised By : Ankita Jodhani 11/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 01:26:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.780	50455456	61473656	20.592m	22.591
28) SA Decachlor...	9.058	7.916	38678325	39245043	20.097	14.379m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110524\
Data File : PL092849.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 15:06
Operator : AR\AJ
Sample : P4693-05
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BP-G4-WC


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/06/2024
Supervised By : Ankita Jodhani 11/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 01:26:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

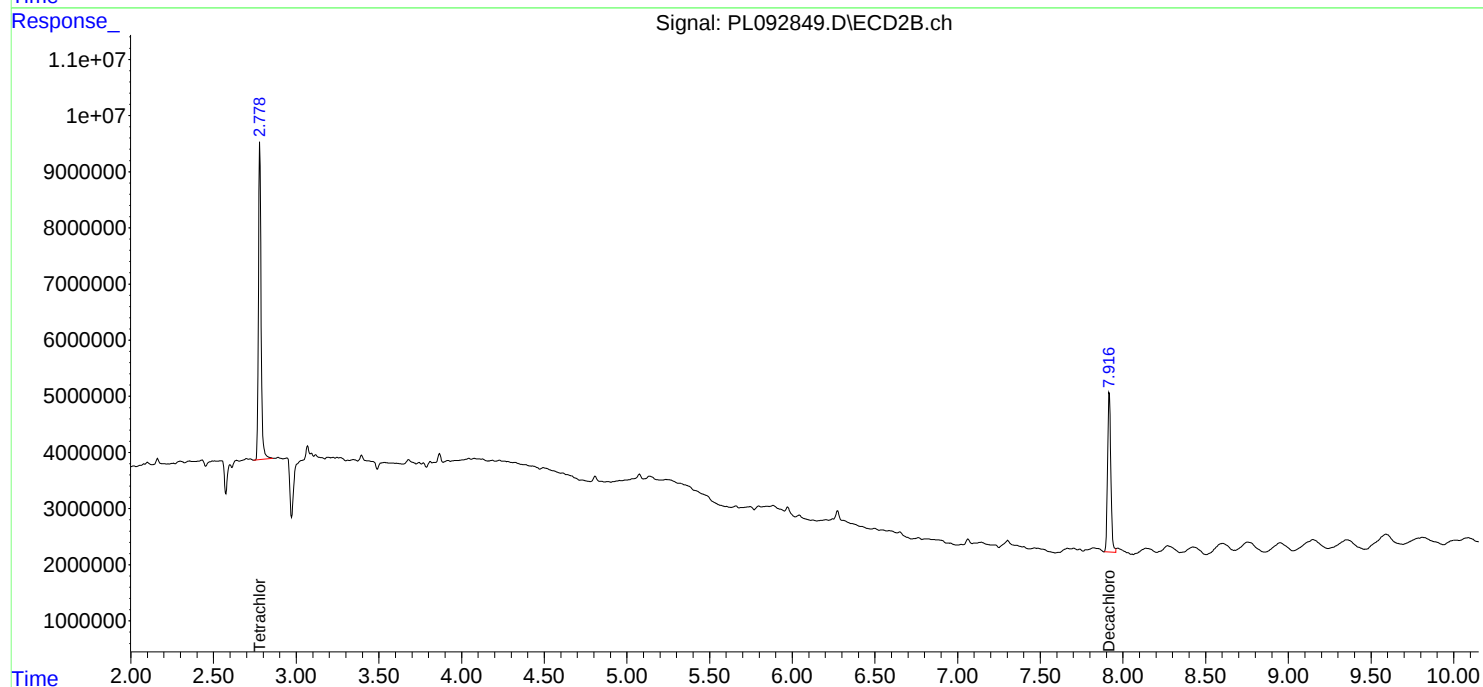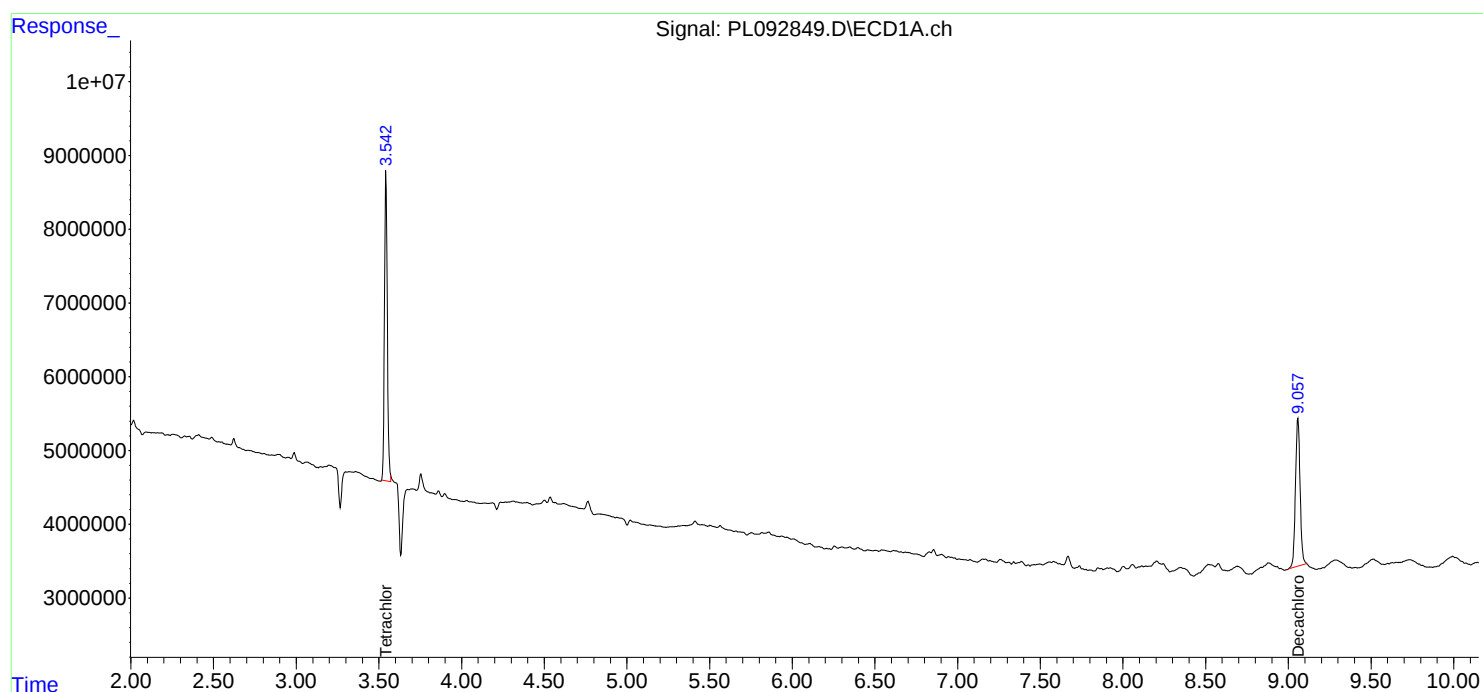

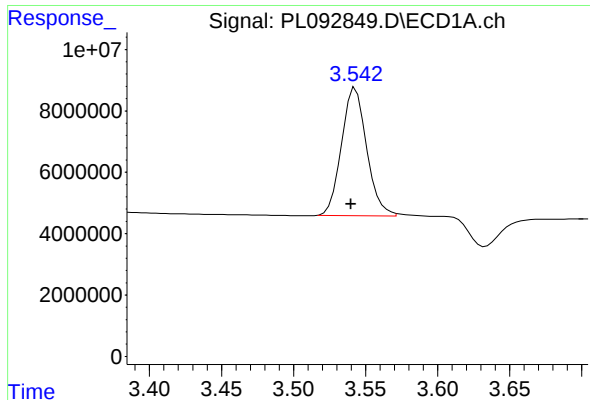


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: 0.002 min
Response: 50455456
Conc: 20.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
BP-G4-WC


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/06/2024
Supervised By :Ankita Jodhani 11/06/2024

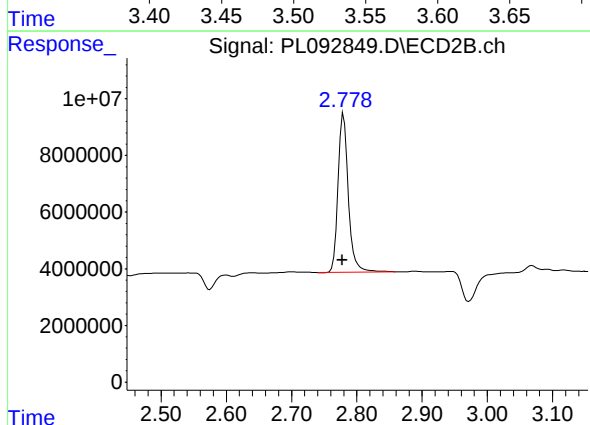


#1 Tetrachloro-m-xylene

R.T.: 2.780 min
Delta R.T.: 0.002 min
Response: 61473656
Conc: 22.59 ng/ml

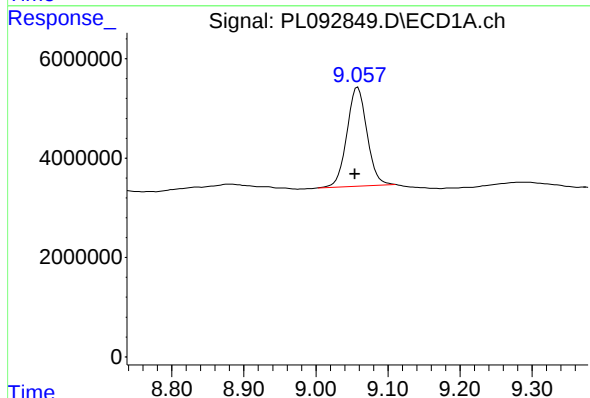

#28 Decachlorobiphenyl

R.T.: 9.058 min
Delta R.T.: 0.004 min
Response: 38678325
Conc: 20.10 ng/ml

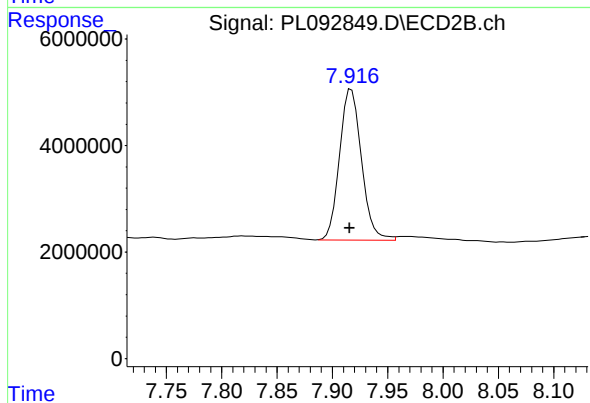

#28 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.000 min
Response: 39245043
Conc: 14.38 ng/ml m