

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
 Data File : PL041854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 11:03
 Operator : AJ\SJ
 Sample : J5805-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-SAMPLES(1-5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 15:44:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.105	110.9E6	60624062	17.407	19.682
28)	SA Decachlor...	8.215	9.238	108.3E6	43627155	16.356	17.027
Target Compounds							
2)	A alpha-BHC	3.872f	0.000	167978	0	0.017	N.D. #
3)	MA gamma-BHC...	0.000	4.835f	0	4221716	N.D.	0.996 #
6)	B beta-BHC	4.408f	0.000	3967676	0	1.053	N.D. #
9)	A Endosulfan I	5.466f	0.000	2419378	0	0.325	N.D. #
10)	B gamma-Chl...	5.466f	0.000	2419378	0	0.297	N.D. #
11)	B alpha-Chl...	5.466	0.000	2419378	0	0.299	N.D. #
23)	Chlordane-1	4.384	0.000	2829011	0	9.978	N.D. #
25)	Chlordane-3	5.466	0.000	2419378	0	2.714	N.D. #
26)	Chlordane-4	5.466	0.000	2419378	0	3.090	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
Data File : PL041854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 11:03
Operator : AJ\SJ
Sample : J5805-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(1-5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 15:44:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

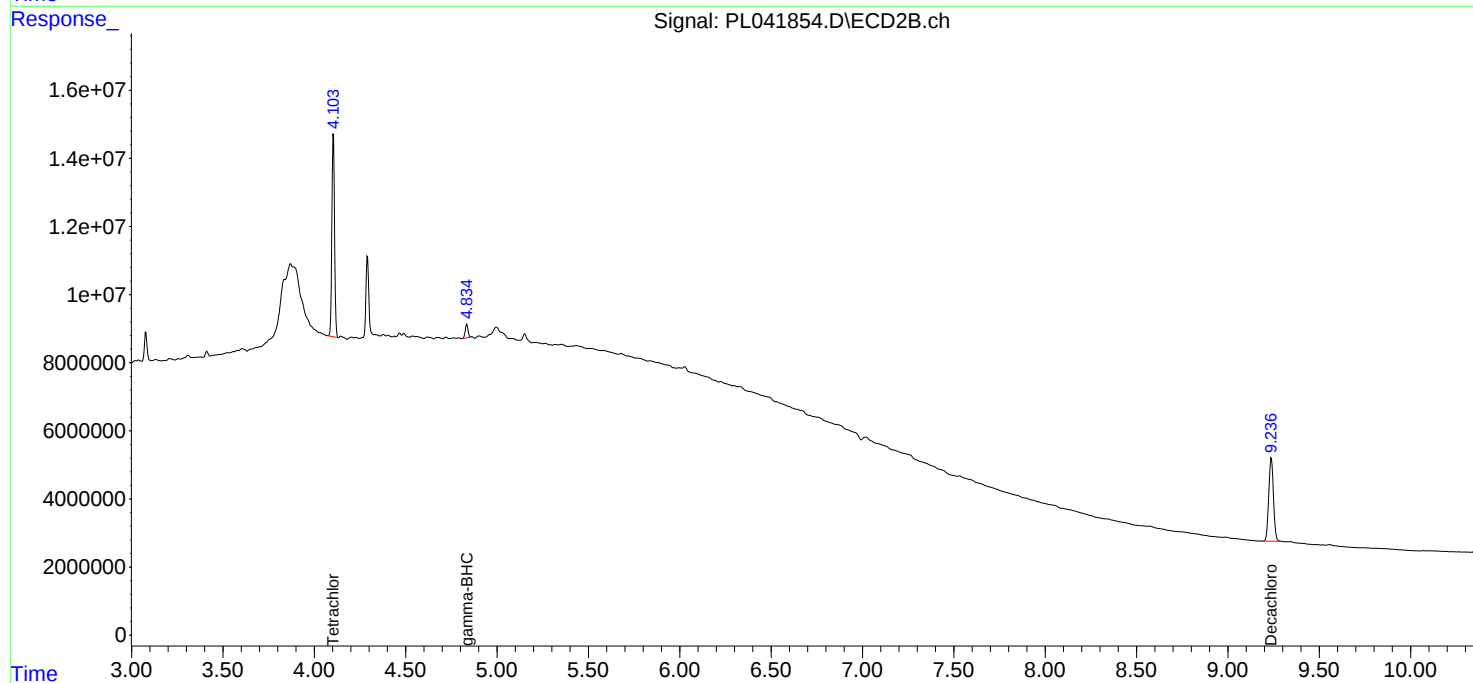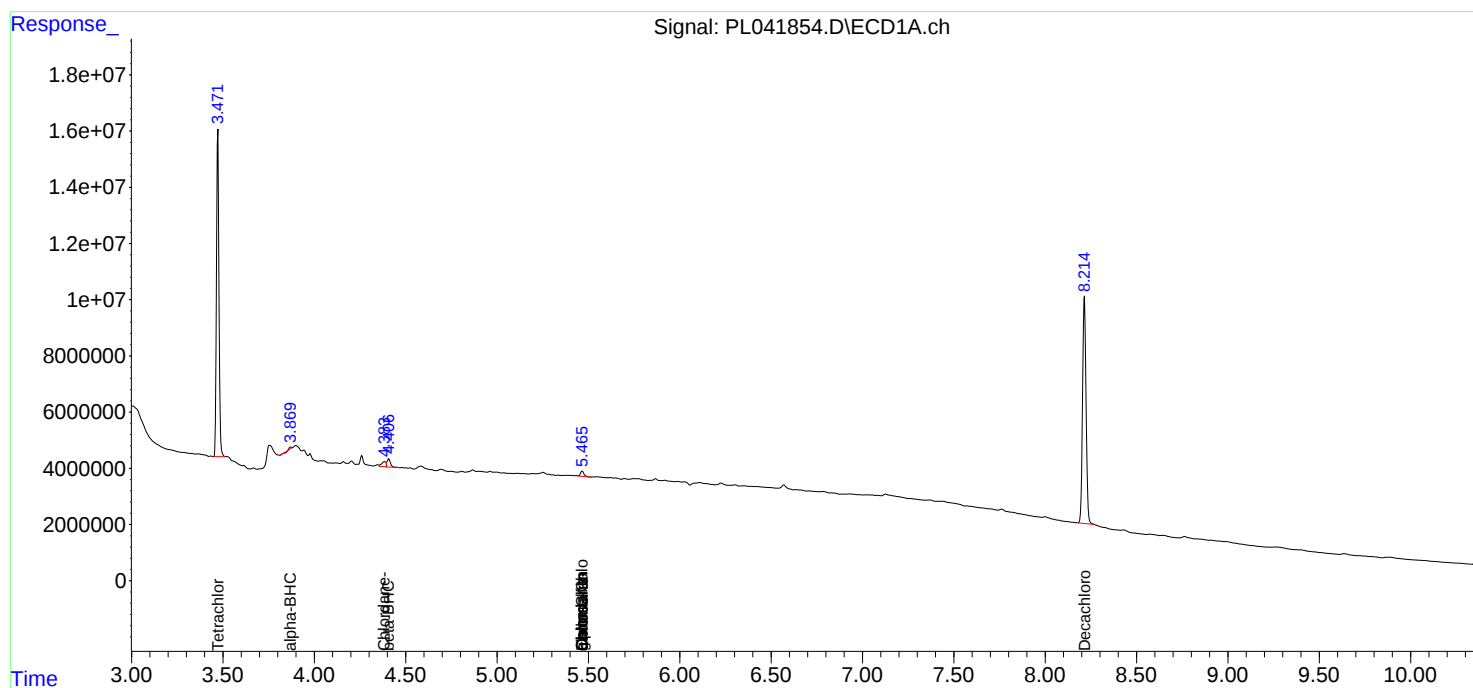


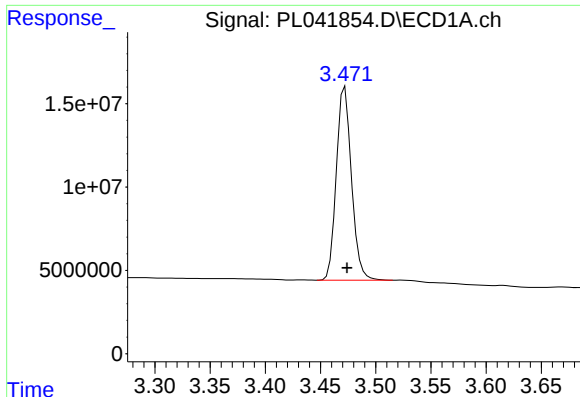

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 110883958
Conc: 17.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(1-5)

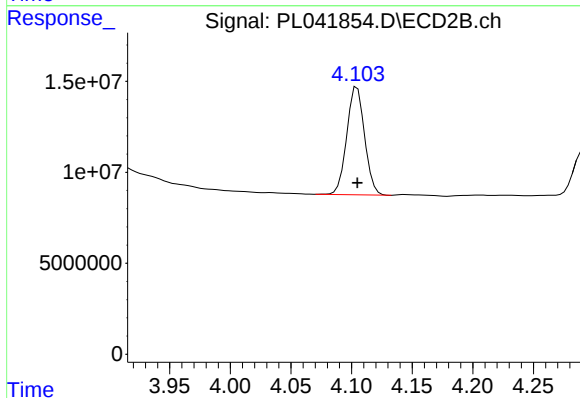


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 60624062
Conc: 19.68 ng/ml

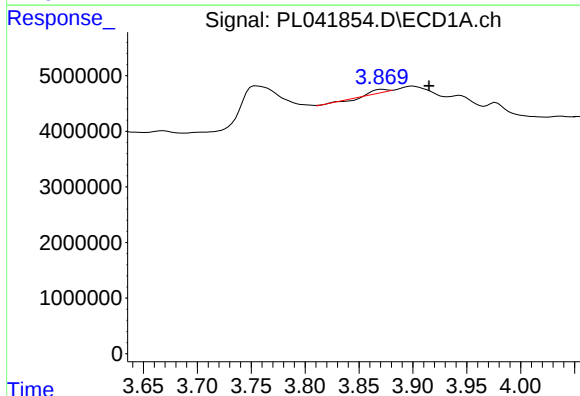


#2 alpha-BHC

R.T.: 3.872 min
Delta R.T.: -0.043 min
Response: 167978
Conc: 0.02 ng/ml

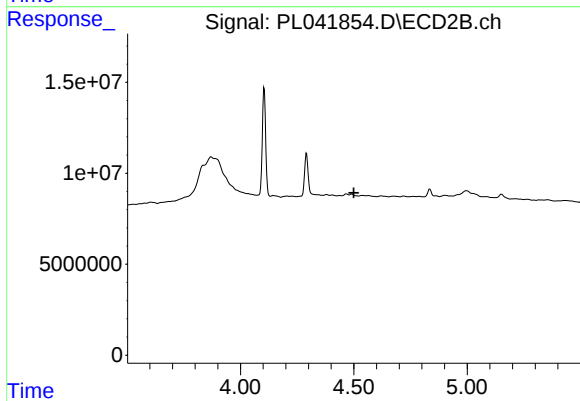

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.501 min
Response: 0
Conc: N.D.

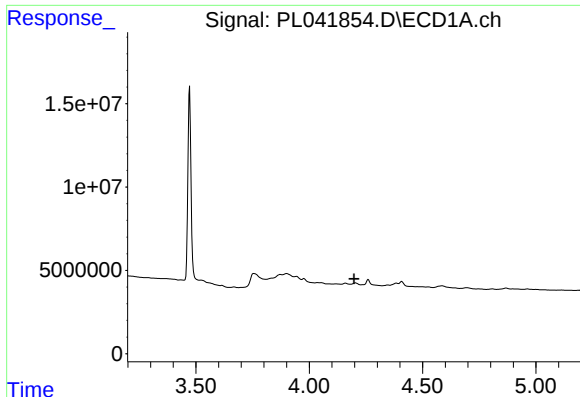

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.198 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(1-5)

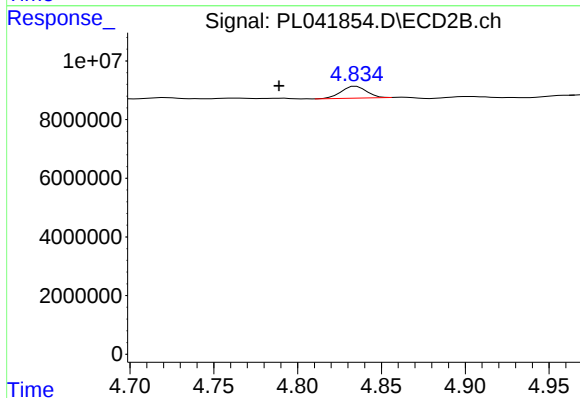


#3 gamma-BHC (Lindane)

R.T.: 4.835 min
Delta R.T.: 0.046 min
Response: 4221716
Conc: 1.00 ng/ml

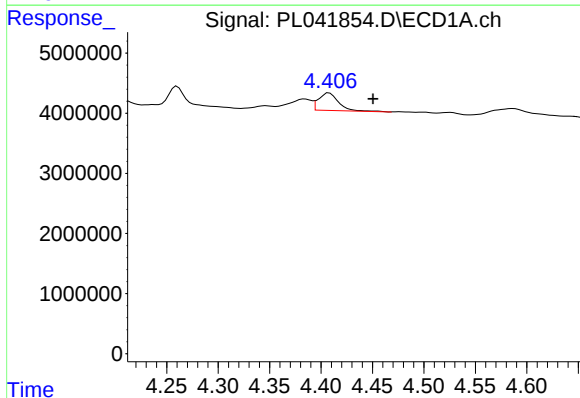


#6 beta-BHC

R.T.: 4.408 min
Delta R.T.: -0.043 min
Response: 3967676
Conc: 1.05 ng/ml

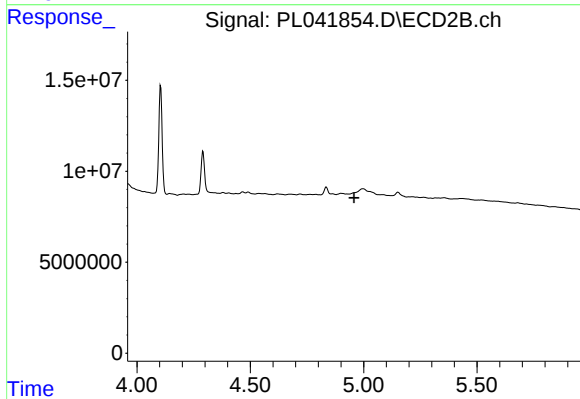

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.957 min
Response: 0
Conc: N.D.

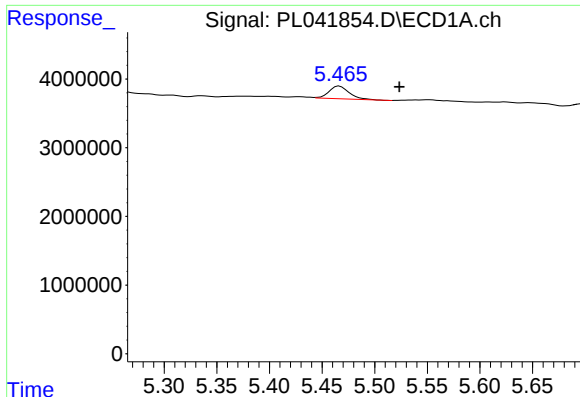

#9 Endosulfan I


R.T.: 5.466 min
Delta R.T.: -0.057 min
Response: 2419378
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(1-5)

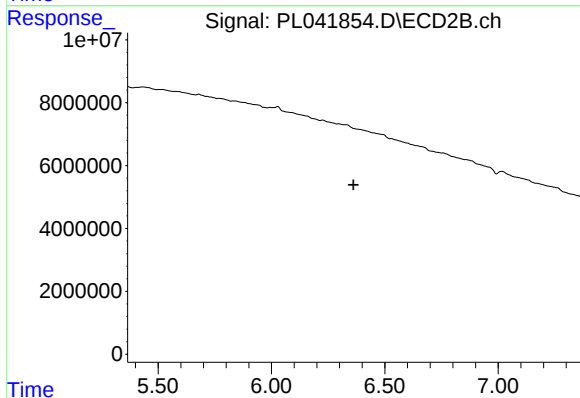


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

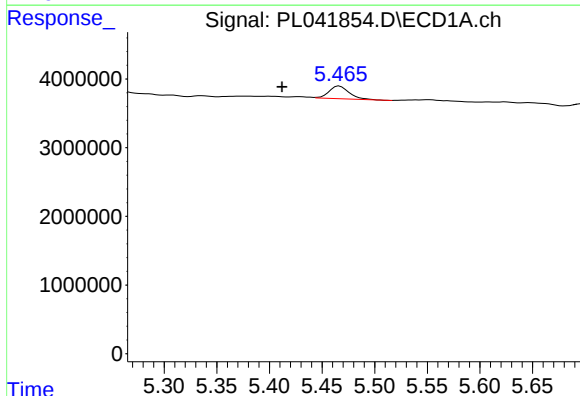


#10 gamma-Chlordane

R.T.: 5.466 min
Delta R.T.: 0.055 min
Response: 2419378
Conc: 0.30 ng/ml

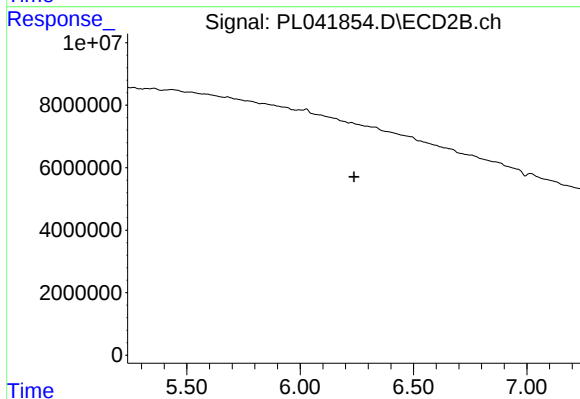

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

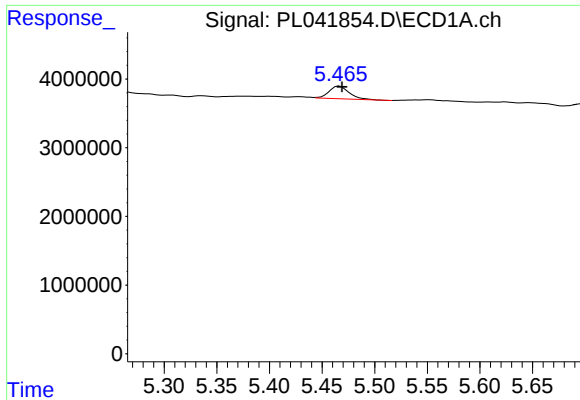

#11 alpha-Chlordane


R.T.: 5.466 min
Delta R.T.: -0.003 min
Response: 2419378
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(1-5)

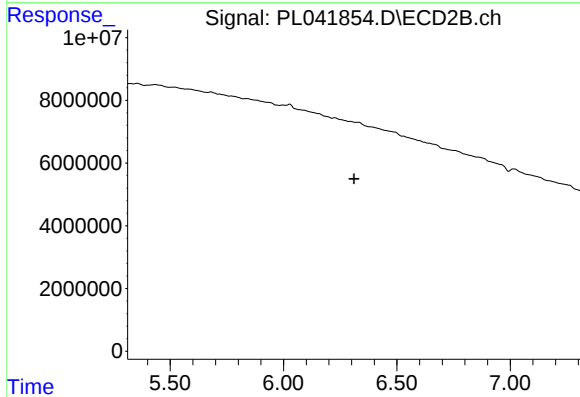


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

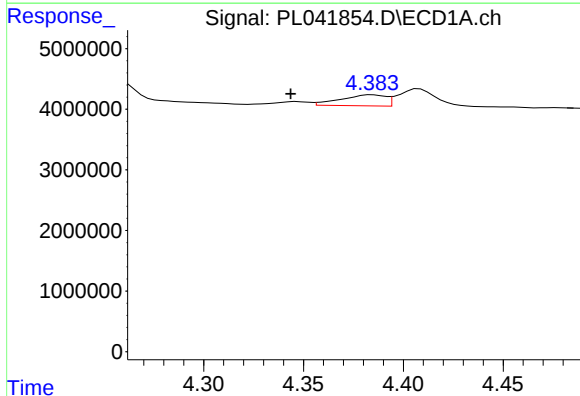


#23 Chlordane-1

R.T.: 4.384 min
Delta R.T.: 0.041 min
Response: 2829011
Conc: 9.98 ng/ml

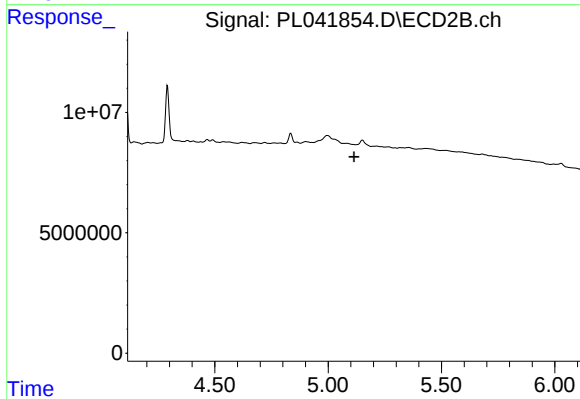

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

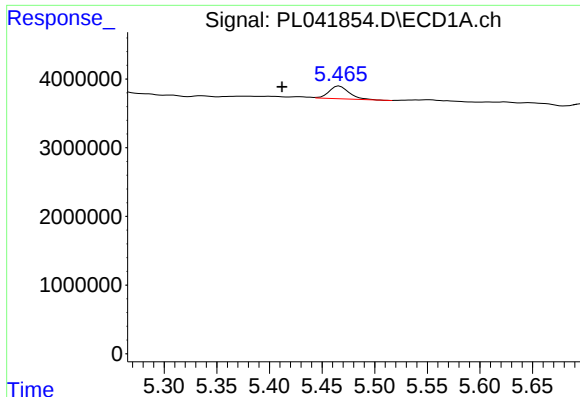

#25 Chlordane-3


R.T.: 5.466 min
Delta R.T.: 0.054 min
Response: 2419378
Conc: 2.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(1-5)

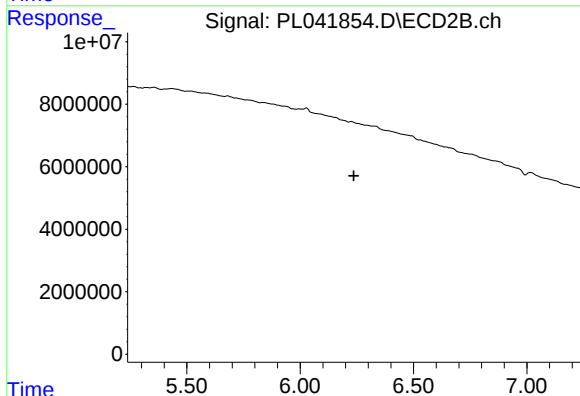


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

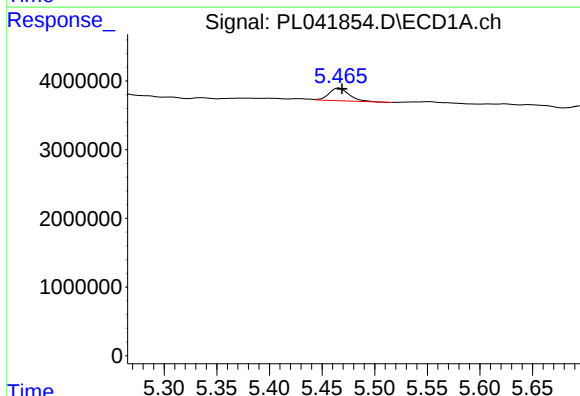


#26 Chlordane-4

R.T.: 5.466 min
Delta R.T.: -0.003 min
Response: 2419378
Conc: 3.09 ng/ml

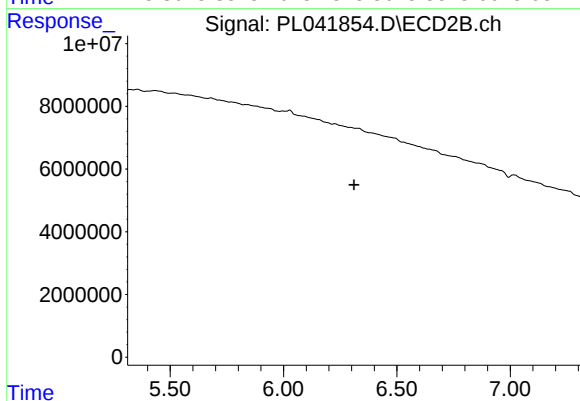

#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

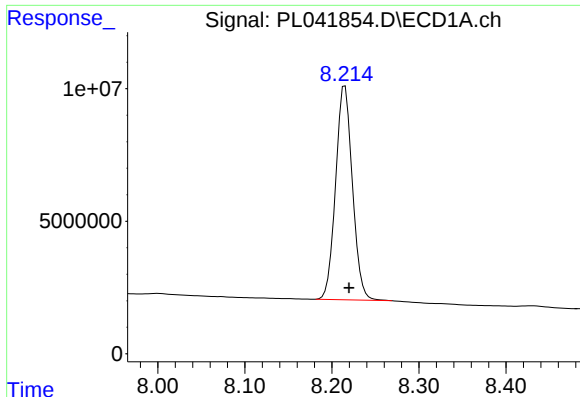

#28 Decachlorobiphenyl


R.T.: 8.215 min

Delta R.T.: -0.004 min

Response: 108341334

Conc: 16.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(1-5)

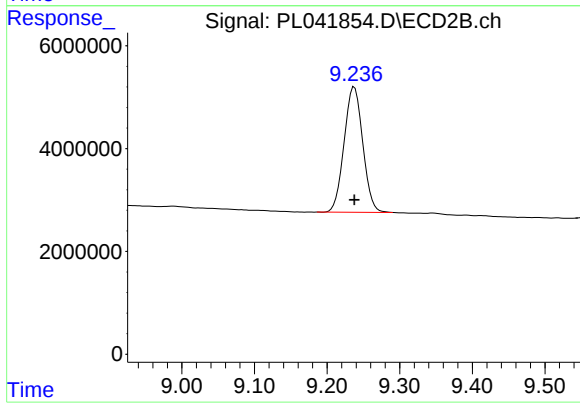

#28 Decachlorobiphenyl

R.T.: 9.238 min

Delta R.T.: 0.000 min

Response: 43627155

Conc: 17.03 ng/ml