

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
 Data File : PL041859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 12:14
 Operator : AJ\SJ
 Sample : J5819-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BES48_WC

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 15:45:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.104	45052581	20175590	7.072	6.550
28)	SA Decachlor...	8.216	9.238	46127574	18945301	6.964	7.394
Target Compounds							
2)	A alpha-BHC	0.000	4.521	0	5419507	N.D.	1.182 #
3)	MA gamma-BHC...	0.000	4.798	0	2922179	N.D.	0.689 #
4)	MA Heptachlor	4.523	0.000	4428889	0	0.483	N.D. #
5)	MB Aldrin	4.769f	0.000	2351502	0	0.279	N.D. #
6)	B beta-BHC	4.438	4.910f	299.9E6	2122363	79.554	1.236 #
7)	B delta-BHC	4.652	0.000	2973452	0	0.358	N.D. #
24)	Chlordane-2	4.894	5.551	2074363	3863512	7.044	29.074 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
Data File : PL041859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 12:14
Operator : AJ\SJ
Sample : J5819-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BES48_WC

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 15:45:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

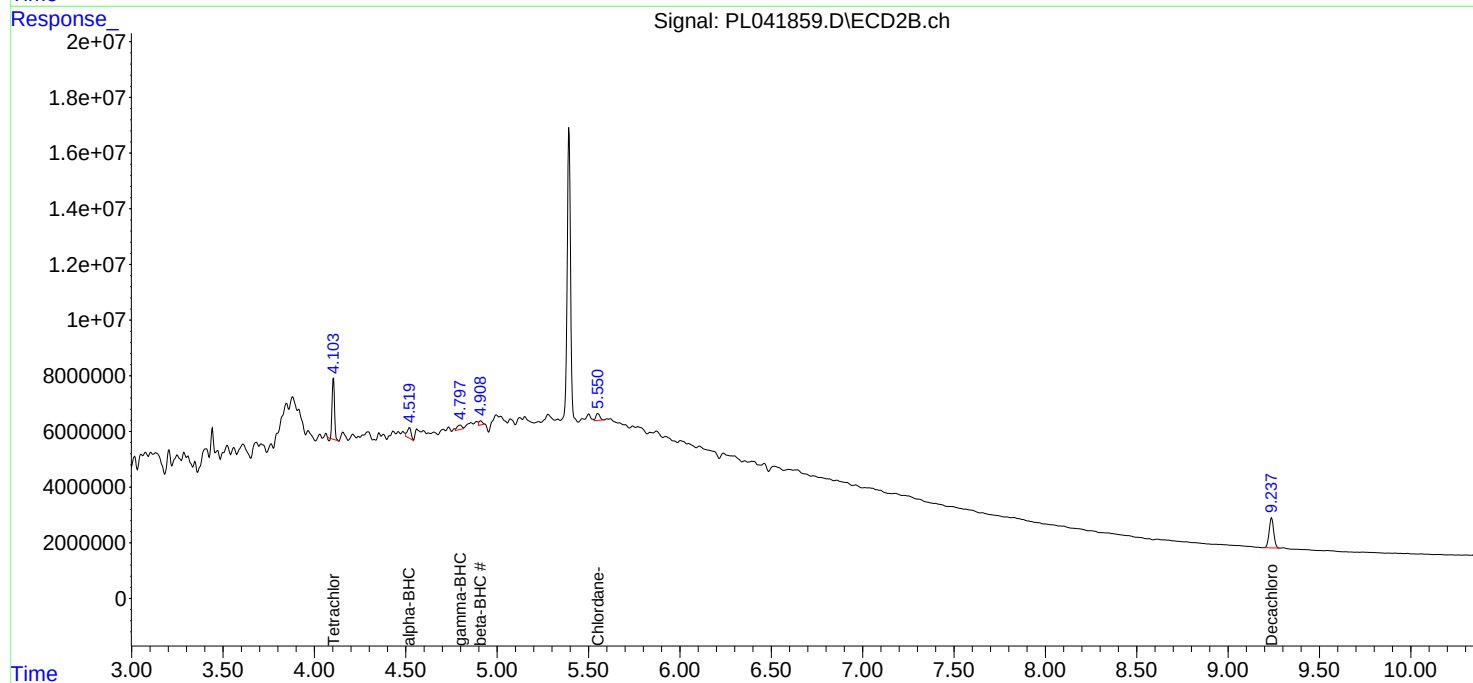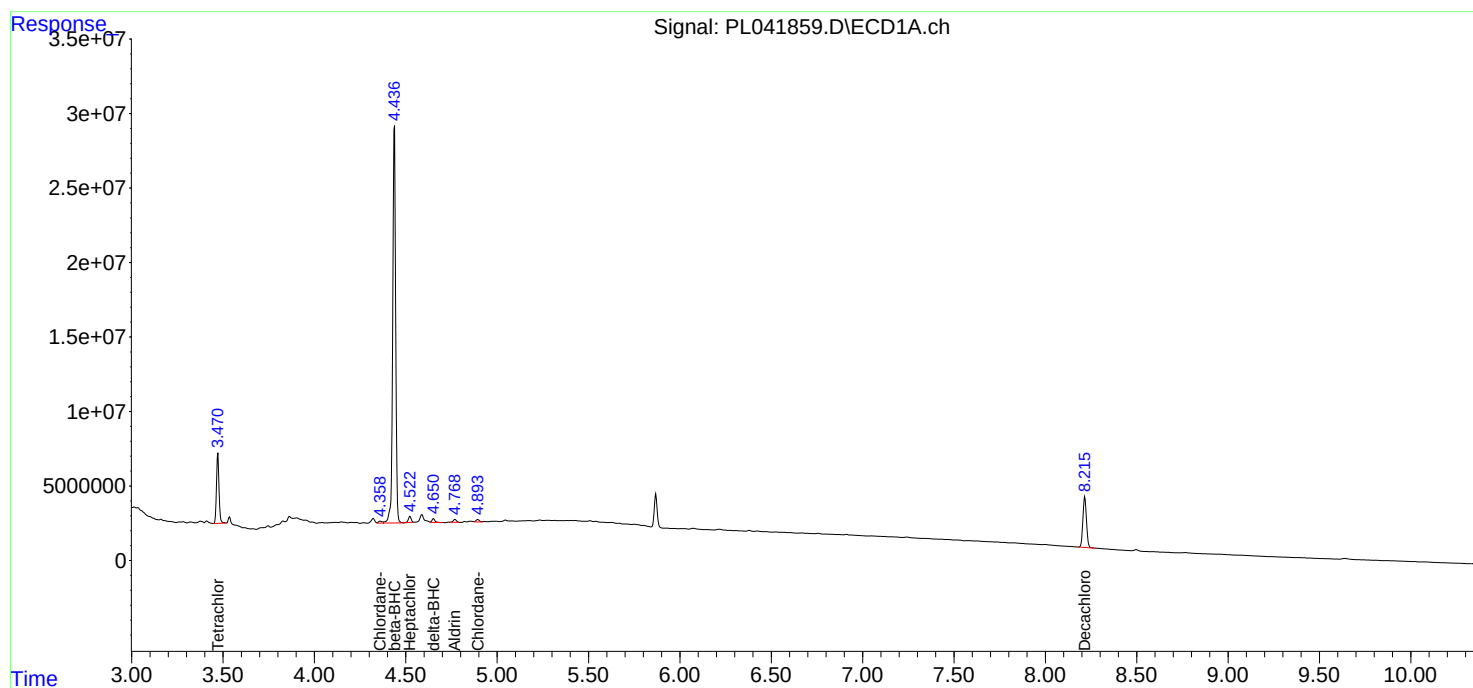


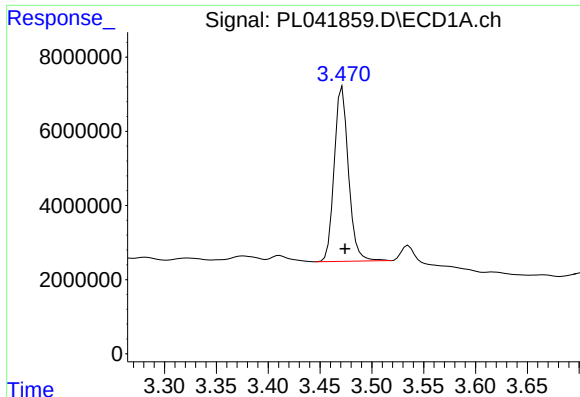

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 45052581
Conc: 7.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
BES48_WC

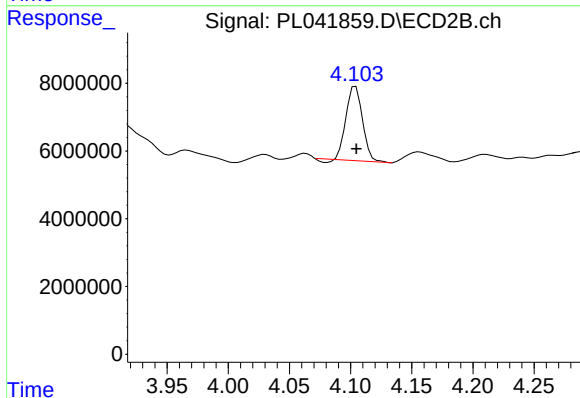


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 20175590
Conc: 6.55 ng/ml

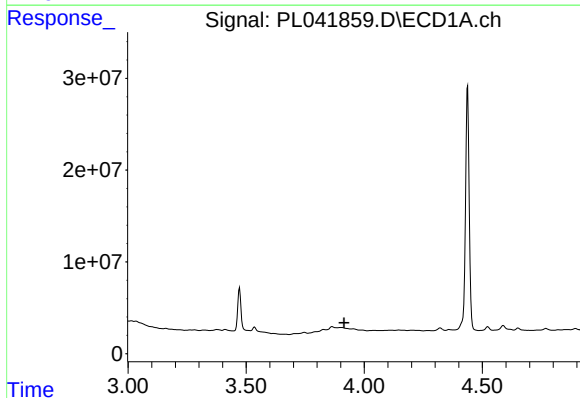


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.915 min
Response: 0
Conc: N.D.

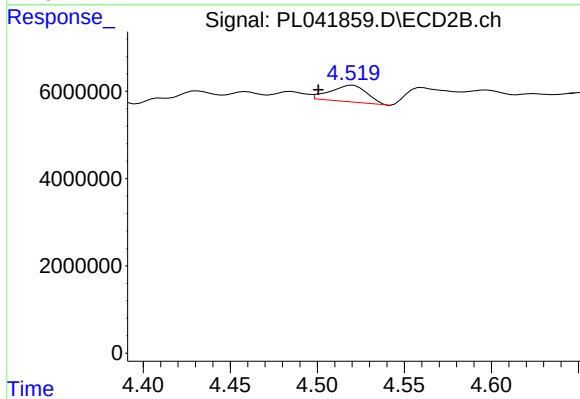

#2 alpha-BHC


R.T.: 4.521 min
Delta R.T.: 0.020 min
Response: 5419507
Conc: 1.18 ng/ml

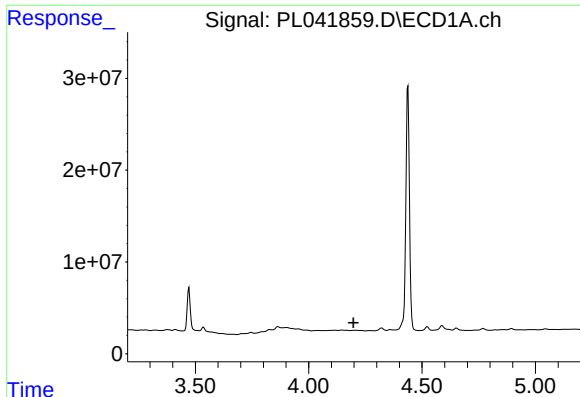

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.198 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BES48_WC

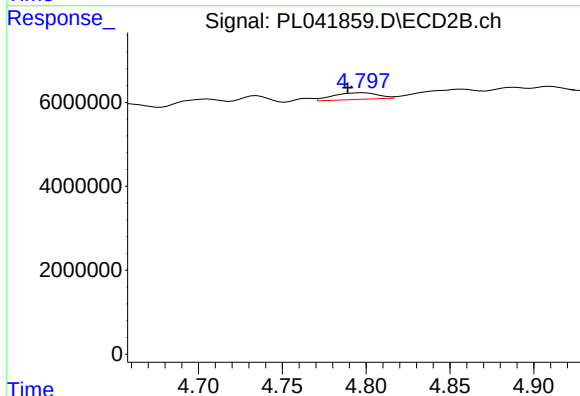


#3 gamma-BHC (Lindane)

R.T.: 4.798 min
Delta R.T.: 0.009 min
Response: 2922179
Conc: 0.69 ng/ml

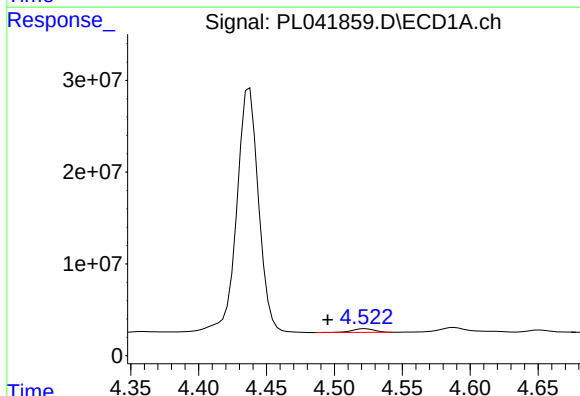


#4 Heptachlor

R.T.: 4.523 min
Delta R.T.: 0.028 min
Response: 4428889
Conc: 0.48 ng/ml

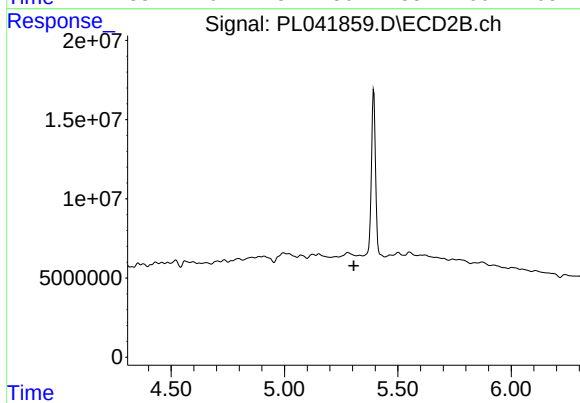

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.305 min
Response: 0
Conc: N.D.

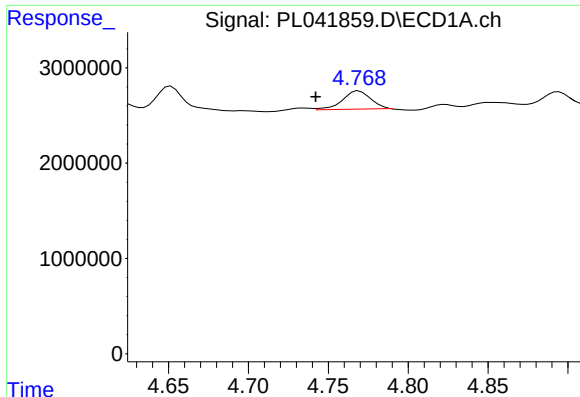

#5 Aldrin


R.T.: 4.769 min
Delta R.T.: 0.027 min
Response: 2351502
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
BES48_WC

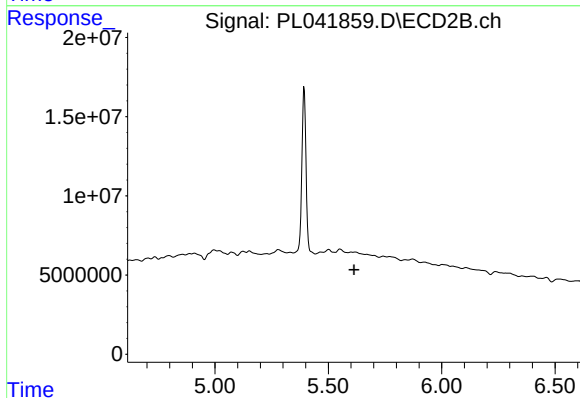


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.614 min
Response: 0
Conc: N.D.

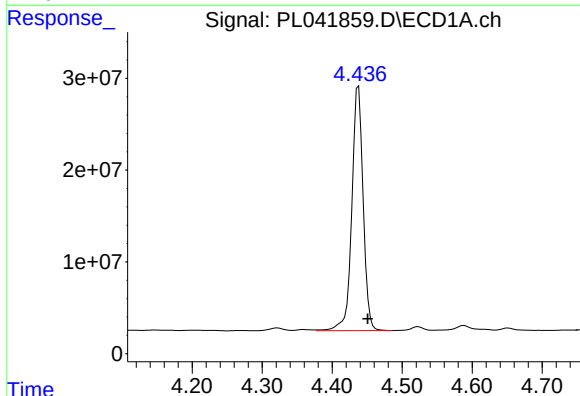


#6 beta-BHC

R.T.: 4.438 min
Delta R.T.: -0.013 min
Response: 299855757
Conc: 79.55 ng/ml

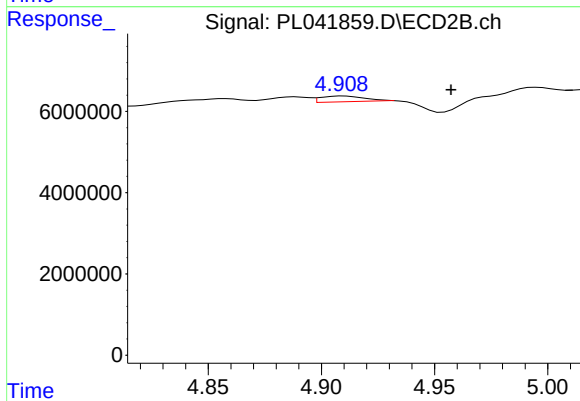

#6 beta-BHC


R.T.: 4.910 min
Delta R.T.: -0.047 min
Response: 2122363
Conc: 1.24 ng/ml

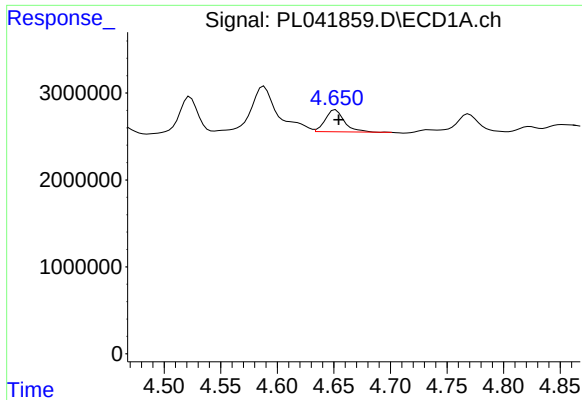

#7 delta-BHC


R.T.: 4.652 min
Delta R.T.: -0.003 min
Response: 2973452
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
BES48_WC

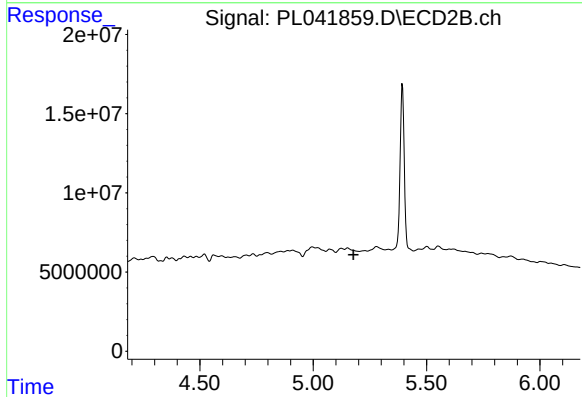


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 5.178 min
Response: 0
Conc: N.D.

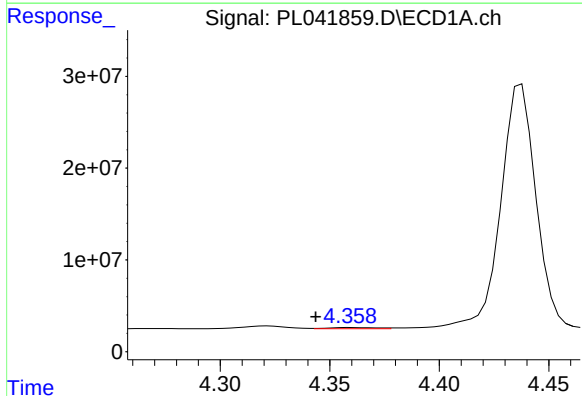


#23 Chlordane-1

R.T.: 4.359 min
Delta R.T.: 0.016 min
Response: 1874819
Conc: 6.61 ng/ml

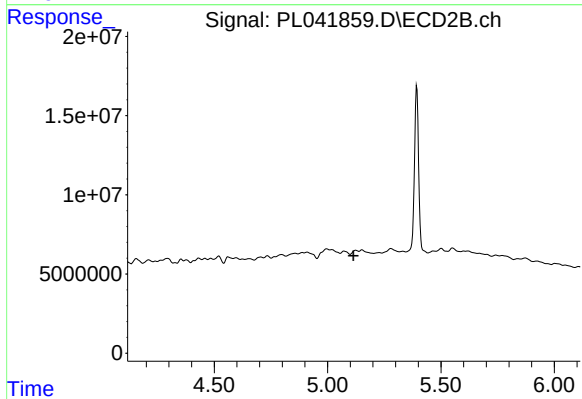

#23 Chlordane-1


R.T.: 5.124 min
Delta R.T.: 0.010 min
Response: -1402536
Conc: N.D.

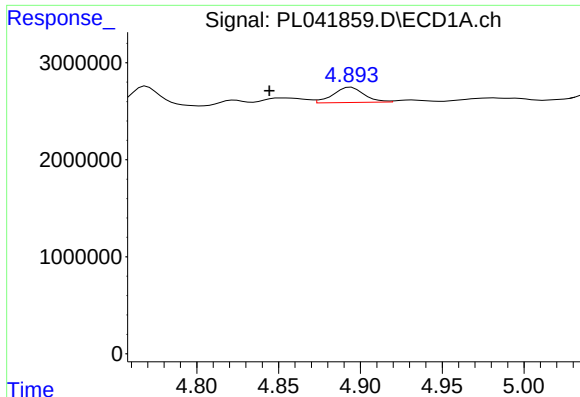

#24 Chlordane-2


R.T.: 4.894 min
Delta R.T.: 0.050 min
Response: 2074363
Conc: 7.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
BES48_WC

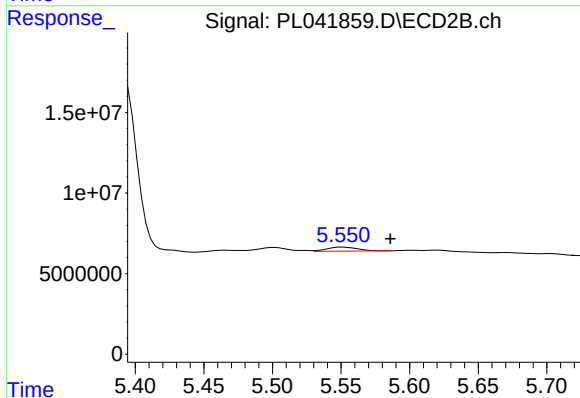


#24 Chlordane-2

R.T.: 5.551 min
Delta R.T.: -0.035 min
Response: 3863512
Conc: 29.07 ng/ml

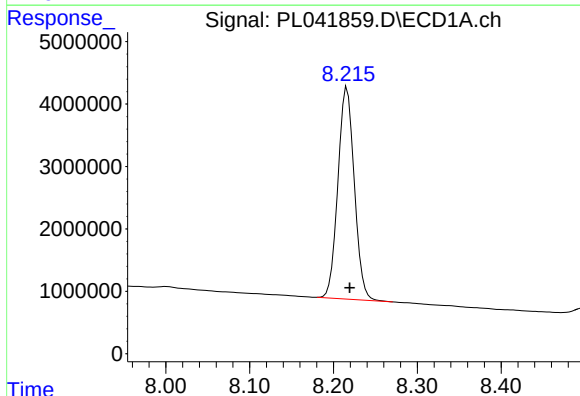

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: -0.003 min
Response: 46127574
Conc: 6.96 ng/ml

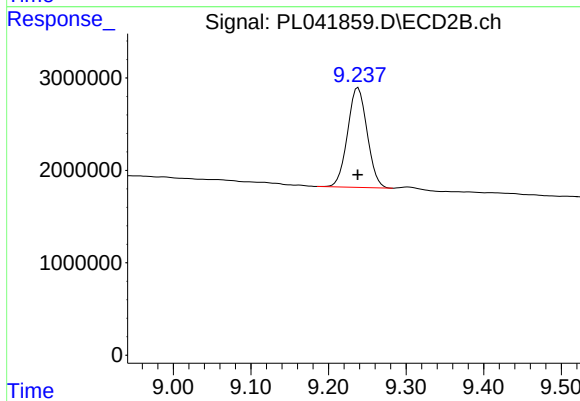

#28 Decachlorobiphenyl

R.T.: 9.238 min
Delta R.T.: 0.000 min
Response: 18945301
Conc: 7.39 ng/ml