

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
 Data File : PL041860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 12:28
 Operator : AJ\SJ
 Sample : J5805-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 15:45:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.105	109.5E6	53051521	17.185	17.223
28)	SA Decachlor...	8.215	9.237	81345577	35510340	12.280	13.860
Target Compounds							
2)	A alpha-BHC	3.946f	4.492	1845344	2375091	0.190	0.518 #
3)	MA gamma-BHC...	0.000	4.835f	0	6860400	N.D.	1.618 #
6)	B beta-BHC	4.408f	0.000	3548591	0	0.941	N.D. #
9)	A Endosulfan I	5.466f	0.000	2083663	0	0.280	N.D. #
10)	B gamma-Chl...	5.466f	0.000	2083663	0	0.256	N.D. #
11)	B alpha-Chl...	5.466	0.000	2083663	0	0.257	N.D. #
23)	Chlordane-1	4.387	0.000	1863281	0	6.572	N.D. #
25)	Chlordane-3	5.466	0.000	2083663	0	2.338	N.D. #
26)	Chlordane-4	5.466	0.000	2083663	0	2.661	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
Data File : PL041860.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 12:28
Operator : AJ\SJ
Sample : J5805-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 15:45:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

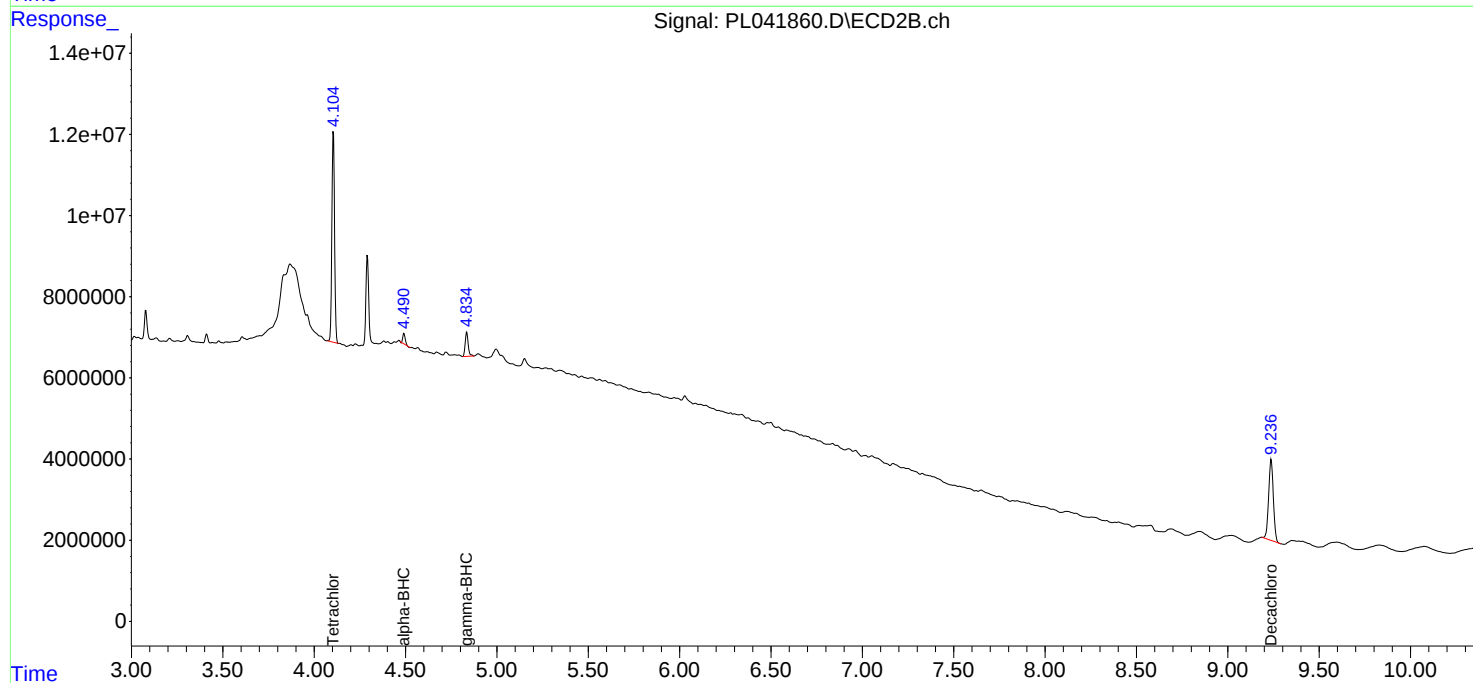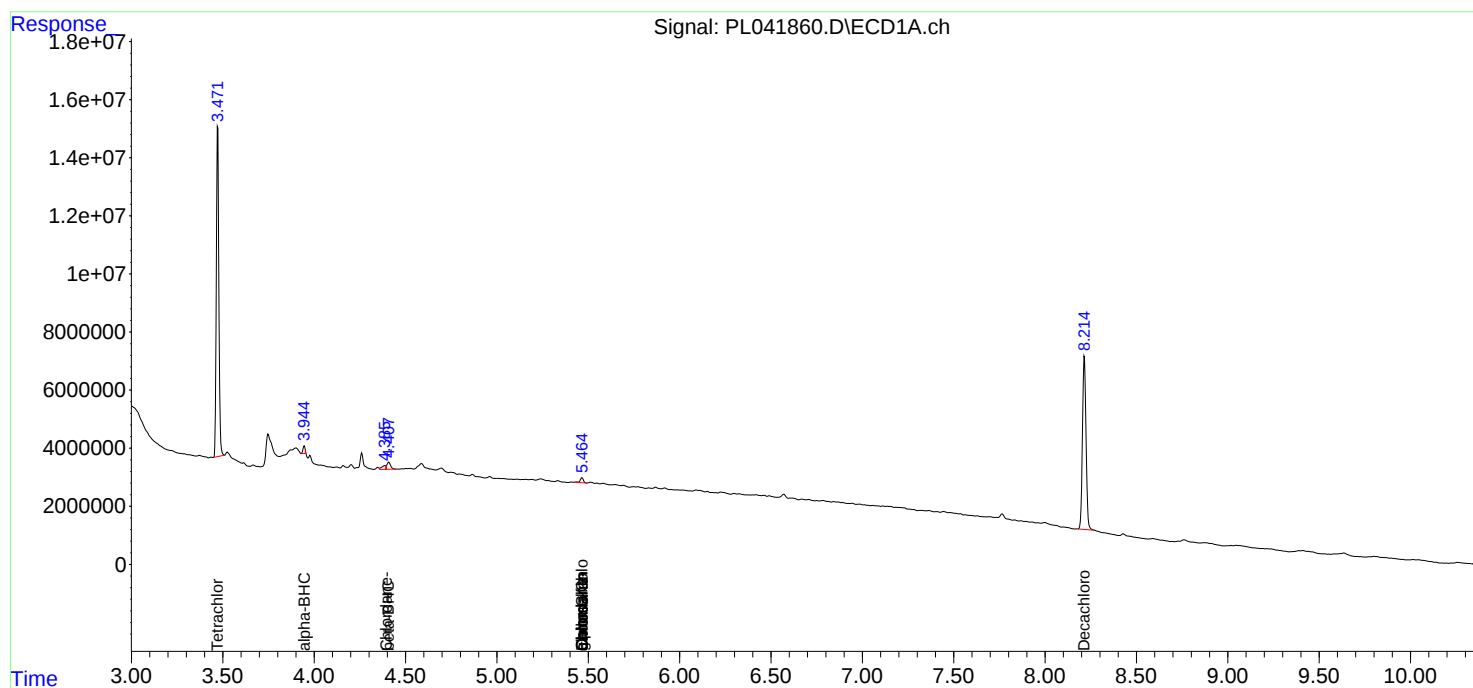


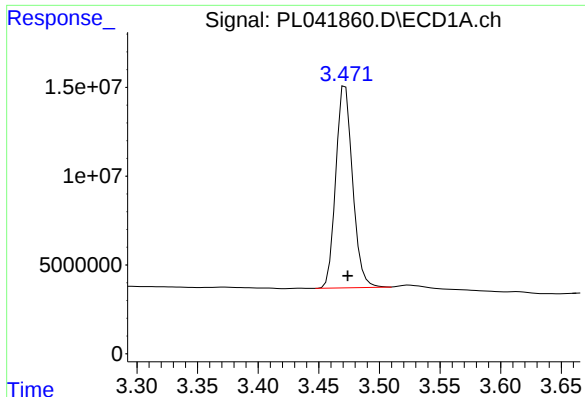

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 109471900
Conc: 17.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

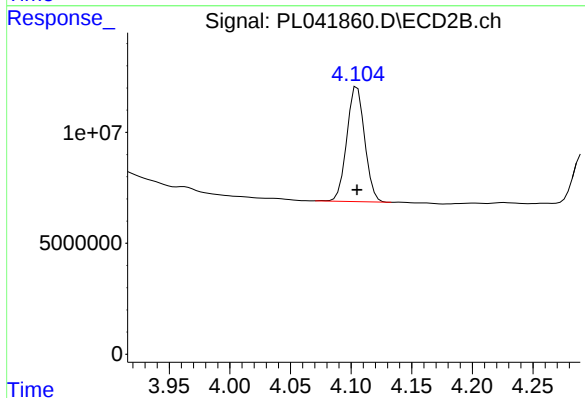


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 53051521
Conc: 17.22 ng/ml

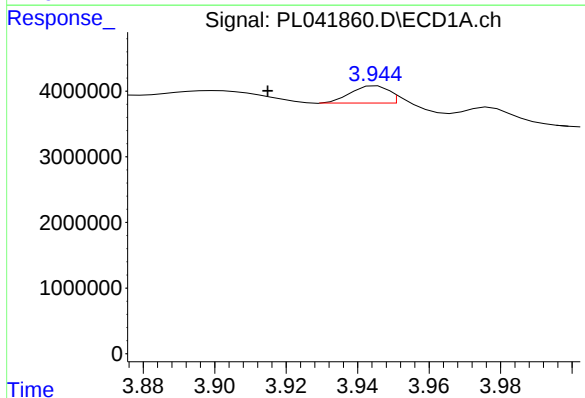


#2 alpha-BHC

R.T.: 3.946 min
Delta R.T.: 0.031 min
Response: 1845344
Conc: 0.19 ng/ml

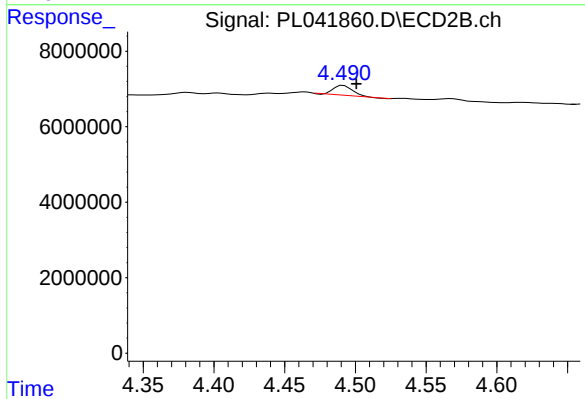

#2 alpha-BHC


R.T.: 4.492 min
Delta R.T.: -0.009 min
Response: 2375091
Conc: 0.52 ng/ml

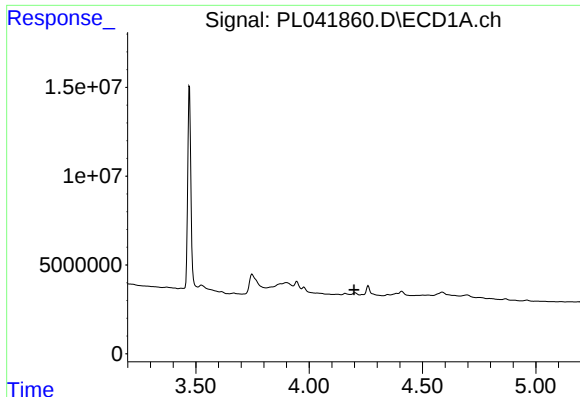

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.198 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

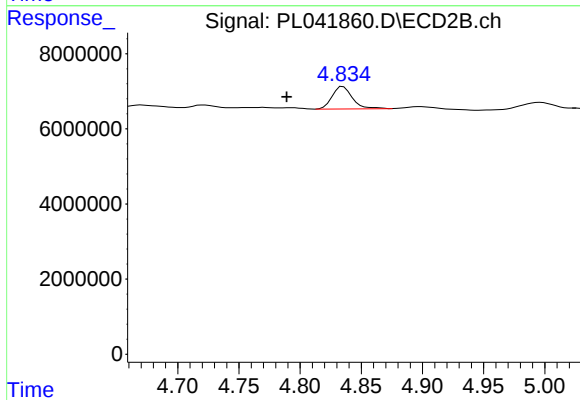


#3 gamma-BHC (Lindane)

R.T.: 4.835 min
Delta R.T.: 0.046 min
Response: 6860400
Conc: 1.62 ng/ml

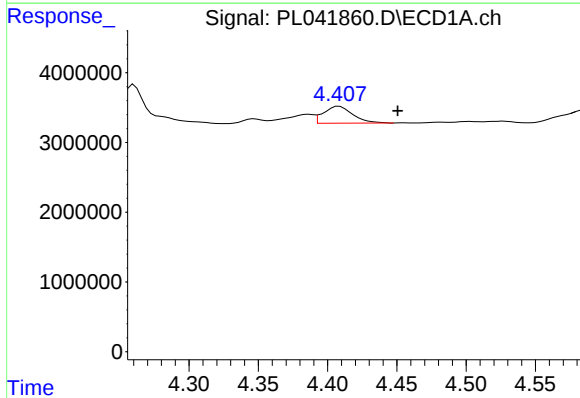


#6 beta-BHC

R.T.: 4.408 min
Delta R.T.: -0.042 min
Response: 3548591
Conc: 0.94 ng/ml

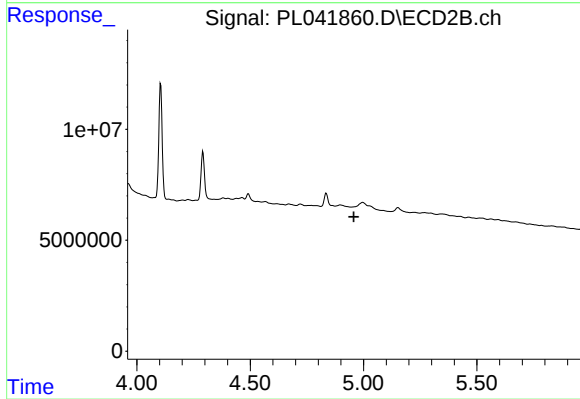

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.957 min
Response: 0
Conc: N.D.

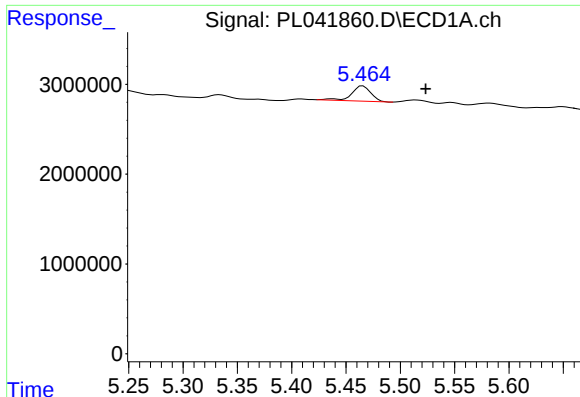

#9 Endosulfan I


R.T.: 5.466 min
Delta R.T.: -0.058 min
Response: 2083663
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

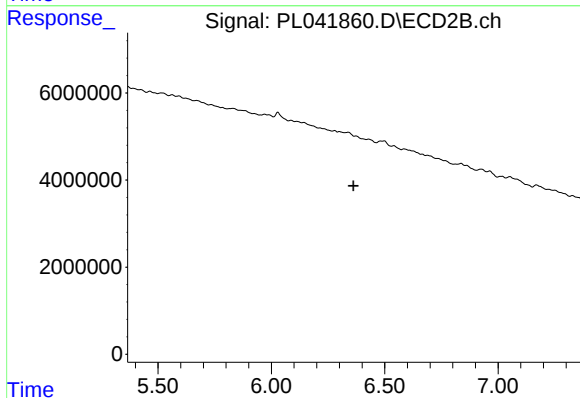


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

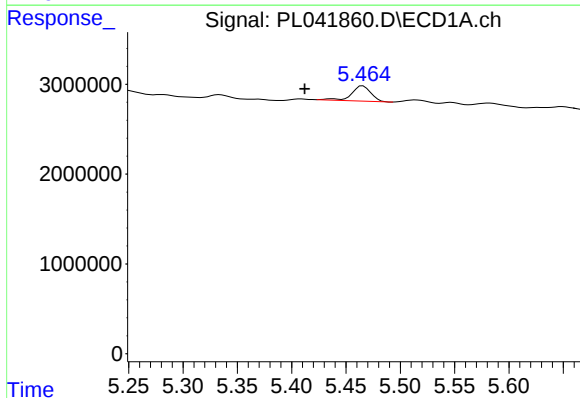


#10 gamma-Chlordane

R.T.: 5.466 min
Delta R.T.: 0.054 min
Response: 2083663
Conc: 0.26 ng/ml

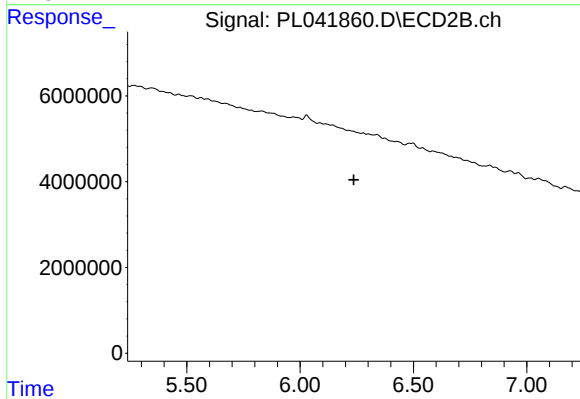

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

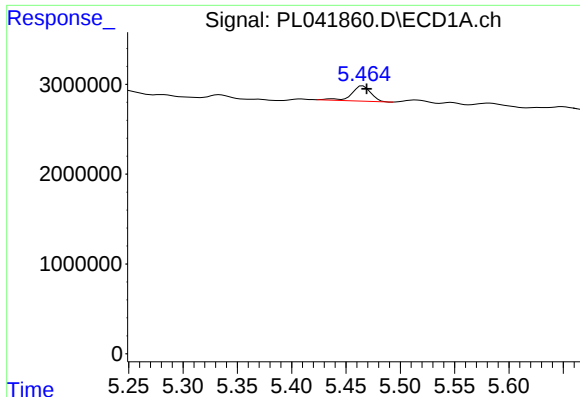

#11 alpha-Chlordane


R.T.: 5.466 min
Delta R.T.: -0.003 min
Response: 2083663
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

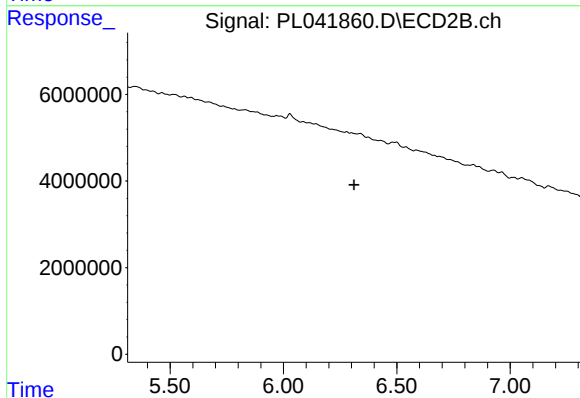


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

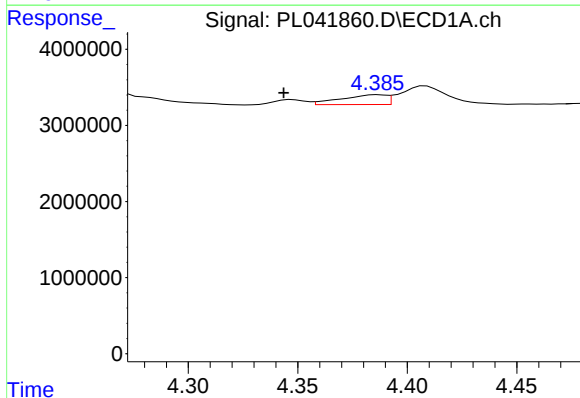


#23 Chlordane-1

R.T.: 4.387 min
Delta R.T.: 0.043 min
Response: 1863281
Conc: 6.57 ng/ml

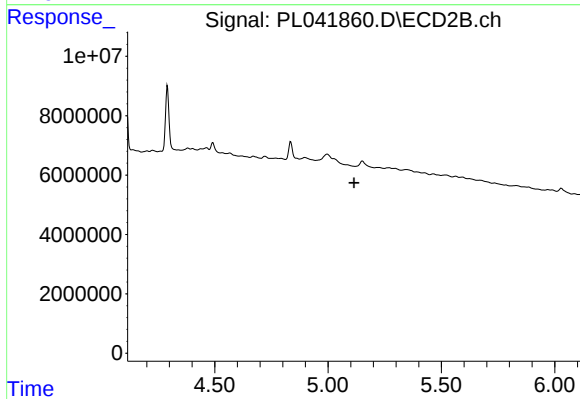

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

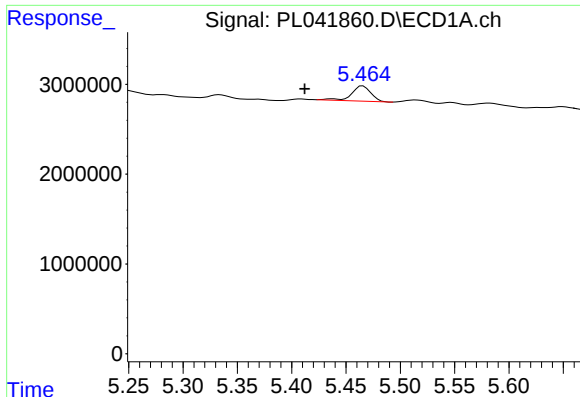

#25 Chlordane-3


R.T.: 5.466 min
Delta R.T.: 0.054 min
Response: 2083663
Conc: 2.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

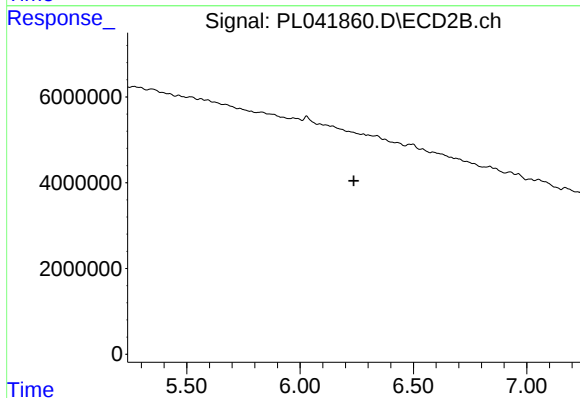


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

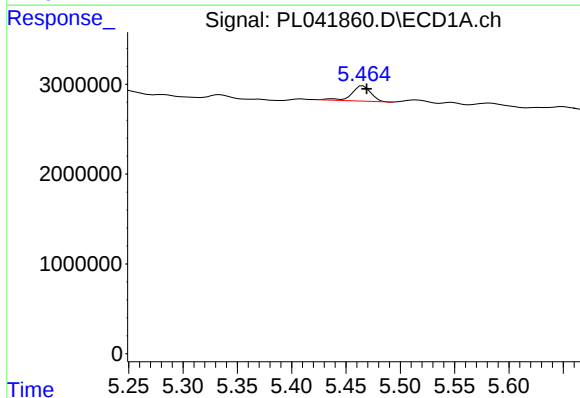


#26 Chlordane-4

R.T.: 5.466 min
Delta R.T.: -0.003 min
Response: 2083663
Conc: 2.66 ng/ml

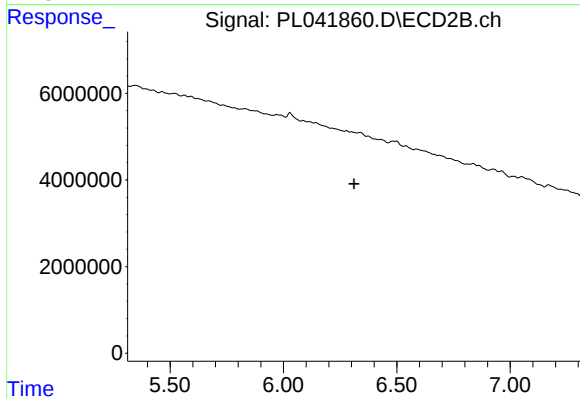

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

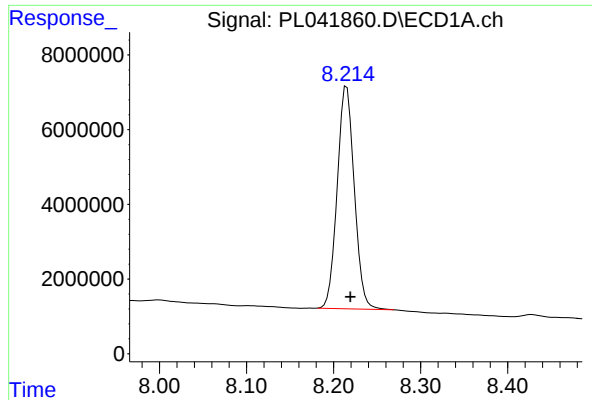

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.004 min
Response: 81345577
Conc: 12.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

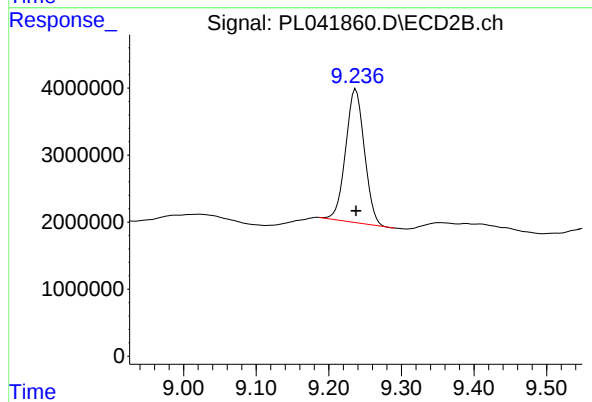

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.000 min
Response: 35510340
Conc: 13.86 ng/ml