

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
 Data File : PL041862.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 12:56
 Operator : AJ\SJ
 Sample : J5805-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-SAMPLES(16-20)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 15:45:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.471	4.105	118.2E6	59429160	18.553	19.294
28)	SA Decachlor...	8.214	9.237	94491214	37247326	14.265	14.537
Target Compounds							
6)	B beta-BHC	4.408f	0.000	2257933	0	0.599	N.D. #
9)	A Endosulfan I	5.465f	0.000	2080856	0	0.280	N.D. #
10)	B gamma-Chl...	5.465f	0.000	2080856	0	0.256	N.D. #
11)	B alpha-Chl...	5.465	0.000	2080856	0	0.257	N.D. #
23)	Chlordane-1	4.408	0.000	2257933	0	7.963	N.D. #
25)	Chlordane-3	5.465	0.000	2080856	0	2.335	N.D. #
26)	Chlordane-4	5.465	0.000	2080856	0	2.658	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
Data File : PL041862.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 12:56
Operator : AJ\SJ
Sample : J5805-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(16-20)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 15:45:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

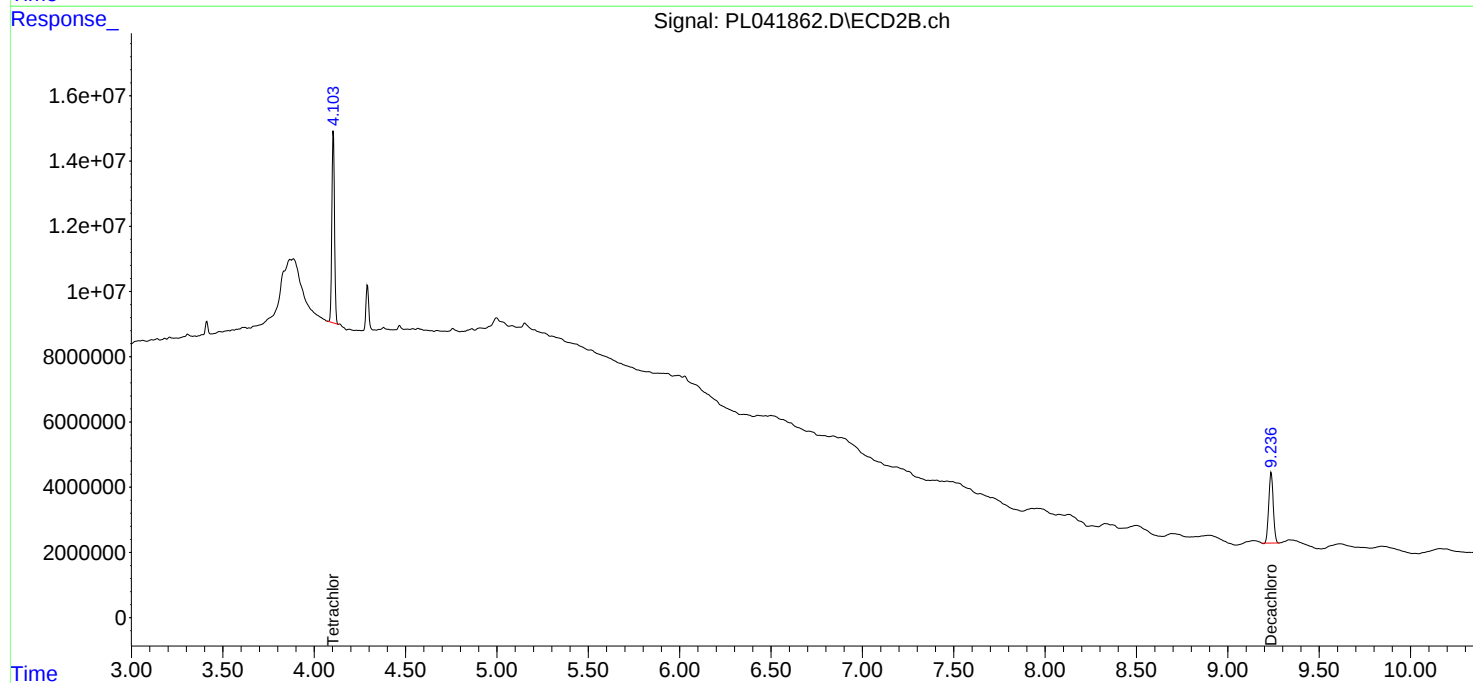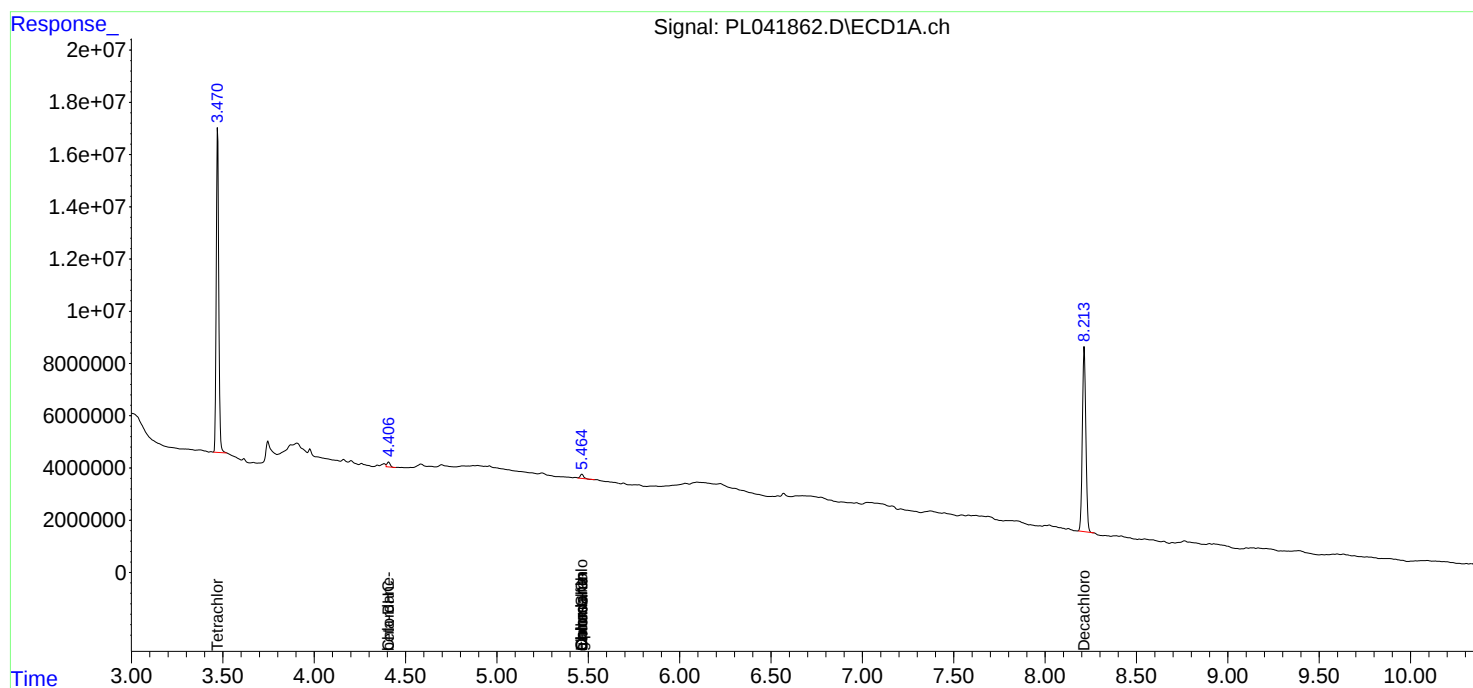


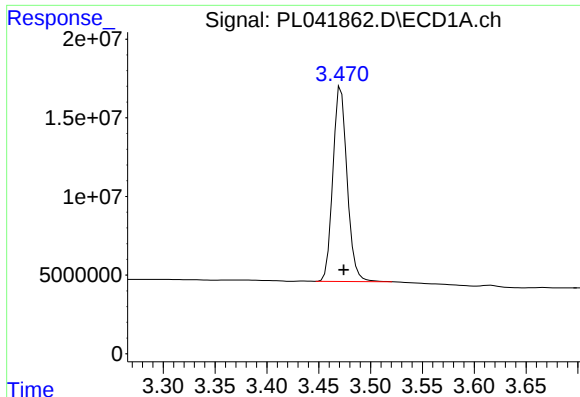

#1 Tetrachloro-m-xylene


R.T.: 3.471 min
Delta R.T.: -0.003 min
Response: 118189359
Conc: 18.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(16-20)

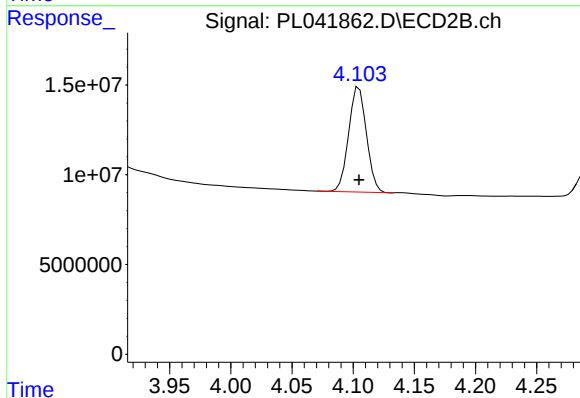


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 59429160
Conc: 19.29 ng/ml

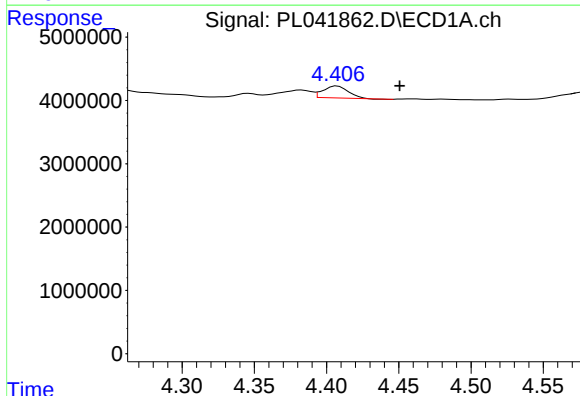


#6 beta-BHC

R.T.: 4.408 min
Delta R.T.: -0.043 min
Response: 2257933
Conc: 0.60 ng/ml

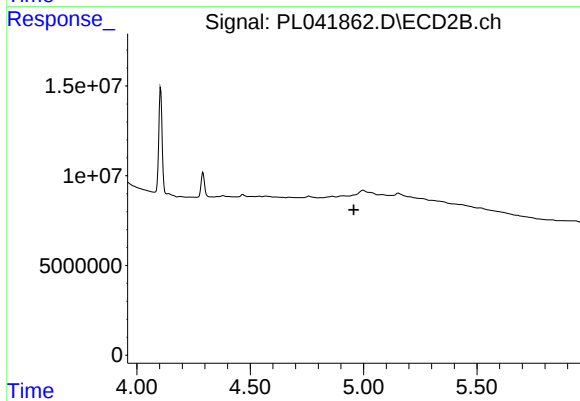

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.957 min
Response: 0
Conc: N.D.

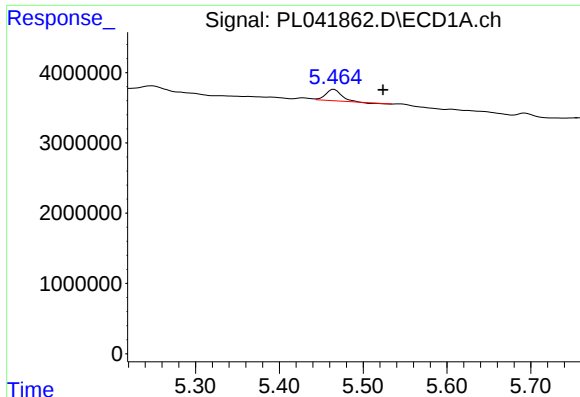

#9 Endosulfan I


R.T.: 5.465 min
Delta R.T.: -0.058 min
Response: 2080856
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(16-20)

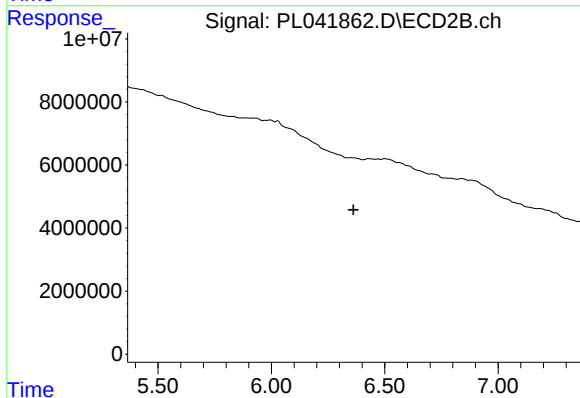


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

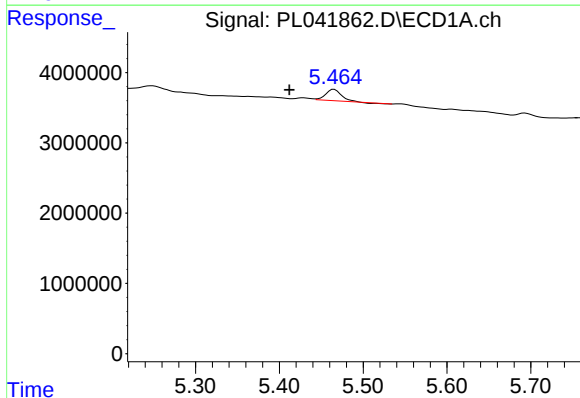


#10 gamma-Chlordane

R.T.: 5.465 min
Delta R.T.: 0.053 min
Response: 2080856
Conc: 0.26 ng/ml

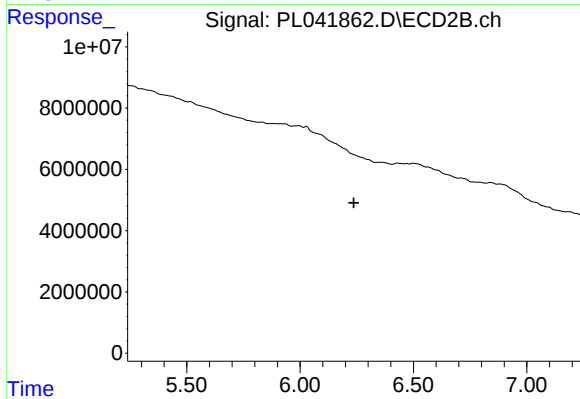

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

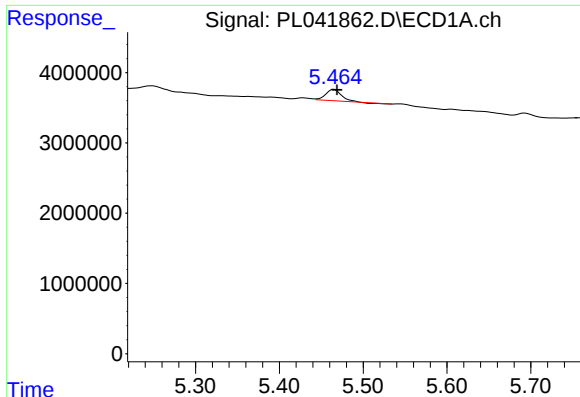

#11 alpha-Chlordane


R.T.: 5.465 min
Delta R.T.: -0.004 min
Response: 2080856
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(16-20)

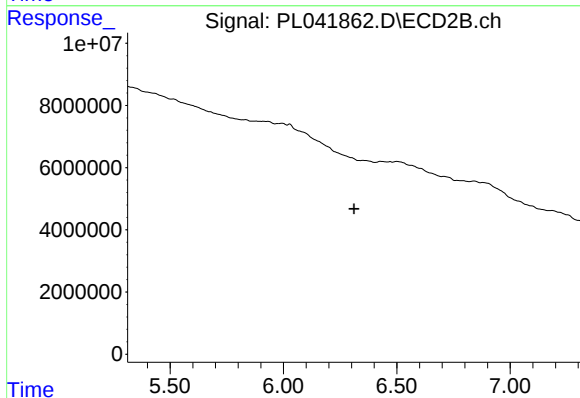


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

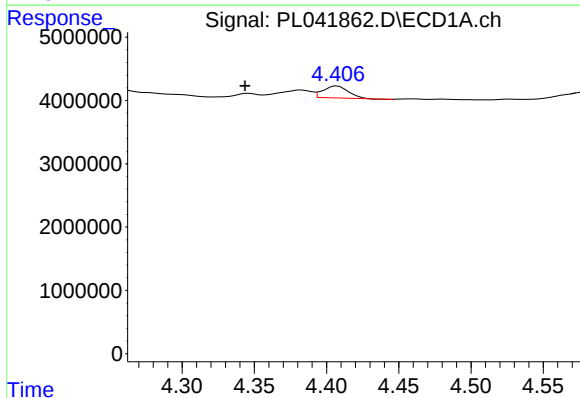


#23 Chlordane-1

R.T.: 4.408 min
Delta R.T.: 0.064 min
Response: 2257933
Conc: 7.96 ng/ml

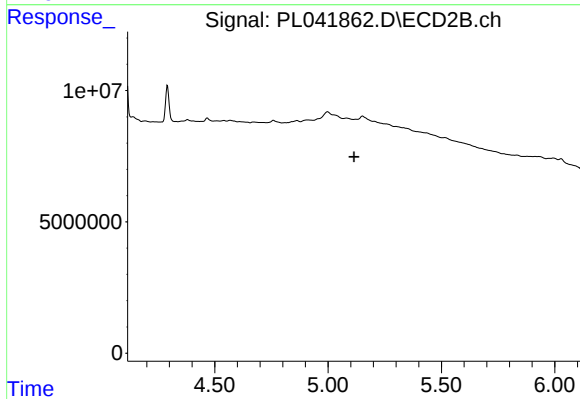

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

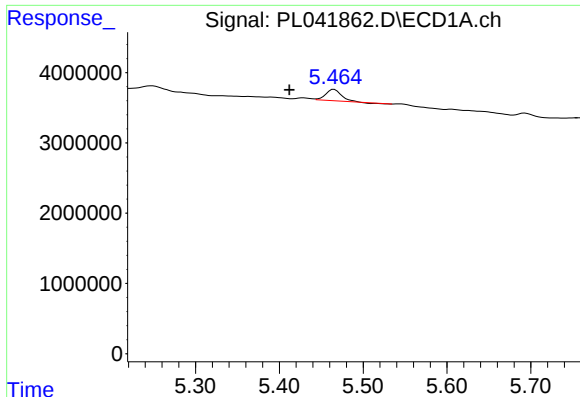

#25 Chlordane-3


R.T.: 5.465 min
Delta R.T.: 0.053 min
Response: 2080856
Conc: 2.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(16-20)

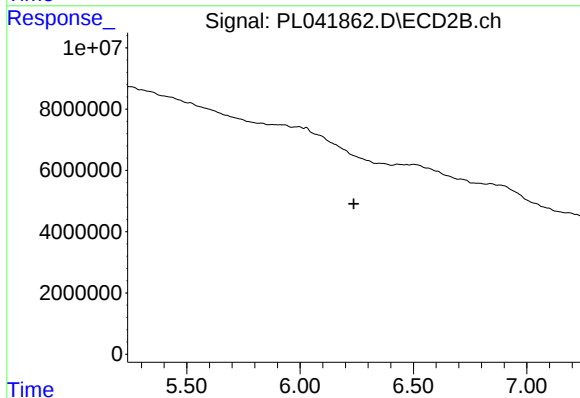


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

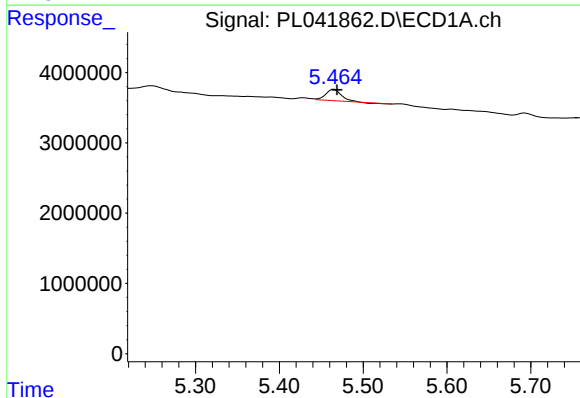


#26 Chlordane-4

R.T.: 5.465 min
Delta R.T.: -0.004 min
Response: 2080856
Conc: 2.66 ng/ml

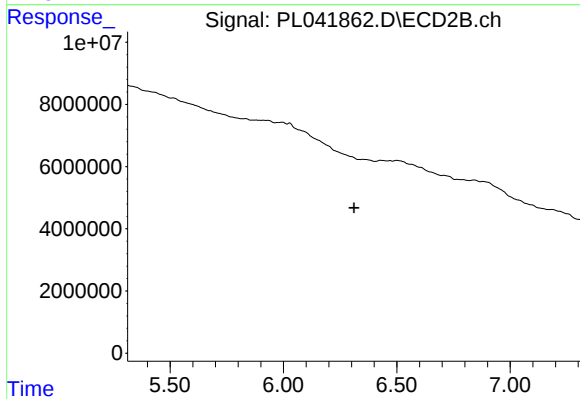

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

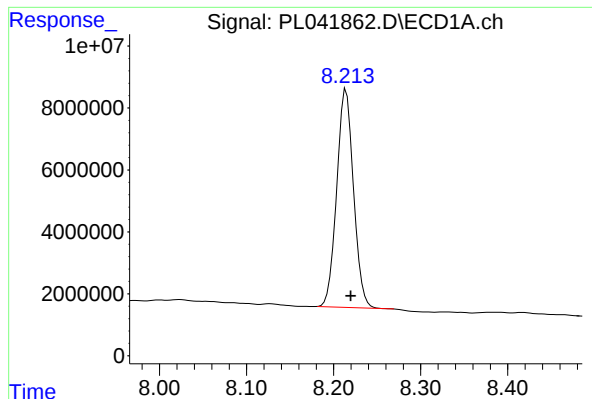

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.005 min
Response: 94491214
Conc: 14.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(16-20)

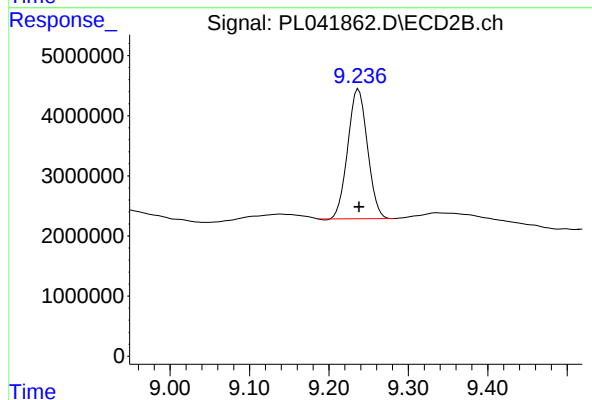

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.000 min
Response: 37247326
Conc: 14.54 ng/ml