

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
 Data File : PL041864.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 13:24
 Operator : AJ\SJ
 Sample : J5805-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 15:45:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.105	122.6E6	64142954	19.252	20.824
28)	SA Decachlor...	8.215	9.237	86797469	37228987	13.104	14.530
Target Compounds							
2)	A alpha-BHC	3.946f	4.491	2109298	-493361	0.217	N.D. #
3)	MA gamma-BHC...	0.000	4.835f	0	5756323	N.D.	1.358 #
6)	B beta-BHC	4.407f	0.000	2417133	0	0.641	N.D. #
8)	B Heptachlo...	5.226f	0.000	1061776	0	0.132	N.D. #
9)	A Endosulfan I	5.466f	0.000	2185014	0	0.294	N.D. #
10)	B gamma-Chl...	5.466f	0.000	2185014	0	0.268	N.D. #
11)	B alpha-Chl...	5.466	0.000	2185014	0	0.270	N.D. #
23)	Chlordane-1	4.346	0.000	1832472	0	6.463	N.D. #
25)	Chlordane-3	5.466	0.000	2185014	0	2.452	N.D. #
26)	Chlordane-4	5.466	0.000	2185014	0	2.791	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
Data File : PL041864.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 13:24
Operator : AJ\SJ
Sample : J5805-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 15:45:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

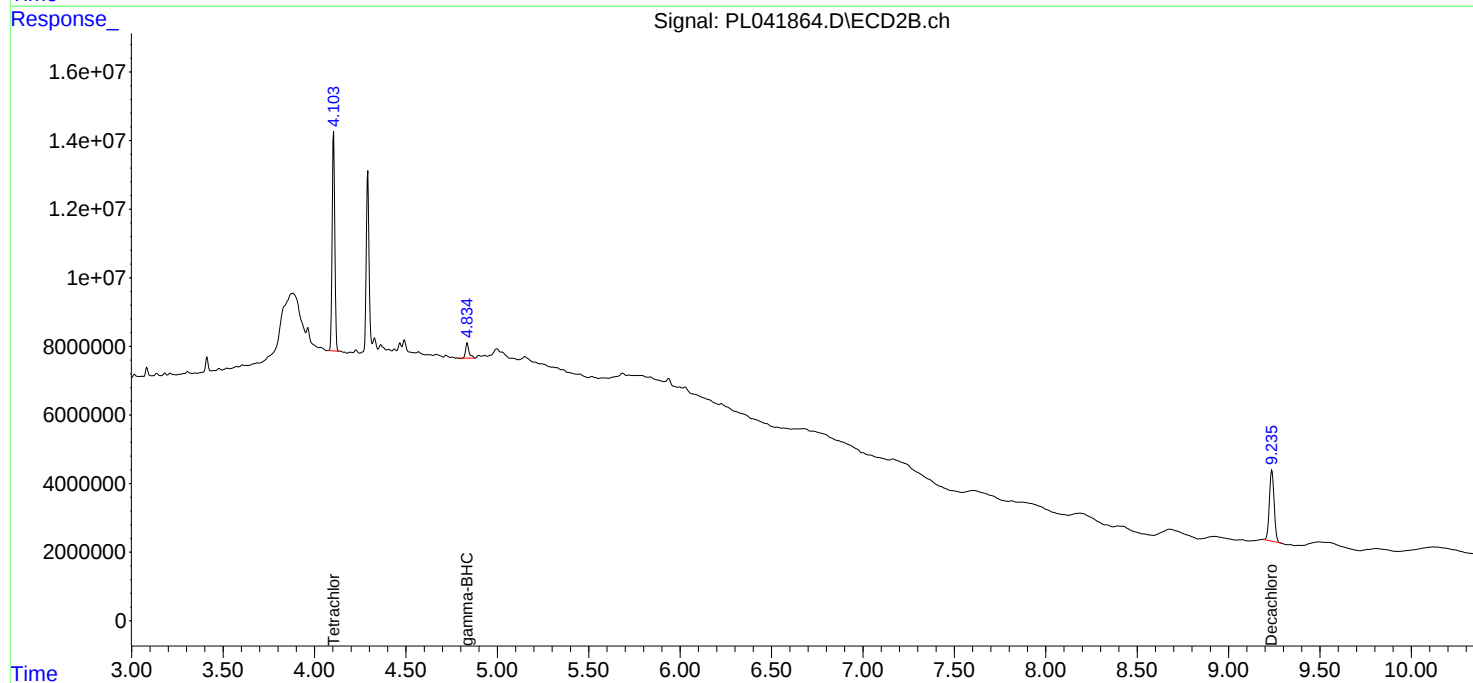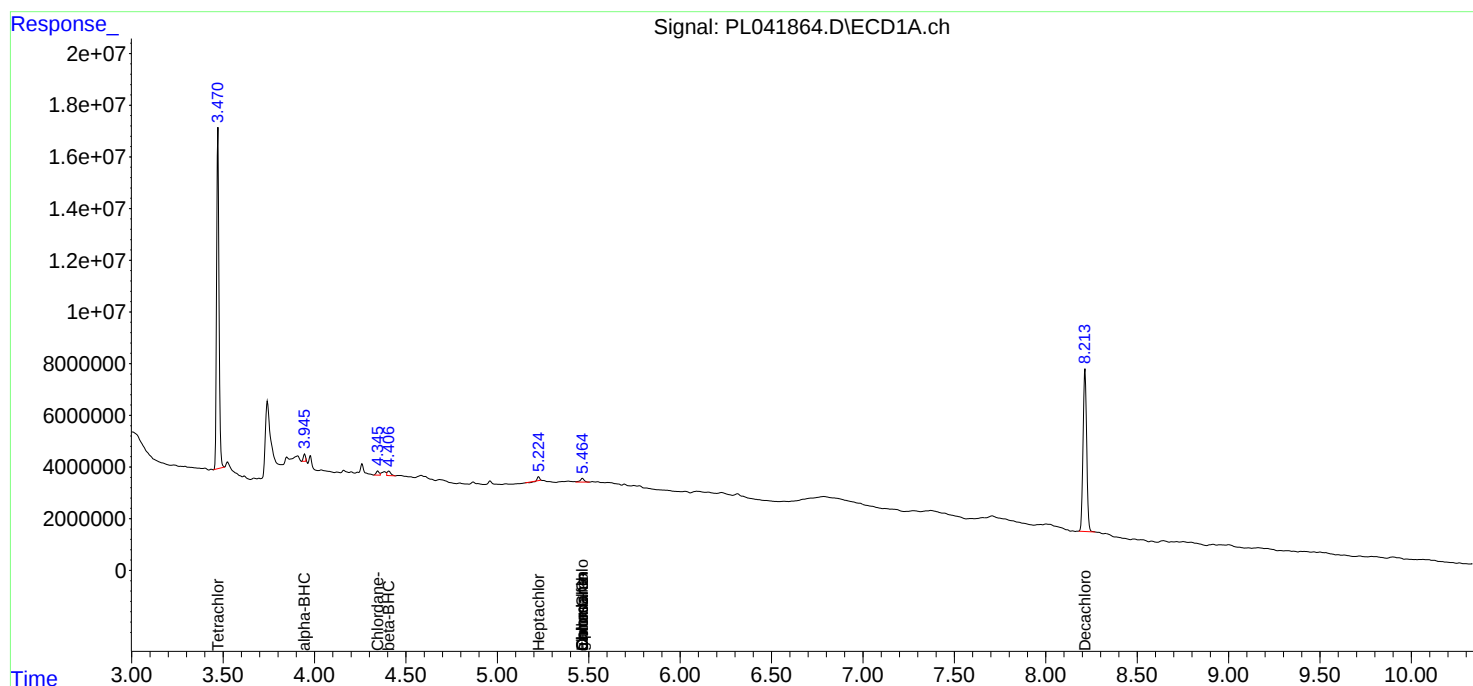


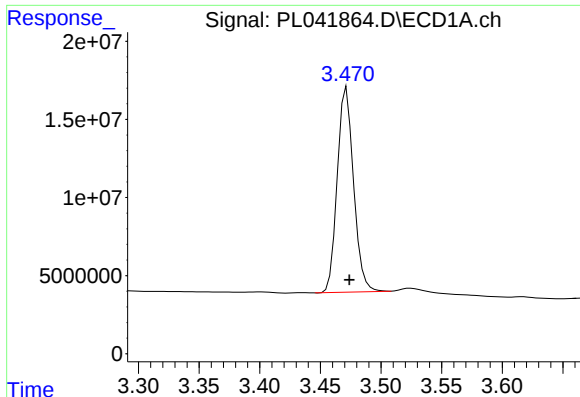

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 122636670
Conc: 19.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

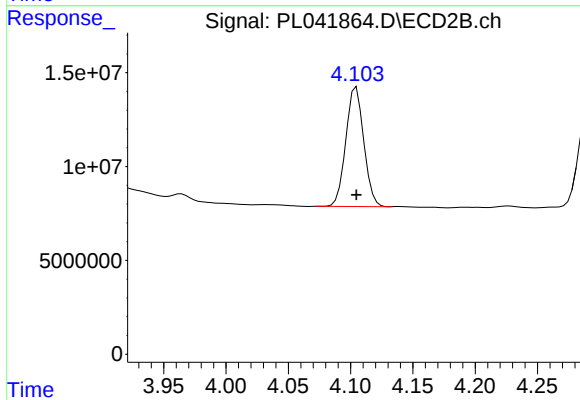


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 64142954
Conc: 20.82 ng/ml

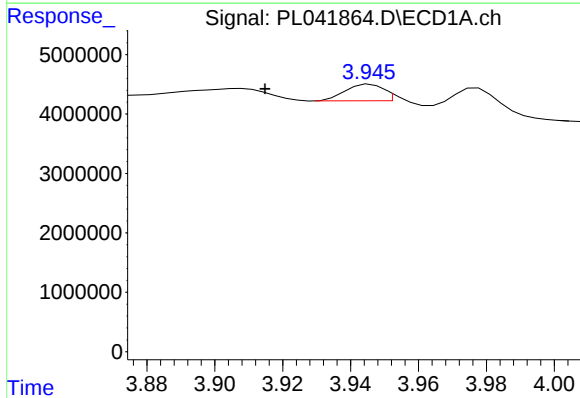


#2 alpha-BHC

R.T.: 3.946 min
Delta R.T.: 0.031 min
Response: 2109298
Conc: 0.22 ng/ml

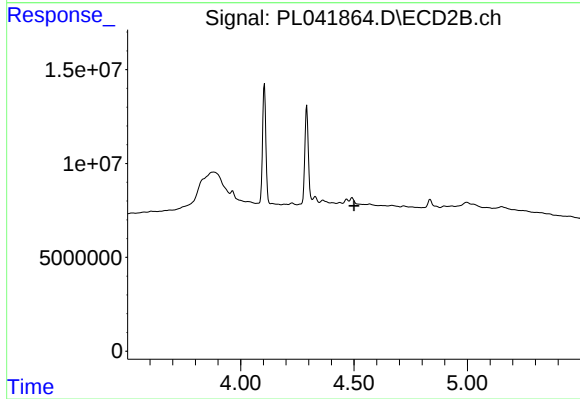

#2 alpha-BHC


R.T.: 4.491 min
Delta R.T.: -0.009 min
Response: -493361
Conc: N.D.

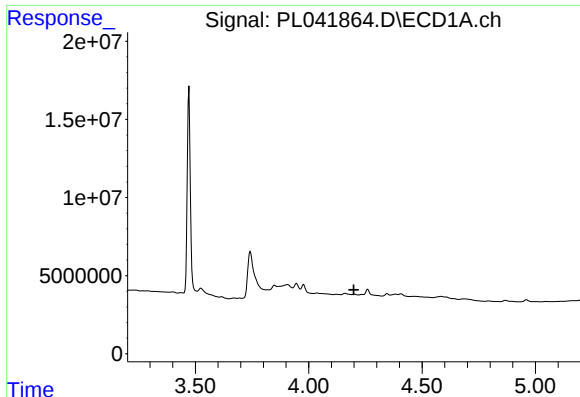

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.198 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

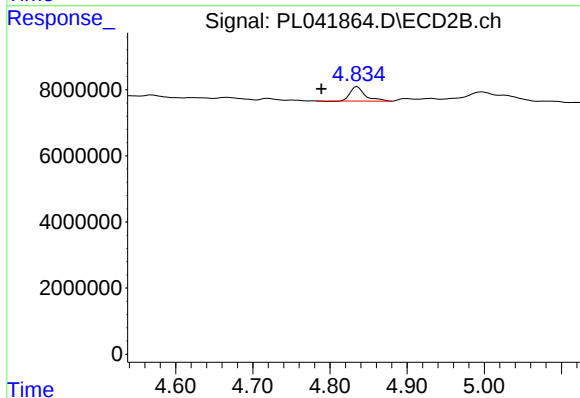


#3 gamma-BHC (Lindane)

R.T.: 4.835 min
Delta R.T.: 0.046 min
Response: 5756323
Conc: 1.36 ng/ml

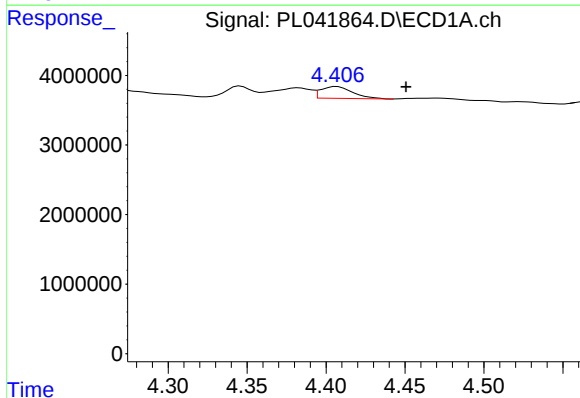


#6 beta-BHC

R.T.: 4.407 min
Delta R.T.: -0.044 min
Response: 2417133
Conc: 0.64 ng/ml

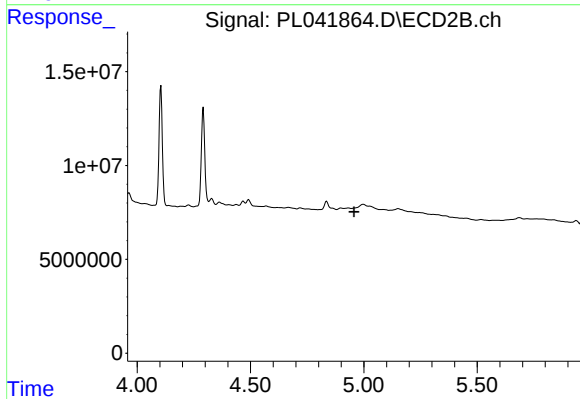

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.957 min
Response: 0
Conc: N.D.

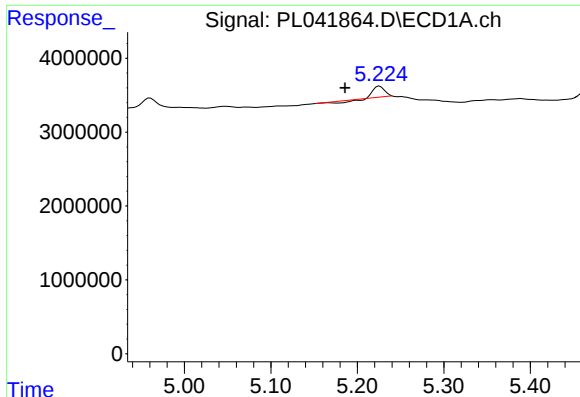

#8 Heptachlor epoxide


R.T.: 5.226 min
Delta R.T.: 0.040 min
Response: 1061776
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

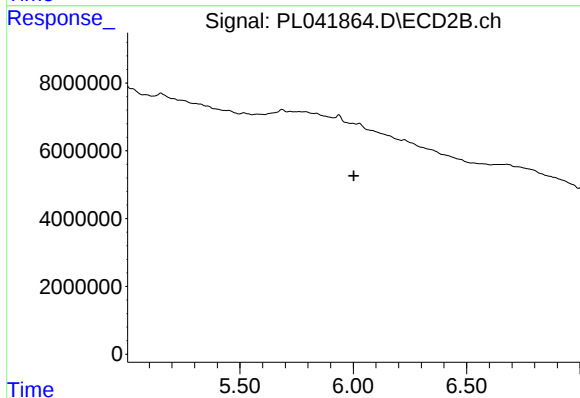


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.002 min
Response: 0
Conc: N.D.

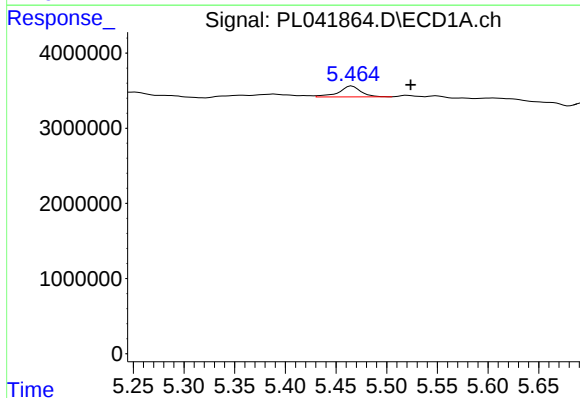


#9 Endosulfan I

R.T.: 5.466 min
Delta R.T.: -0.058 min
Response: 2185014
Conc: 0.29 ng/ml

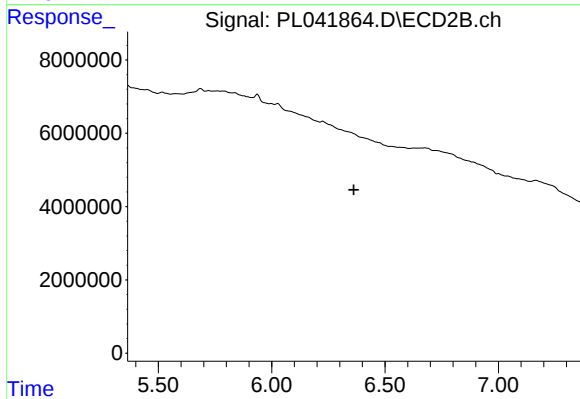

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

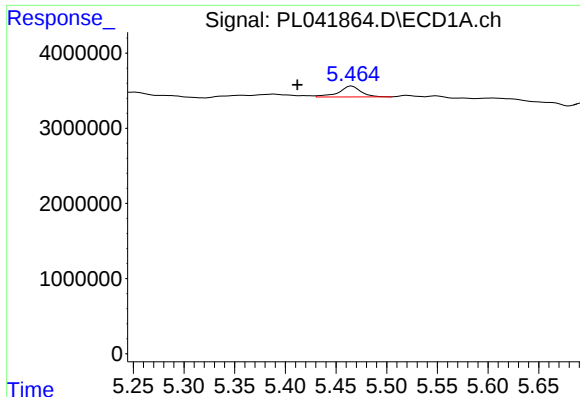

#10 gamma-Chlordane


R.T.: 5.466 min
Delta R.T.: 0.054 min
Response: 2185014
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

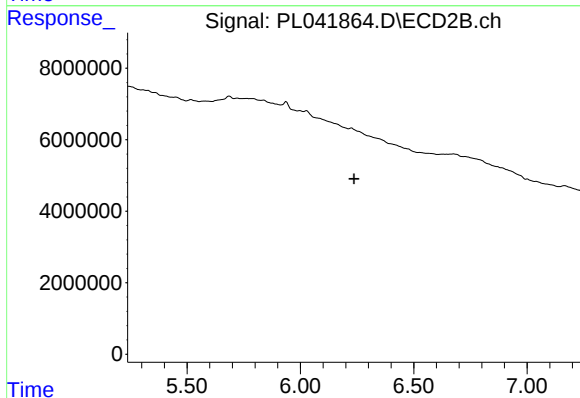


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

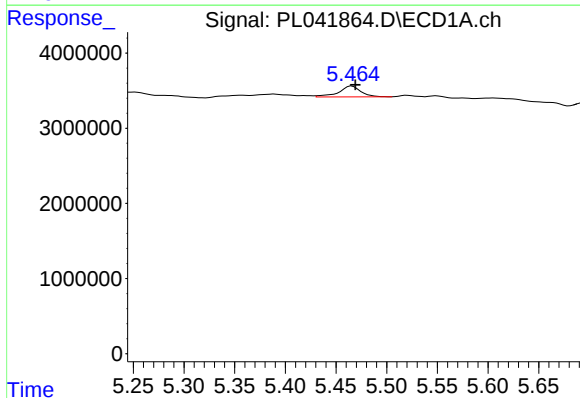


#11 alpha-Chlordane

R.T.: 5.466 min
Delta R.T.: -0.003 min
Response: 2185014
Conc: 0.27 ng/ml

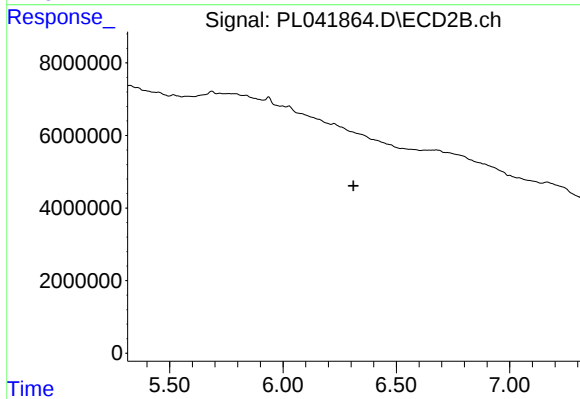

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

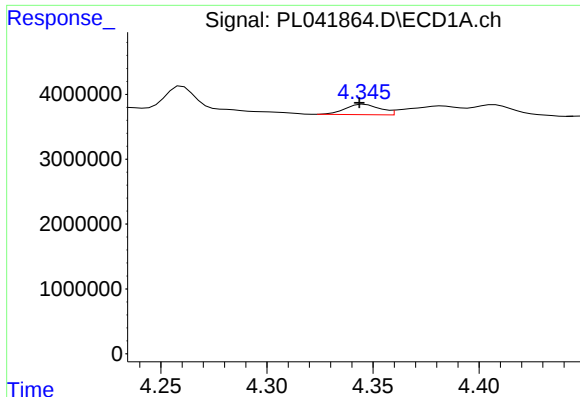

#23 Chlordane-1


R.T.: 4.346 min
Delta R.T.: 0.002 min
Response: 1832472
Conc: 6.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

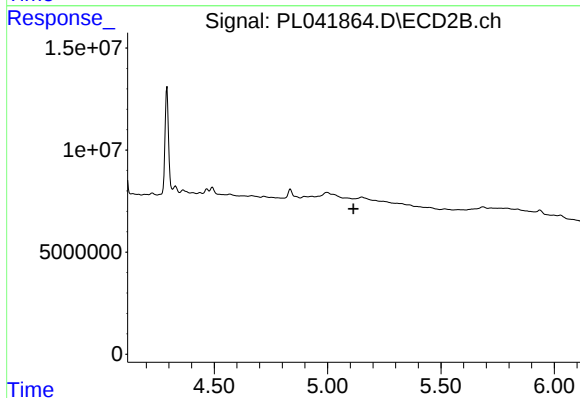


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

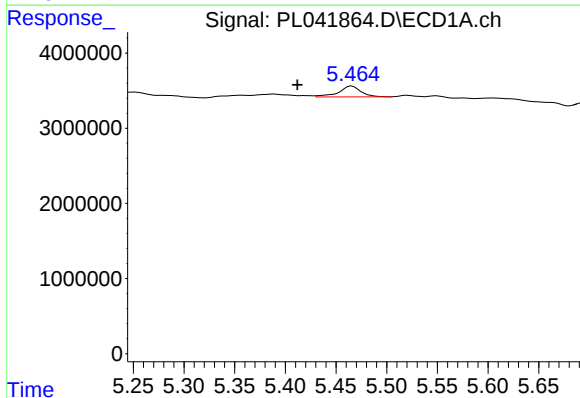


#25 Chlordane-3

R.T.: 5.466 min
Delta R.T.: 0.054 min
Response: 2185014
Conc: 2.45 ng/ml

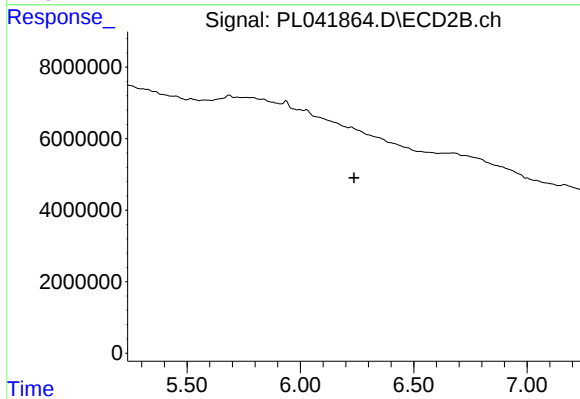

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

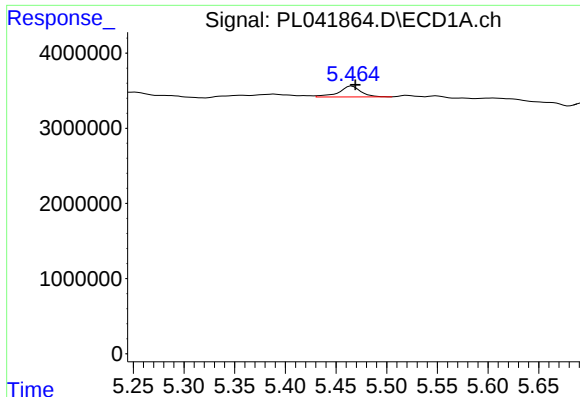

#26 Chlordane-4


R.T.: 5.466 min
Delta R.T.: -0.003 min
Response: 2185014
Conc: 2.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

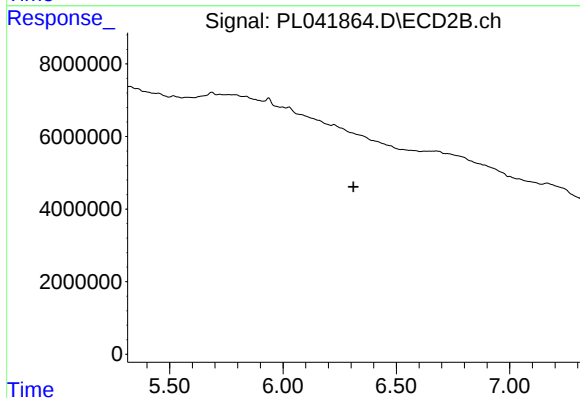


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

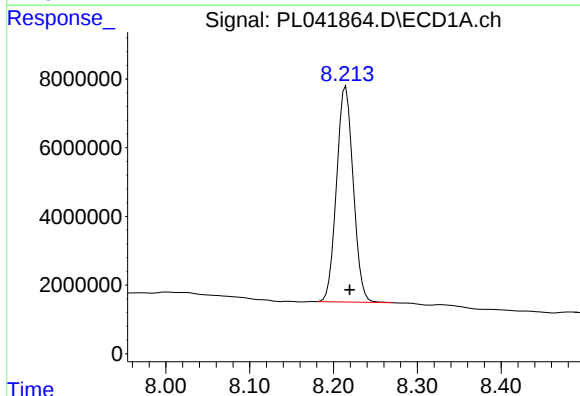

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.005 min
Response: 86797469
Conc: 13.10 ng/ml

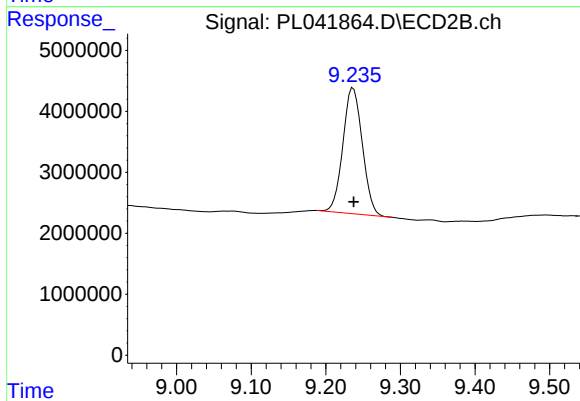

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: -0.001 min
Response: 37228987
Conc: 14.53 ng/ml