

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
 Data File : PL041865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 13:38
 Operator : AJ\SJ
 Sample : J5805-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-SAMPLES(31-35)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 15:46:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.105	125.8E6	65770734	19.742	21.353
28)	SA Decachlor...	8.214	9.239	101.9E6	41902288	15.377	16.354
Target Compounds							
3)	MA gamma-BHC...	0.000	4.836f	0	3341627	N.D.	0.788 #
8)	B Heptachlo...	5.225f	5.938f	277106	1589090	0.034	0.452 #
9)	A Endosulfan I	5.466f	0.000	2473818	0	0.332	N.D. #
10)	B gamma-Chl...	5.466f	0.000	2473818	0	0.304	N.D. #
11)	B alpha-Chl...	5.466	0.000	2473818	0	0.306	N.D. #
23)	Chlordane-1	4.383	0.000	5658780	0	19.958	N.D. #
25)	Chlordane-3	5.466	0.000	2473818	0	2.776	N.D. #
26)	Chlordane-4	5.466	0.000	2473818	0	3.160	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
Data File : PL041865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 13:38
Operator : AJ\SJ
Sample : J5805-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(31-35)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 15:46:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

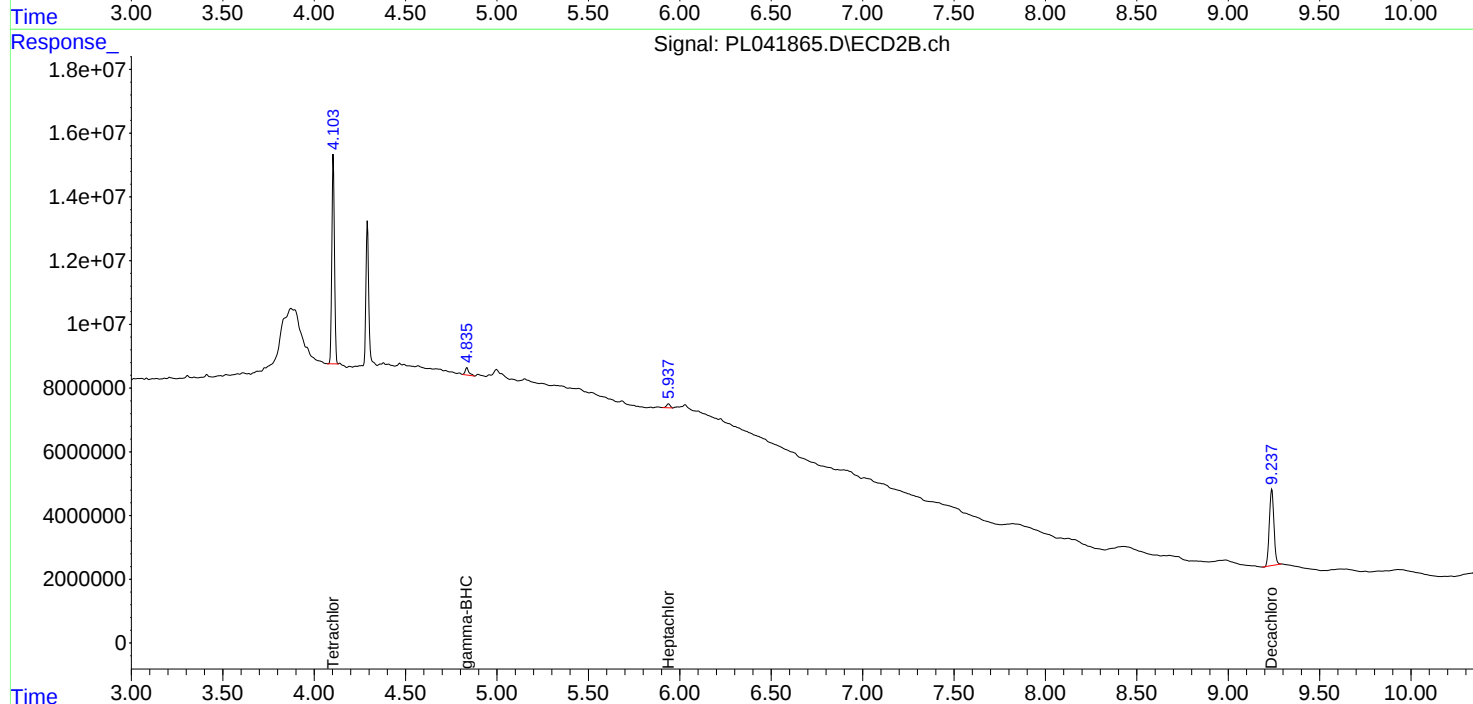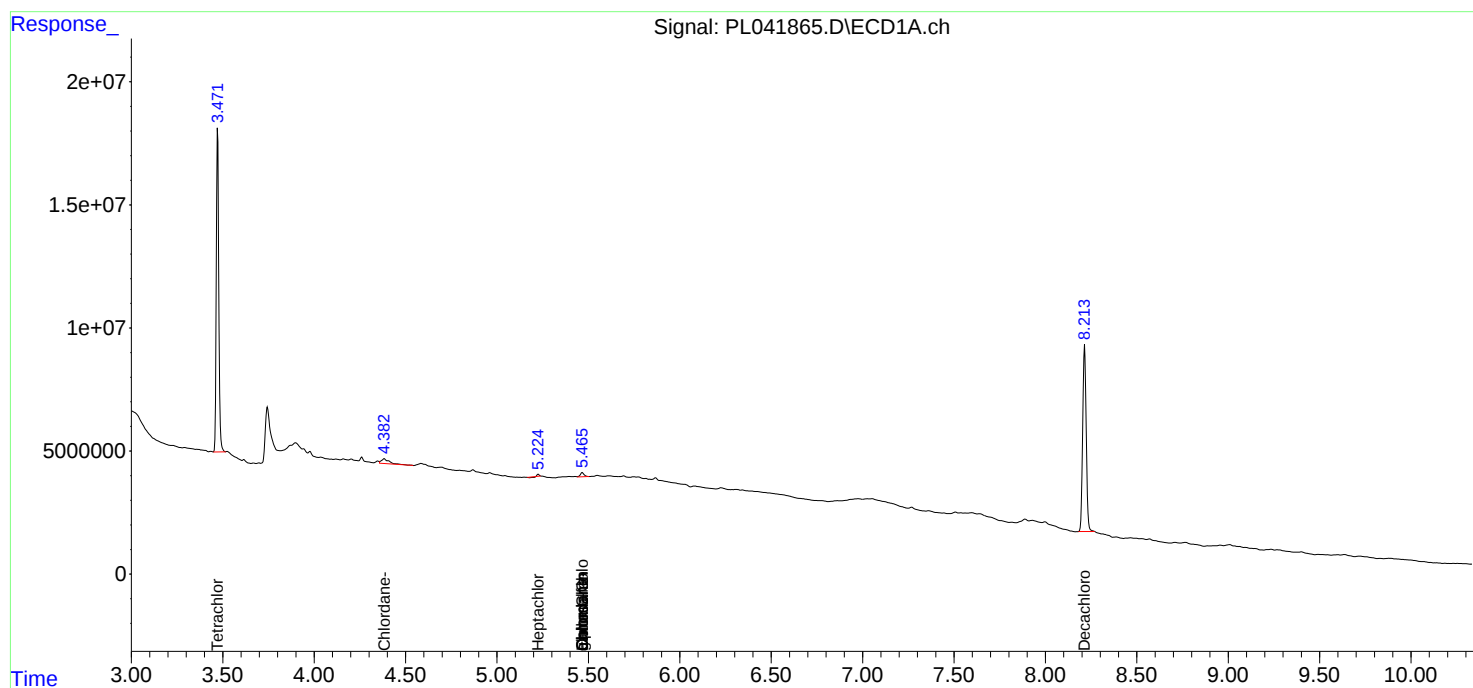


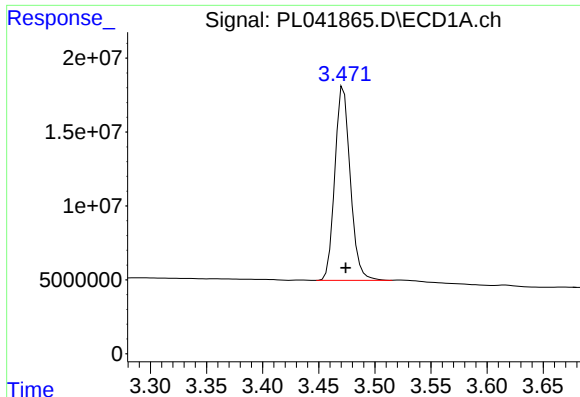

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 125760351
Conc: 19.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(31-35)

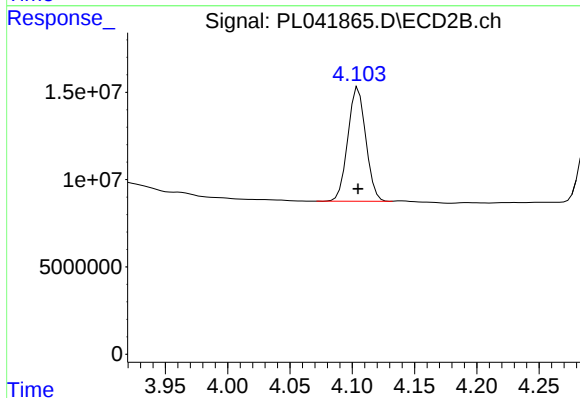


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 65770734
Conc: 21.35 ng/ml

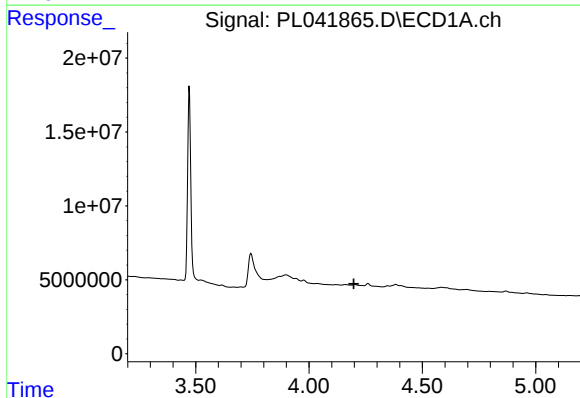


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.198 min
Response: 0
Conc: N.D.

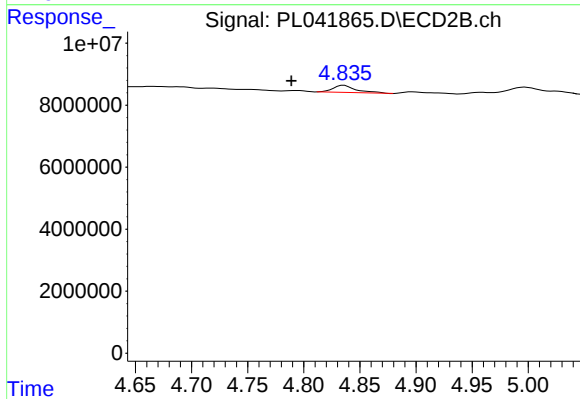

#3 gamma-BHC (Lindane)


R.T.: 4.836 min
Delta R.T.: 0.047 min
Response: 3341627
Conc: 0.79 ng/ml

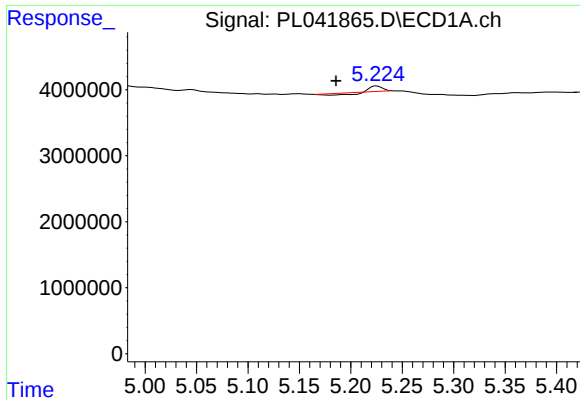

#8 Heptachlor epoxide


R.T.: 5.225 min
Delta R.T.: 0.040 min
Response: 277106
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(31-35)

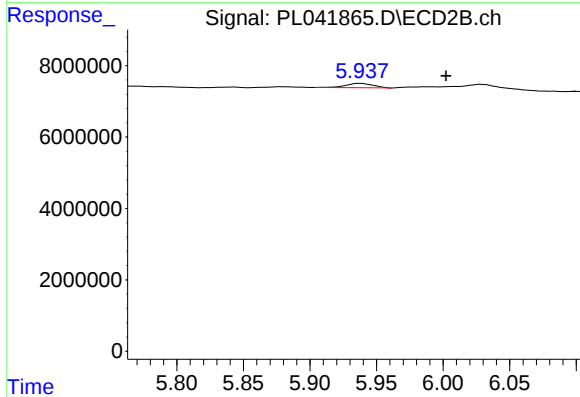


#8 Heptachlor epoxide

R.T.: 5.938 min
Delta R.T.: -0.064 min
Response: 1589090
Conc: 0.45 ng/ml

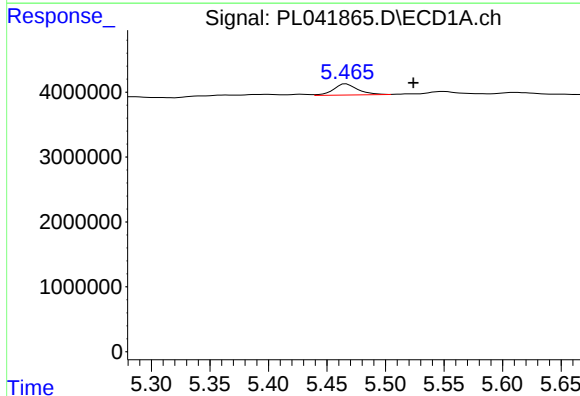


#9 Endosulfan I

R.T.: 5.466 min
Delta R.T.: -0.057 min
Response: 2473818
Conc: 0.33 ng/ml

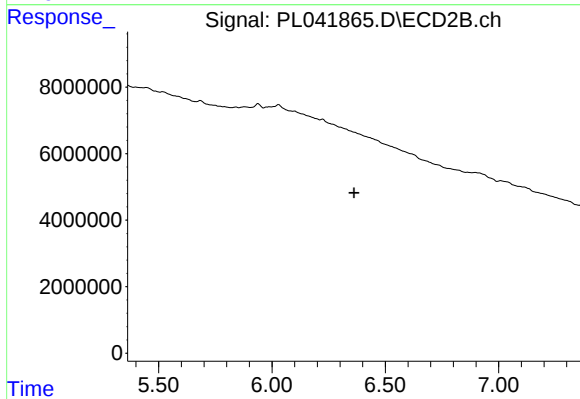

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

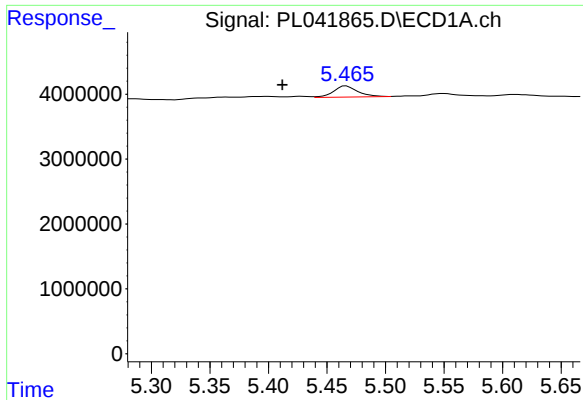

#10 gamma-Chlordane


R.T.: 5.466 min
Delta R.T.: 0.054 min
Response: 2473818
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(31-35)

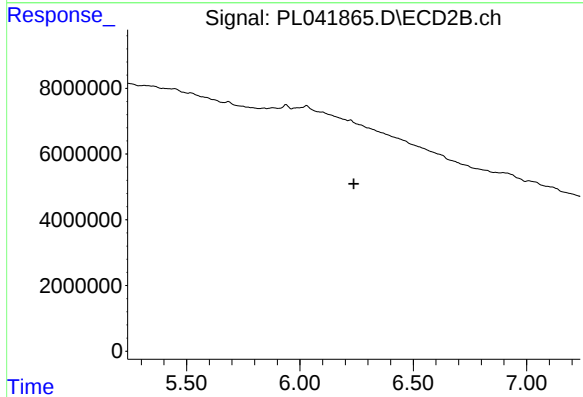


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

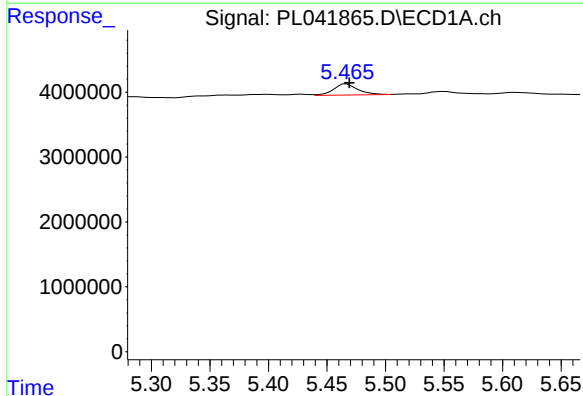


#11 alpha-Chlordane

R.T.: 5.466 min
Delta R.T.: -0.003 min
Response: 2473818
Conc: 0.31 ng/ml

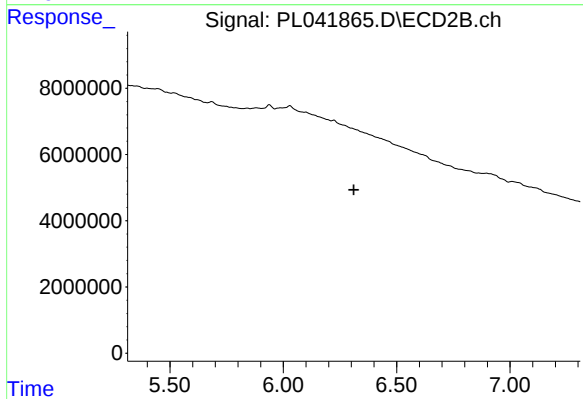

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

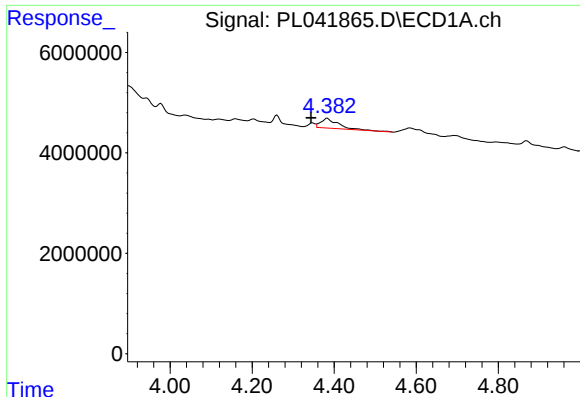

#23 Chlordane-1


R.T.: 4.383 min
Delta R.T.: 0.040 min
Response: 5658780
Conc: 19.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(31-35)

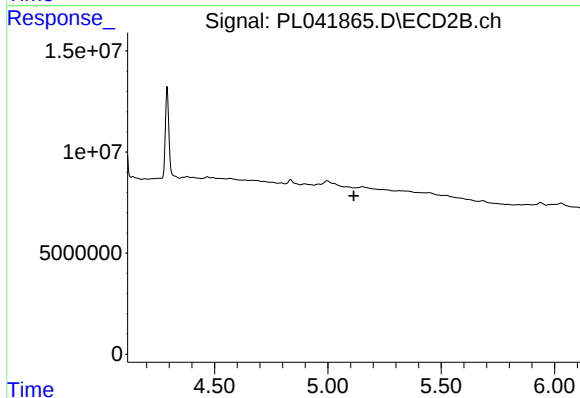


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

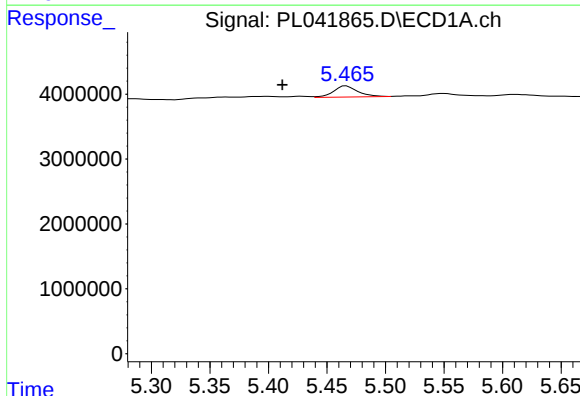


#25 Chlordane-3

R.T.: 5.466 min
Delta R.T.: 0.054 min
Response: 2473818
Conc: 2.78 ng/ml

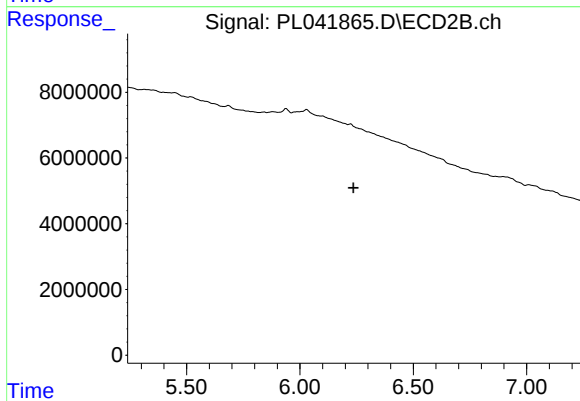

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

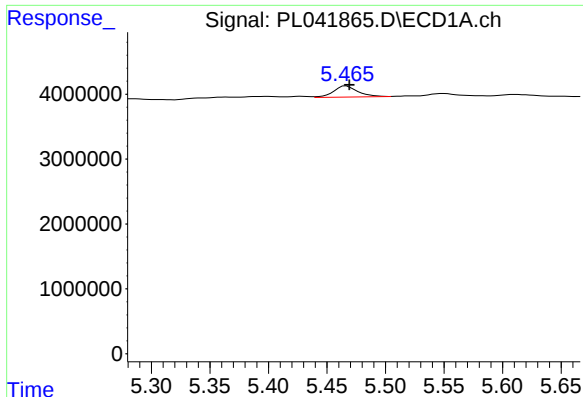

#26 Chlordane-4


R.T.: 5.466 min
Delta R.T.: -0.003 min
Response: 2473818
Conc: 3.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-SAMPLES(31-35)

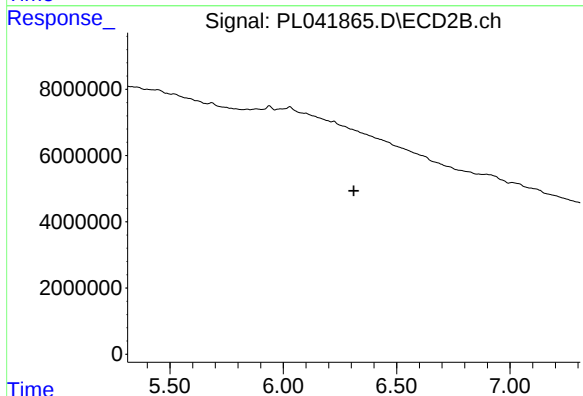


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.311 min
Response: 0
Conc: N.D.

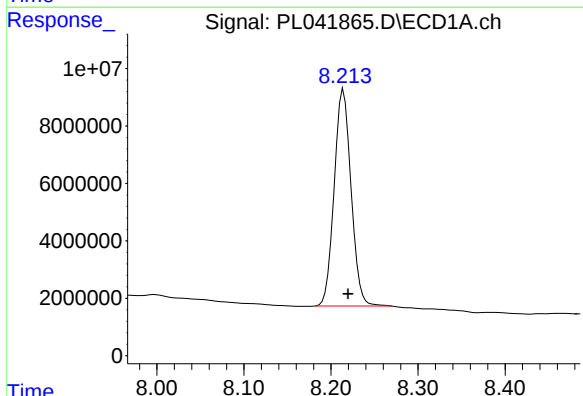

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.005 min
Response: 101856652
Conc: 15.38 ng/ml

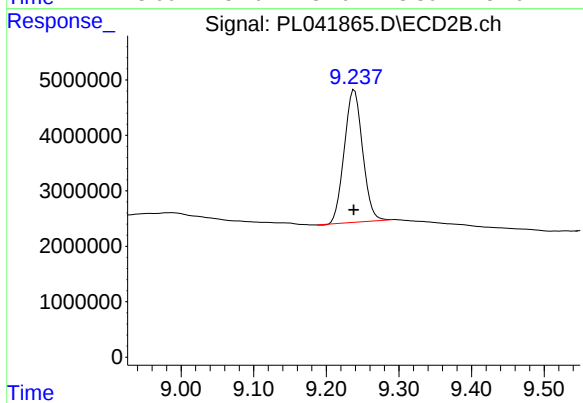

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.000 min
Response: 41902288
Conc: 16.35 ng/ml