

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL110618\  
 Data File : PL041866.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 06 Nov 2018 13:52  
 Operator : AJ\SJ  
 Sample : J5805-08  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 COMP-SAMPLES(36-40)

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 06 15:46:11 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL102918.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Oct 30 01:26:00 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|--------|
| -----                       |                 |        |       |          |          |        |        |
| System Monitoring Compounds |                 |        |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.472  | 4.105 | 117.9E6  | 61714718 | 18.506 | 20.036 |
| 28)                         | SA Decachlor... | 8.214  | 9.238 | 98653638 | 41718024 | 14.893 | 16.282 |
| Target Compounds            |                 |        |       |          |          |        |        |
| 6)                          | B beta-BHC      | 4.407f | 0.000 | 3176491  | 0        | 0.843  | N.D. # |
| 9)                          | A Endosulfan I  | 5.466f | 0.000 | 1945512  | 0        | 0.261  | N.D. # |
| 10)                         | B gamma-Chl...  | 5.466f | 0.000 | 1945512  | 0        | 0.239  | N.D. # |
| 11)                         | B alpha-Chl...  | 5.466  | 0.000 | 1945512  | 0        | 0.240  | N.D. # |
| 23)                         | Chlordane-1     | 4.383  | 0.000 | 2920749  | 0        | 10.301 | N.D. # |
| 25)                         | Chlordane-3     | 5.466  | 0.000 | 1945512  | 0        | 2.183  | N.D. # |
| 26)                         | Chlordane-4     | 5.466  | 0.000 | 1945512  | 0        | 2.485  | N.D. # |
| -----                       |                 |        |       |          |          |        |        |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL110618\  
Data File : PL041866.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 06 Nov 2018 13:52  
Operator : AJ\SJ  
Sample : J5805-08  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
COMP-SAMPLES(36-40)

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 06 15:46:11 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL102918.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 30 01:26:00 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

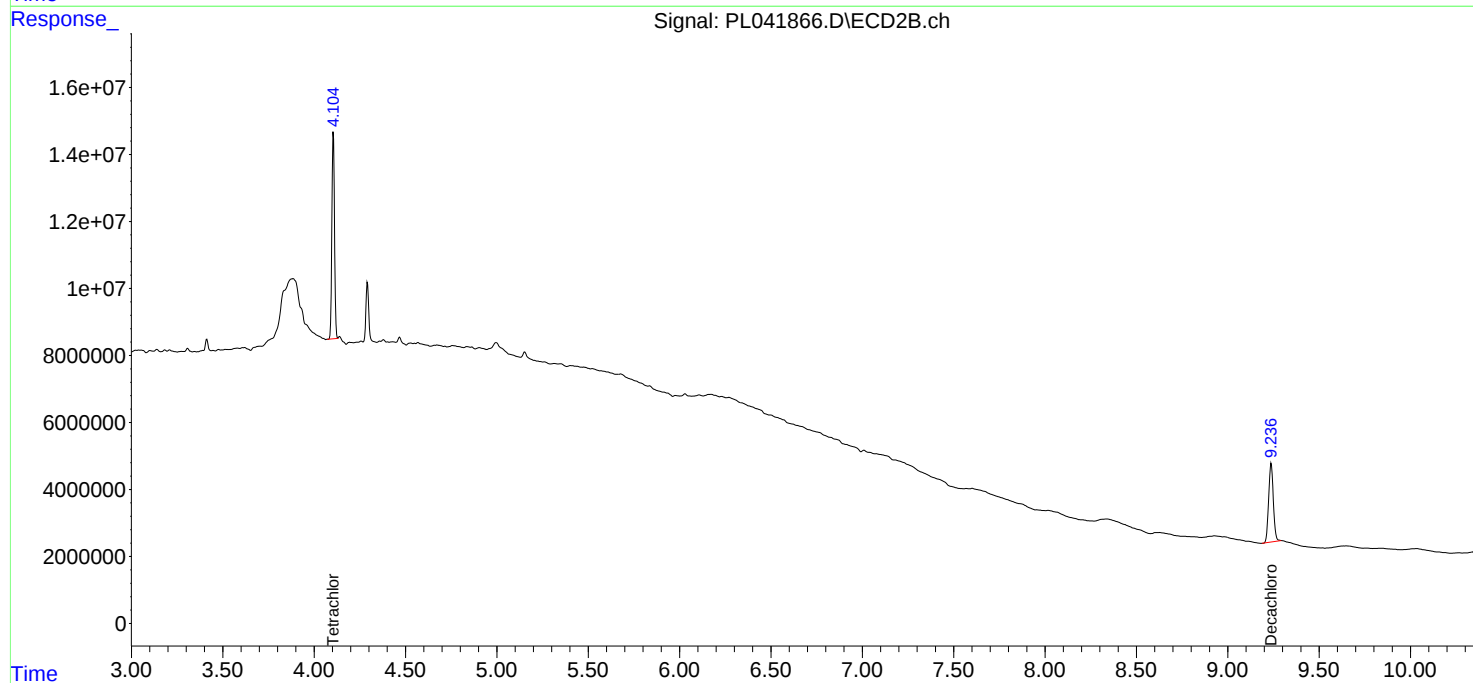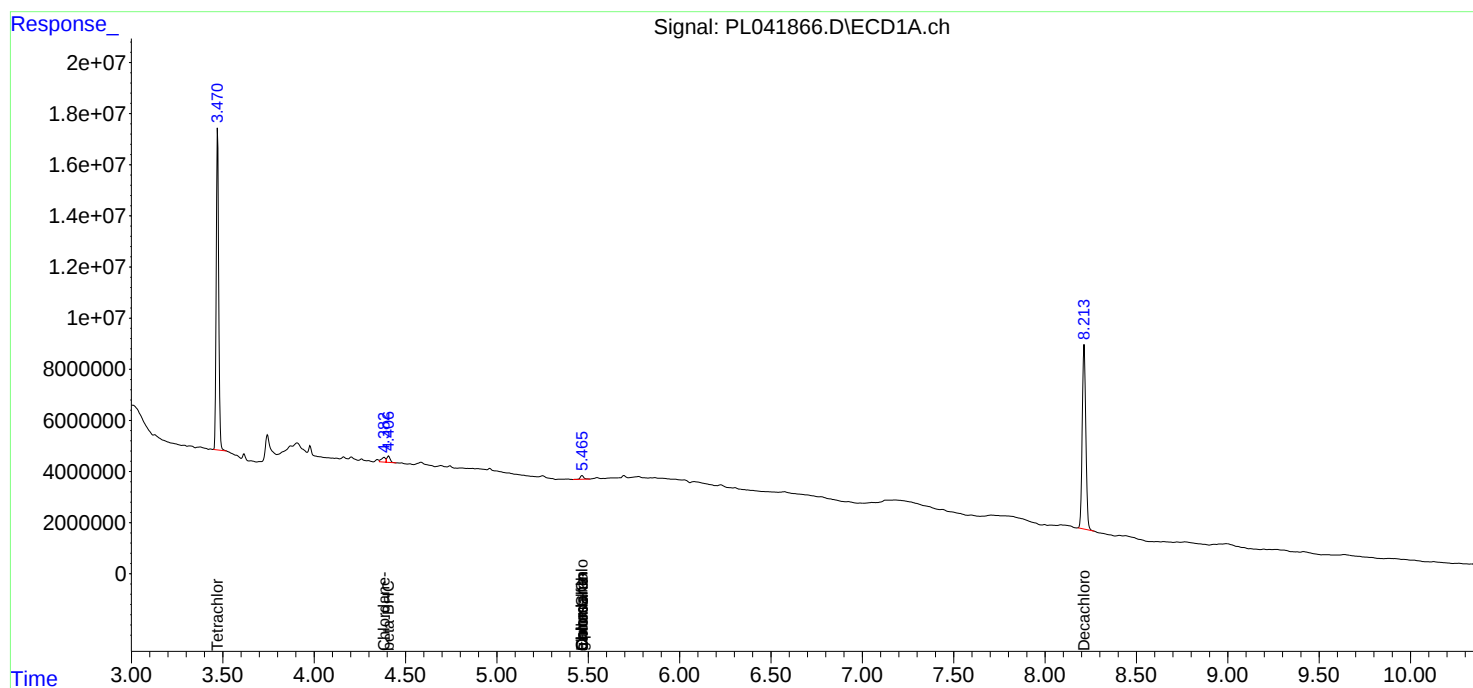


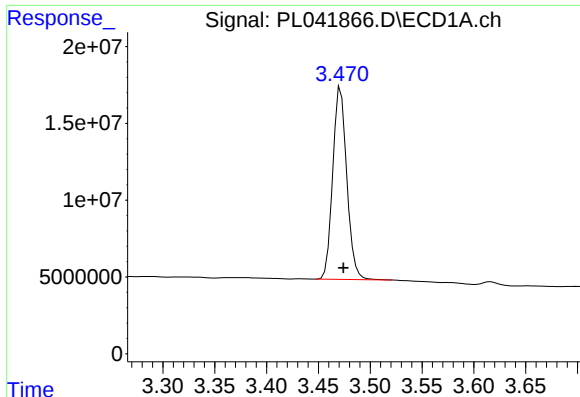

#1 Tetrachloro-m-xylene


R.T.: 3.472 min  
Delta R.T.: -0.002 min  
Response: 117888194  
Conc: 18.51 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
COMP-SAMPLES(36-40)

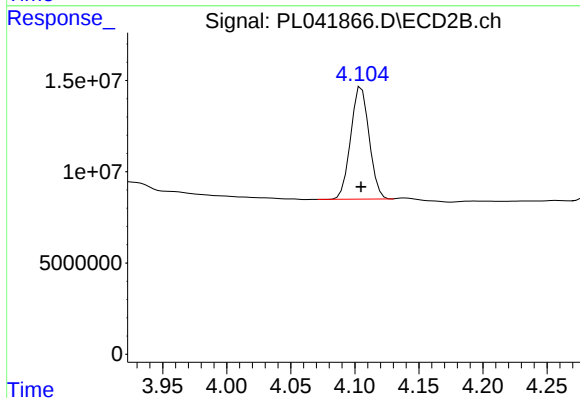


#1 Tetrachloro-m-xylene

R.T.: 4.105 min  
Delta R.T.: 0.000 min  
Response: 61714718  
Conc: 20.04 ng/ml

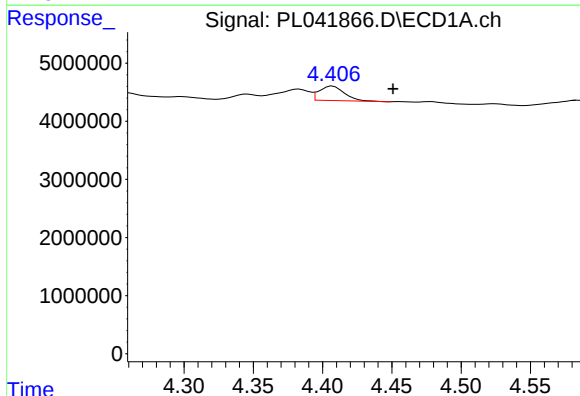


#6 beta-BHC

R.T.: 4.407 min  
Delta R.T.: -0.043 min  
Response: 3176491  
Conc: 0.84 ng/ml

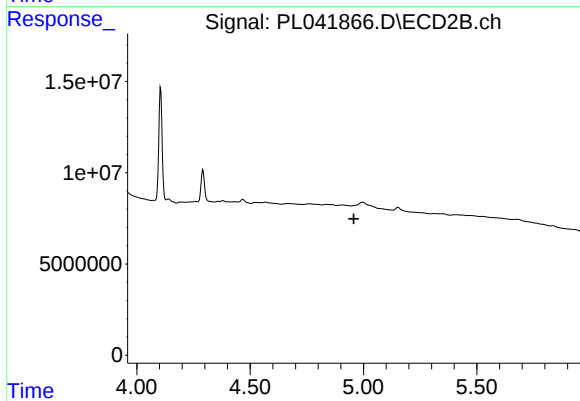

#6 beta-BHC


R.T.: 0.000 min  
Exp R.T.: 4.957 min  
Response: 0  
Conc: N.D.

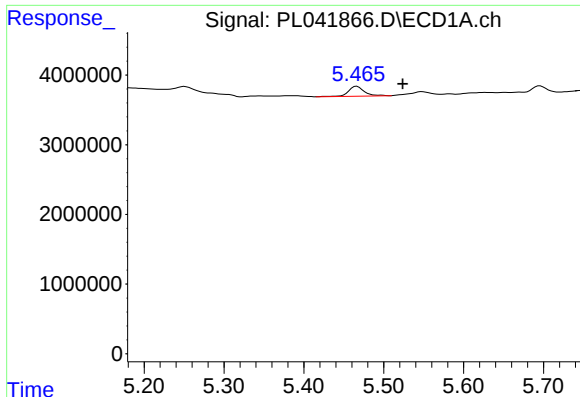

#9 Endosulfan I


R.T.: 5.466 min  
Delta R.T.: -0.057 min  
Response: 1945512  
Conc: 0.26 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
COMP-SAMPLES(36-40)

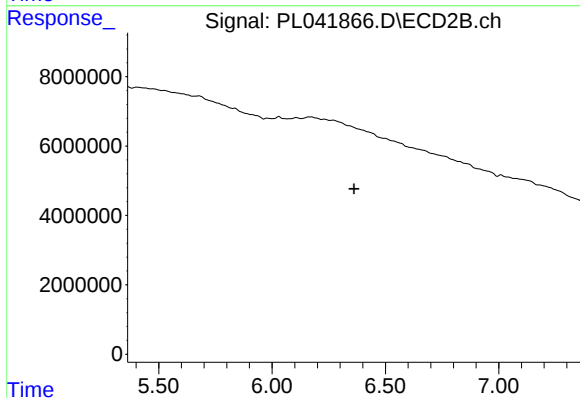


#9 Endosulfan I

R.T.: 0.000 min  
Exp R.T. : 6.363 min  
Response: 0  
Conc: N.D.

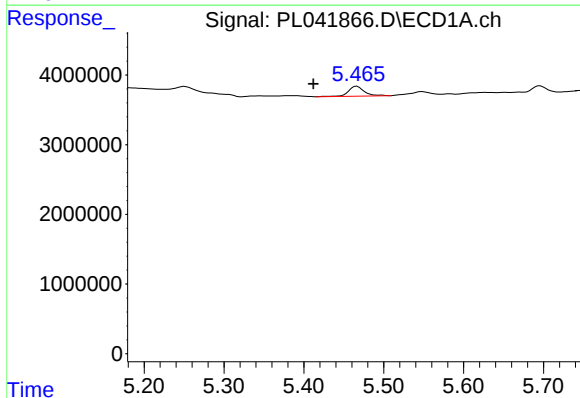


#10 gamma-Chlordane

R.T.: 5.466 min  
Delta R.T.: 0.054 min  
Response: 1945512  
Conc: 0.24 ng/ml

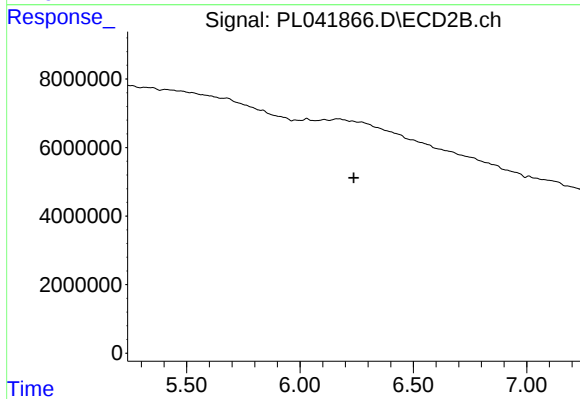

#10 gamma-Chlordane


R.T.: 0.000 min  
Exp R.T. : 6.237 min  
Response: 0  
Conc: N.D.

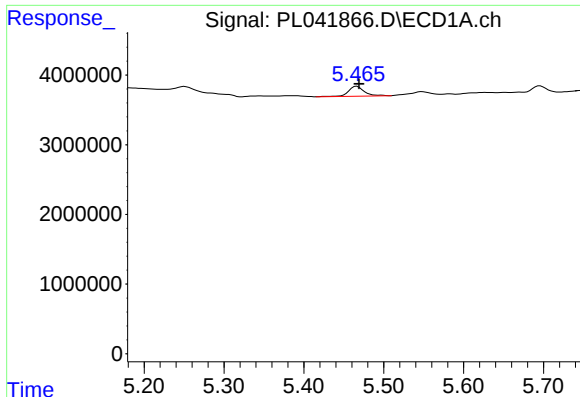

#11 alpha-Chlordane


R.T.: 5.466 min  
Delta R.T.: -0.003 min  
Response: 1945512  
Conc: 0.24 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
COMP-SAMPLES(36-40)

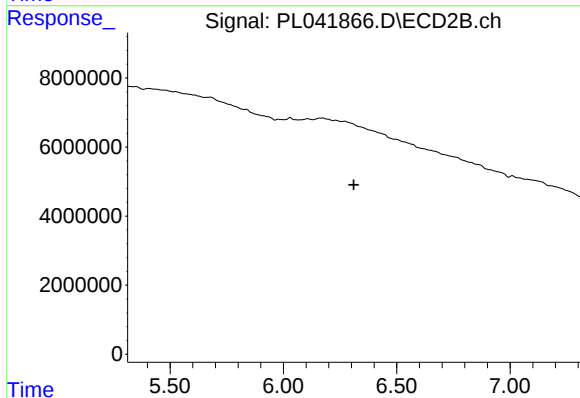


#11 alpha-Chlordane

R.T.: 0.000 min  
Exp R.T. : 6.311 min  
Response: 0  
Conc: N.D.

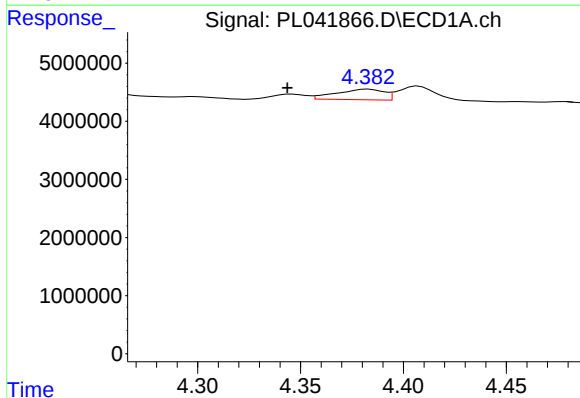


#23 Chlordane-1

R.T.: 4.383 min  
Delta R.T.: 0.039 min  
Response: 2920749  
Conc: 10.30 ng/ml

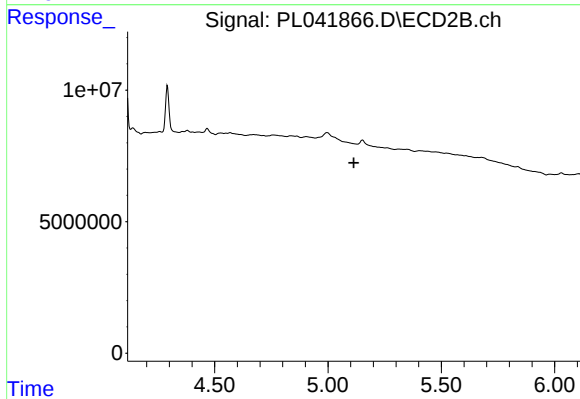

#23 Chlordane-1


R.T.: 0.000 min  
Exp R.T. : 5.115 min  
Response: 0  
Conc: N.D.

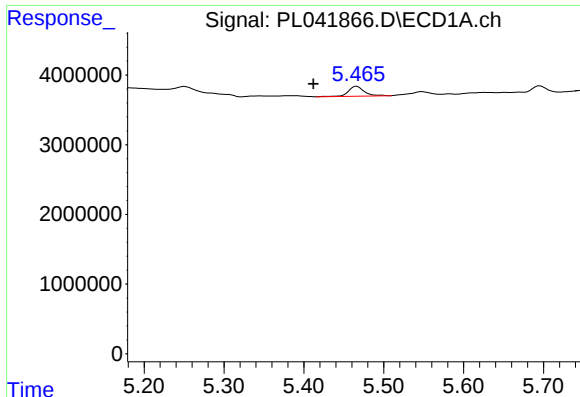

#25 Chlordane-3


R.T.: 5.466 min  
Delta R.T.: 0.054 min  
Response: 1945512  
Conc: 2.18 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
COMP-SAMPLES(36-40)

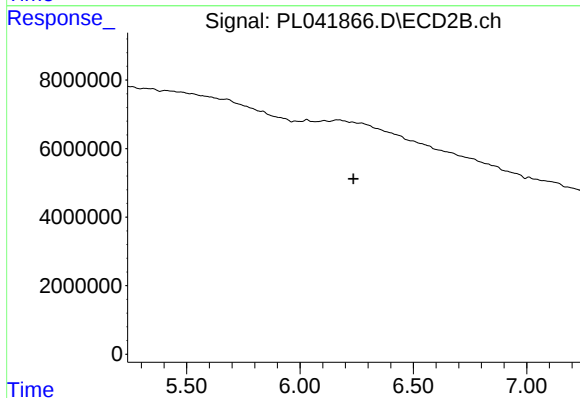


#25 Chlordane-3

R.T.: 0.000 min  
Exp R.T. : 6.237 min  
Response: 0  
Conc: N.D.

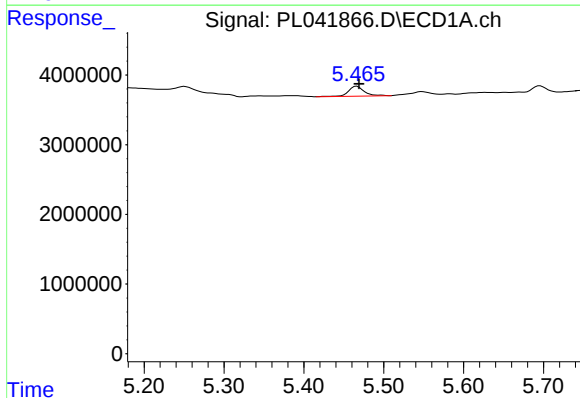


#26 Chlordane-4

R.T.: 5.466 min  
Delta R.T.: -0.003 min  
Response: 1945512  
Conc: 2.48 ng/ml

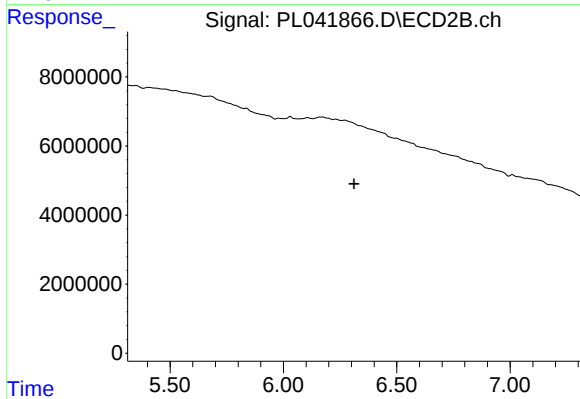

#26 Chlordane-4


R.T.: 0.000 min  
Exp R.T. : 6.311 min  
Response: 0  
Conc: N.D.

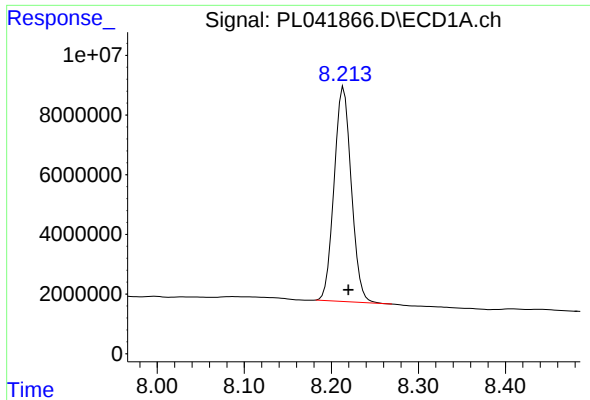

#28 Decachlorobiphenyl

R.T.: 8.214 min  
Delta R.T.: -0.005 min  
Response: 98653638  
Conc: 14.89 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
COMP-SAMPLES(36-40)

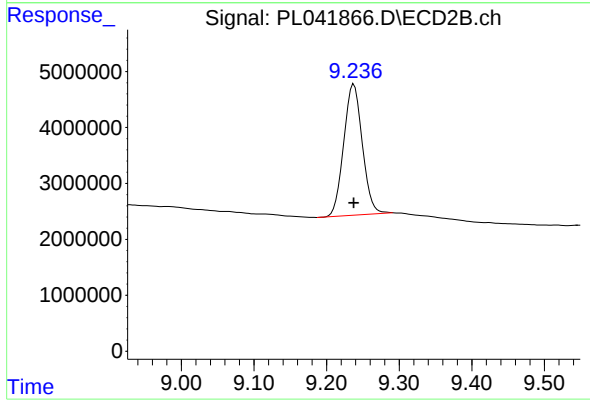

#28 Decachlorobiphenyl

R.T.: 9.238 min  
Delta R.T.: 0.000 min  
Response: 41718024  
Conc: 16.28 ng/ml