

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
 Data File : PL041871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 15:02
 Operator : AJ\SJ
 Sample : J5812-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP2-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 15:46:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.105	118.9E6	62805093	18.659	20.390
28)	SA Decachlor...	8.215	9.238	104.2E6	42403493	15.724	16.550
Target Compounds							
6)	B beta-BHC	4.408f	0.000	2225470	0	0.590	N.D. #
23)	Chlordane-1	4.383	0.000	2972038	0	10.482	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
Data File : PL041871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 15:02
Operator : AJ\SJ
Sample : J5812-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP2-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 15:46:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

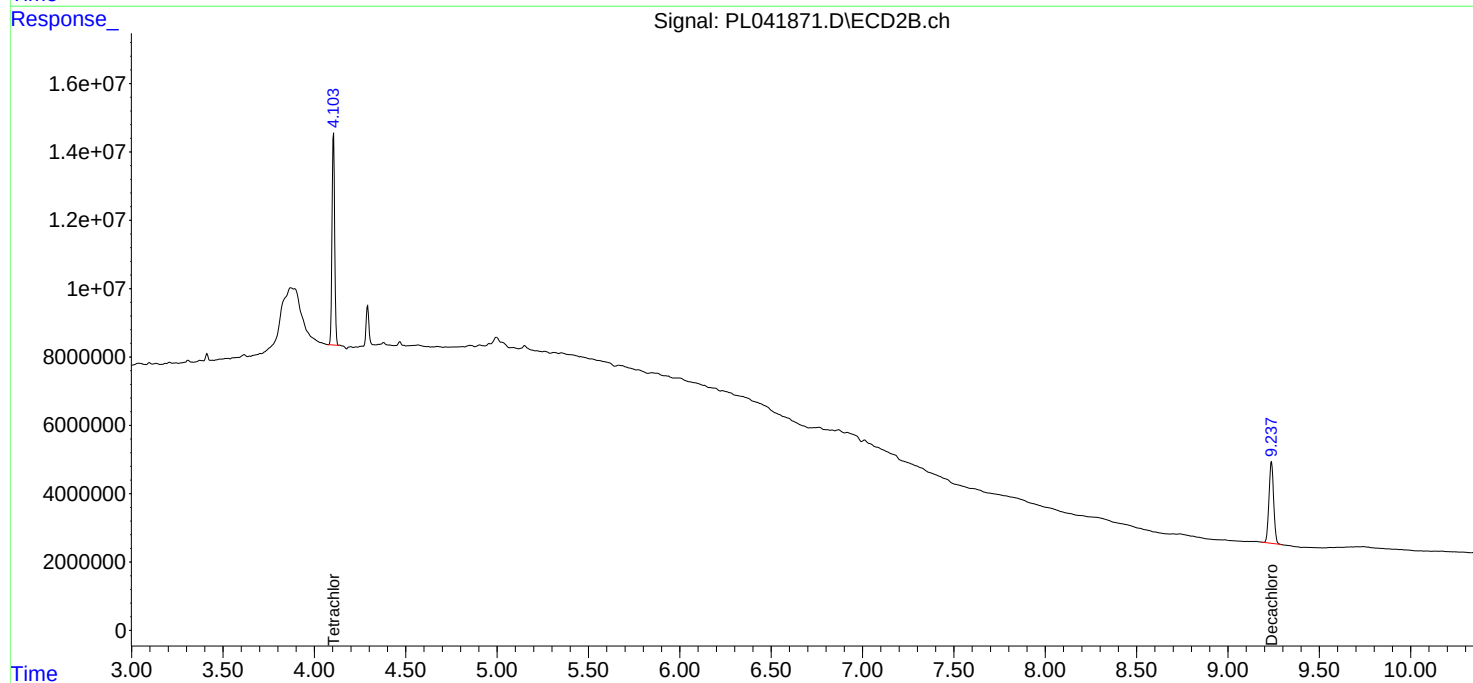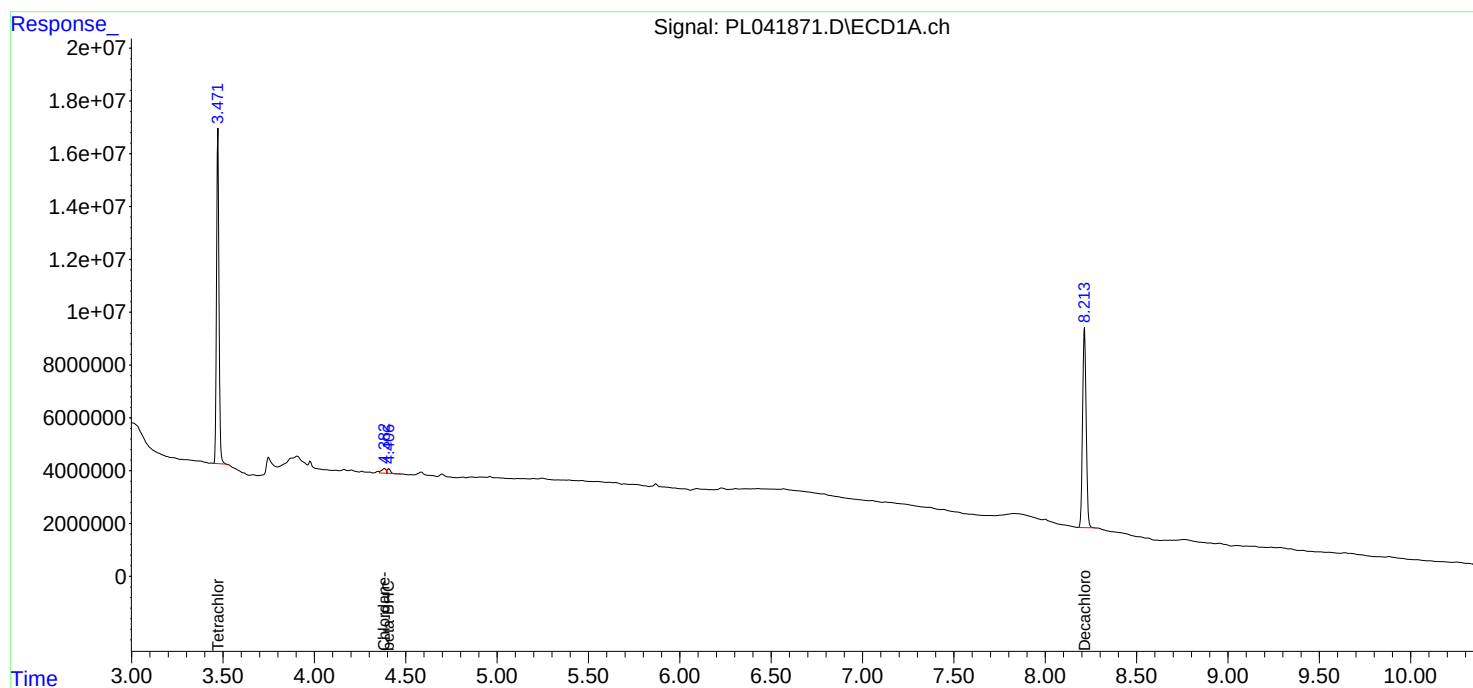


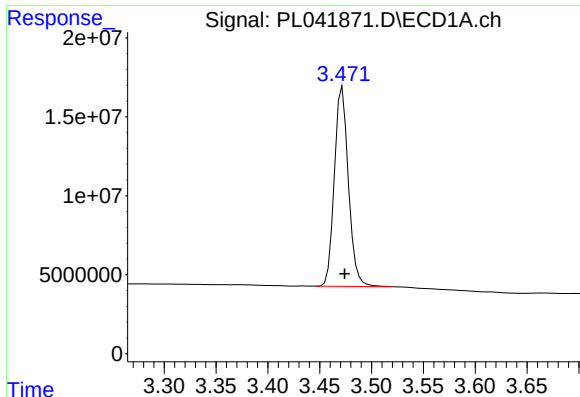

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 118859870
Conc: 18.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP2-B

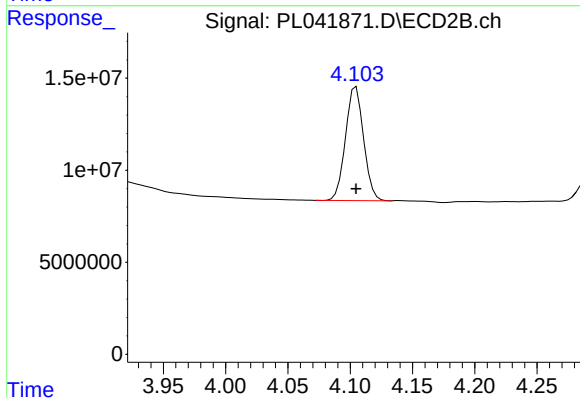


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 62805093
Conc: 20.39 ng/ml

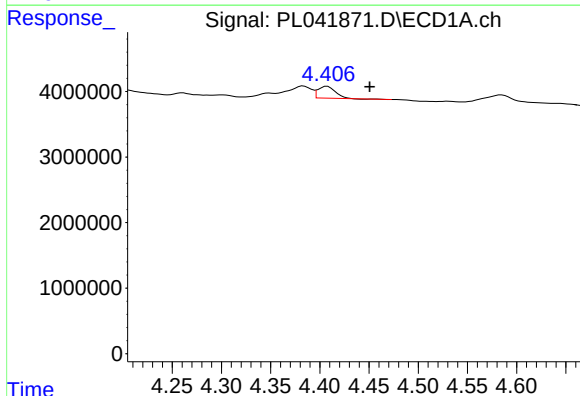


#6 beta-BHC

R.T.: 4.408 min
Delta R.T.: -0.043 min
Response: 2225470
Conc: 0.59 ng/ml

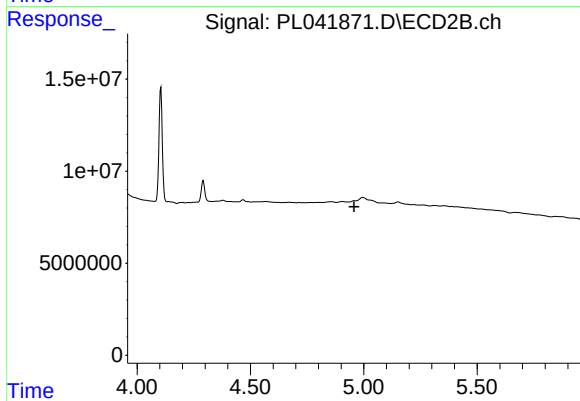

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.957 min
Response: 0
Conc: N.D.

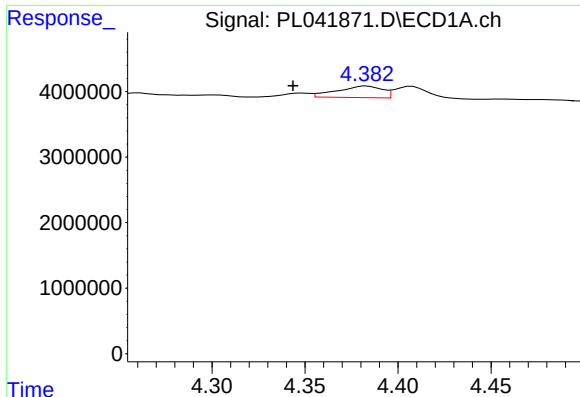

#23 Chlordane-1


R.T.: 4.383 min
Delta R.T.: 0.040 min
Response: 2972038
Conc: 10.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP2-B

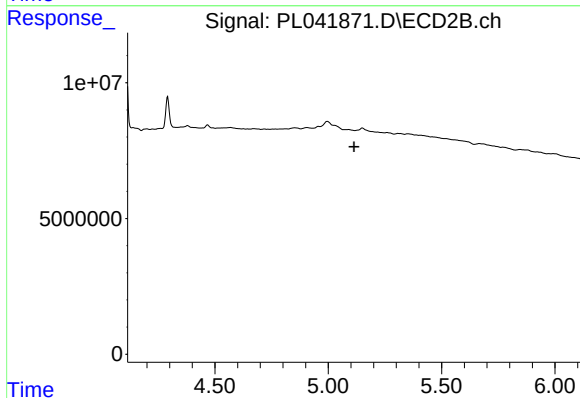


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.115 min
Response: 0
Conc: N.D.

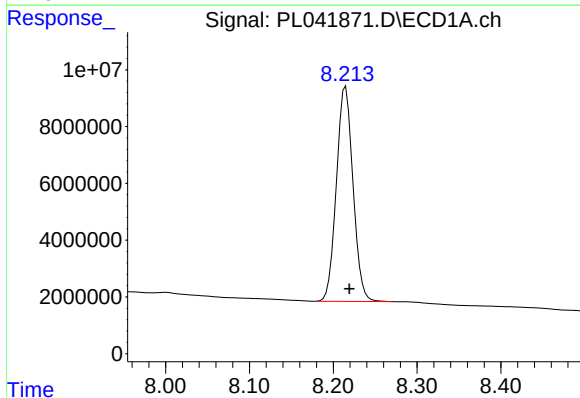

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.005 min
Response: 104157120
Conc: 15.72 ng/ml

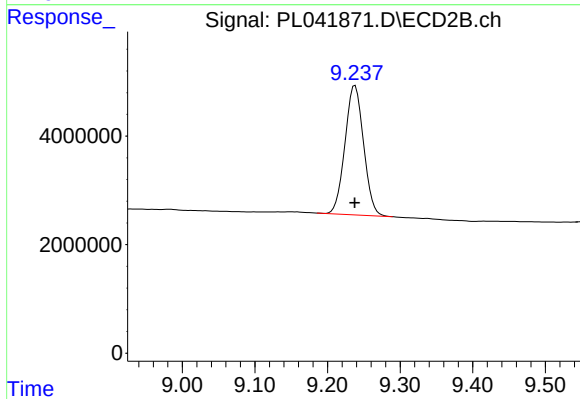

#28 Decachlorobiphenyl

R.T.: 9.238 min
Delta R.T.: 0.000 min
Response: 42403493
Conc: 16.55 ng/ml