

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
 Data File : PL041874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 15:45
 Operator : AJ\SJ
 Sample : J5812-28
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP4-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 16:04:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.105	121.4E6	64269509	19.060	20.865
28)	SA Decachlor...	8.214	9.237	110.2E6	43835158	16.632	17.109
Target Compounds							
2)	A alpha-BHC	3.867f	0.000	370399	0	0.038	N.D. #
6)	B beta-BHC	4.408f	0.000	3245958	0	0.861	N.D. #
9)	A Endosulfan I	5.548	0.000	7906456	0	1.062	N.D. #
10)	B gamma-Chl...	0.000	6.168f	0	3470744	N.D.	1.028 #
20)	A Methoxychlor	6.934	0.000	2207759	0	0.657	N.D. #
23)	Chlordane-1	4.383	0.000	3627542	0	12.794	N.D. #
25)	Chlordane-3	0.000	6.168	0	3470744	N.D.	7.712 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
Data File : PL041874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 15:45
Operator : AJ\SJ
Sample : J5812-28
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP4-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 16:04:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

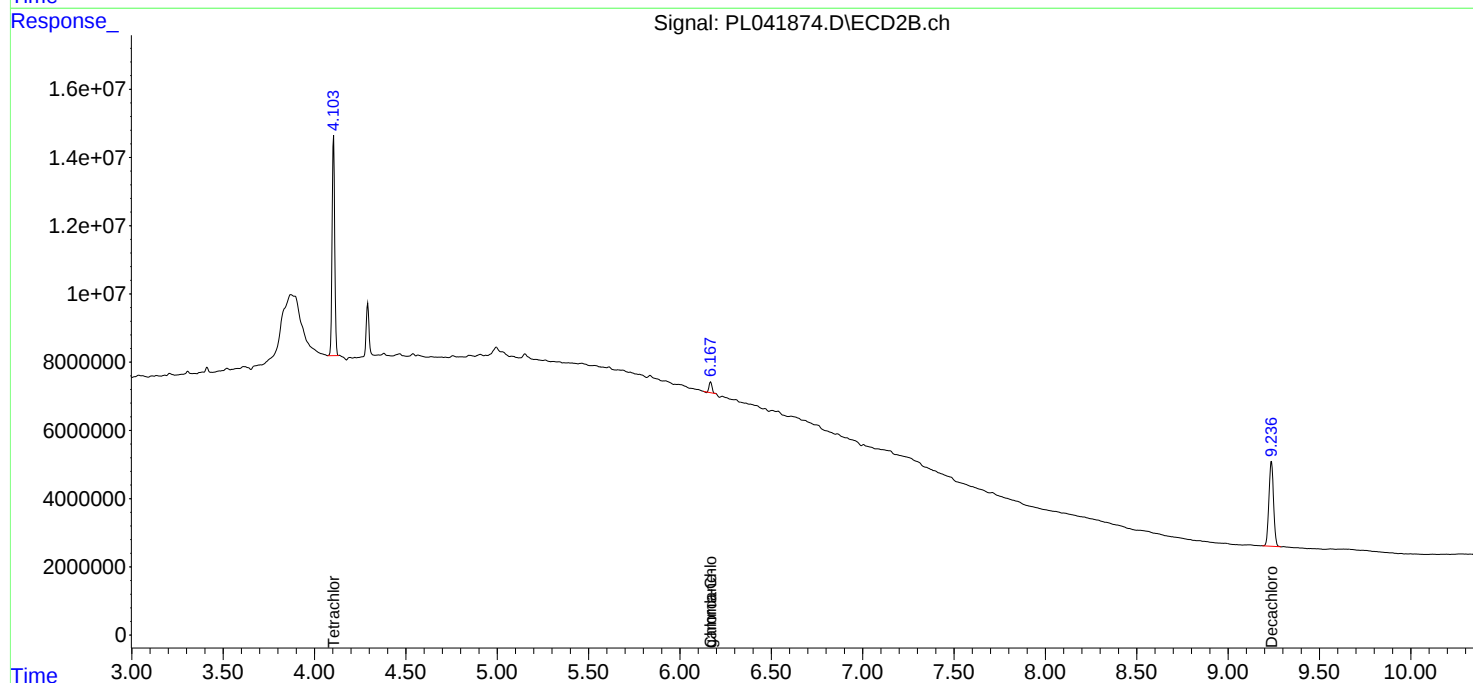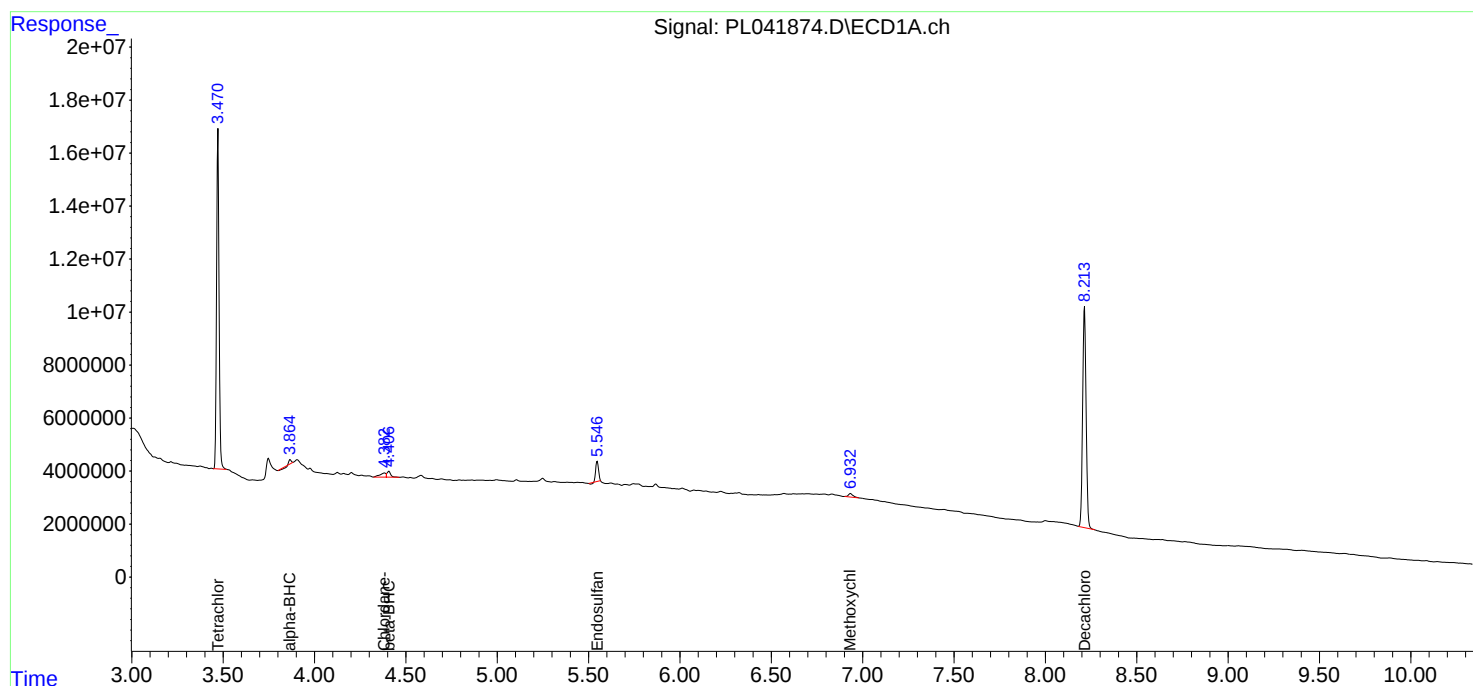


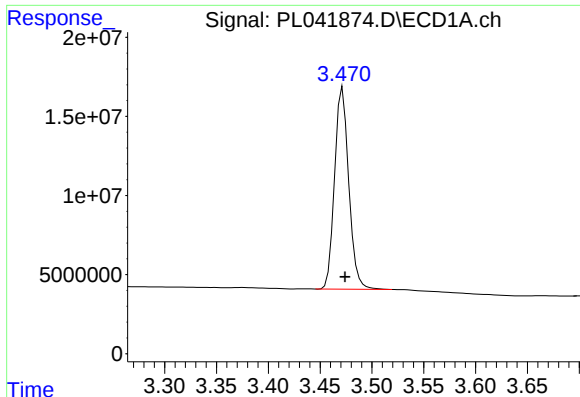

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 121417849
Conc: 19.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP4-A

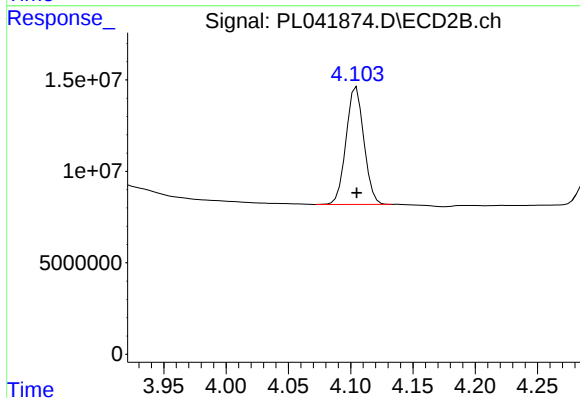


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 64269509
Conc: 20.87 ng/ml

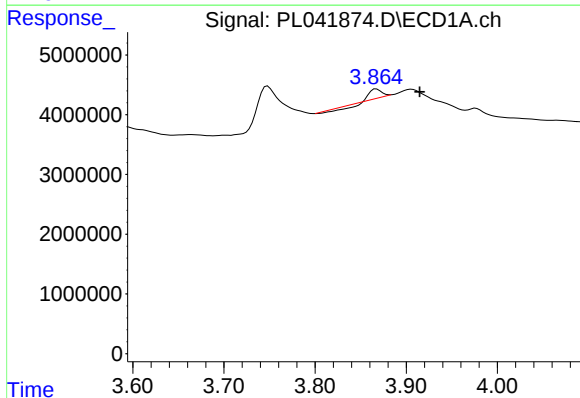


#2 alpha-BHC

R.T.: 3.867 min
Delta R.T.: -0.048 min
Response: 370399
Conc: 0.04 ng/ml

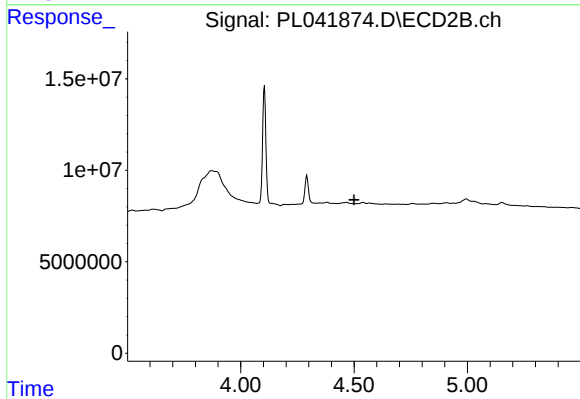

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.501 min
Response: 0
Conc: N.D.

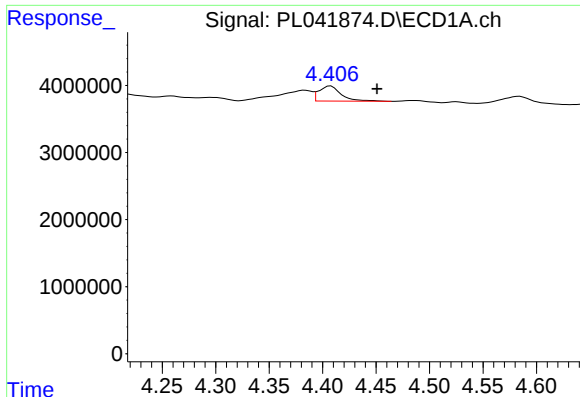

#6 beta-BHC


R.T.: 4.408 min
Delta R.T.: -0.043 min
Response: 3245958
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP4-A

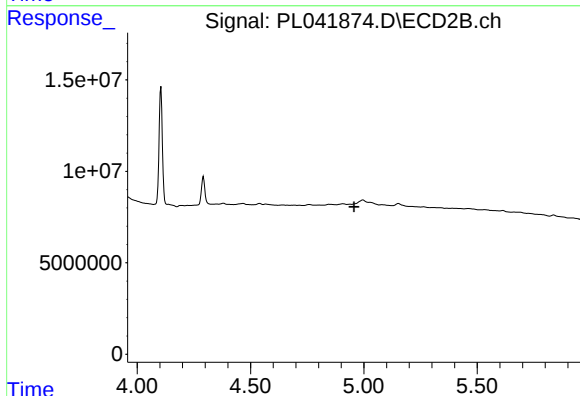


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

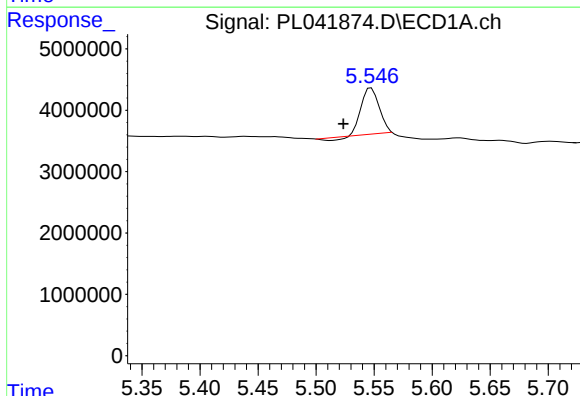


#9 Endosulfan I

R.T.: 5.548 min
Delta R.T.: 0.024 min
Response: 7906456
Conc: 1.06 ng/ml

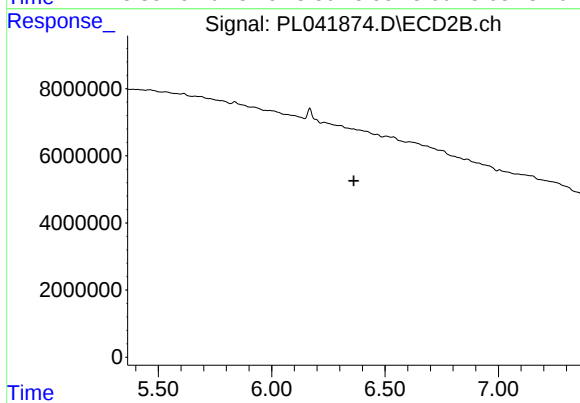

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

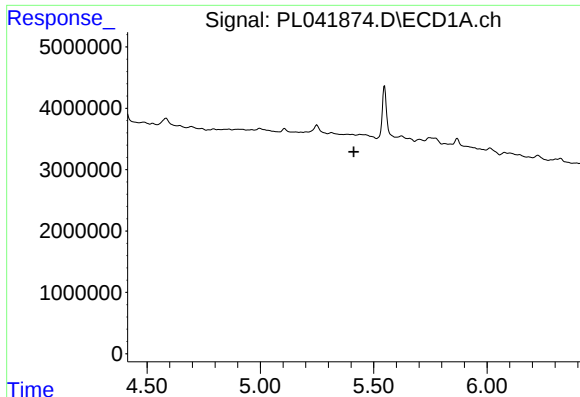

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP4-A

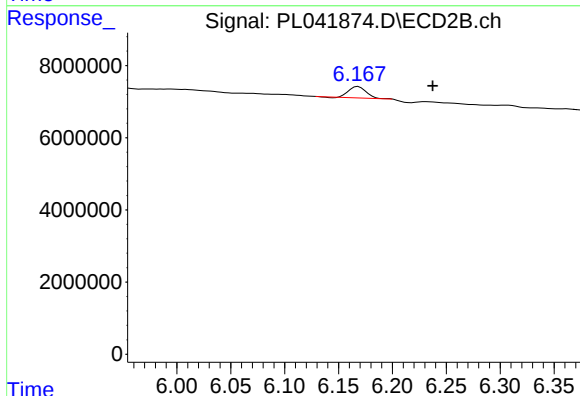


#10 gamma-Chlordane

R.T.: 6.168 min
Delta R.T.: -0.069 min
Response: 3470744
Conc: 1.03 ng/ml

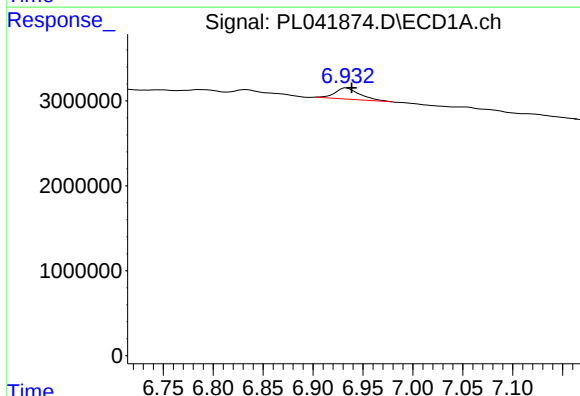


#20 Methoxychlor

R.T.: 6.934 min
Delta R.T.: -0.005 min
Response: 2207759
Conc: 0.66 ng/ml

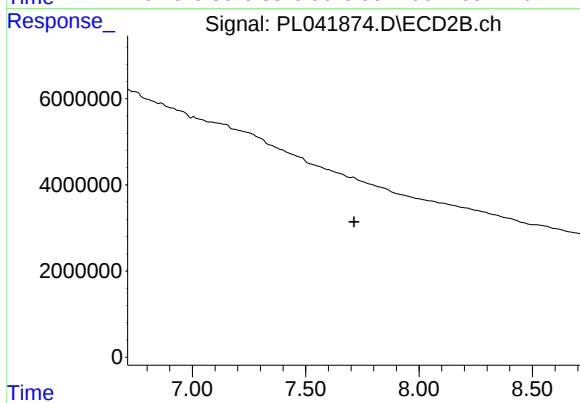

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.713 min
Response: 0
Conc: N.D.

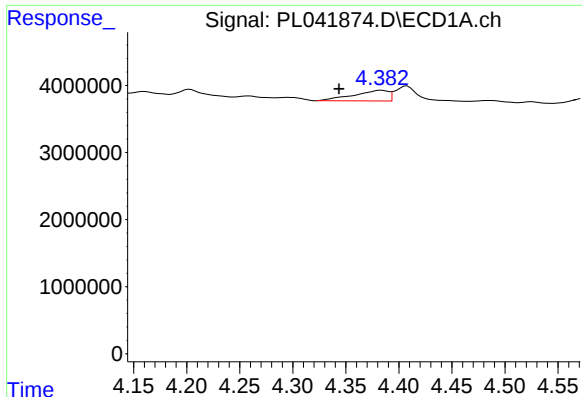

#23 Chlordane-1


R.T.: 4.383 min
Delta R.T.: 0.040 min
Response: 3627542
Conc: 12.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP4-A

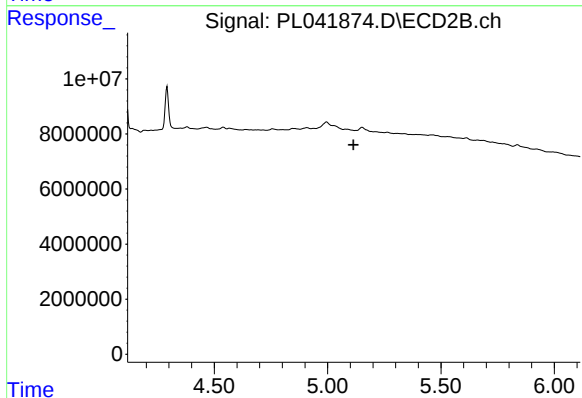


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

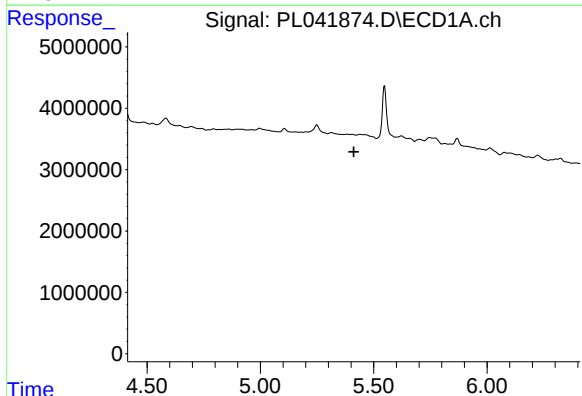


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.412 min
Response: 0
Conc: N.D.

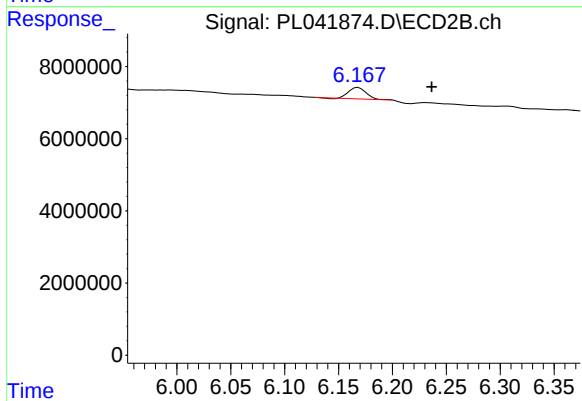

#25 Chlordane-3

R.T.: 6.168 min
Delta R.T.: -0.068 min
Response: 3470744
Conc: 7.71 ng/ml

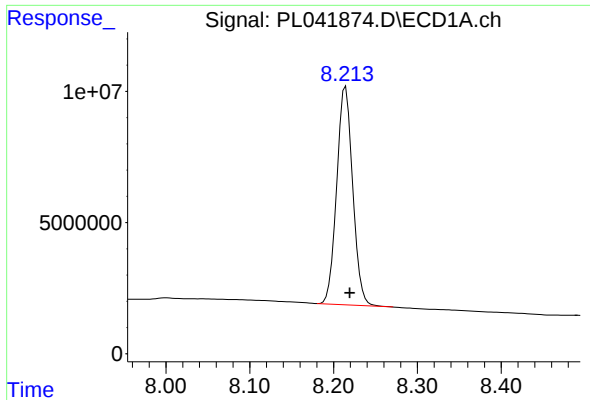

#28 Decachlorobiphenyl


R.T.: 8.214 min

Delta R.T.: -0.005 min

Response: 110167296

Conc: 16.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP4-A

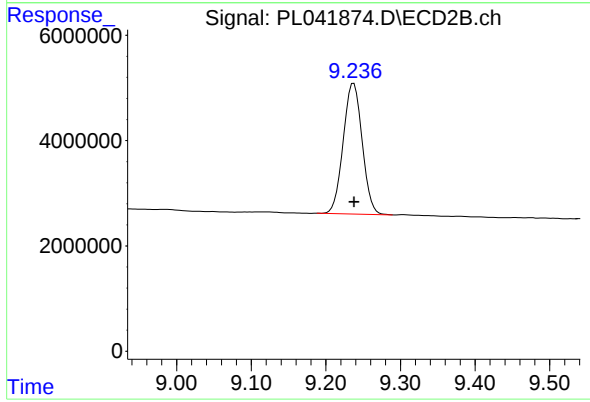

#28 Decachlorobiphenyl

R.T.: 9.237 min

Delta R.T.: 0.000 min

Response: 43835158

Conc: 17.11 ng/ml