

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
 Data File : PL041875.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 15:59
 Operator : AJ\SJ
 Sample : J5812-32
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP4-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 16:34:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.105	116.8E6	61434761	18.338	19.945
28)	SA Decachlor...	8.215	9.237	105.5E6	42604779	15.926	16.628
Target Compounds							
2)	A alpha-BHC	3.869f	0.000	1459399	0	0.150	N.D. #
6)	B beta-BHC	4.408f	0.000	3006776	0	0.798	N.D. #
9)	A Endosulfan I	5.549	0.000	5666363	0	0.761	N.D. #
14)	MA Endrin	0.000	6.864	0	31741263	N.D.	11.676 #
15)	B Endosulfa...	6.331	0.000	1474567	0	0.213	N.D. #
16)	A 4,4'-DDD	6.099f	0.000	14168939	0	2.438	N.D. #
17)	MA 4,4'-DDT	6.331f	0.000	1474567	0	0.242	N.D. #
23)	Chlordane-1	4.384	0.000	4109448	0	14.493	N.D. #
27)	Chlordane-5	6.331	0.000	1474567	0	5.913	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
Data File : PL041875.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 15:59
Operator : AJ\SJ
Sample : J5812-32
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP4-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 16:34:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

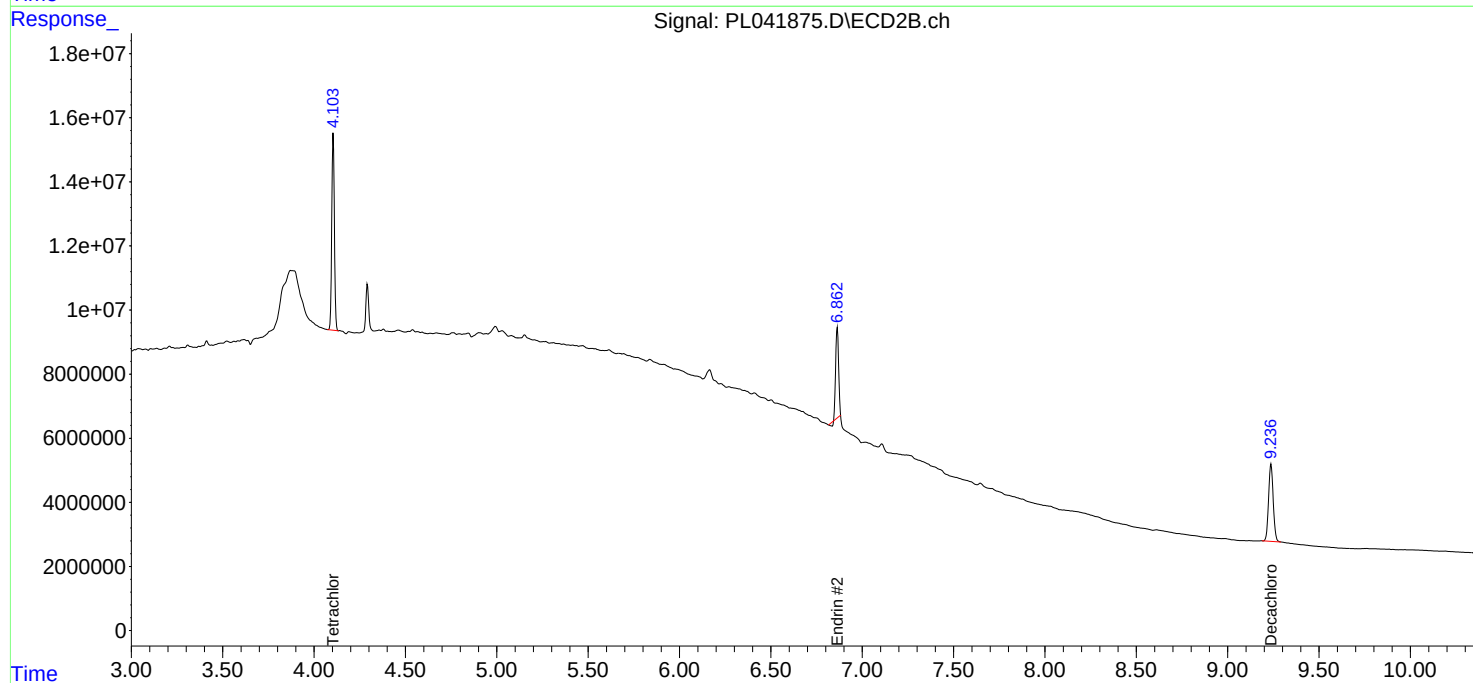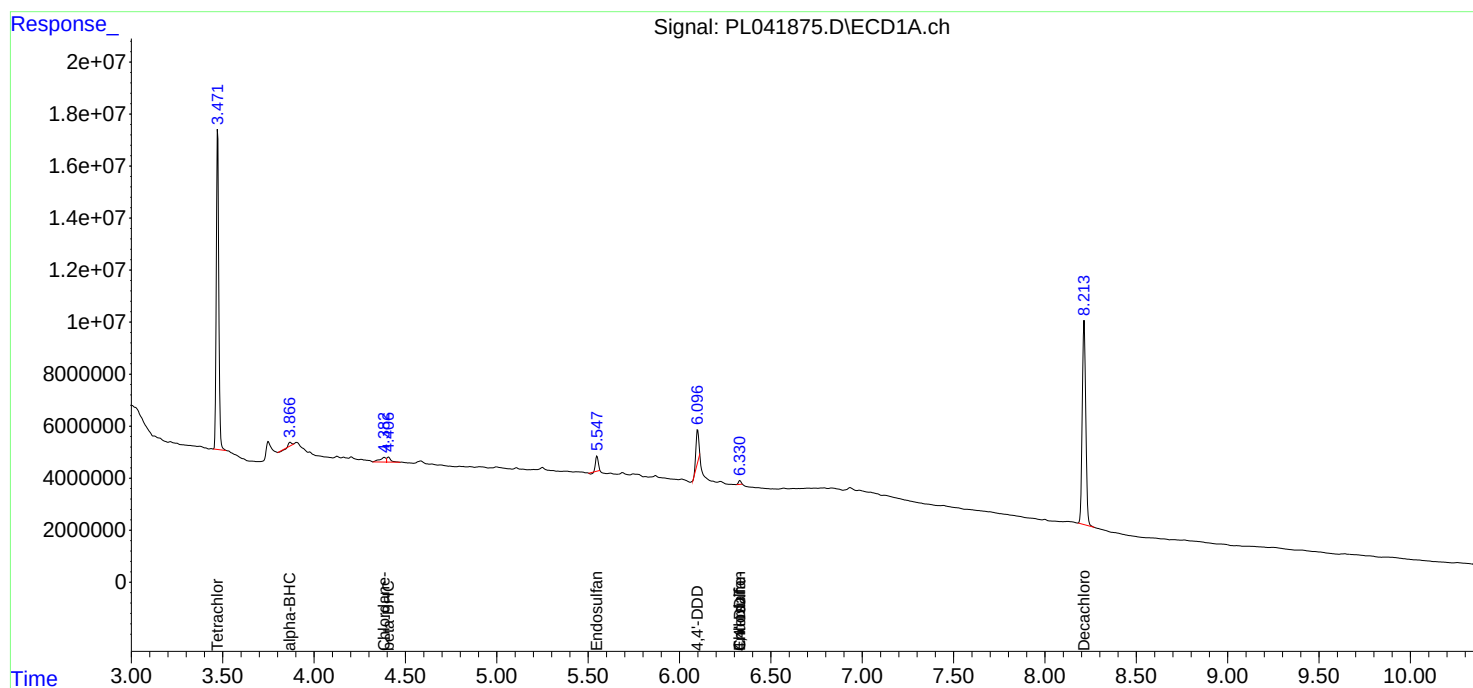


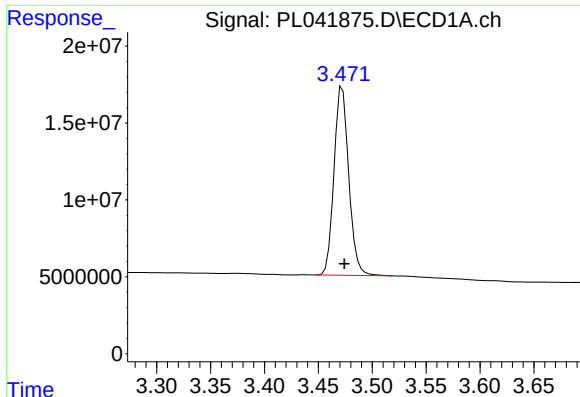

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 116815566
Conc: 18.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP4-B

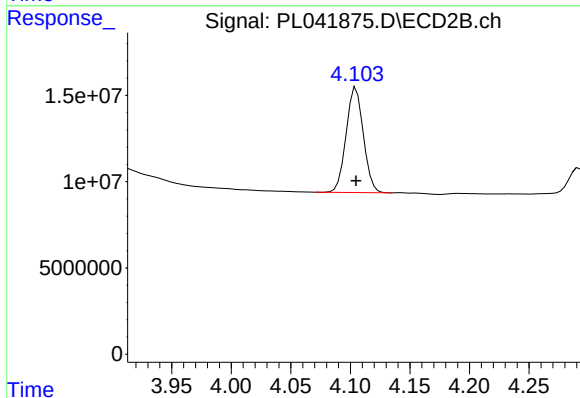


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 61434761
Conc: 19.94 ng/ml

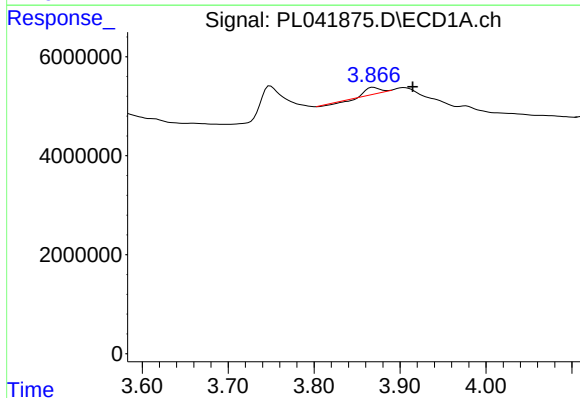


#2 alpha-BHC

R.T.: 3.869 min
Delta R.T.: -0.046 min
Response: 1459399
Conc: 0.15 ng/ml

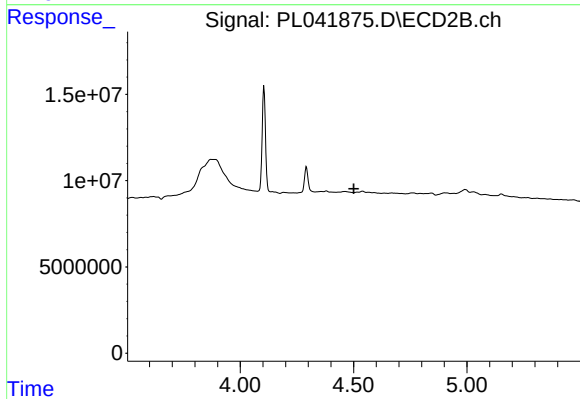

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.501 min
Response: 0
Conc: N.D.

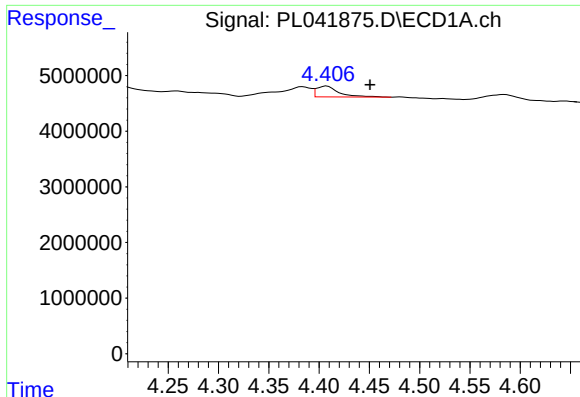

#6 beta-BHC


R.T.: 4.408 min
Delta R.T.: -0.043 min
Response: 3006776
Conc: 0.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP4-B

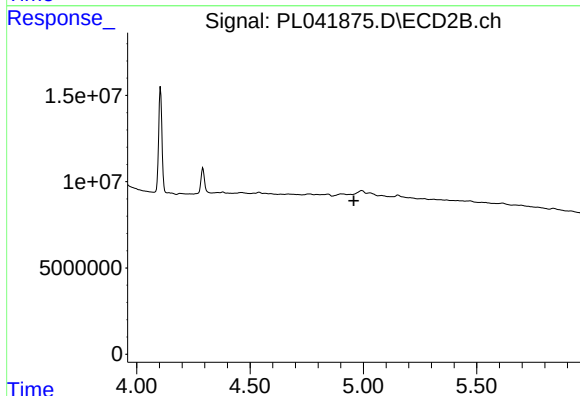


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

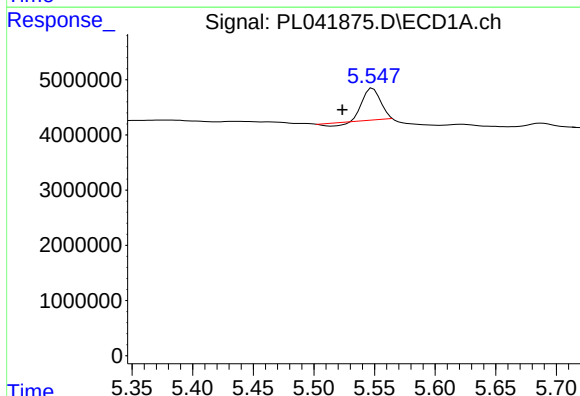


#9 Endosulfan I

R.T.: 5.549 min
Delta R.T.: 0.025 min
Response: 5666363
Conc: 0.76 ng/ml

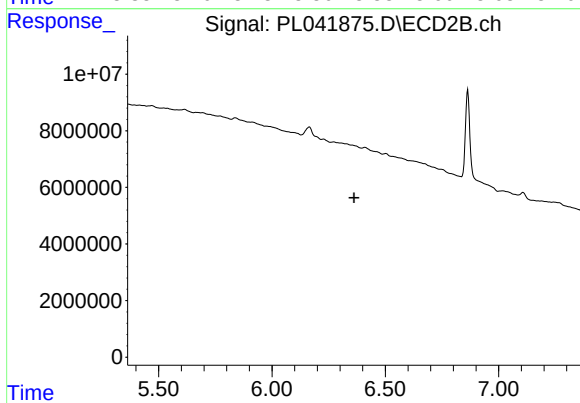

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

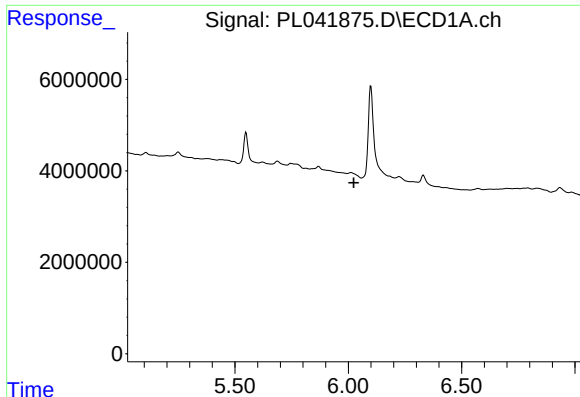

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP4-B

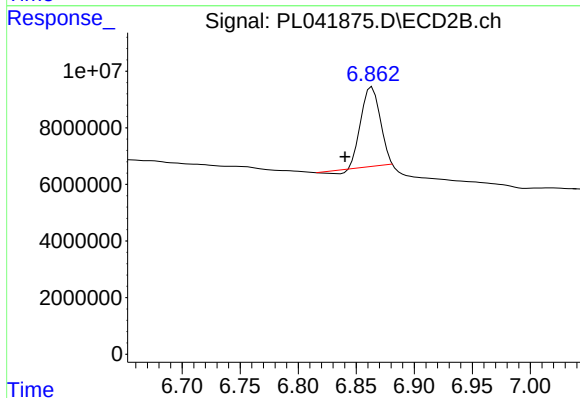


#14 Endrin

R.T.: 6.864 min
Delta R.T.: 0.023 min
Response: 31741263
Conc: 11.68 ng/ml

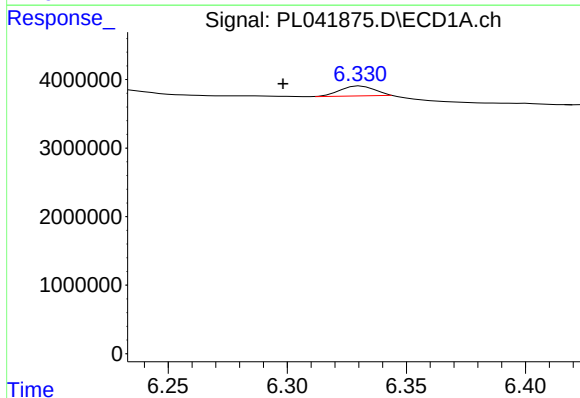


#15 Endosulfan II

R.T.: 6.331 min
Delta R.T.: 0.033 min
Response: 1474567
Conc: 0.21 ng/ml

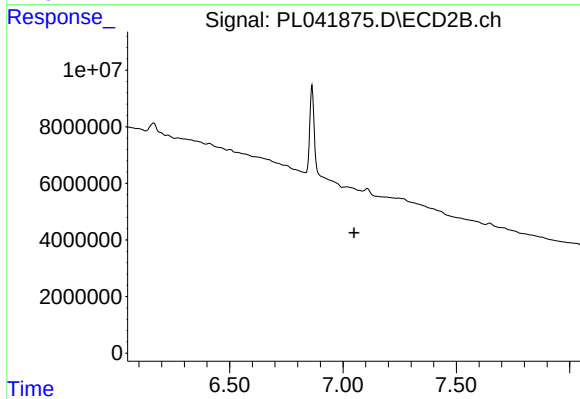

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.048 min
Response: 0
Conc: N.D.

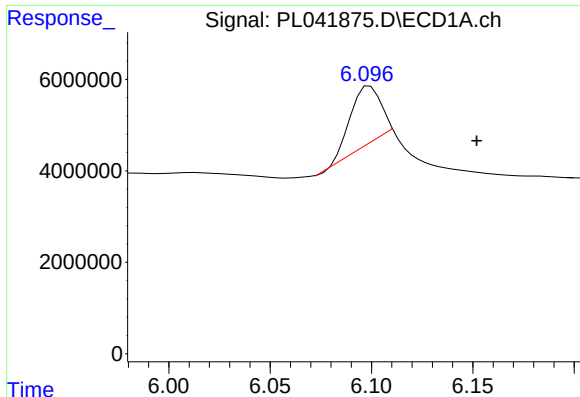

#16 4,4'-DDD


R.T.: 6.099 min
Delta R.T.: -0.053 min
Response: 14168939
Conc: 2.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP4-B

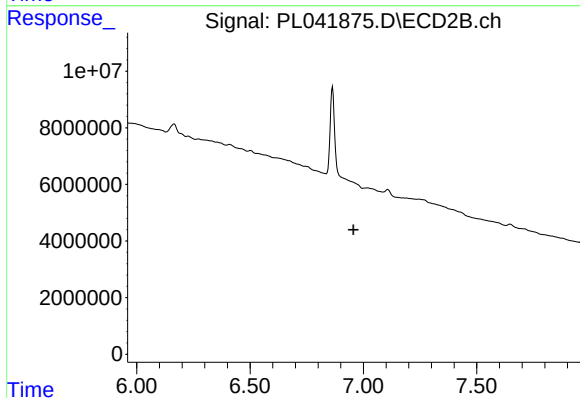


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.957 min
Response: 0
Conc: N.D.

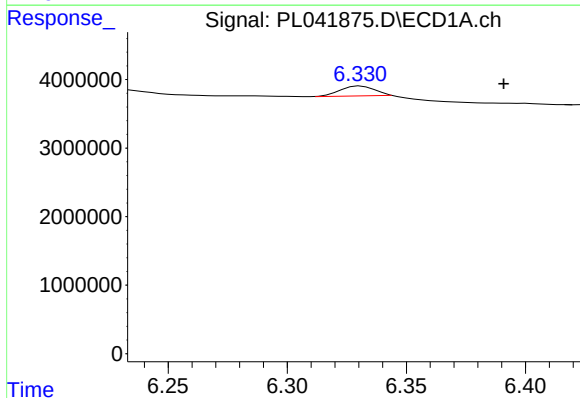


#17 4,4'-DDT

R.T.: 6.331 min
Delta R.T.: -0.060 min
Response: 1474567
Conc: 0.24 ng/ml

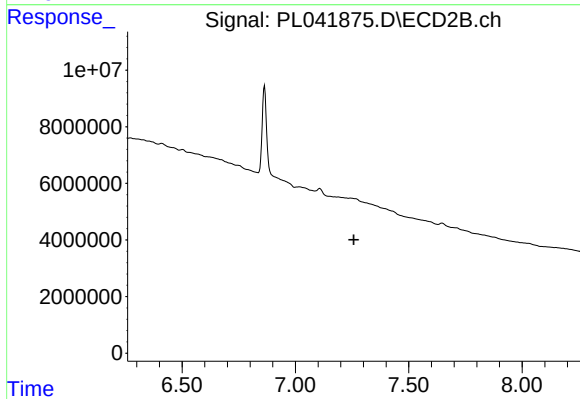

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.258 min
Response: 0
Conc: N.D.

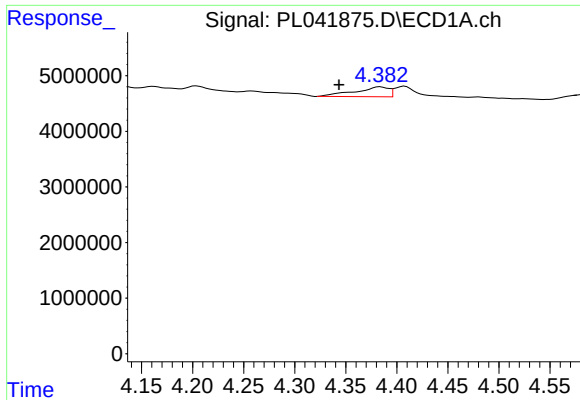

#23 Chlordane-1


R.T.: 4.384 min
Delta R.T.: 0.040 min
Response: 4109448
Conc: 14.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP4-B

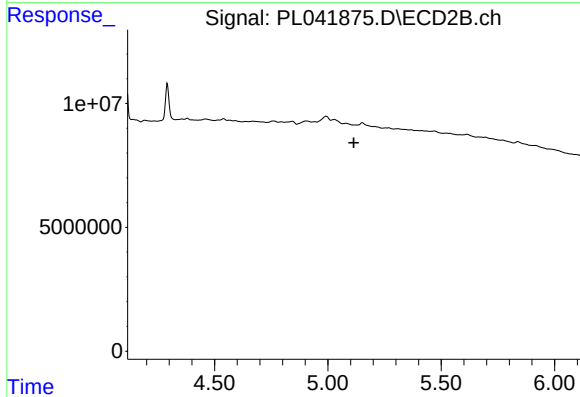


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

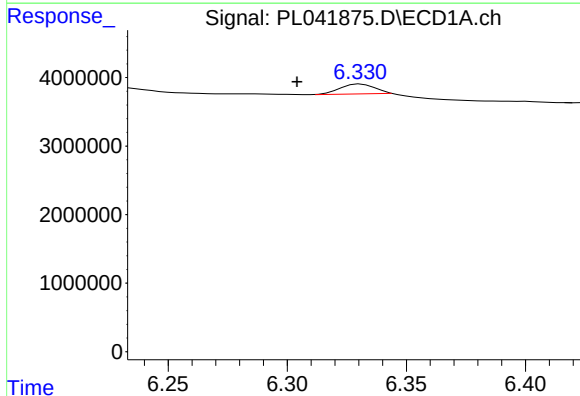


#27 Chlordane-5

R.T.: 6.331 min
Delta R.T.: 0.027 min
Response: 1474567
Conc: 5.91 ng/ml

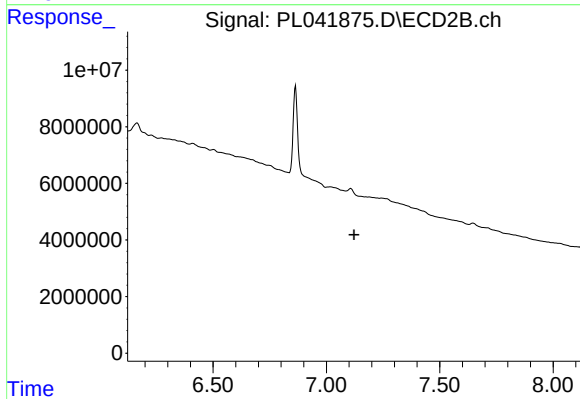

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.123 min
Response: 0
Conc: N.D.

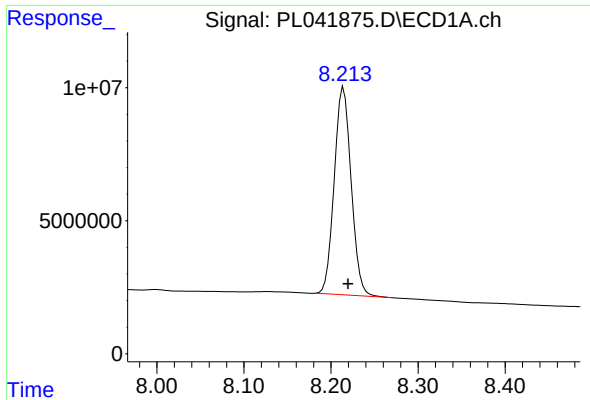

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.005 min
Response: 105494410
Conc: 15.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP4-B

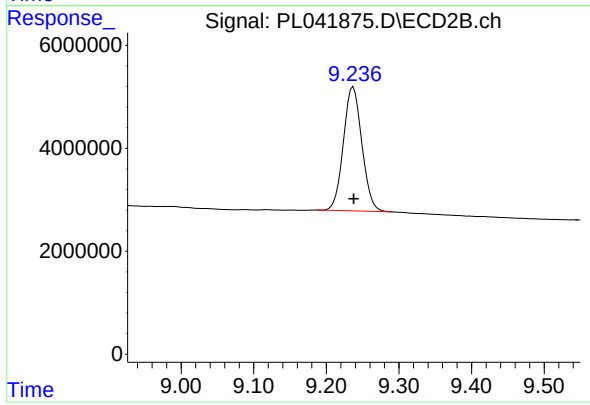

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.000 min
Response: 42604779
Conc: 16.63 ng/ml