

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL110618\  
 Data File : PL041892.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 06 Nov 2018 20:14  
 Operator : AJ\SJ  
 Sample : J5820-17  
 Misc :  
 ALS Vial : 40 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 07 08:13:10 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL102918.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Oct 30 01:26:00 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|--------|
| -----                       |                 |        |       |          |          |        |        |
| System Monitoring Compounds |                 |        |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.473  | 4.105 | 102.6E6  | 51347009 | 16.105 | 16.670 |
| 28)                         | SA Decachlor... | 8.215  | 9.238 | 85184638 | 33193334 | 12.860 | 12.955 |
| Target Compounds            |                 |        |       |          |          |        |        |
| 4)                          | MA Heptachlor   | 4.524  | 0.000 | 1228452  | 0        | 0.134  | N.D. # |
| 6)                          | B beta-BHC      | 4.408f | 0.000 | 2597803  | 0        | 0.689  | N.D. # |
| 15)                         | B Endosulfa...  | 6.232f | 0.000 | 2071380  | 0        | 0.300  | N.D. # |
| 23)                         | Chlordane-1     | 4.384  | 0.000 | 3055222  | 0        | 10.775 | N.D. # |
| -----                       |                 |        |       |          |          |        |        |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL110618\  
Data File : PL041892.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 06 Nov 2018 20:14  
Operator : AJ\SJ  
Sample : J5820-17  
Misc :  
ALS Vial : 40 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampled :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 07 08:13:10 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL102918.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 30 01:26:00 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

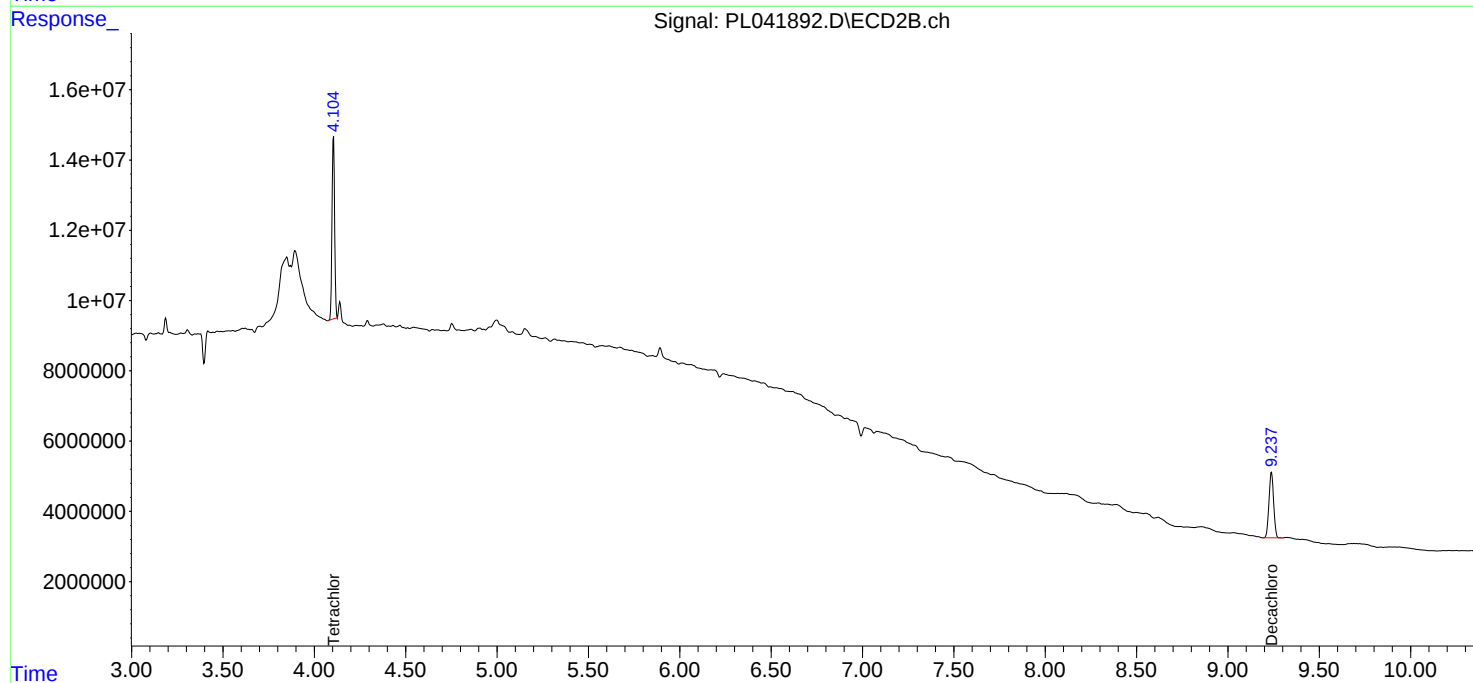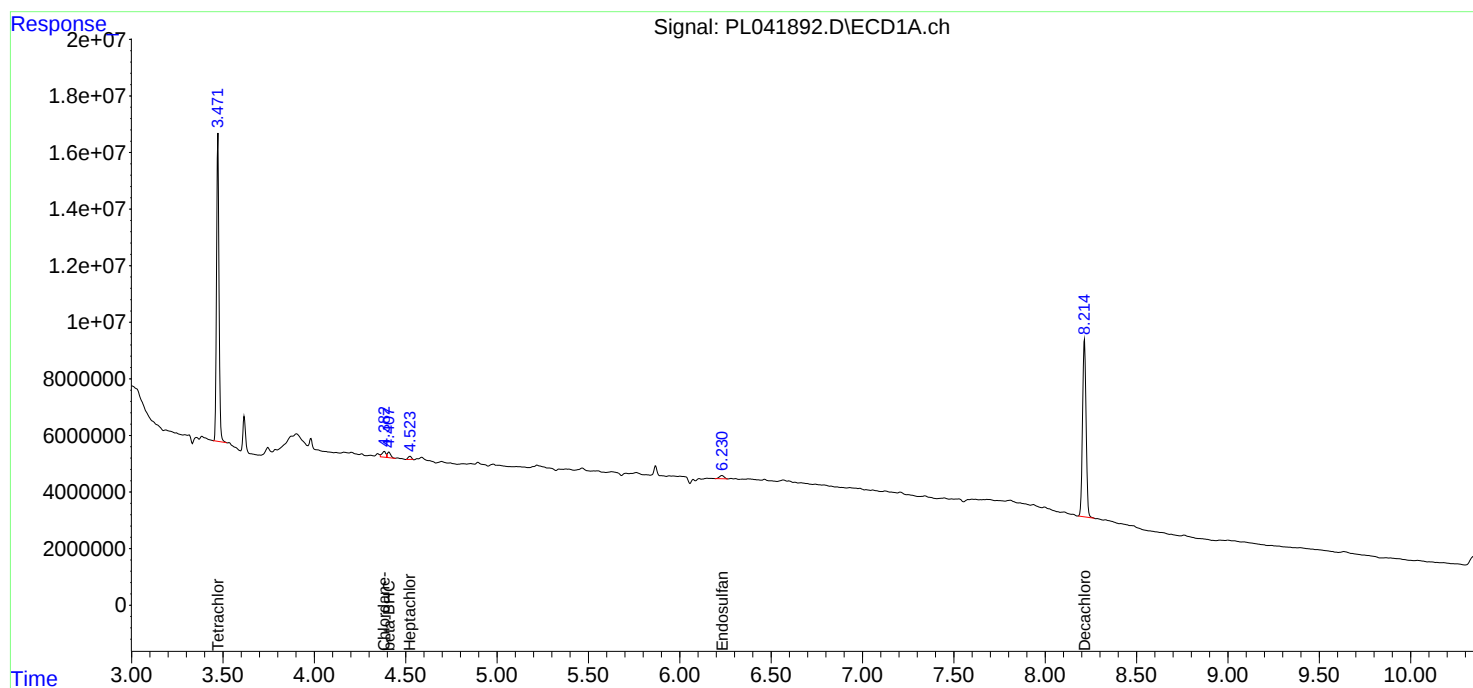


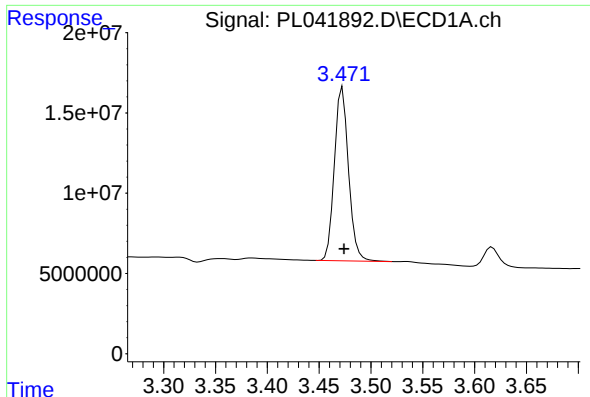

#1 Tetrachloro-m-xylene


R.T.: 3.473 min  
Delta R.T.: -0.001 min  
Response: 102595407  
Conc: 16.11 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

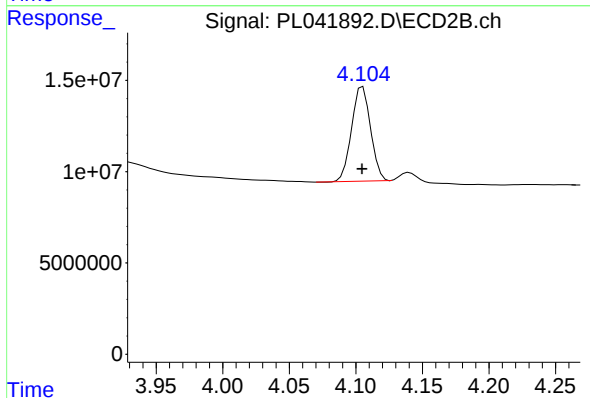


#1 Tetrachloro-m-xylene

R.T.: 4.105 min  
Delta R.T.: 0.000 min  
Response: 51347009  
Conc: 16.67 ng/ml

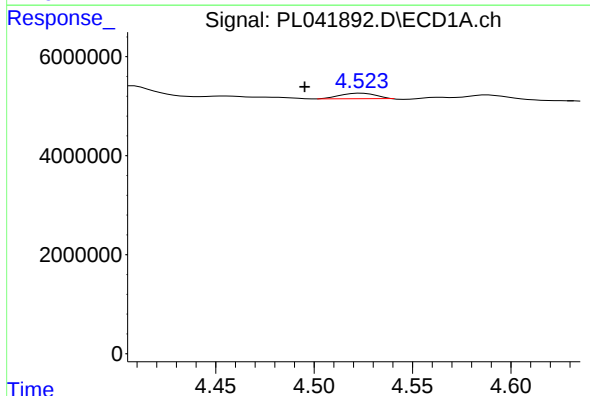


#4 Heptachlor

R.T.: 4.524 min  
Delta R.T.: 0.029 min  
Response: 1228452  
Conc: 0.13 ng/ml

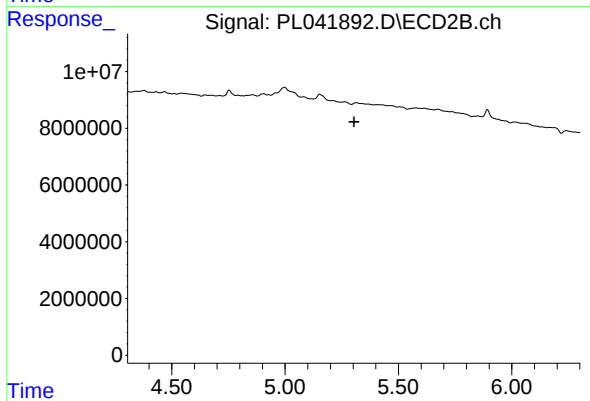

#4 Heptachlor


R.T.: 0.000 min  
Exp R.T. : 5.305 min  
Response: 0  
Conc: N.D.

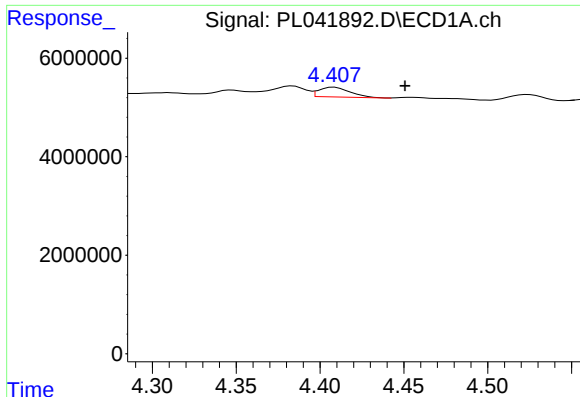

#6 beta-BHC


R.T.: 4.408 min  
Delta R.T.: -0.042 min  
Response: 2597803  
Conc: 0.69 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

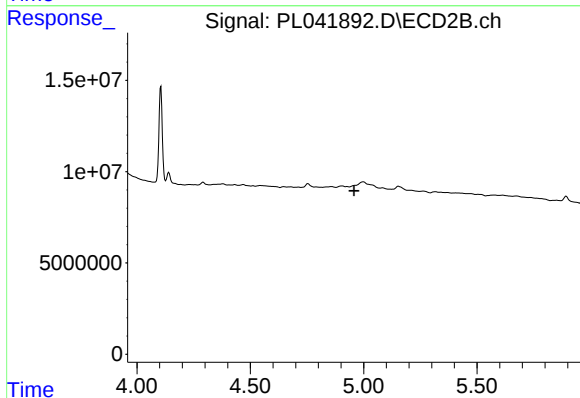


#6 beta-BHC

R.T.: 0.000 min  
Exp R.T. : 4.957 min  
Response: 0  
Conc: N.D.

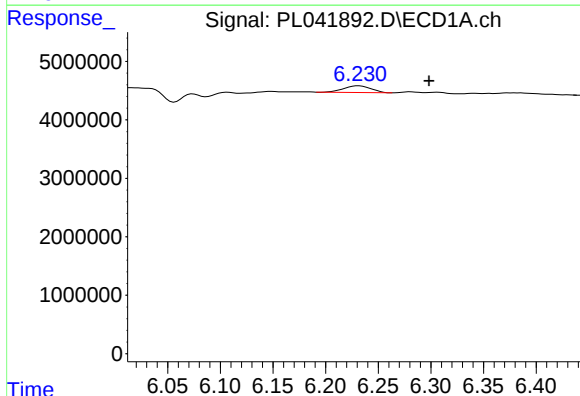


#15 Endosulfan II

R.T.: 6.232 min  
Delta R.T.: -0.067 min  
Response: 2071380  
Conc: 0.30 ng/ml

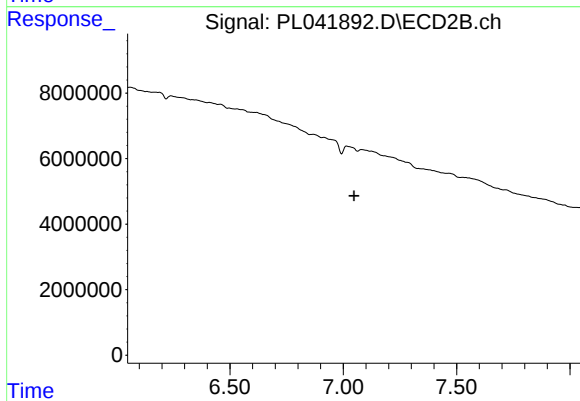

#15 Endosulfan II


R.T.: 0.000 min  
Exp R.T. : 7.048 min  
Response: 0  
Conc: N.D.

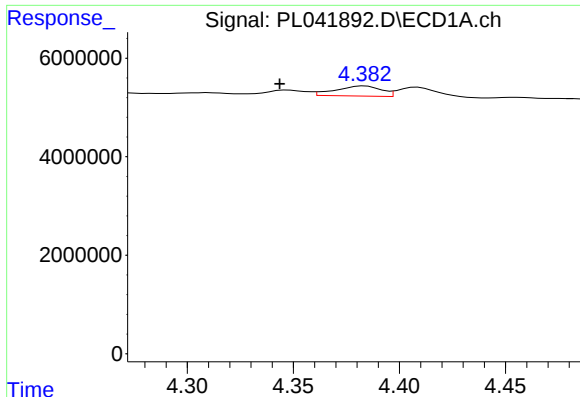

#23 Chlordane-1


R.T.: 4.384 min  
Delta R.T.: 0.040 min  
Response: 3055222  
Conc: 10.78 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

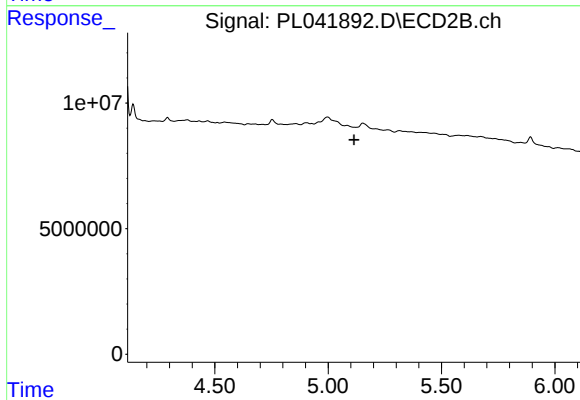


#23 Chlordane-1

R.T.: 0.000 min  
Exp R.T. : 5.115 min  
Response: 0  
Conc: N.D.

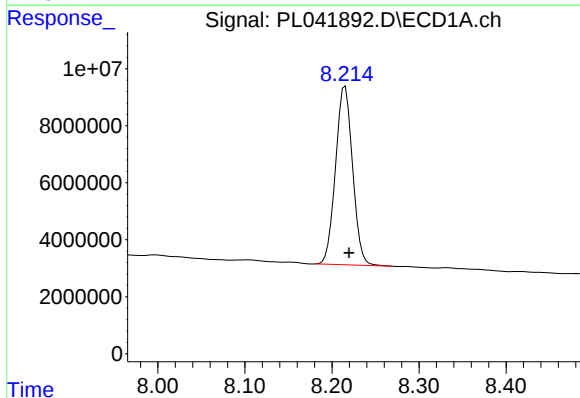

#28 Decachlorobiphenyl

R.T.: 8.215 min  
Delta R.T.: -0.004 min  
Response: 85184638  
Conc: 12.86 ng/ml

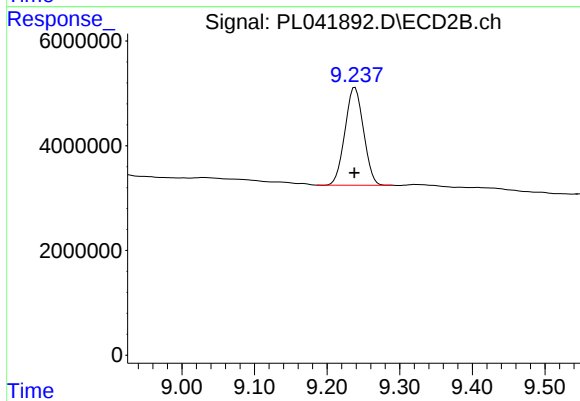

#28 Decachlorobiphenyl

R.T.: 9.238 min  
Delta R.T.: 0.000 min  
Response: 33193334  
Conc: 12.96 ng/ml