

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
 Data File : PL041912.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2018 00:56
 Operator : AJ\SJ
 Sample : J5827-50
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 08:15:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.104	119.4E6	65108129	18.738	21.137
28)	SA Decachlor...	8.213	9.235	137.4E6	53645177	20.742	20.937
Target Compounds							
2)	A alpha-BHC	3.868f	0.000	963366	0	0.099	N.D. #
6)	B beta-BHC	4.408f	0.000	8680726	0	2.303	N.D. #
7)	B delta-BHC	0.000	5.151f	0	602955	N.D.	0.149 #
23)	Chlordane-1	4.384	5.151	2261918	602955	7.977	4.341 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
Data File : PL041912.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2018 00:56
Operator : AJ\SJ
Sample : J5827-50
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SP-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 08:15:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

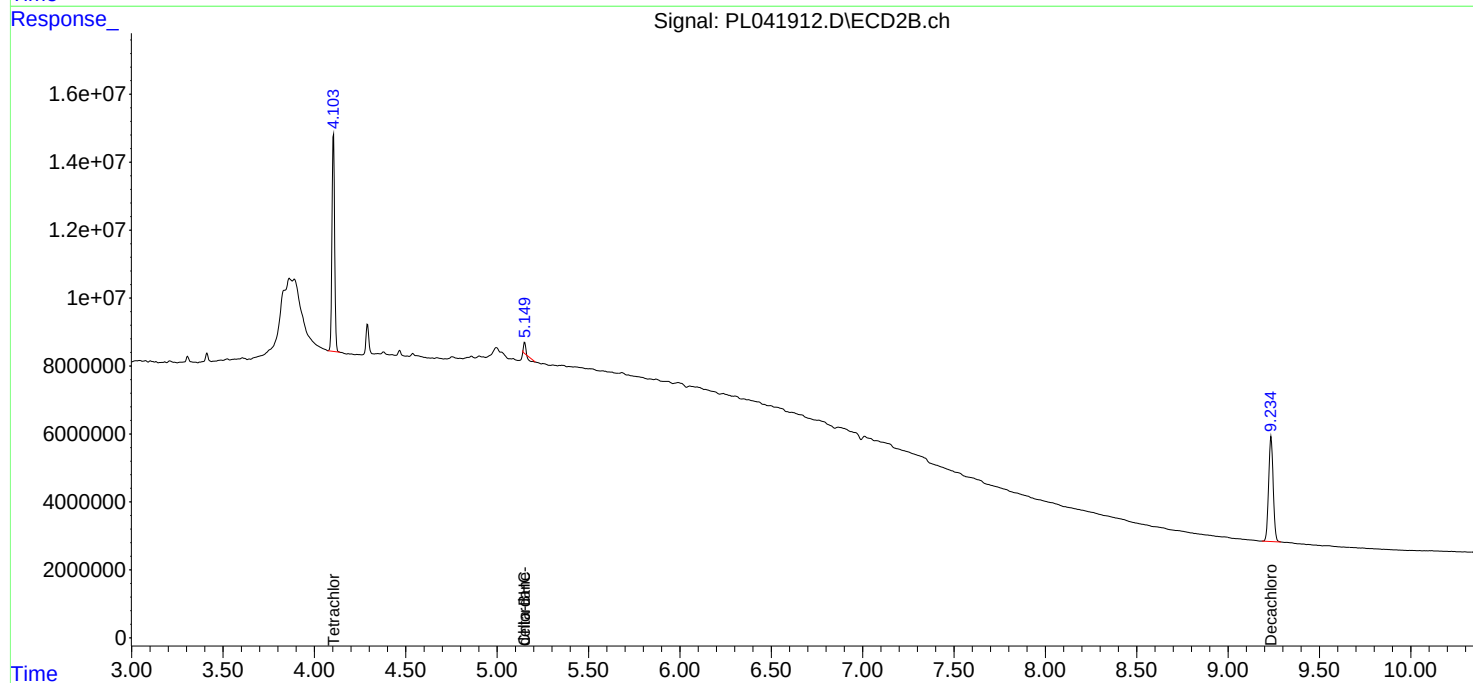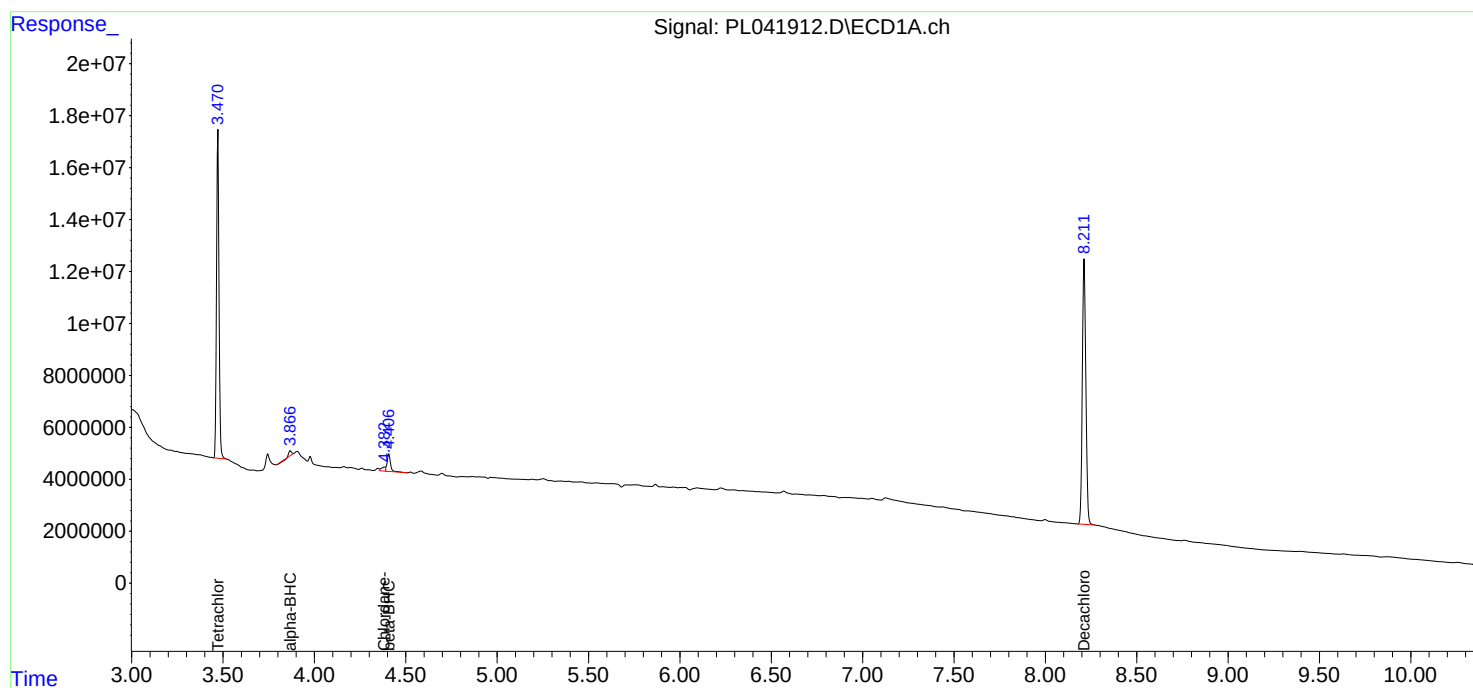


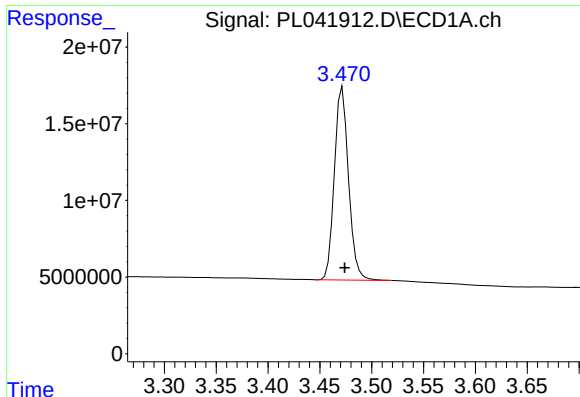

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 119364586
Conc: 18.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-E

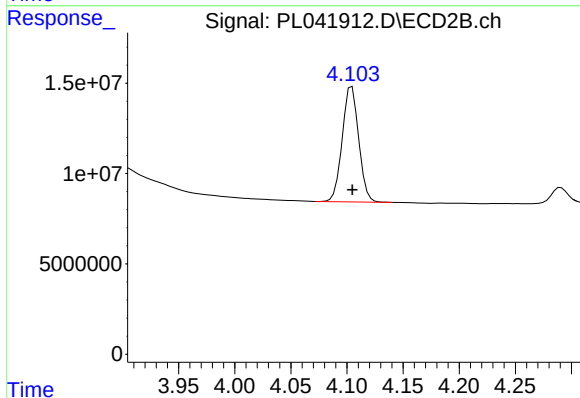


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 65108129
Conc: 21.14 ng/ml

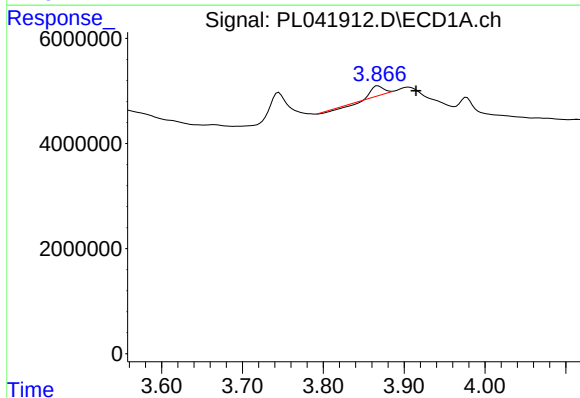


#2 alpha-BHC

R.T.: 3.868 min
Delta R.T.: -0.047 min
Response: 963366
Conc: 0.10 ng/ml

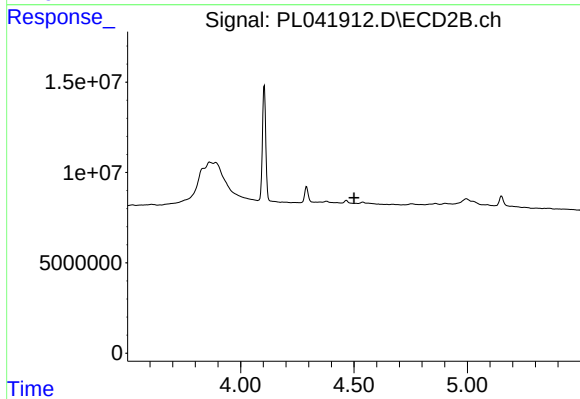

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.501 min
Response: 0
Conc: N.D.

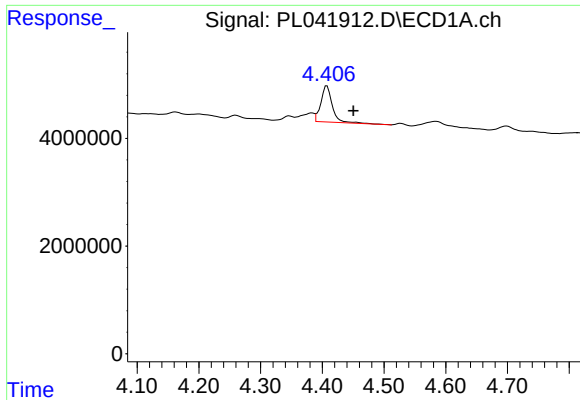

#6 beta-BHC


R.T.: 4.408 min
Delta R.T.: -0.043 min
Response: 8680726
Conc: 2.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-E

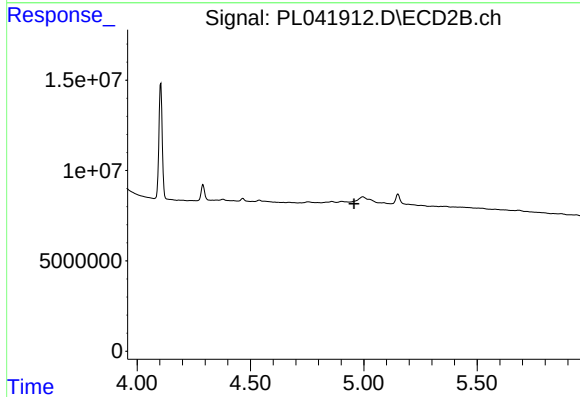


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

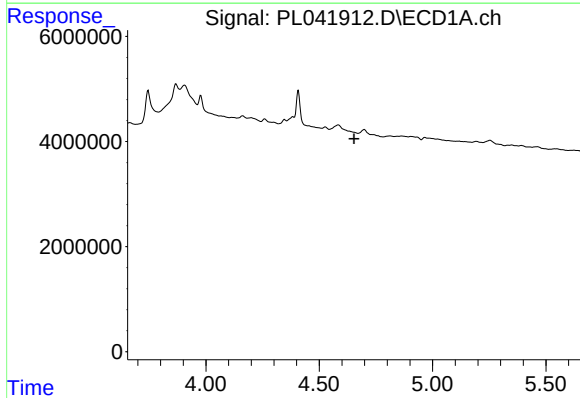


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.654 min
Response: 0
Conc: N.D.

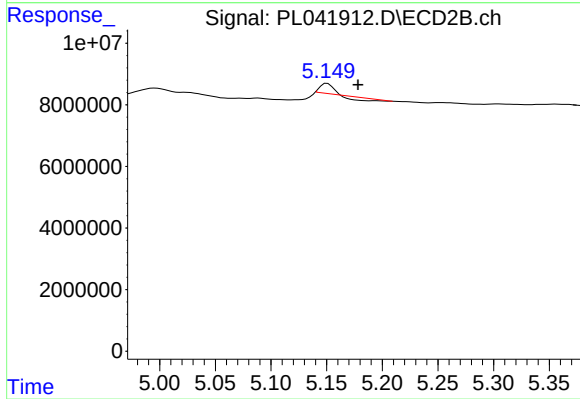

#7 delta-BHC


R.T.: 5.151 min
Delta R.T.: -0.027 min
Response: 602955
Conc: 0.15 ng/ml

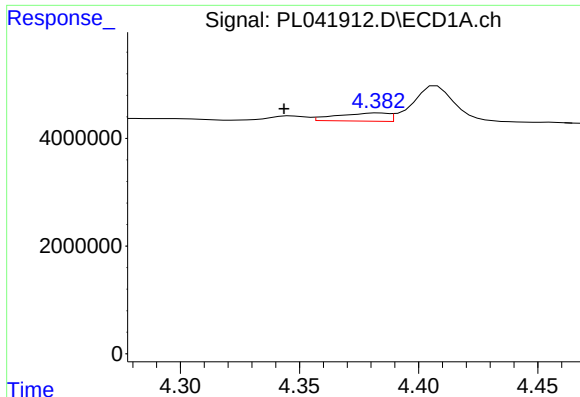

#23 Chlordane-1


R.T.: 4.384 min
Delta R.T.: 0.040 min
Response: 2261918
Conc: 7.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-E

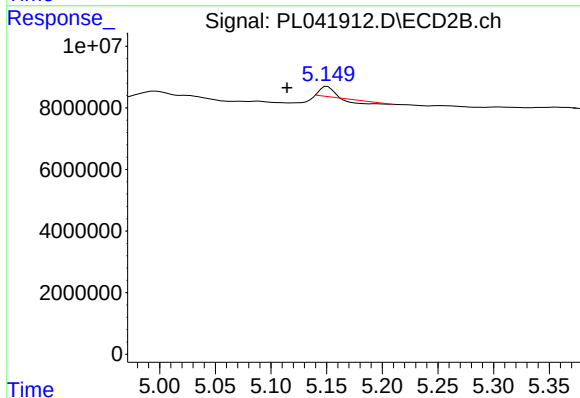


#23 Chlordane-1

R.T.: 5.151 min
Delta R.T.: 0.036 min
Response: 602955
Conc: 4.34 ng/ml

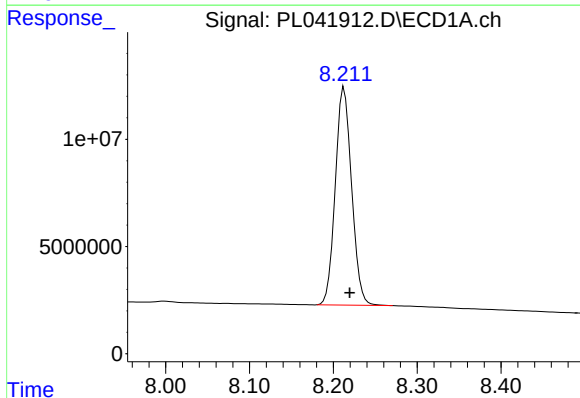

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.007 min
Response: 137395499
Conc: 20.74 ng/ml

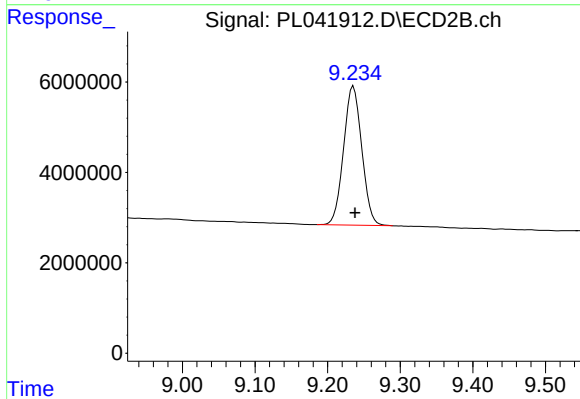

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: -0.002 min
Response: 53645177
Conc: 20.94 ng/ml