

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
 Data File : PL041915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2018 01:38
 Operator : AJ\SJ
 Sample : J5816-04
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-9-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 08:15:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.104	121.4E6	65060179	19.061	21.122
28)	SA Decachlor...	8.214	9.237	133.1E6	52209633	20.092	20.377
Target Compounds							
6)	B beta-BHC	4.408f	0.000	5287161	0	1.403	N.D. #
23)	Chlordane-1	4.408	0.000	5287161	0	18.647	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110618\
Data File : PL041915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2018 01:38
Operator : AJ\SJ
Sample : J5816-04
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-9-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 08:15:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

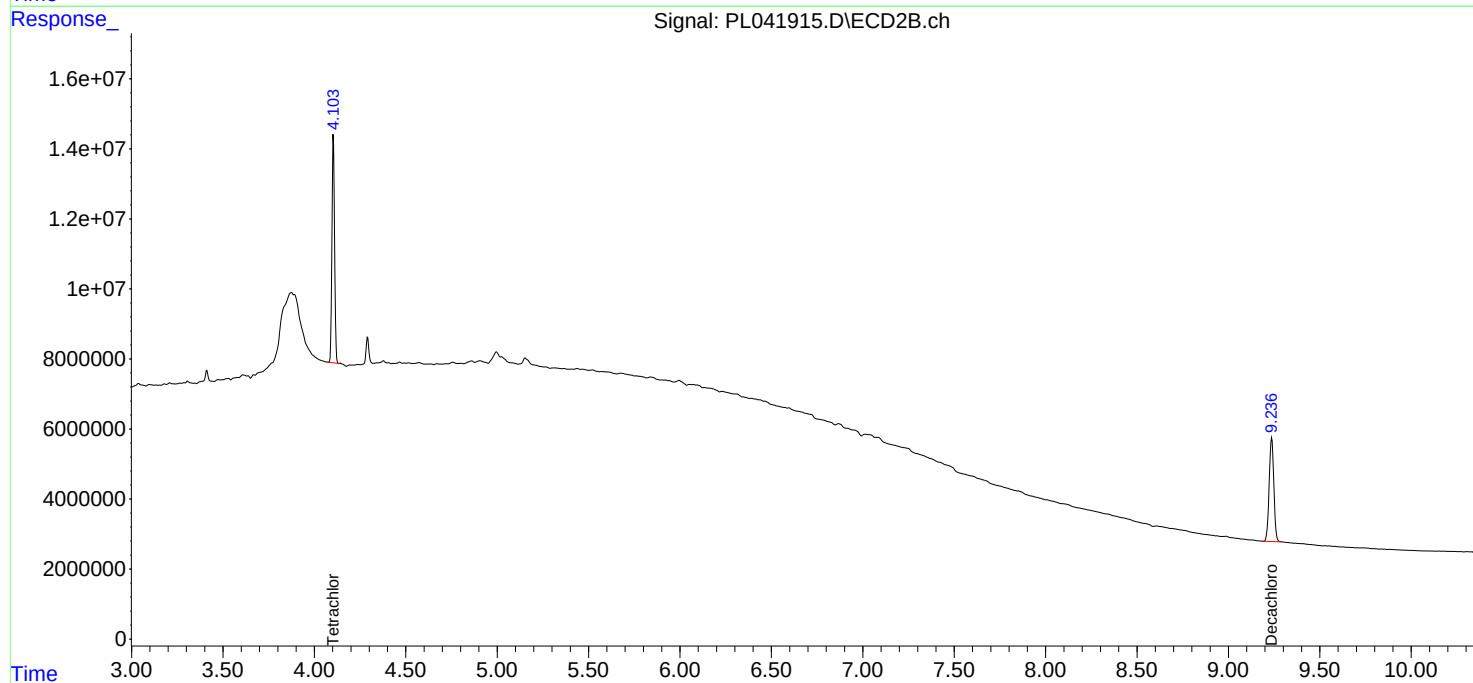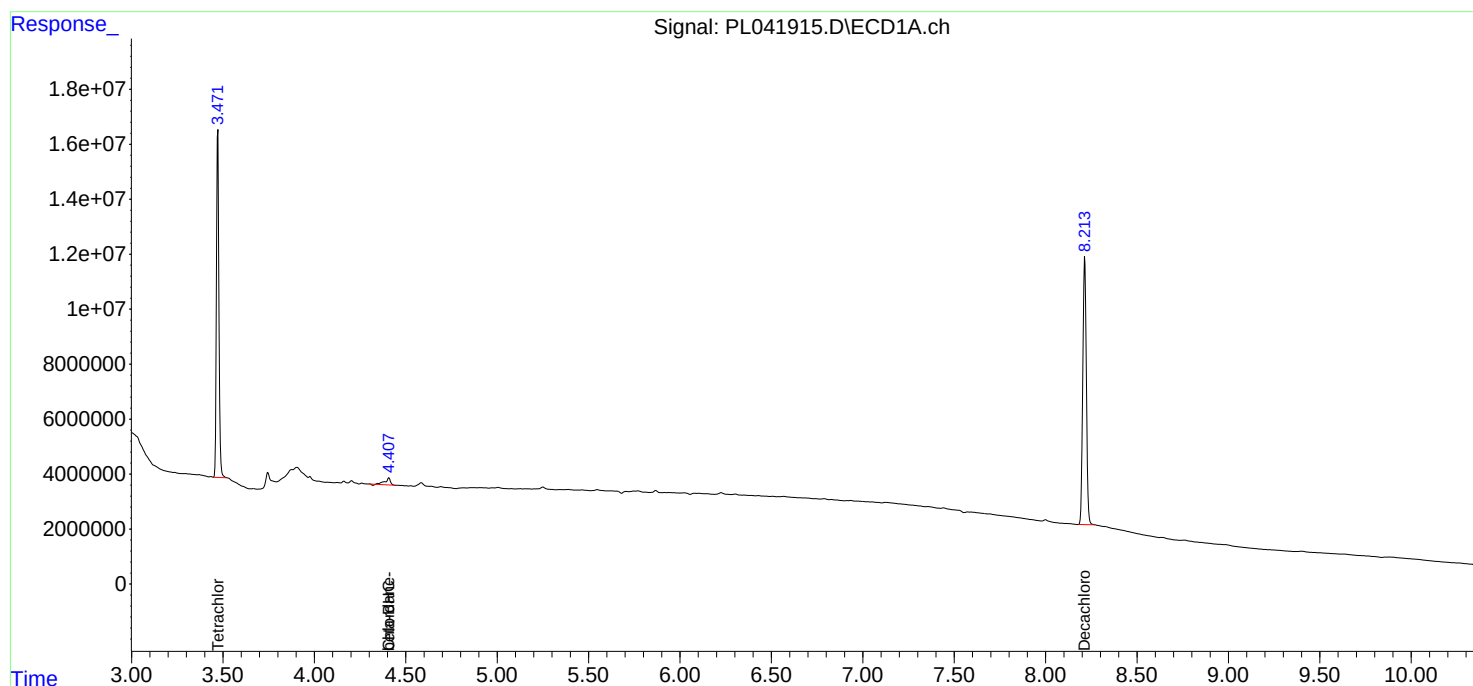


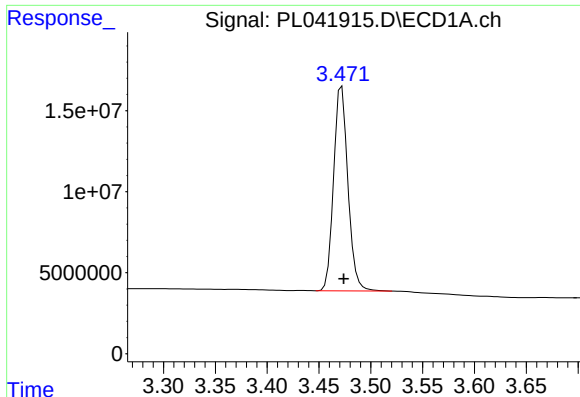

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 121425063
Conc: 19.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-9-S

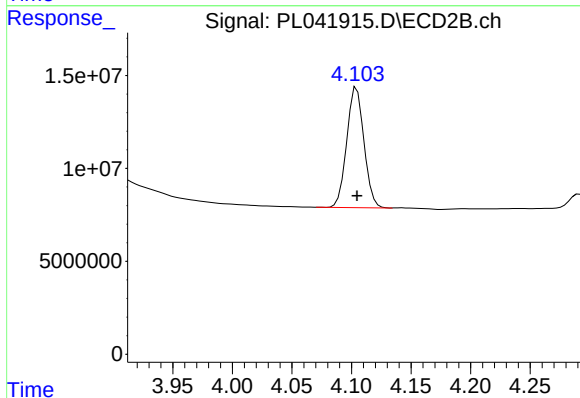


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 65060179
Conc: 21.12 ng/ml

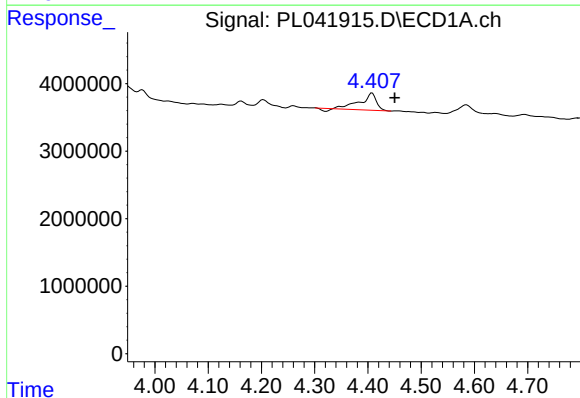


#6 beta-BHC

R.T.: 4.408 min
Delta R.T.: -0.043 min
Response: 5287161
Conc: 1.40 ng/ml

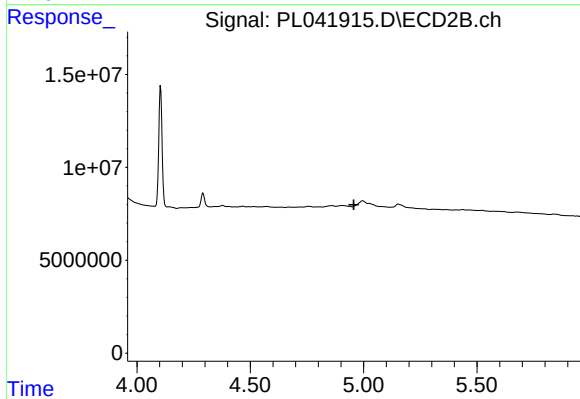

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

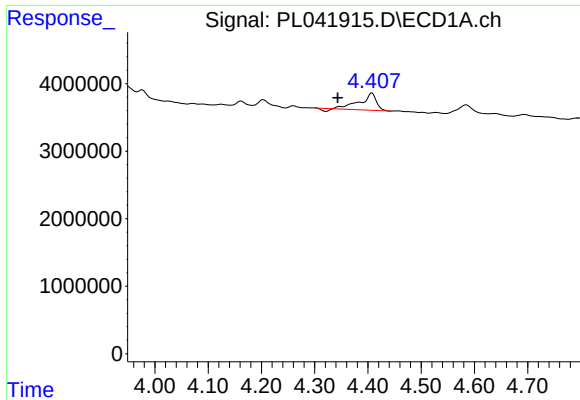

#23 Chlordane-1


R.T.: 4.408 min
Delta R.T.: 0.064 min
Response: 5287161
Conc: 18.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-9-S

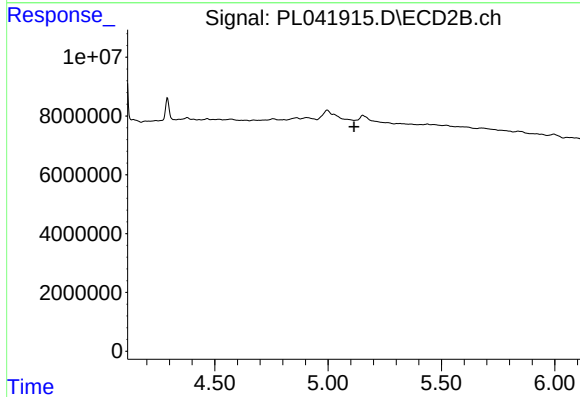


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

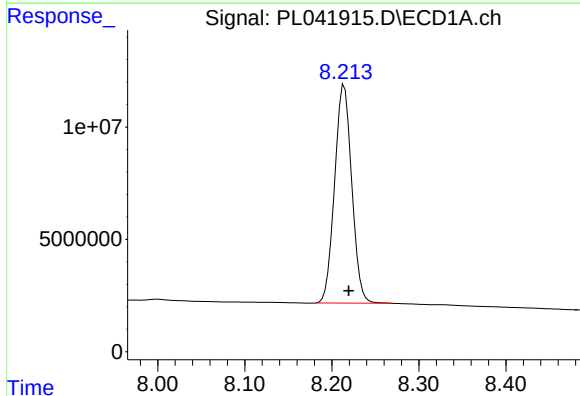

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.005 min
Response: 133091657
Conc: 20.09 ng/ml

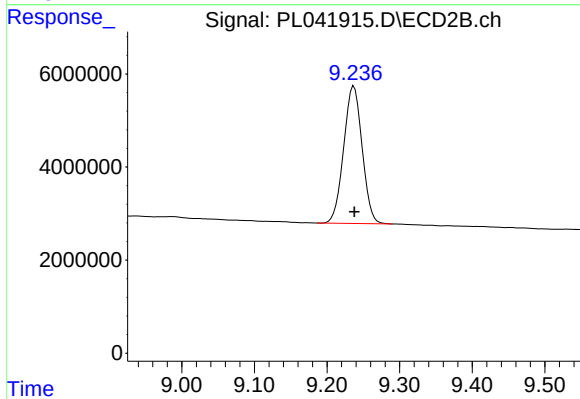

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.000 min
Response: 52209633
Conc: 20.38 ng/ml