

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110619\
 Data File : PL054040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2019 08:28
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 01:02:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
6)	B	beta-BHC	4.517	0.000	1503577	0	0.228 N.D. #
8)	B	Heptachlo...	5.282	5.915	74750065	35337785	5.537 12.117 #
9)	A	Endosulfan I	5.624	0.000	86929284	0	7.072 N.D. #
11)	B	alpha-Chl...	5.557	0.000	130.9E6	0	9.839 N.D. #
12)	B	4,4'-DDE	5.759f	0.000	19738101	0	1.661 N.D. #
14)	MA	Endrin	6.126	6.747	10838209	8207553	0.935 3.381 #
16)	A	4,4'-DDD	6.272f	0.000	4960797	0	0.557 N.D. #
17)	MA	4,4'-DDT	6.469f	7.177	20357880	2022031	2.055 0.874 #
24)		Chlordane-2	4.916f	0.000	82127858	0	213.144 N.D. #
26)		Chlordane-4	5.557	0.000	130.9E6	0	139.621 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110619\
Data File : PL054040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2019 08:28
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 01:02:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

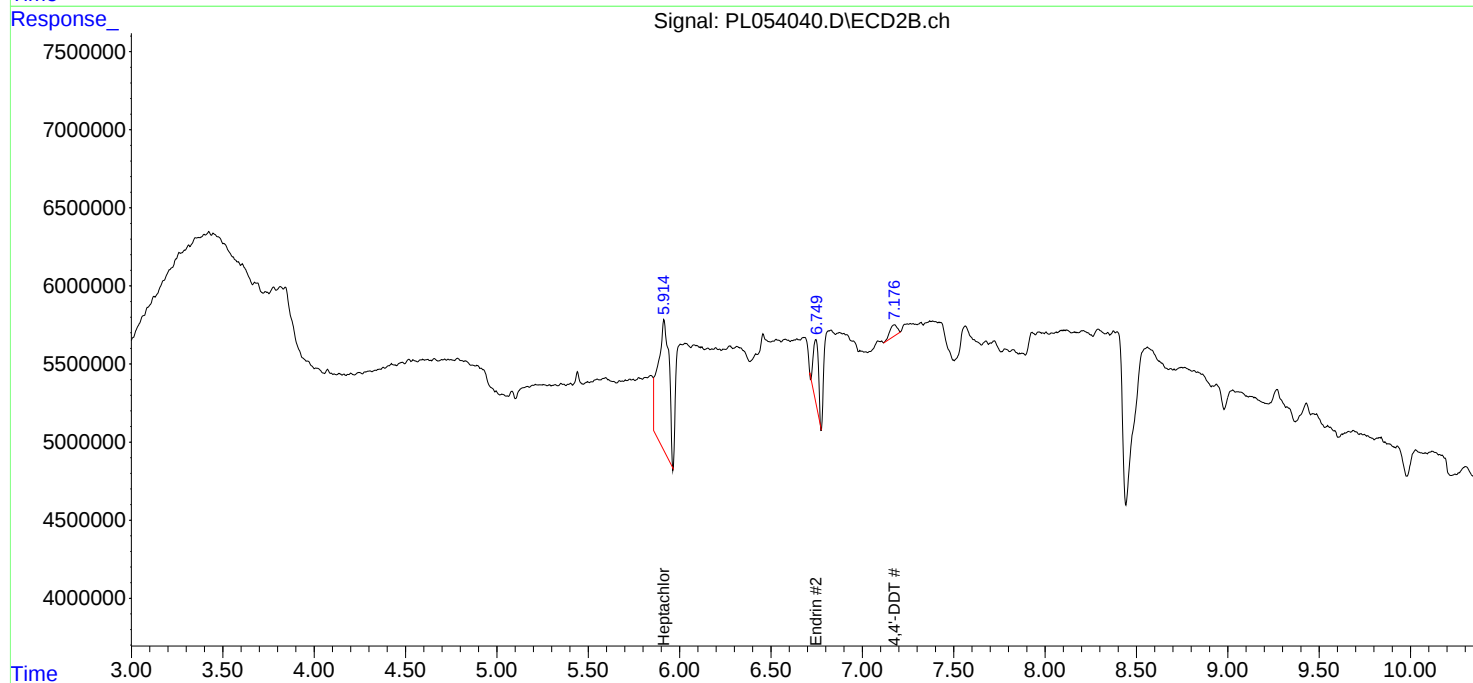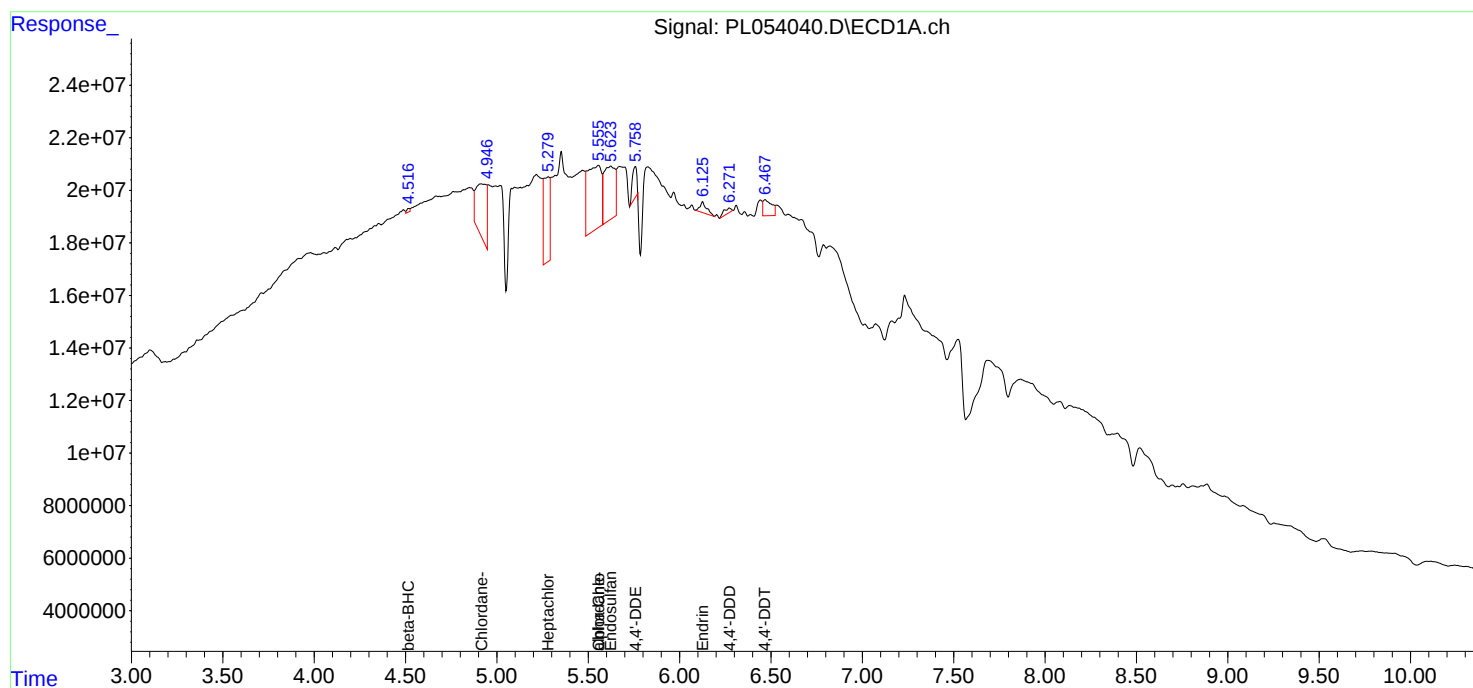


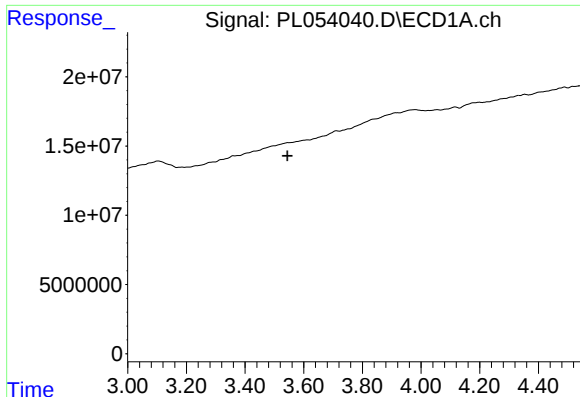

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.544 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

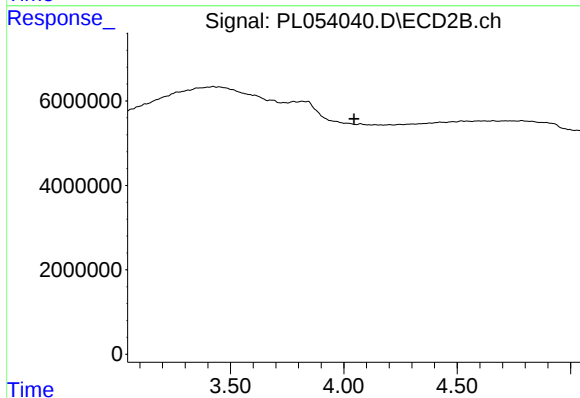


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.046 min
Response: 0
Conc: N.D.

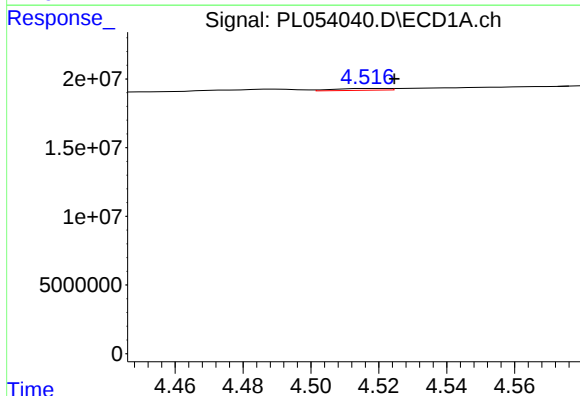


#6 beta-BHC

R.T.: 4.517 min
Delta R.T.: -0.007 min
Response: 1503577
Conc: 0.23 ng/ml

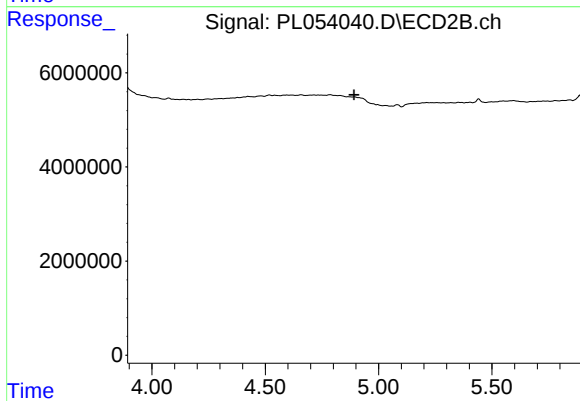

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.892 min
Response: 0
Conc: N.D.

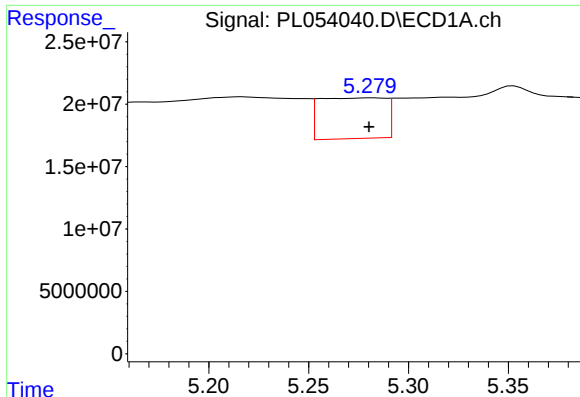

#8 Heptachlor epoxide


R.T.: 5.282 min
Delta R.T.: 0.002 min
Response: 74750065
Conc: 5.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

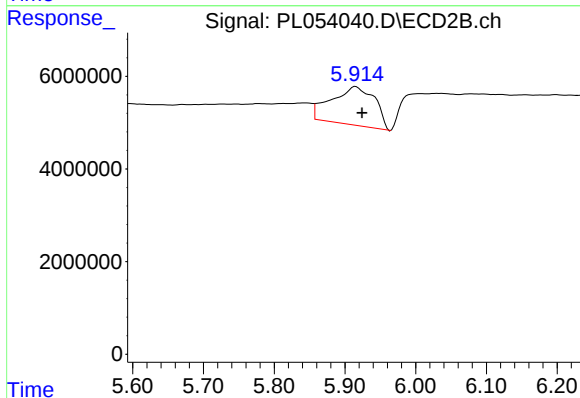


#8 Heptachlor epoxide

R.T.: 5.915 min
Delta R.T.: -0.010 min
Response: 35337785
Conc: 12.12 ng/ml

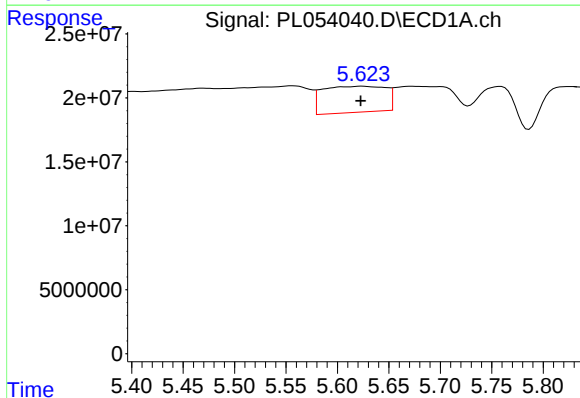


#9 Endosulfan I

R.T.: 5.624 min
Delta R.T.: 0.002 min
Response: 86929284
Conc: 7.07 ng/ml

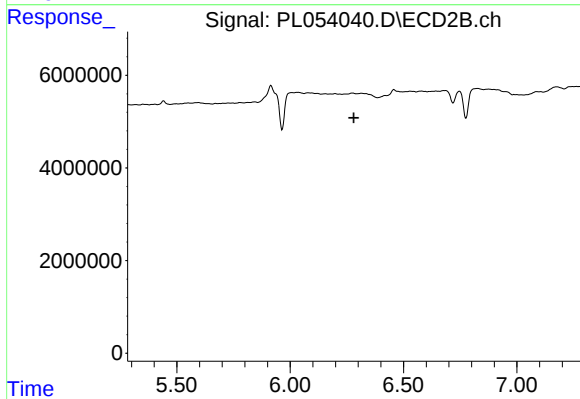

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

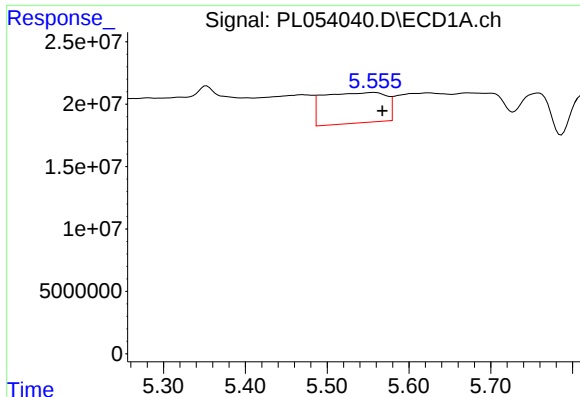

#11 alpha-Chlordane


R.T.: 5.557 min
Delta R.T.: -0.011 min
Response: 130887994
Conc: 9.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

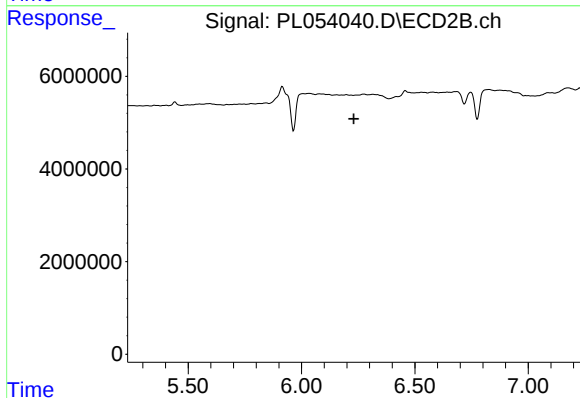


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

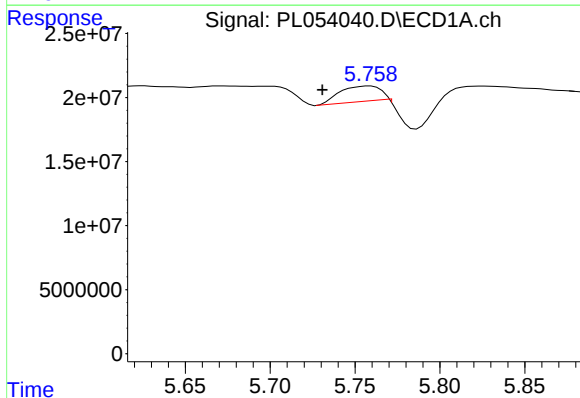


#12 4,4'-DDE

R.T.: 5.759 min
Delta R.T.: 0.028 min
Response: 19738101
Conc: 1.66 ng/ml

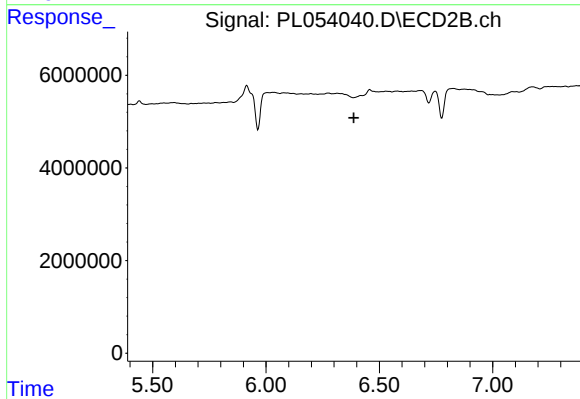

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.387 min
Response: 0
Conc: N.D.

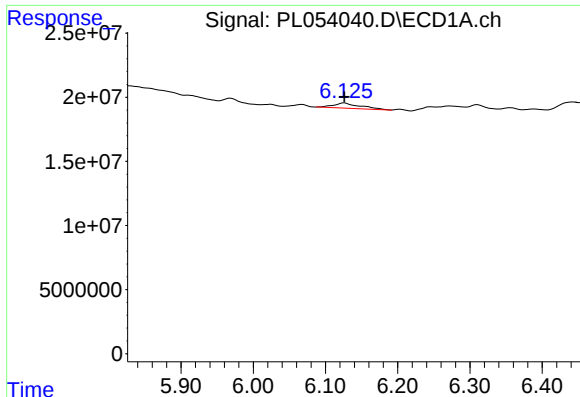

#14 Endrin


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 10838209
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

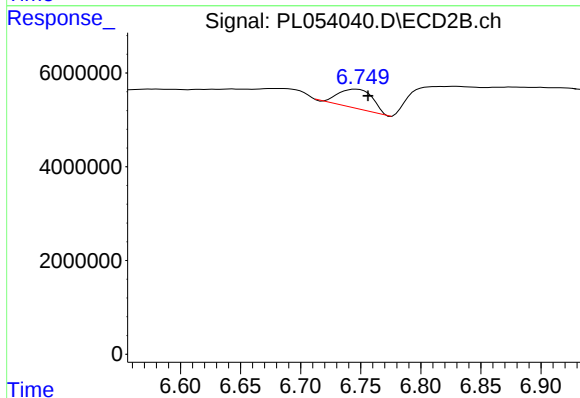


#14 Endrin

R.T.: 6.747 min
Delta R.T.: -0.010 min
Response: 8207553
Conc: 3.38 ng/ml

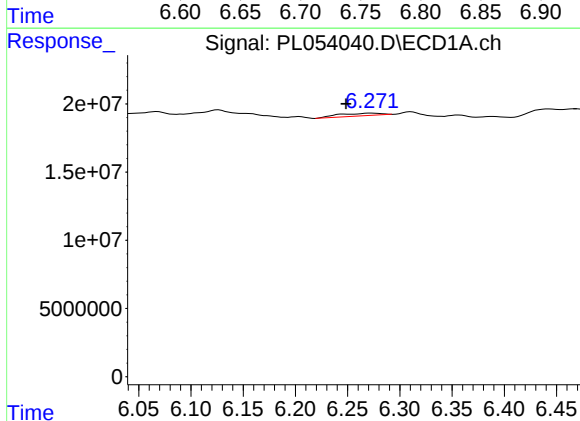


#16 4,4'-DDD

R.T.: 6.272 min
Delta R.T.: 0.024 min
Response: 4960797
Conc: 0.56 ng/ml

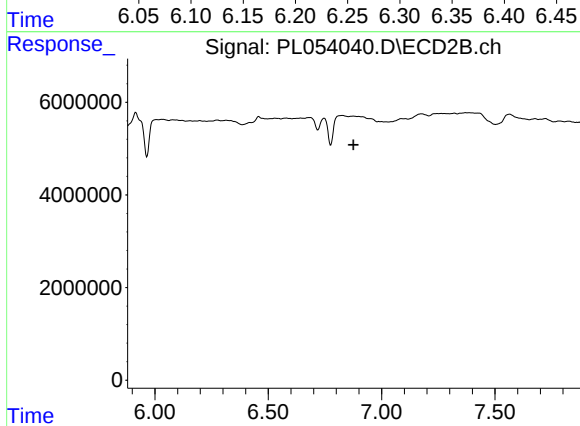

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.877 min
Response: 0
Conc: N.D.

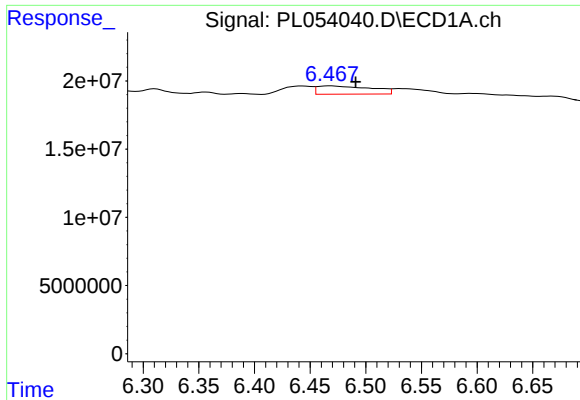

#17 4,4'-DDT


R.T.: 6.469 min
Delta R.T.: -0.023 min
Response: 20357880
Conc: 2.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

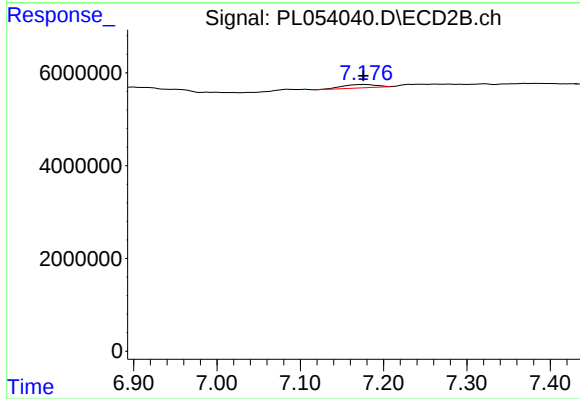


#17 4,4'-DDT

R.T.: 7.177 min
Delta R.T.: 0.001 min
Response: 2022031
Conc: 0.87 ng/ml

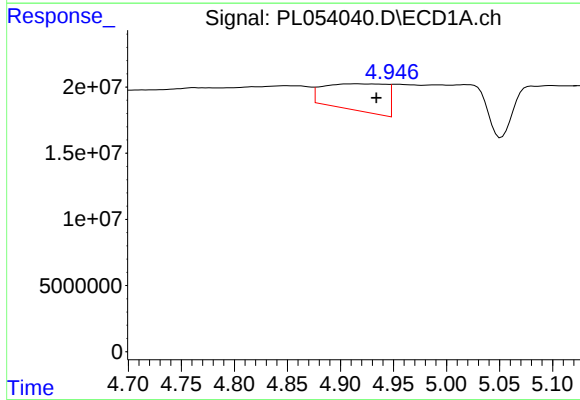


#24 Chlordane-2

R.T.: 4.916 min
Delta R.T.: -0.018 min
Response: 82127858
Conc: 213.14 ng/ml

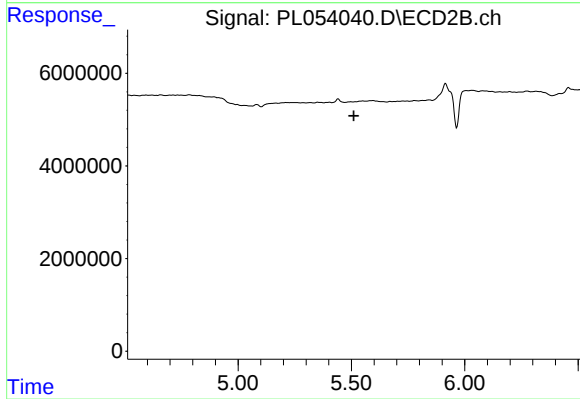

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.510 min
Response: 0
Conc: N.D.

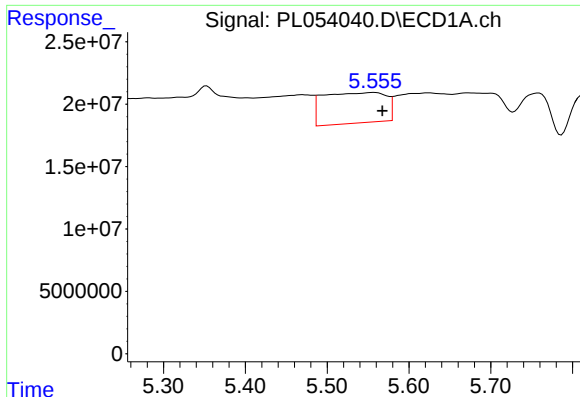

#26 Chlordane-4


R.T.: 5.557 min
Delta R.T.: -0.011 min
Response: 130887994
Conc: 139.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

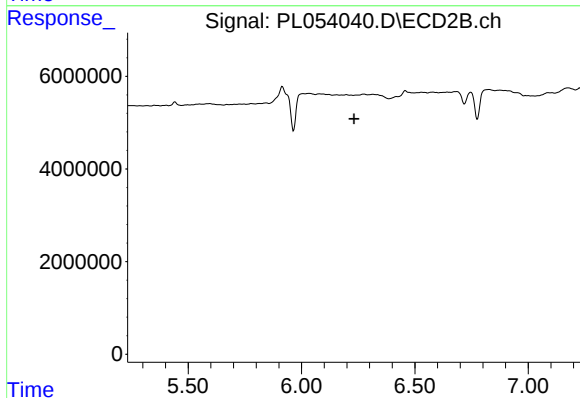


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.232 min
Response: 0
Conc: N.D.

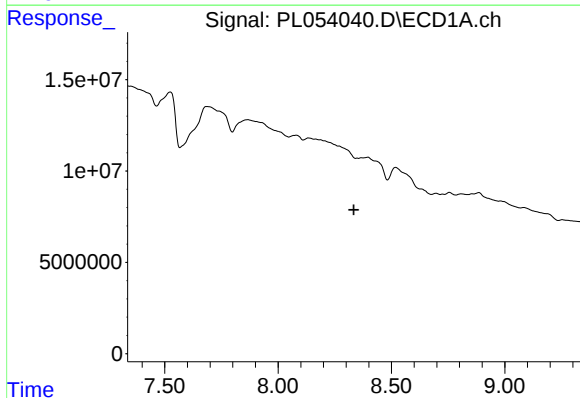

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.334 min
Response: 0
Conc: N.D.

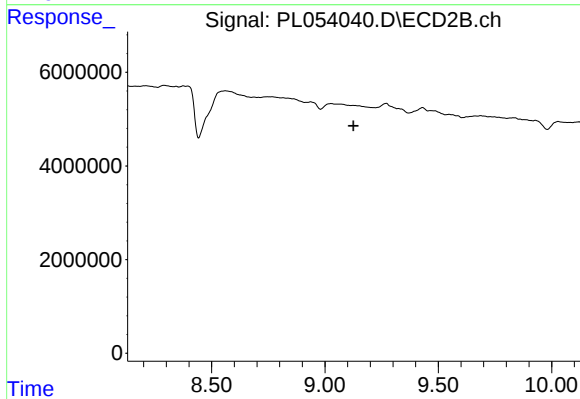

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.126 min
Response: 0
Conc: N.D.