

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110620\
 Data File : PL062862.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2020 08:29
 Operator : DD\AJ
 Sample : HEHANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEHANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:30:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	5.104	5.811	822835	8437849	0.451	2.605 #
16) A	4,4'-DDD	6.065	0.000	735635	0	0.520	N.D. #
17) MA	4,4'-DDT	6.302	7.073	5182922	10765491	3.884	4.795
18) B	Endrin al...	6.381	6.969	3664685	4506760	2.524	1.976
20) A	Methoxychlor	6.851	0.000	3185087	0	3.698	N.D. #
21) B	Endrin ke...	7.057	0.000	2836061	0	1.573	N.D. #
23)	Chlordane-1	4.270	0.000	74323	0	1.442	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110620\
Data File : PL062862.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2020 08:29
Operator : DD\AJ
Sample : HEHANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
HEHANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:30:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

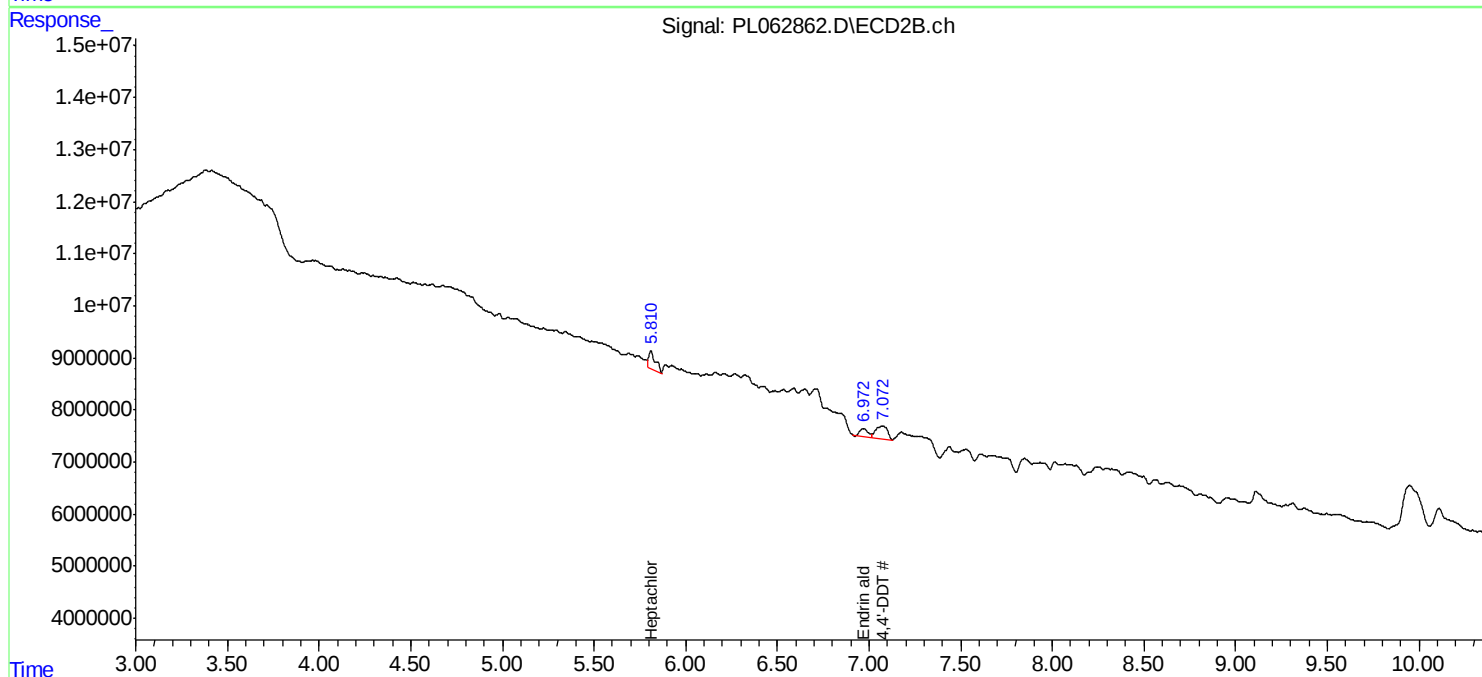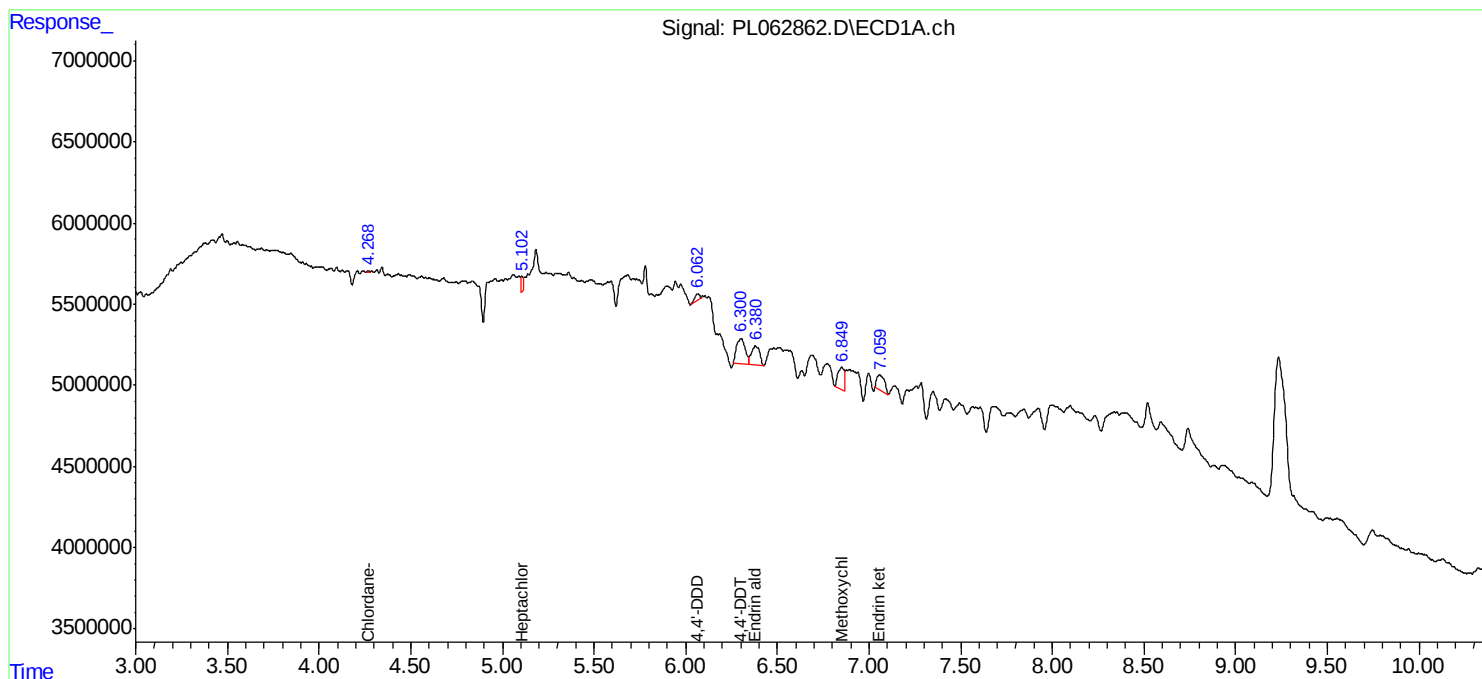


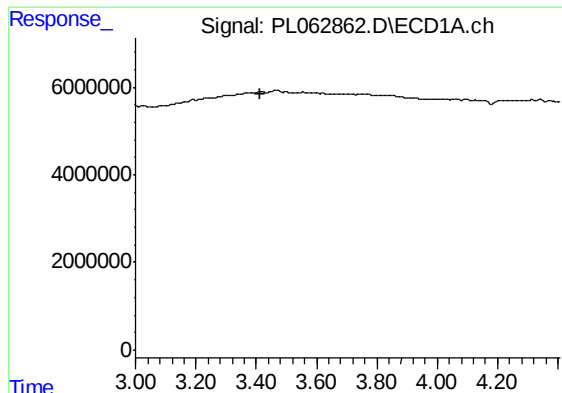

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEHANE

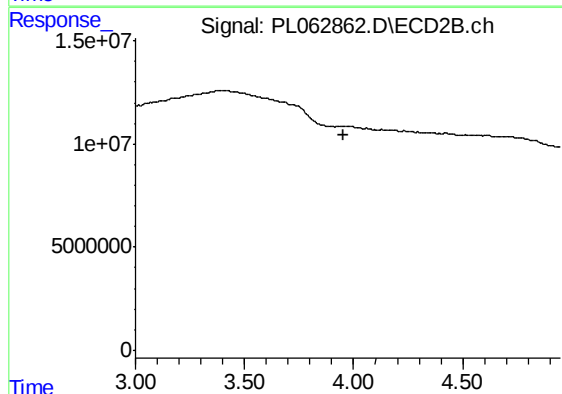


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.952 min
Response: 0
Conc: N.D.

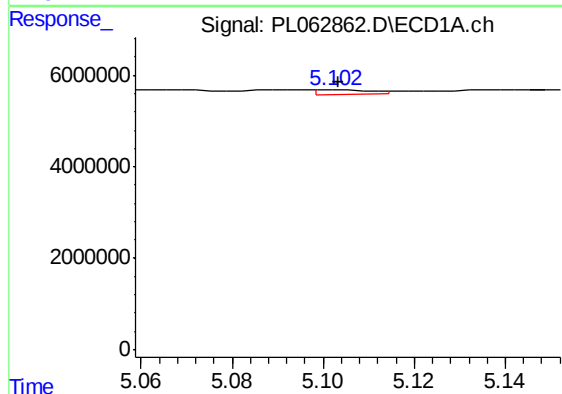


#8 Heptachlor epoxide

R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 822835
Conc: 0.45 ng/ml

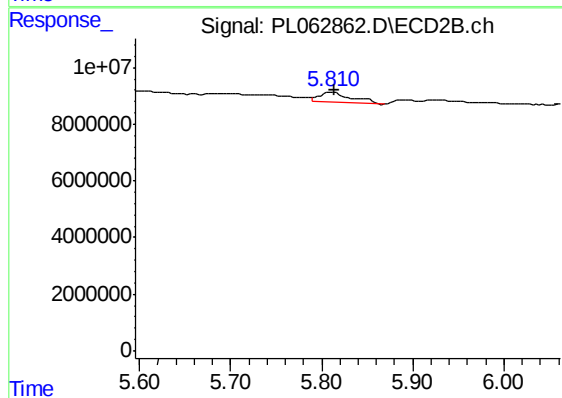

#8 Heptachlor epoxide


R.T.: 5.811 min
Delta R.T.: -0.003 min
Response: 8437849
Conc: 2.61 ng/ml

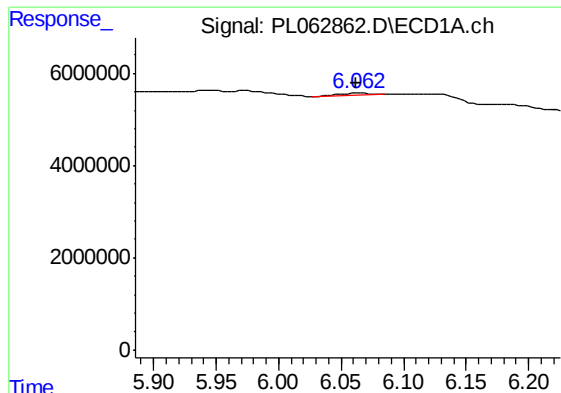

#16 4,4'-DDD


R.T.: 6.065 min
Delta R.T.: 0.003 min
Response: 735635
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEHANE

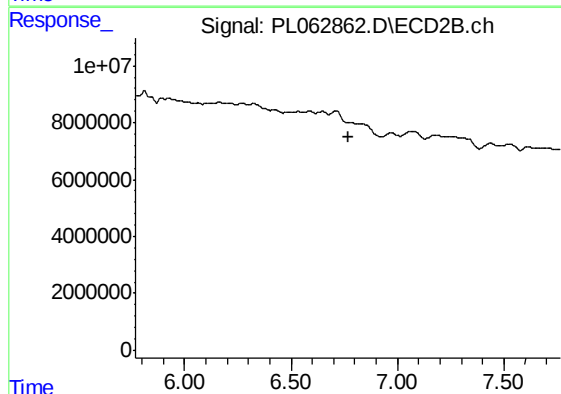


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

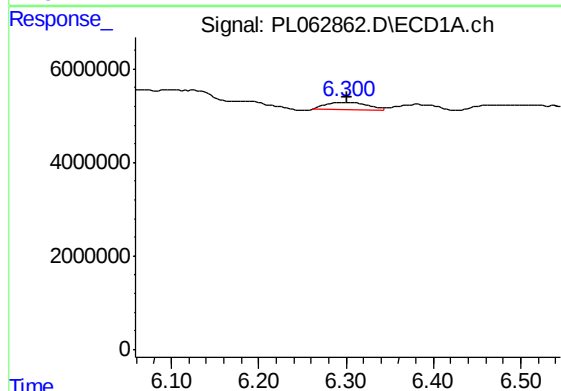


#17 4,4'-DDT

R.T.: 6.302 min
Delta R.T.: 0.000 min
Response: 5182922
Conc: 3.88 ng/ml

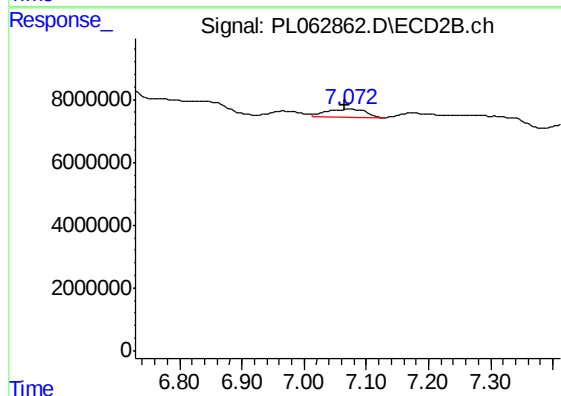

#17 4,4'-DDT


R.T.: 7.073 min
Delta R.T.: 0.007 min
Response: 10765491
Conc: 4.79 ng/ml

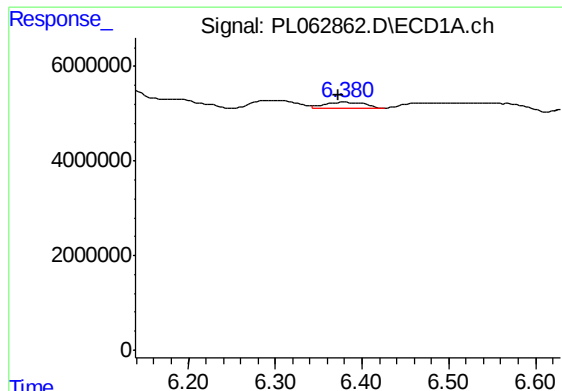

#18 Endrin aldehyde


R.T.: 6.381 min
Delta R.T.: 0.009 min
Response: 3664685
Conc: 2.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEHANE

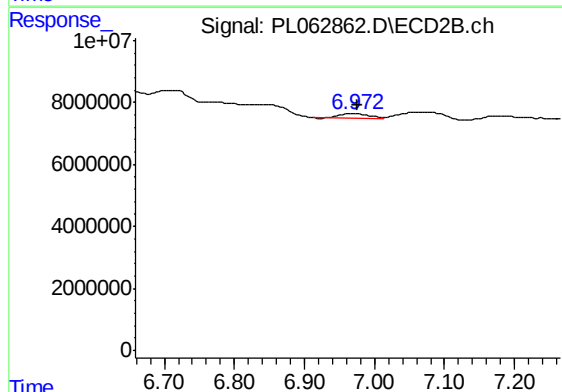


#18 Endrin aldehyde

R.T.: 6.969 min
Delta R.T.: -0.008 min
Response: 4506760
Conc: 1.98 ng/ml

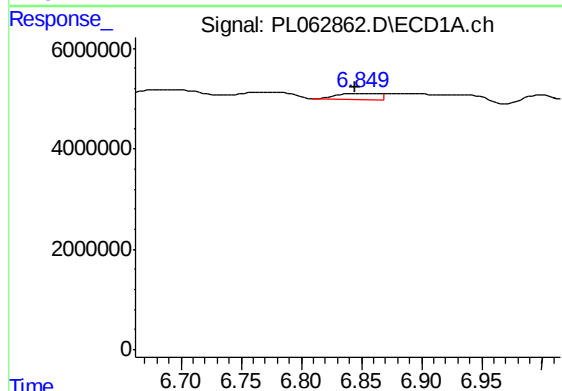


#20 Methoxychlor

R.T.: 6.851 min
Delta R.T.: 0.006 min
Response: 3185087
Conc: 3.70 ng/ml

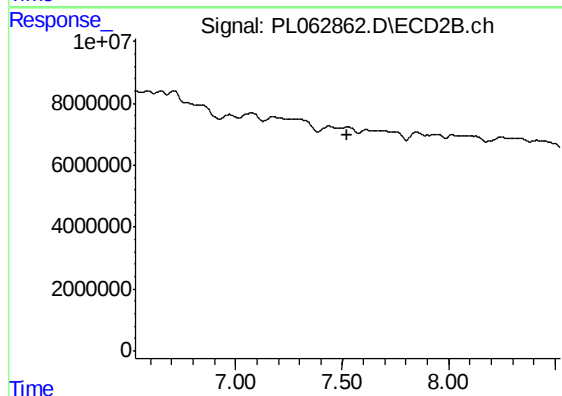

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.526 min
Response: 0
Conc: N.D.

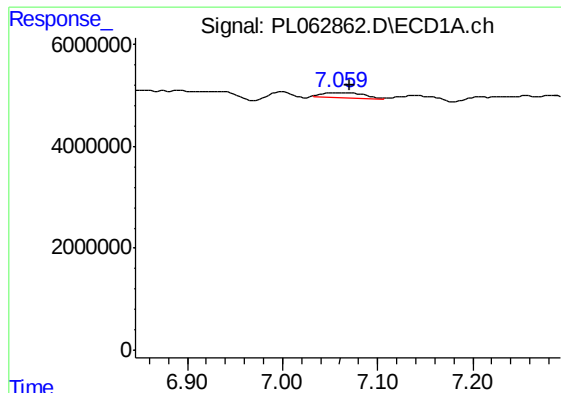

#21 Endrin ketone


R.T.: 7.057 min
Delta R.T.: -0.014 min
Response: 2836061
Conc: 1.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEHANE

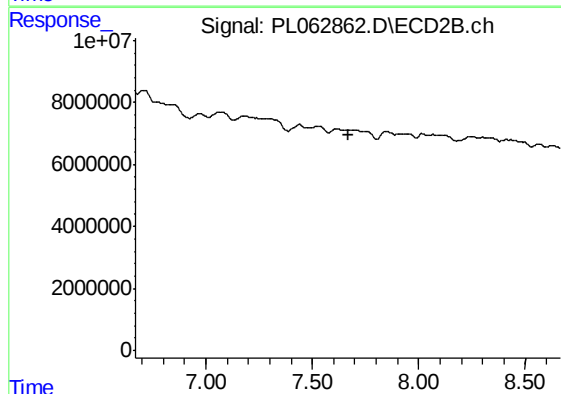


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.668 min
Response: 0
Conc: N.D.

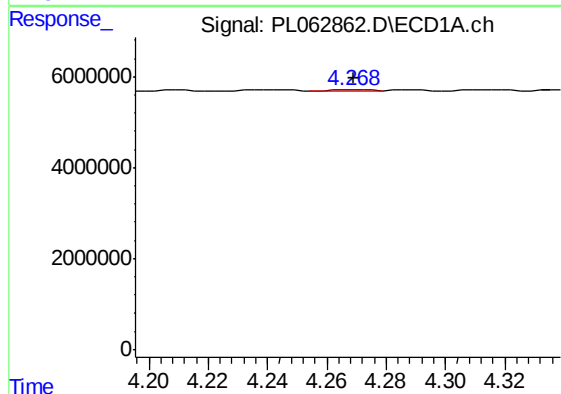


#23 Chlordane-1

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 74323
Conc: 1.44 ng/ml

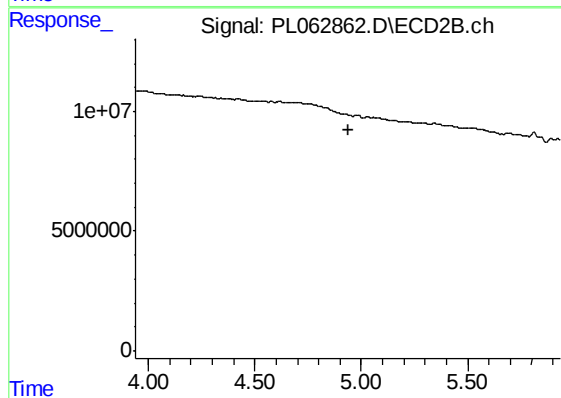

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

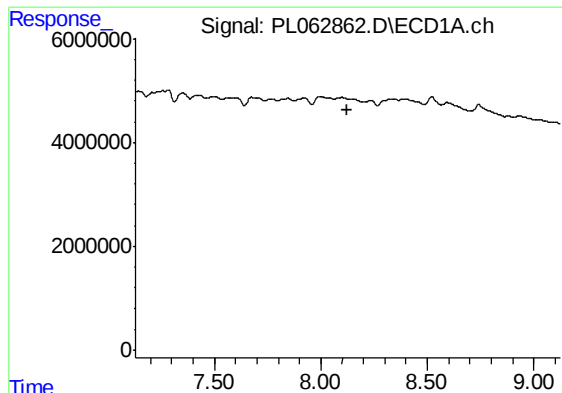

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.126 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEHANE

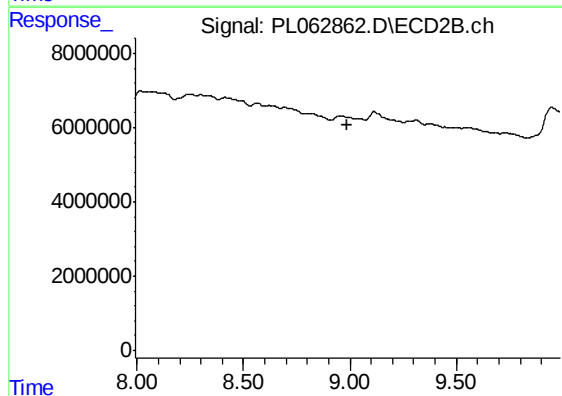

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.989 min
Response: 0
Conc: N.D.