

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110620\
 Data File : PL062874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2020 13:49
 Operator : DD\AJ
 Sample : L4653-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-7-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:35:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	40294170	70550848	23.426	24.007
28)	SA Decachlor...	8.124	8.988	37513224	45838636	23.383	21.901
Target Compounds							
9)	A Endosulfan I	5.458f	0.000	972107	0	0.582	N.D. #
10)	B gamma-Chl...	0.000	6.068f	0	3071921	N.D.	0.913 #
15)	B Endosulfa...	0.000	6.865	0	7049160	N.D.	2.466 #
18)	B Endrin al...	0.000	6.988	0	2781310	N.D.	1.220 #
21)	B Endrin ke...	0.000	7.670	0	3160694	N.D.	1.334 #
23)	Chlordane-1	4.274	0.000	1265143	0	24.542	N.D. #
25)	Chlordane-3	0.000	6.068f	0	3071921	N.D.	7.605 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110620\
Data File : PL062874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2020 13:49
Operator : DD\AJ
Sample : L4653-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-7-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:35:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

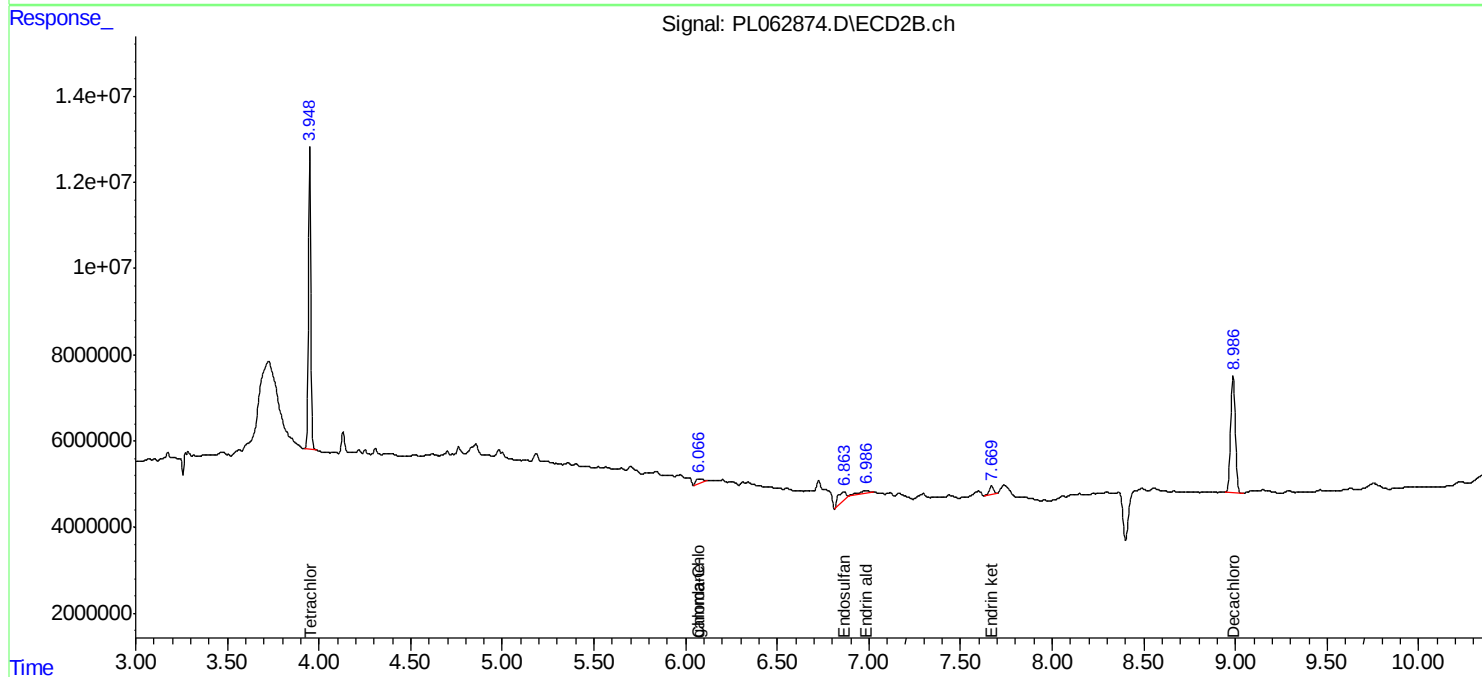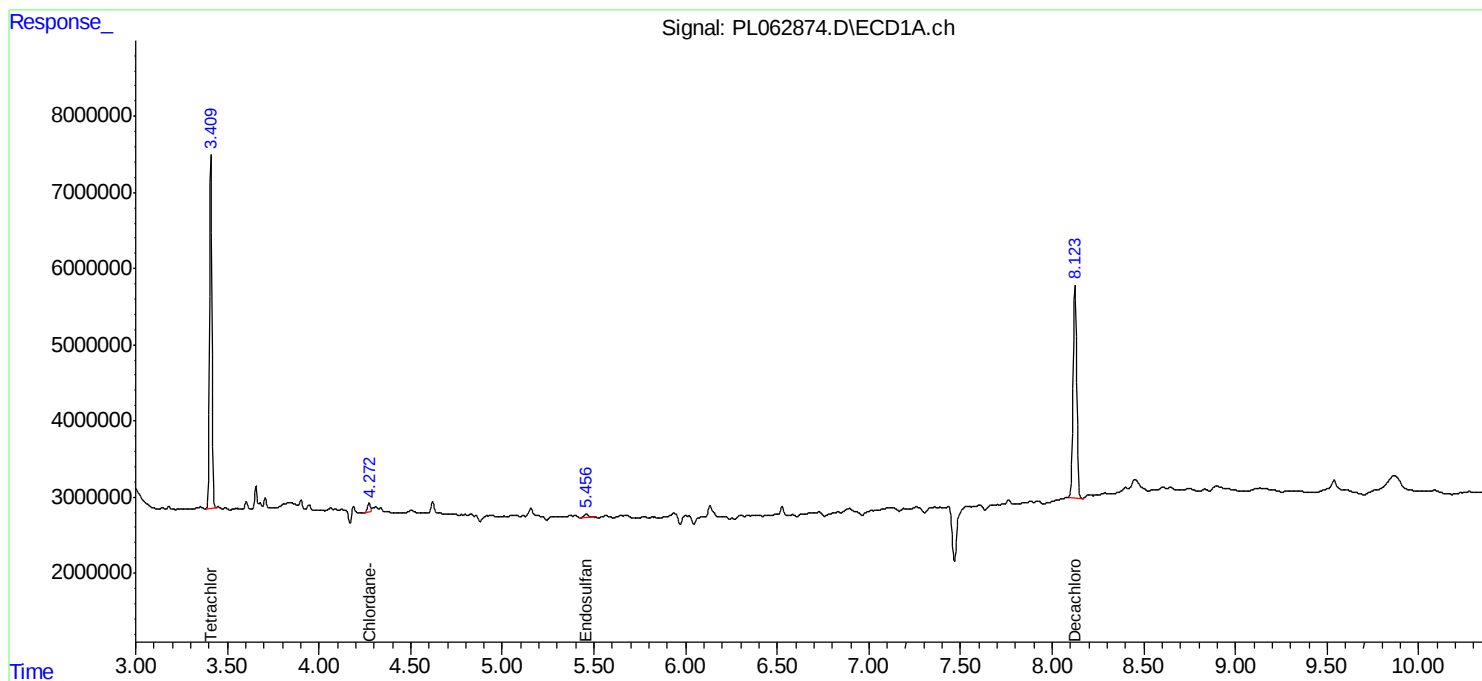


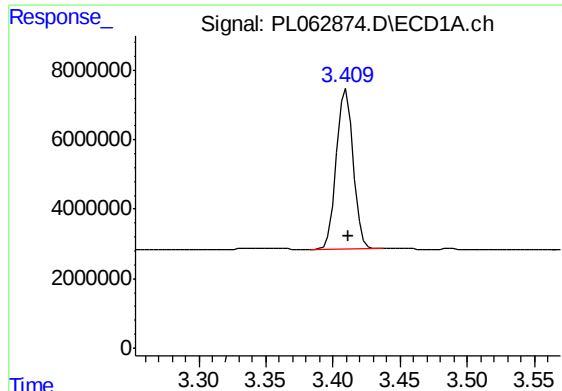

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 40294170
Conc: 23.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-COMP

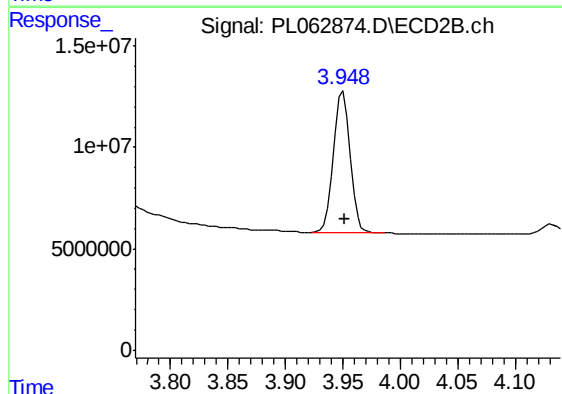


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 70550848
Conc: 24.01 ng/ml

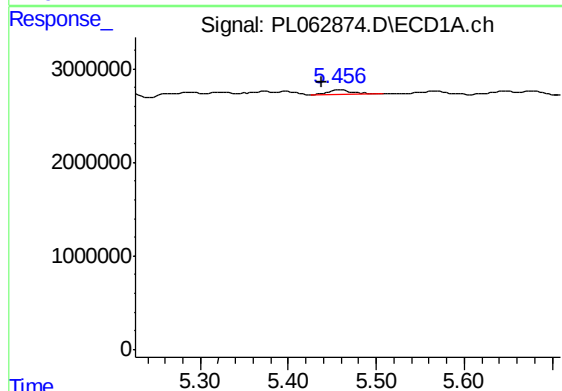


#9 Endosulfan I

R.T.: 5.458 min
Delta R.T.: 0.020 min
Response: 972107
Conc: 0.58 ng/ml

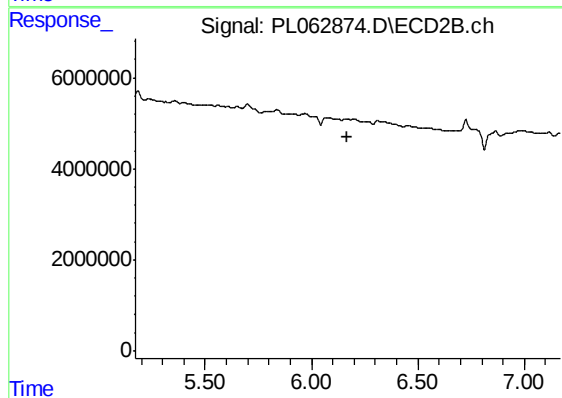

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

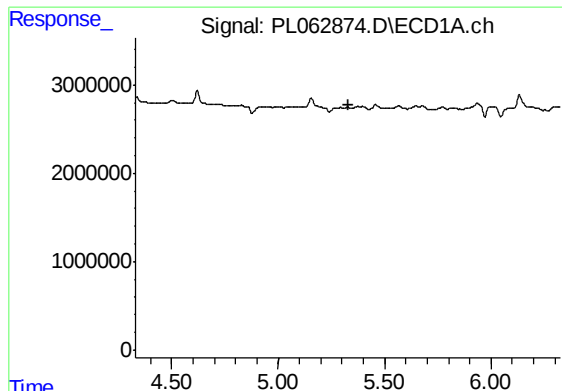

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-7-COMP

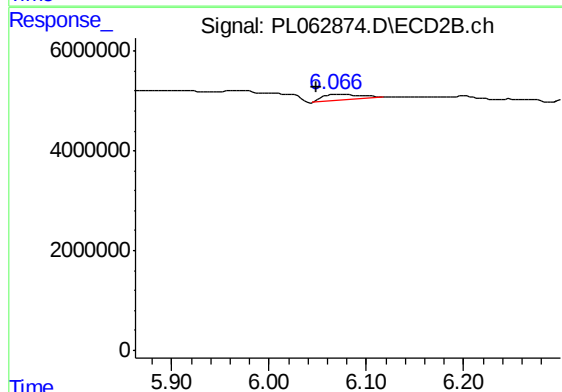


#10 gamma-Chlordane

R.T.: 6.068 min
Delta R.T.: 0.019 min
Response: 3071921
Conc: 0.91 ng/ml

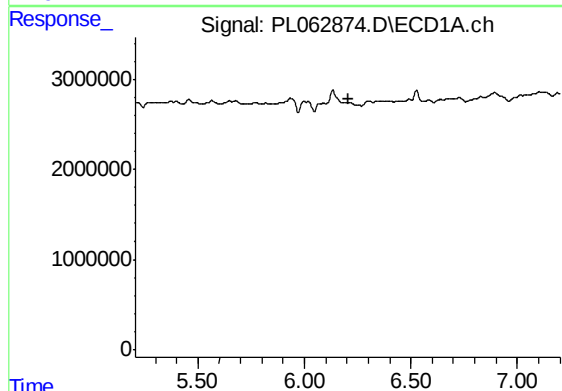


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

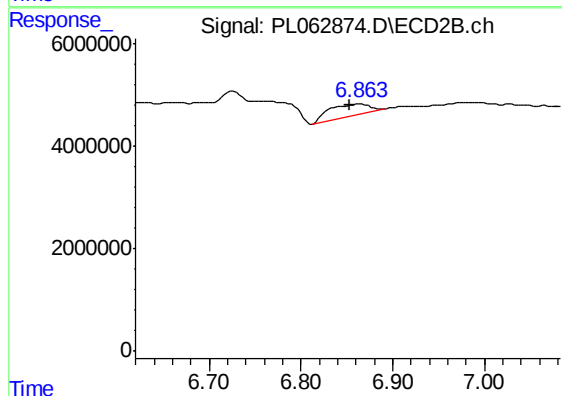

#15 Endosulfan II


R.T.: 6.865 min
Delta R.T.: 0.013 min
Response: 7049160
Conc: 2.47 ng/ml

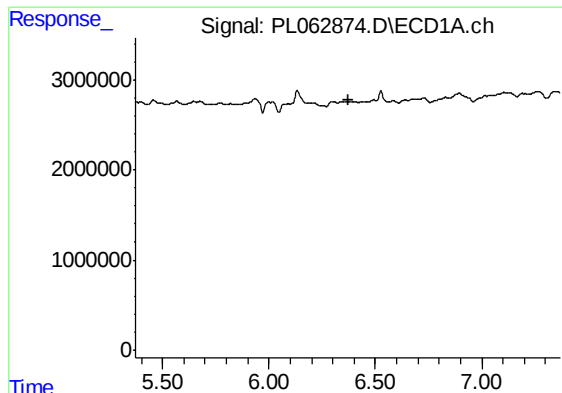

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-7-COMP

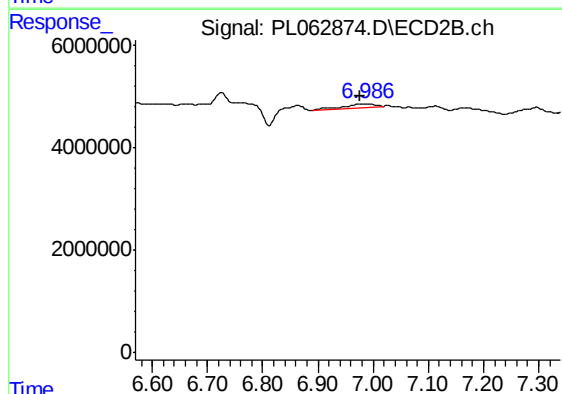


#18 Endrin aldehyde

R.T.: 6.988 min
Delta R.T.: 0.012 min
Response: 2781310
Conc: 1.22 ng/ml

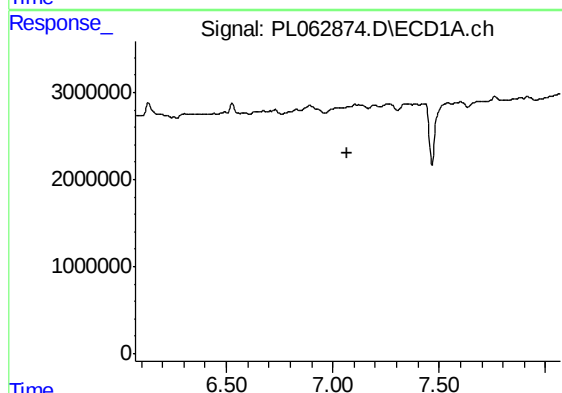


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.071 min
Response: 0
Conc: N.D.

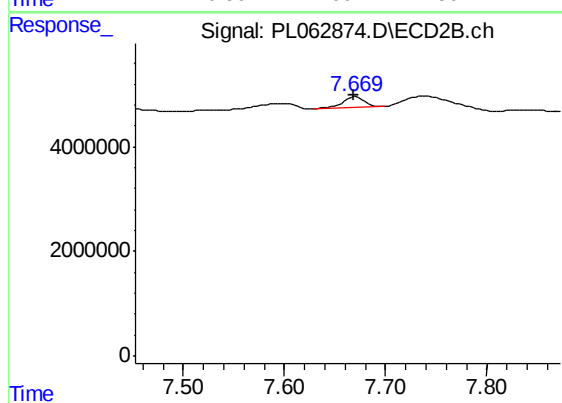

#21 Endrin ketone


R.T.: 7.670 min
Delta R.T.: 0.002 min
Response: 3160694
Conc: 1.33 ng/ml

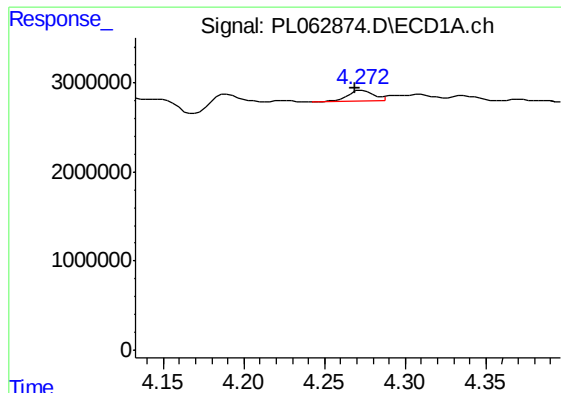

#23 Chlordane-1


R.T.: 4.274 min
Delta R.T.: 0.004 min
Response: 1265143
Conc: 24.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-COMP

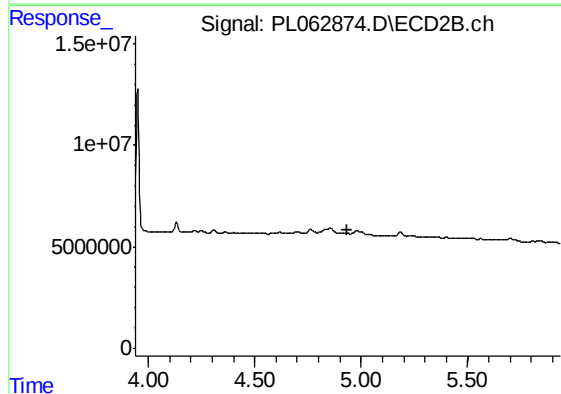


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

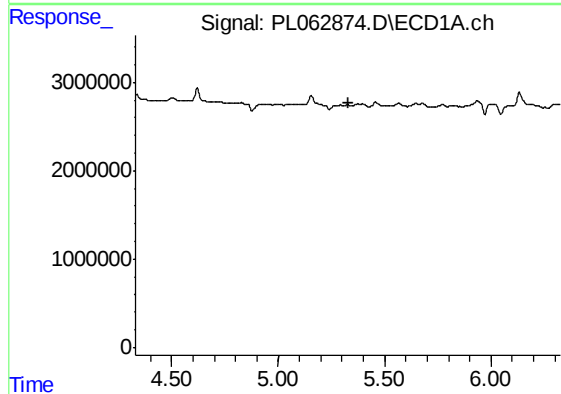


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

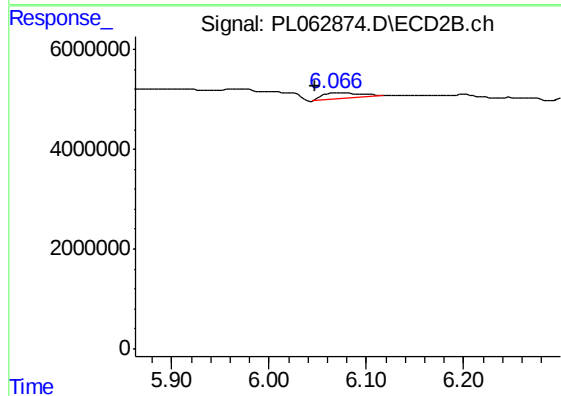

#25 Chlordane-3


R.T.: 6.068 min
Delta R.T.: 0.019 min
Response: 3071921
Conc: 7.60 ng/ml

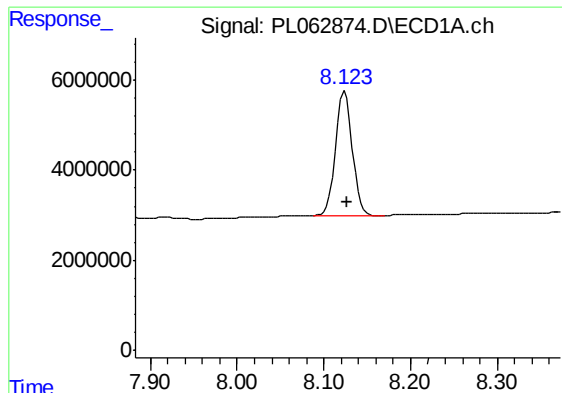

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.002 min
Response: 37513224
Conc: 23.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-COMP

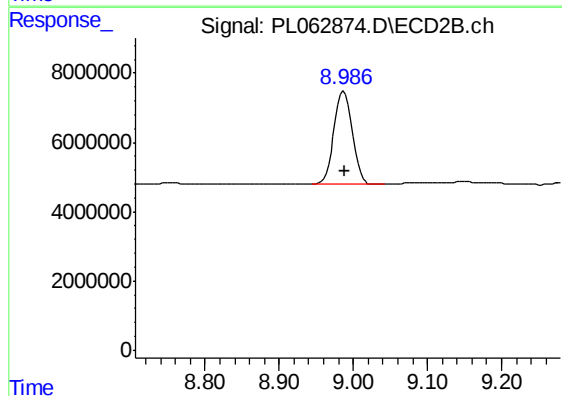

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.001 min
Response: 45838636
Conc: 21.90 ng/ml