

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110620\
 Data File : PL062875.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2020 14:03
 Operator : DD\AJ
 Sample : L4657-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PAV-B49-110520-0-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:35:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	27937368	47414974	16.242	16.135
28)	SA Decachlor...	8.124	8.988	23966917	30883639	14.939	14.756
Target Compounds							
2)	A alpha-BHC	0.000	4.361f	0	1599535	N.D.	0.360 #
6)	B beta-BHC	0.000	4.812f	0	1743664	N.D.	0.926 #
8)	B Heptachlo...	5.093	5.811	1645355	4526726	0.902	1.398 #
9)	A Endosulfan I	5.448	0.000	3433950	0	2.054	N.D. #
10)	B gamma-Chl...	0.000	6.047	0	3423988	N.D.	1.017 #
14)	MA Endrin	5.936	0.000	2237833	0	1.345	N.D. #
15)	B Endosulfa...	0.000	6.826f	0	1122634	N.D.	0.393 #
17)	MA 4,4'-DDT	6.298	7.064	1034306	6722422	0.775	2.994 #
23)	Chlordane-1	4.264	0.000	2524494	0	48.972	N.D. #
25)	Chlordane-3	0.000	6.047	0	3423988	N.D.	8.476 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110620\
Data File : PL062875.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2020 14:03
Operator : DD\AJ
Sample : L4657-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PAV-B49-110520-0-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:35:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

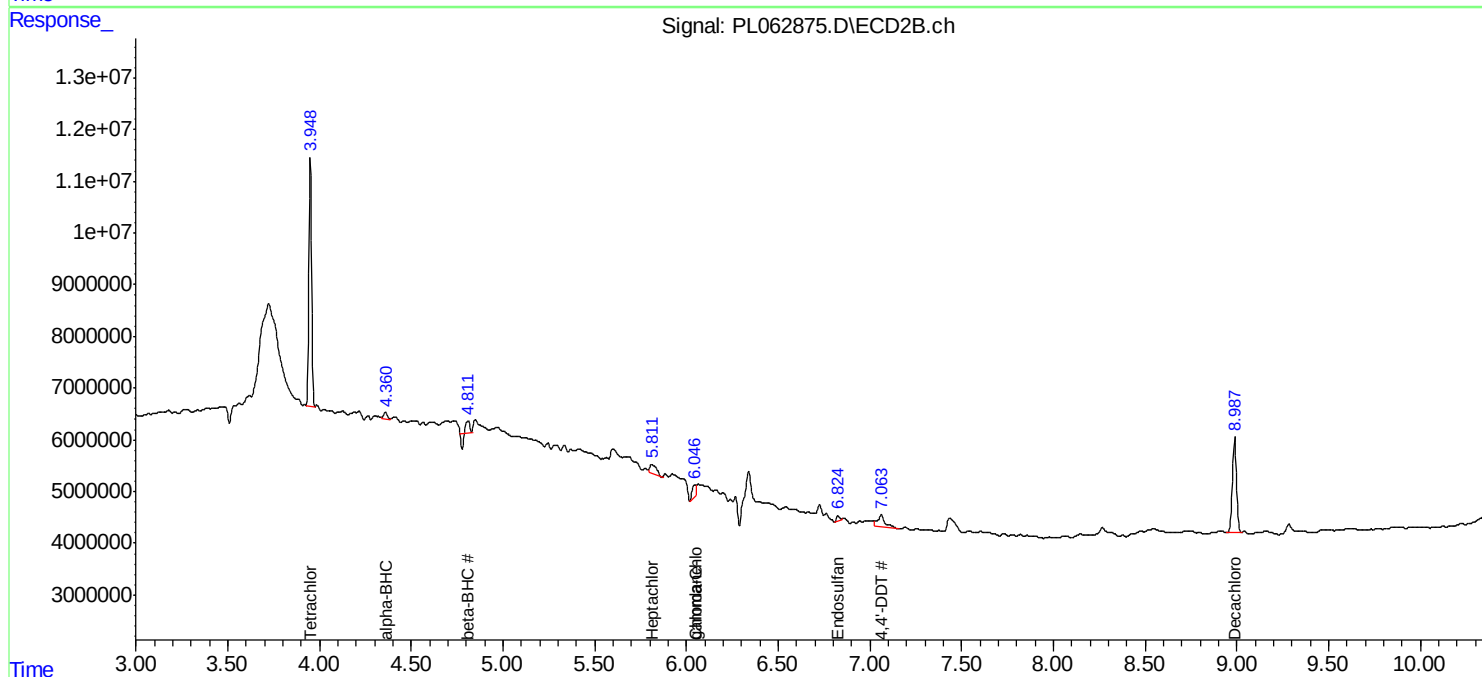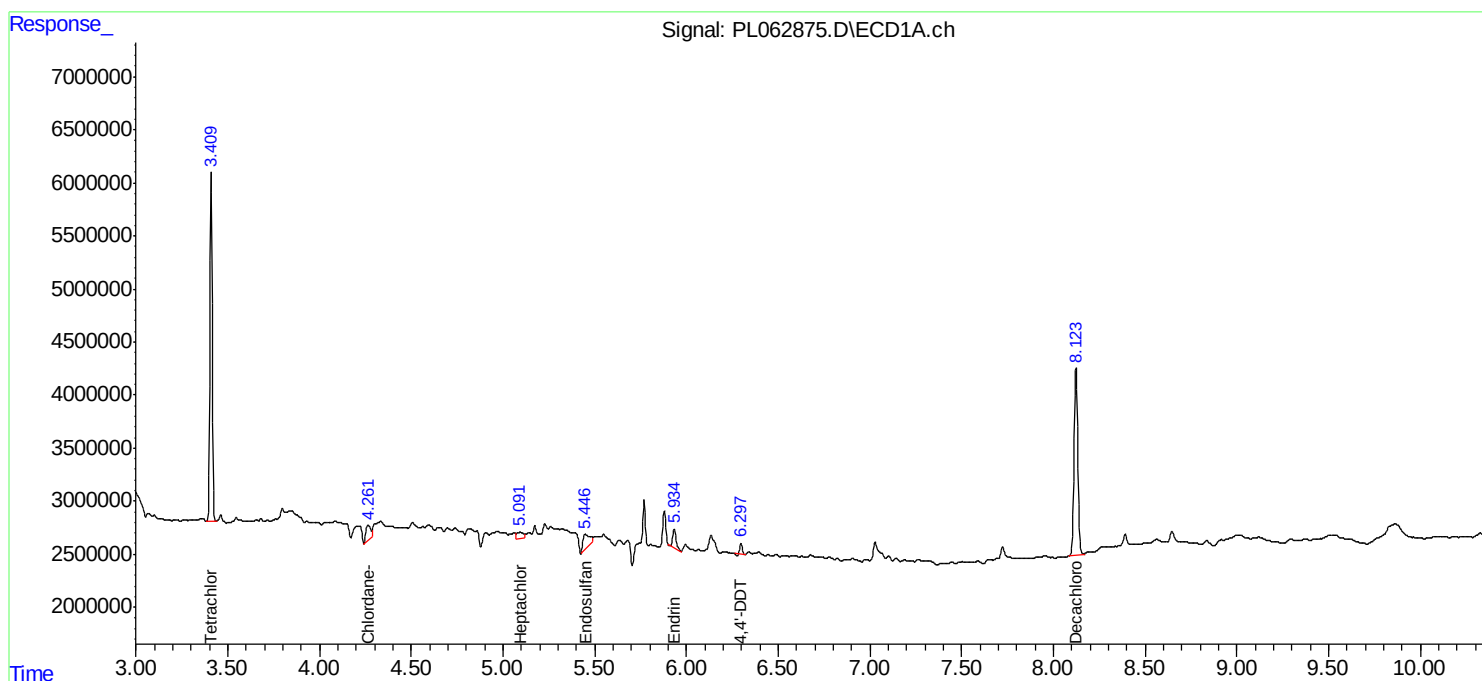


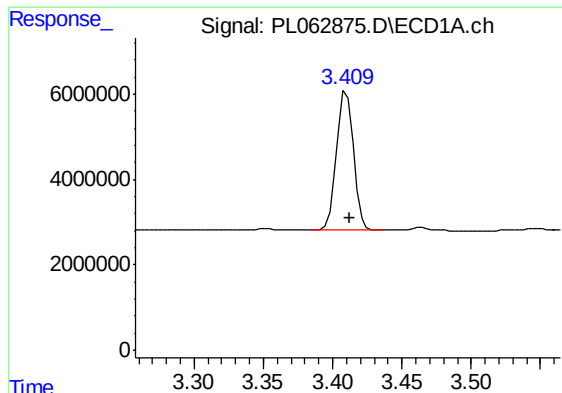

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 27937368
Conc: 16.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B49-110520-0-10

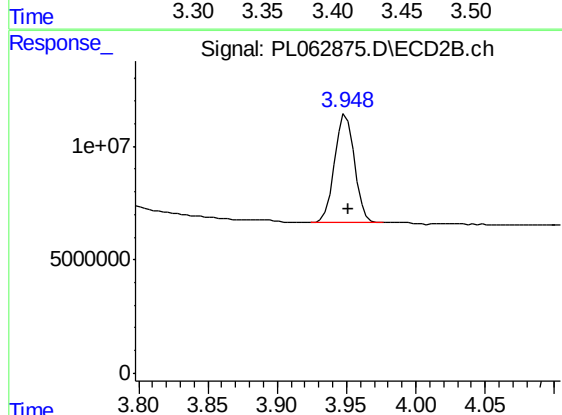


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 47414974
Conc: 16.13 ng/ml

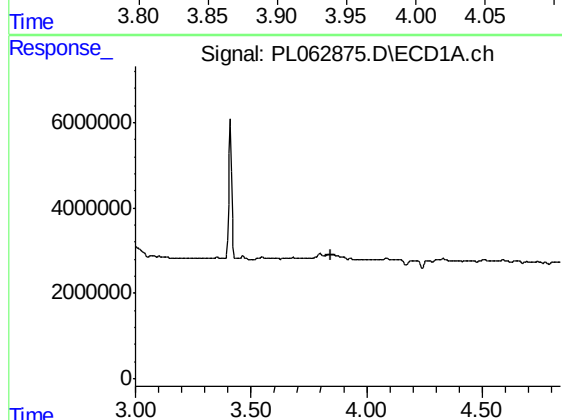


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.844 min
Response: 0
Conc: N.D.

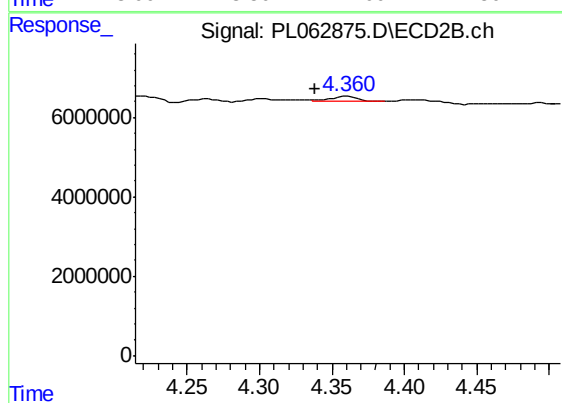

#2 alpha-BHC


R.T.: 4.361 min
Delta R.T.: 0.023 min
Response: 1599535
Conc: 0.36 ng/ml

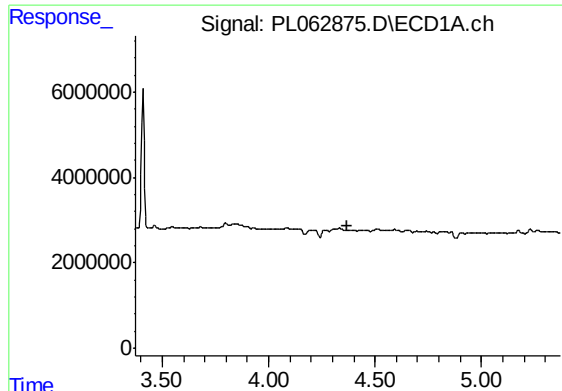

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PAV-B49-110520-0-10

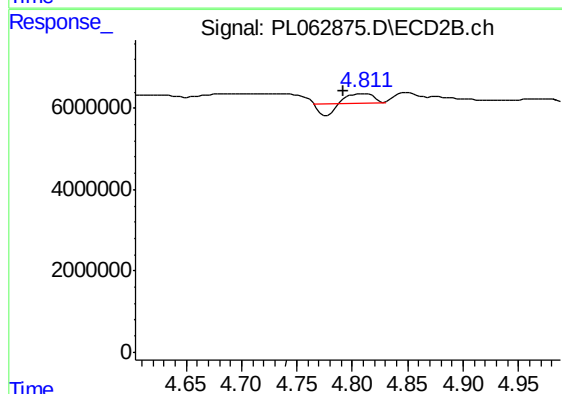


#6 beta-BHC

R.T.: 4.812 min
Delta R.T.: 0.020 min
Response: 1743664
Conc: 0.93 ng/ml

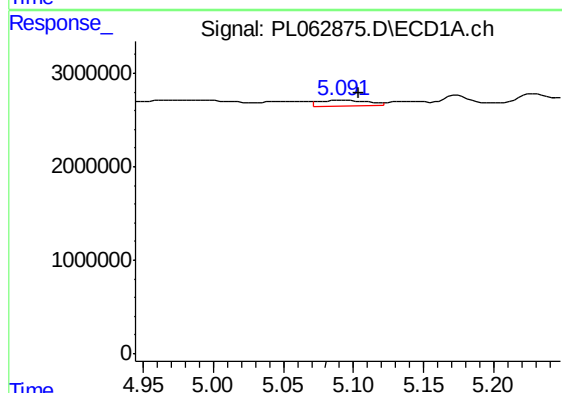


#8 Heptachlor epoxide

R.T.: 5.093 min
Delta R.T.: -0.011 min
Response: 1645355
Conc: 0.90 ng/ml

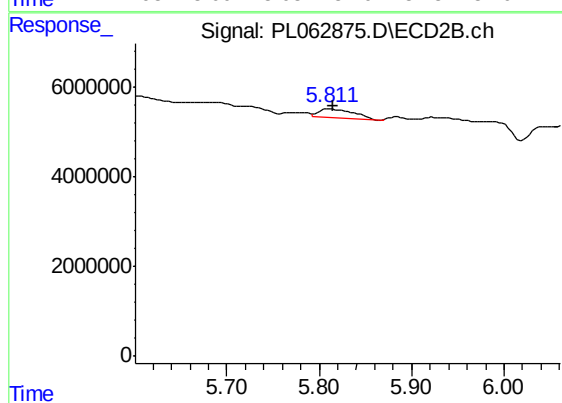

#8 Heptachlor epoxide


R.T.: 5.811 min
Delta R.T.: -0.003 min
Response: 4526726
Conc: 1.40 ng/ml

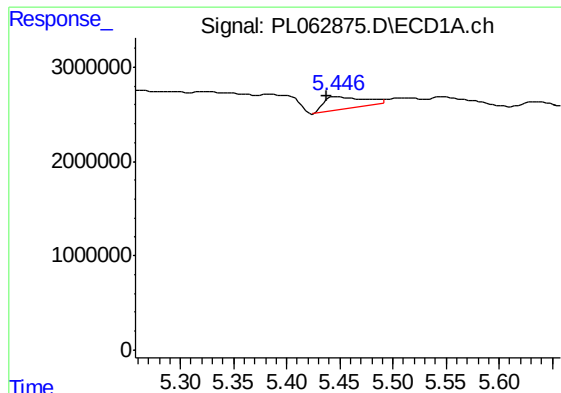

#9 Endosulfan I


R.T.: 5.448 min
Delta R.T.: 0.010 min
Response: 3433950
Conc: 2.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B49-110520-0-10

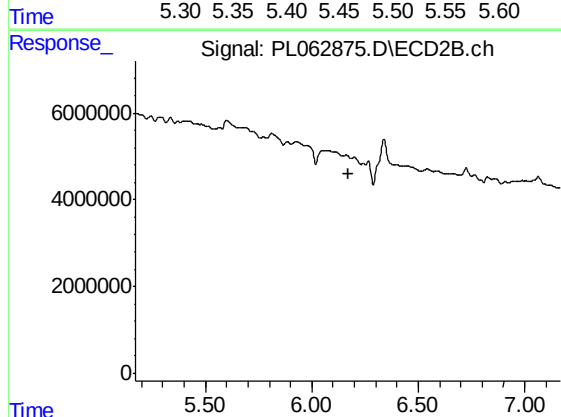


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

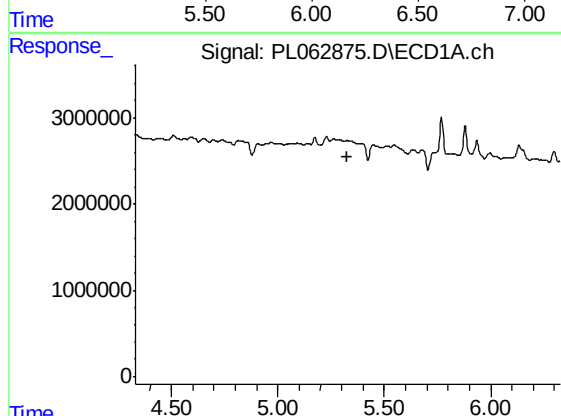


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

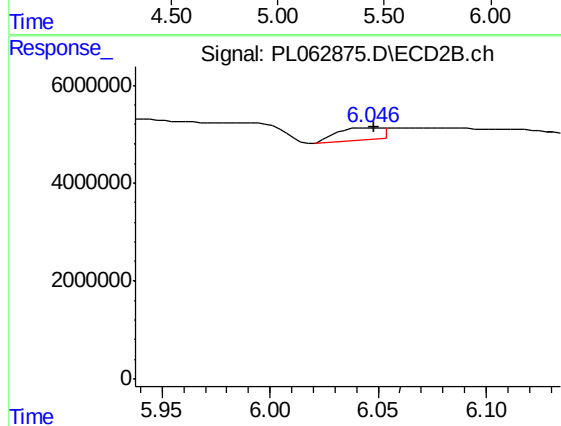

#10 gamma-Chlordane


R.T.: 6.047 min
Delta R.T.: -0.001 min
Response: 3423988
Conc: 1.02 ng/ml

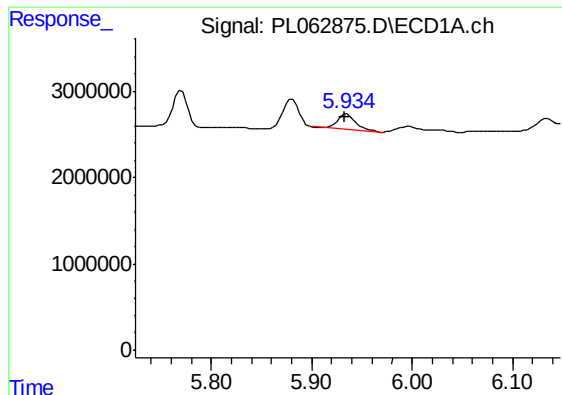

#14 Endrin


R.T.: 5.936 min
Delta R.T.: 0.002 min
Response: 2237833
Conc: 1.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B49-110520-0-10

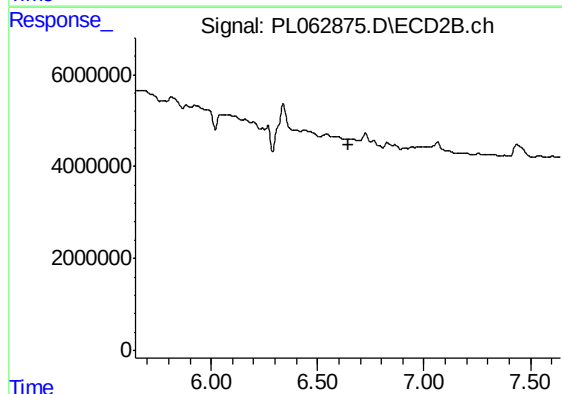


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

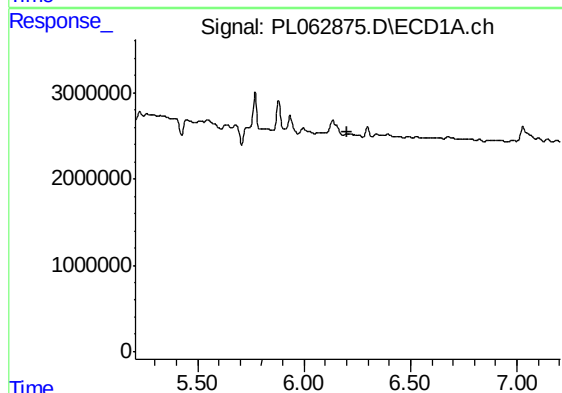


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

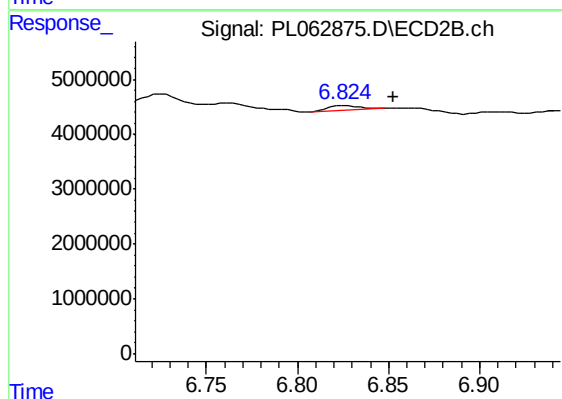

#15 Endosulfan II


R.T.: 6.826 min
Delta R.T.: -0.027 min
Response: 1122634
Conc: 0.39 ng/ml

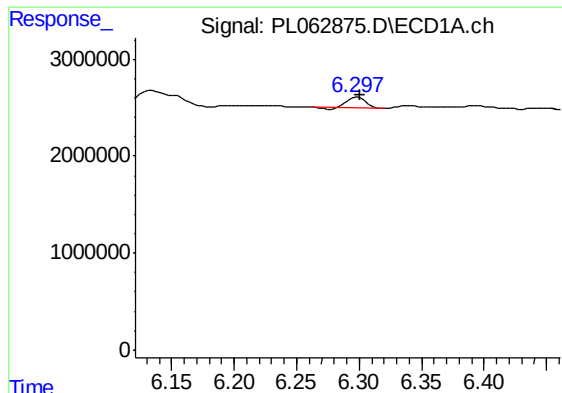

#17 4,4'-DDT


R.T.: 6.298 min
Delta R.T.: -0.003 min
Response: 1034306
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B49-110520-0-10

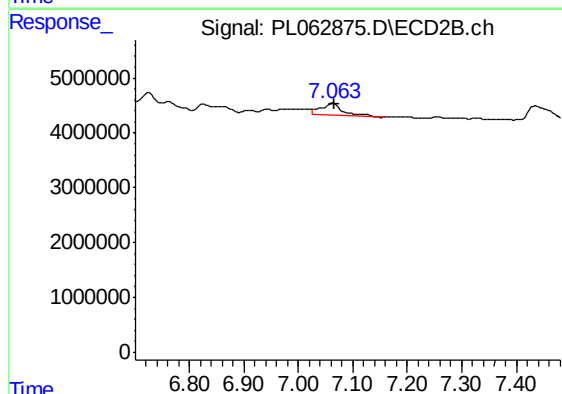


#17 4,4'-DDT

R.T.: 7.064 min
Delta R.T.: -0.002 min
Response: 6722422
Conc: 2.99 ng/ml

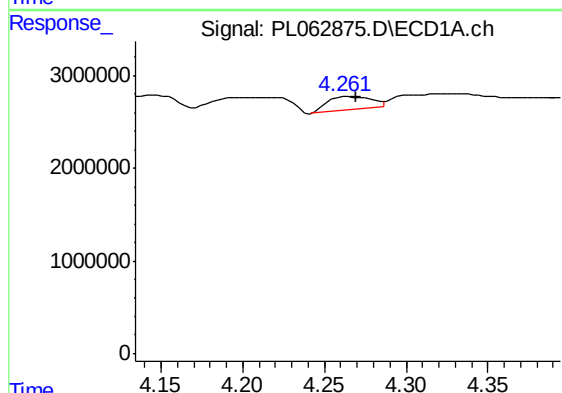


#23 Chlordane-1

R.T.: 4.264 min
Delta R.T.: -0.005 min
Response: 2524494
Conc: 48.97 ng/ml

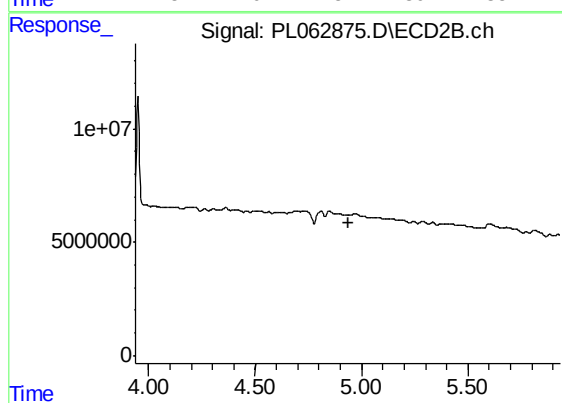

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

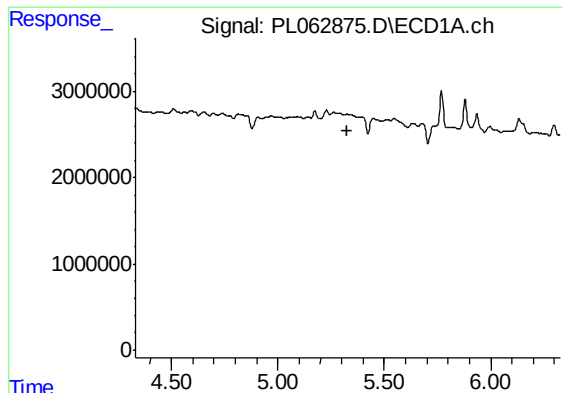

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PAV-B49-110520-0-10

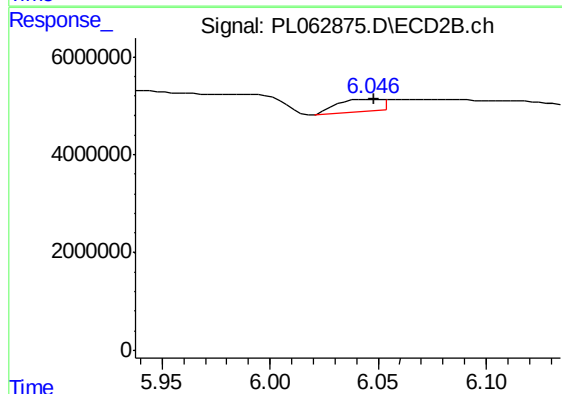


#25 Chlordane-3

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 3423988
Conc: 8.48 ng/ml

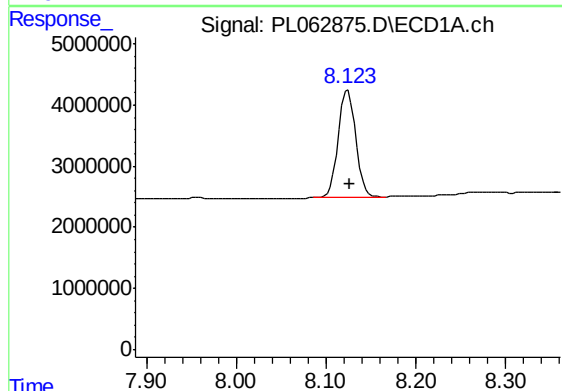

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.002 min
Response: 23966917
Conc: 14.94 ng/ml

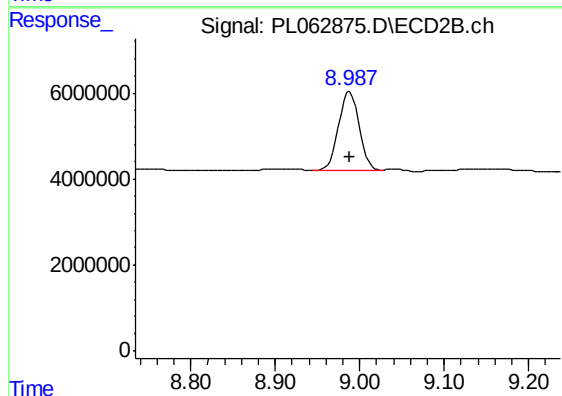

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 30883639
Conc: 14.76 ng/ml