

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110620\
 Data File : PL062875.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2020 14:03
 Operator : DD\AJ
 Sample : L4657-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PAV-B49-110520-0-10

Manual Integrations
 APPROVED

Ankita
 11/9/2020 2:56:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:35:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	27937368	47414974	16.242	16.135
28)	SA Decachlor...	8.124	8.988	23966917	30883639	14.939	14.756
Target Compounds							
17)	MA 4,4'-DDT	6.297	7.063	1369515	2915257	1.026m	1.298m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110620\
Data File : PL062875.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2020 14:03
Operator : DD\AJ
Sample : L4657-02
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
PAV-B49-110520-0-10


Manual Integrations
APPROVED

Ankita
11/9/2020 2:56:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:35:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

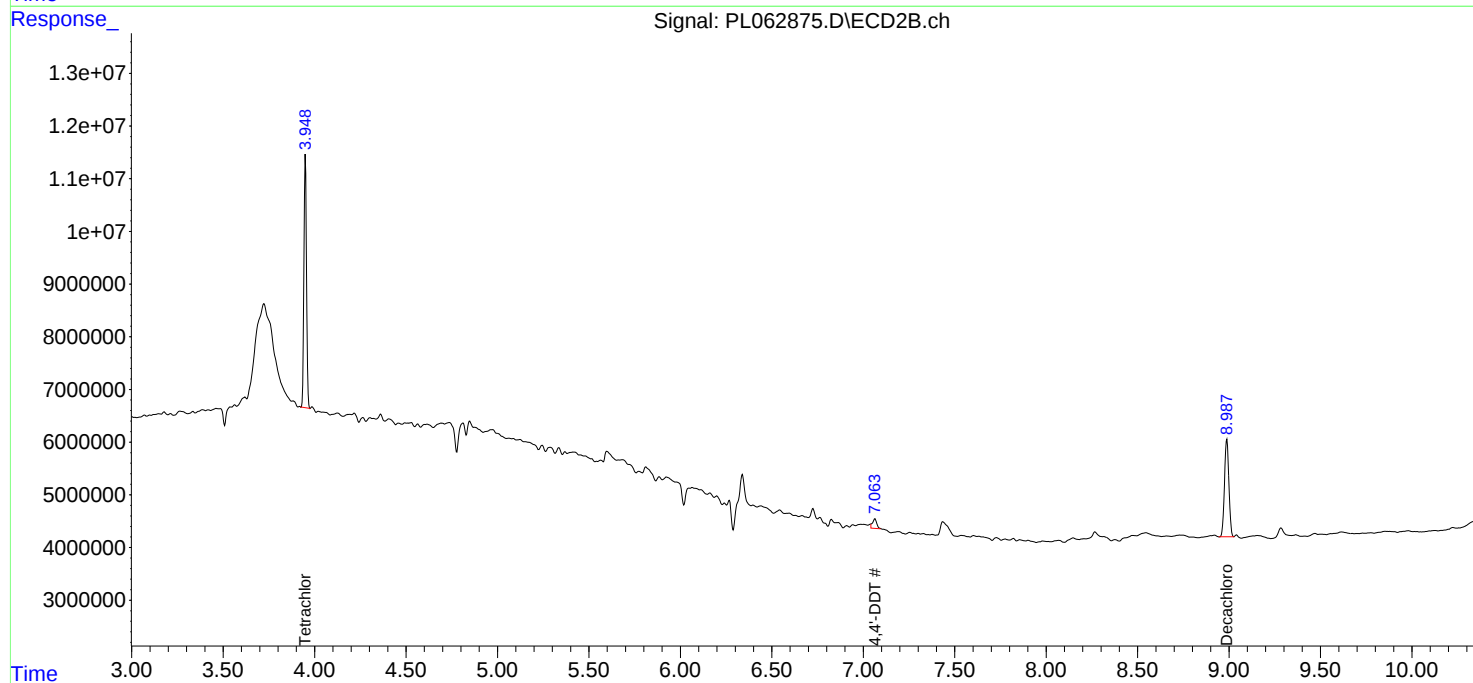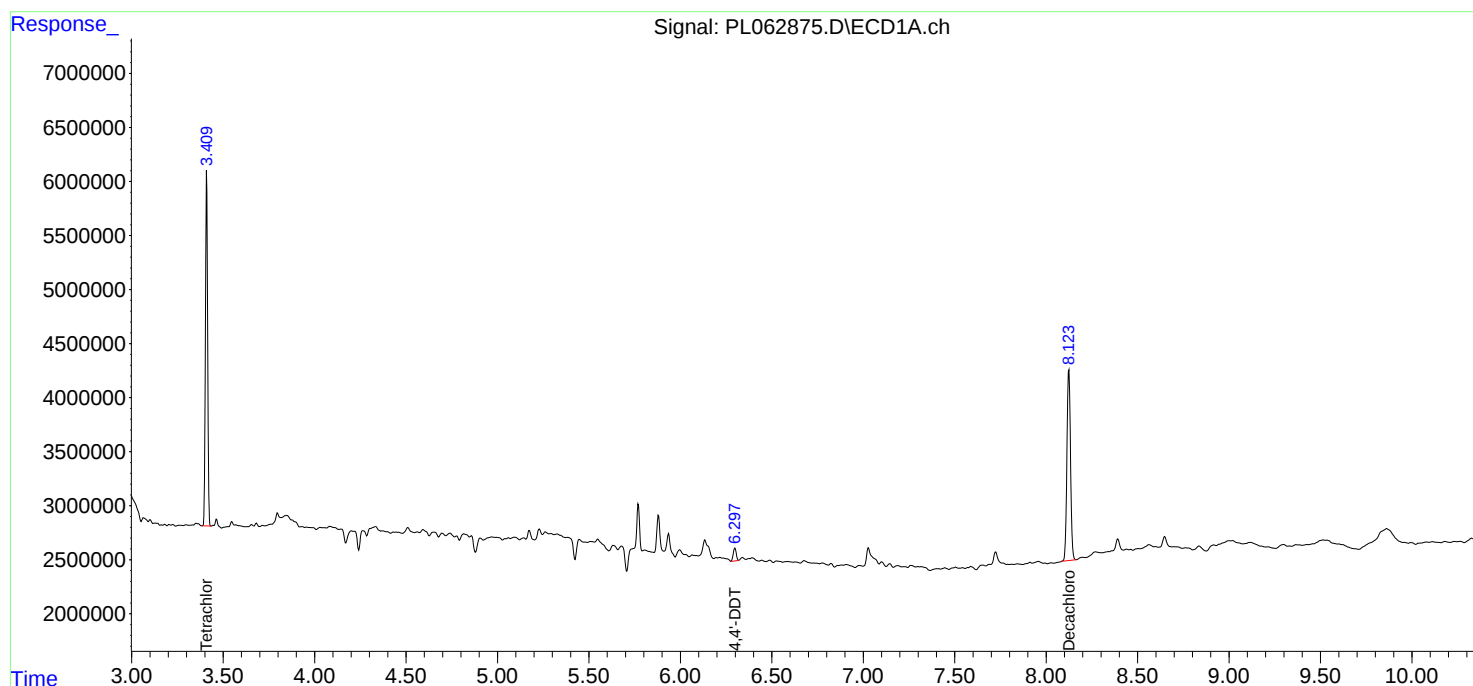

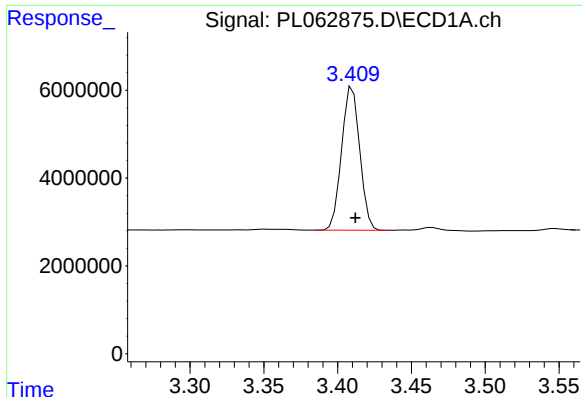


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 27937368
Conc: 16.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B49-110520-0-10


Manual Integrations
APPROVED

Ankita
11/9/2020 2:56:43 PM

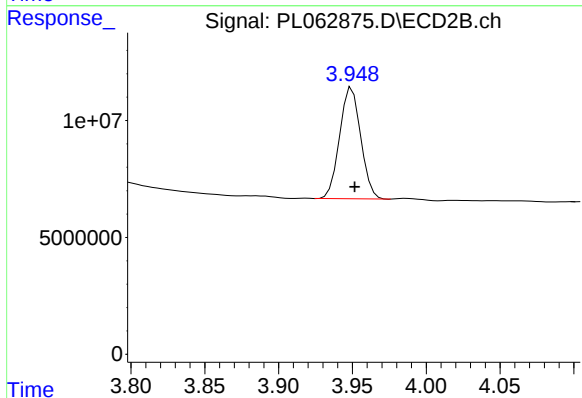


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 47414974
Conc: 16.13 ng/ml

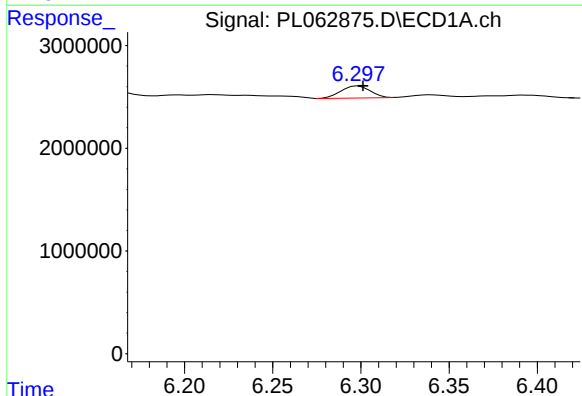


#17 4,4'-DDT

R.T.: 6.297 min
Delta R.T.: -0.004 min
Response: 1369515
Conc: 1.03 ng/ml m

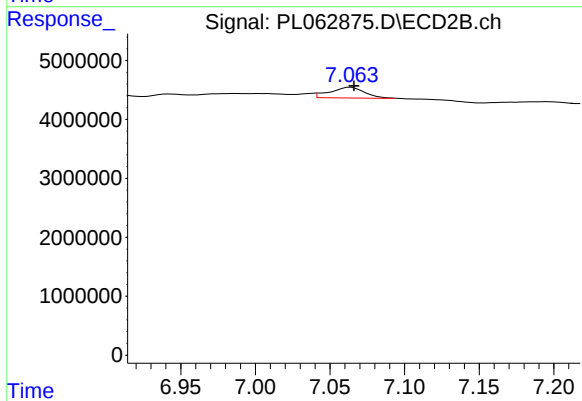

#17 4,4'-DDT

R.T.: 7.063 min
Delta R.T.: -0.003 min
Response: 2915257
Conc: 1.30 ng/ml m

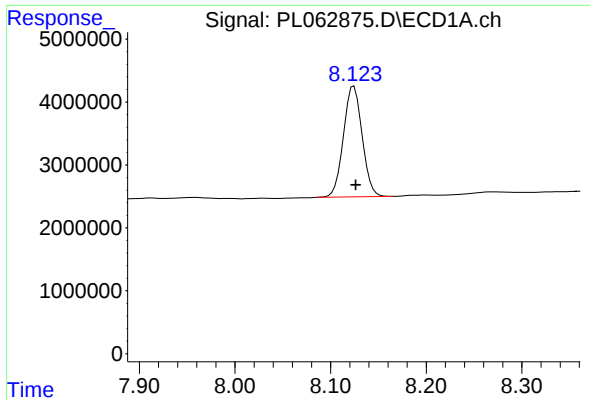


#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.002 min
Response: 23966917
Conc: 14.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B49-110520-0-10

Manual Integrations
APPROVED

Ankita
11/9/2020 2:56:43 PM

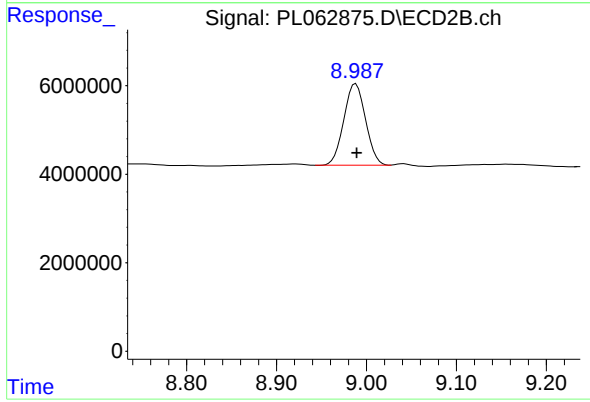

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 30883639
Conc: 14.76 ng/ml