

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110620\
 Data File : PL062883.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2020 16:15
 Operator : DD\AJ
 Sample : L4625-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CONTAINER-001-A-B-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:37:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	34764227	61000969	20.211	20.758
28)	SA Decachlor...	8.125	8.988	29836491	37964478	18.598	18.139

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110620\
Data File : PL062883.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2020 16:15
Operator : DD\AJ
Sample : L4625-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CONTAINER-001-A-B-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:37:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

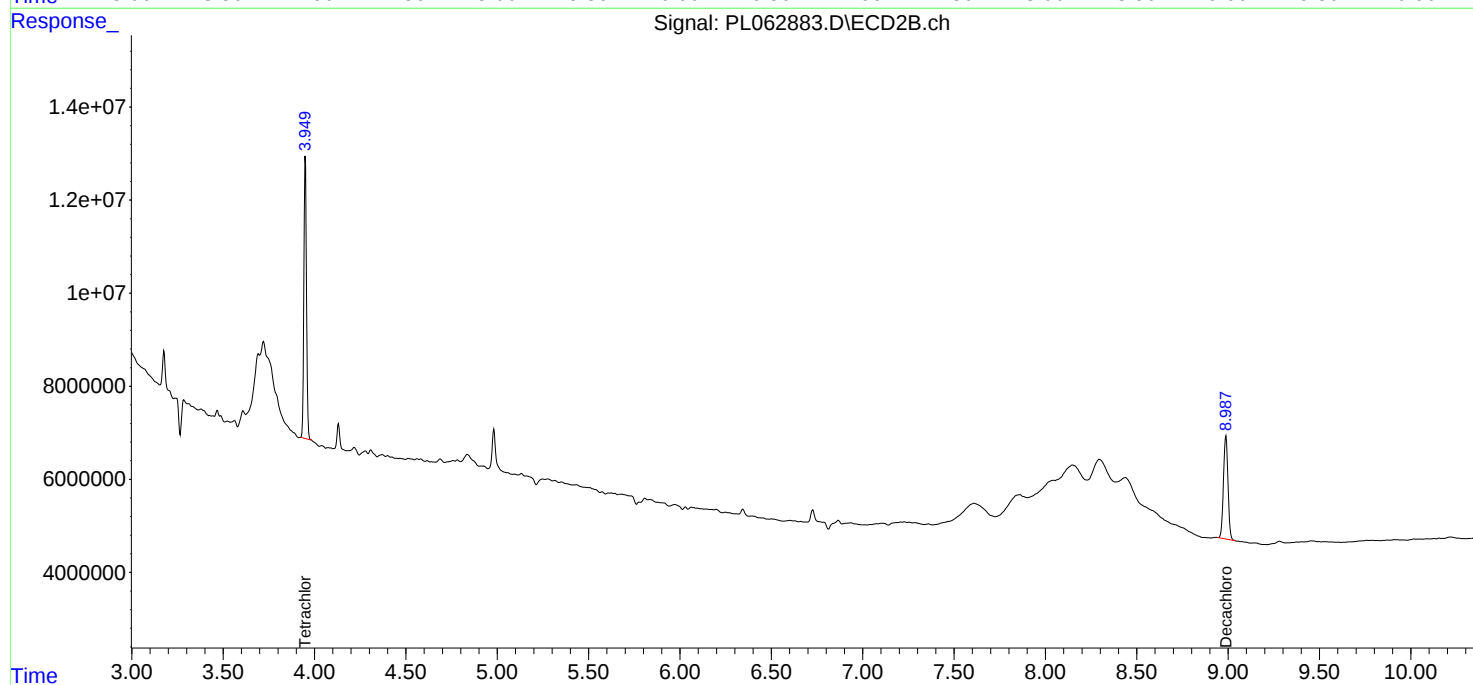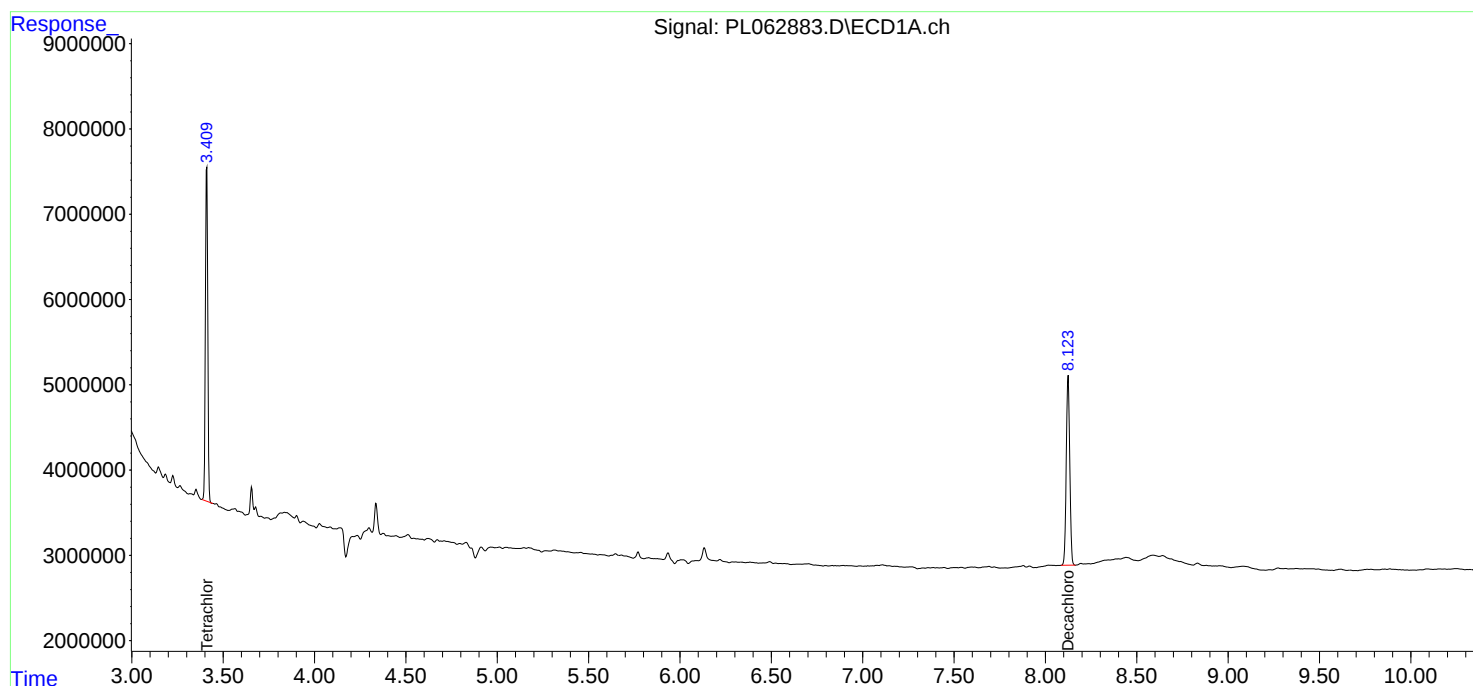


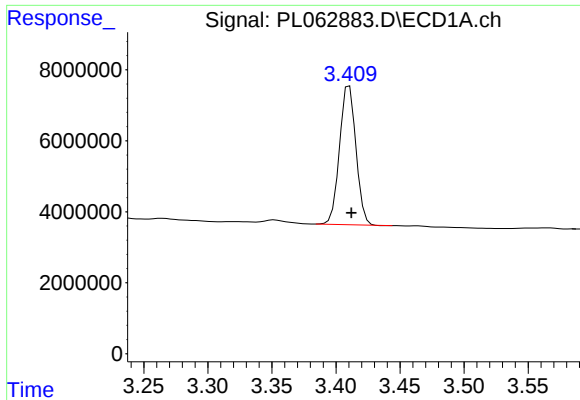

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 34764227
Conc: 20.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
CONTAINER-001-A-B-COMP

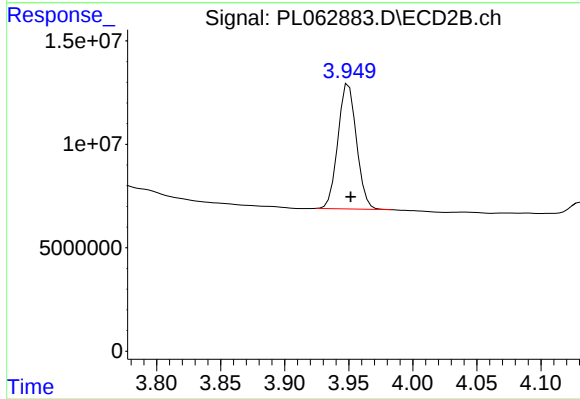


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 61000969
Conc: 20.76 ng/ml

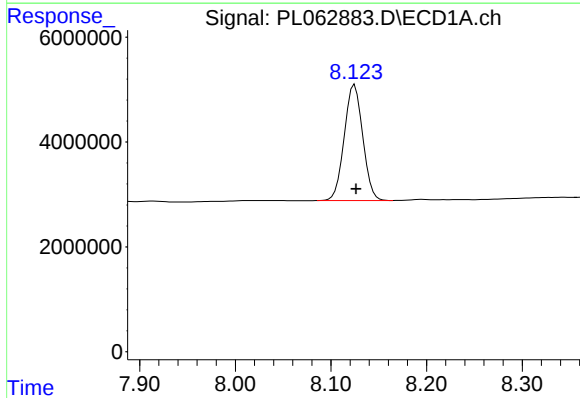

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: -0.002 min
Response: 29836491
Conc: 18.60 ng/ml

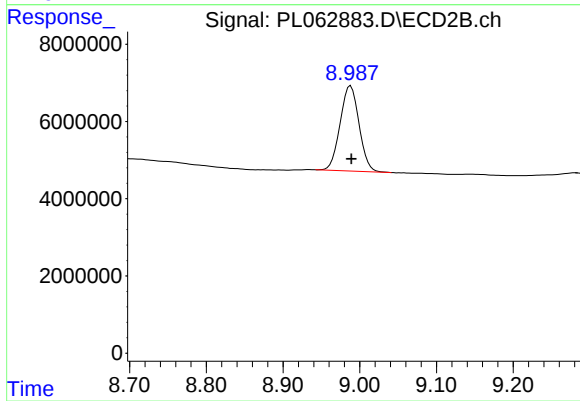

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 37964478
Conc: 18.14 ng/ml