

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110624\
 Data File : PL092876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 14:32
 Operator : AR\AJ
 Sample : PB164707BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB164707BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:05:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.778	49015429	52519239	20.004	19.300
28)	SA Decachlor...	9.058	7.918	38990617	45263923	20.260	16.585
Target Compounds							
2)	A alpha-BHC	0.000	3.271	0	150456	N.D.	0.038 #
5)	MB Aldrin	0.000	4.210f	0	55989	N.D.	0.015 #
7)	B delta-BHC	4.767	4.143	3020173	161986	0.965	0.042 #
8)	B Heptachlo...	0.000	4.755f	0	20102	N.D.	0.006 #
10)	B gamma-Chl...	0.000	4.973	0	599288	N.D.	0.178 #
11)	B alpha-Chl...	0.000	5.026f	0	980534	N.D.	0.295 #
14)	MA Endrin	0.000	5.635	0	195764	N.D.	0.068 #
23)	Chlordane-1	0.000	3.804f	0	150058	N.D.	1.414 #
24)	Chlordane-2	0.000	4.346	0	38758	N.D.	0.313 #
25)	Chlordane-3	0.000	4.973	0	599288	N.D.	1.652 #
26)	Chlordane-4	0.000	5.026f	0	980534	N.D.	2.803 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110624\
Data File : PL092876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 14:32
Operator : AR\AJ
Sample : PB164707BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB164707BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:05:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

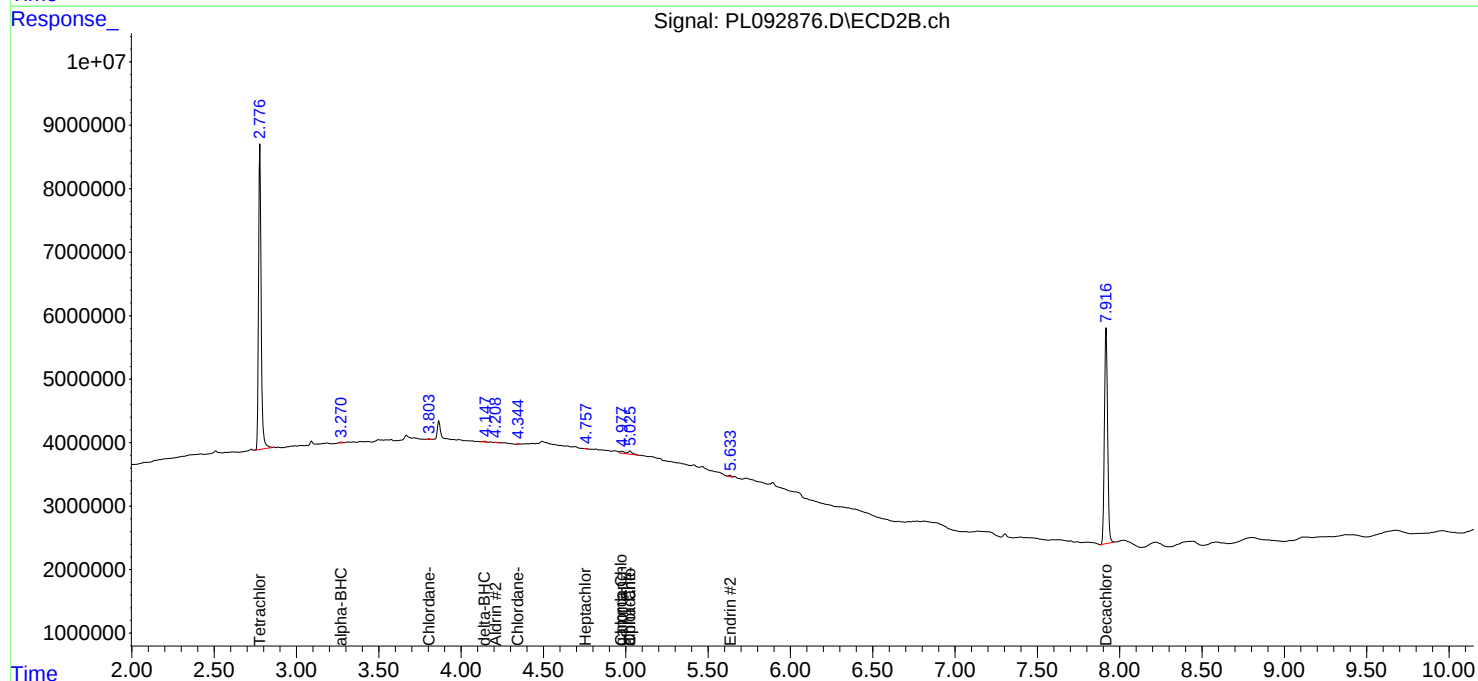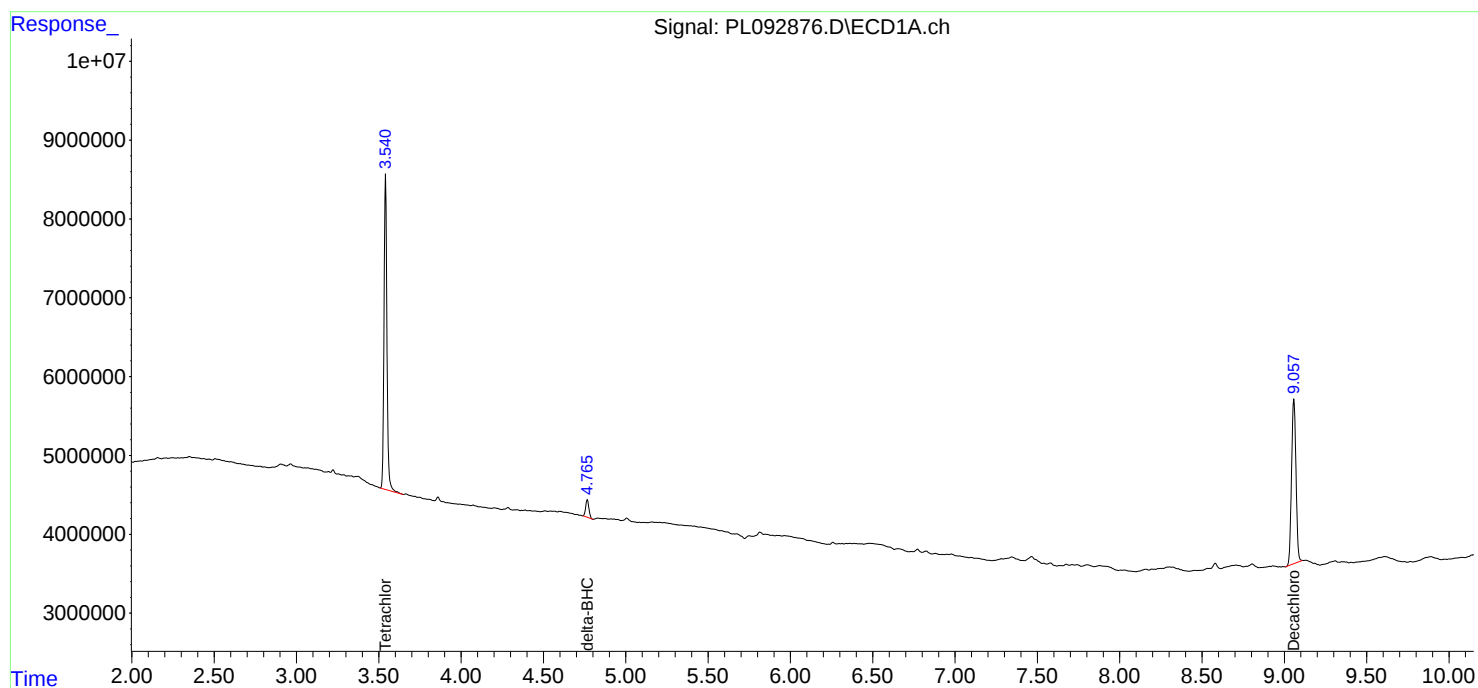


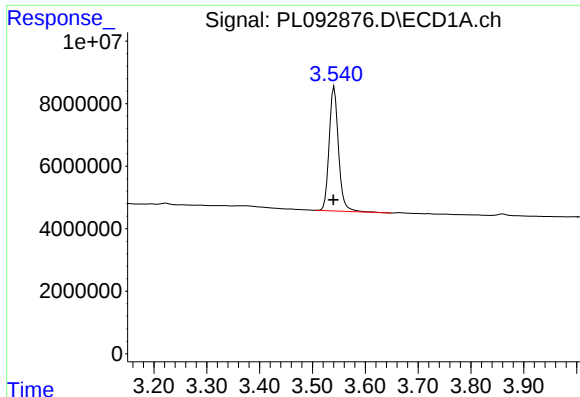

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: 0.001 min
Response: 49015429
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB164707BL

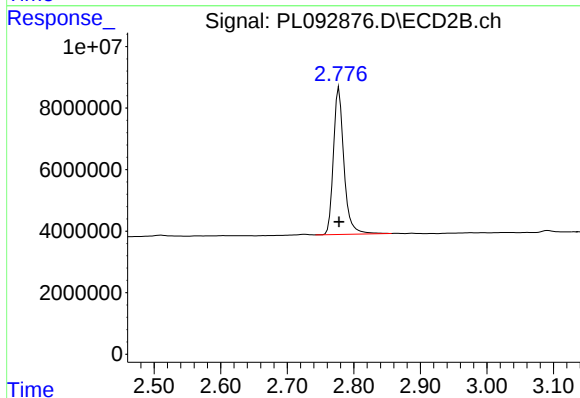


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 52519239
Conc: 19.30 ng/ml

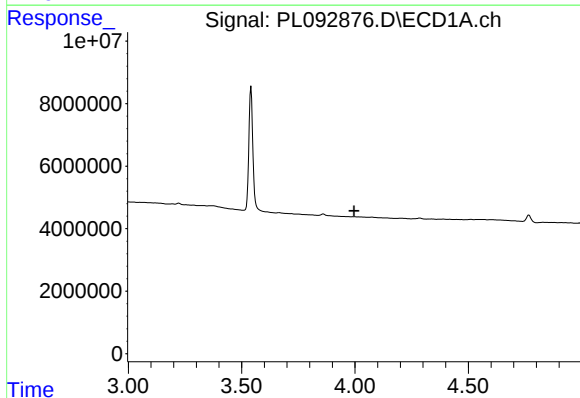


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.996 min
Response: 0
Conc: N.D.

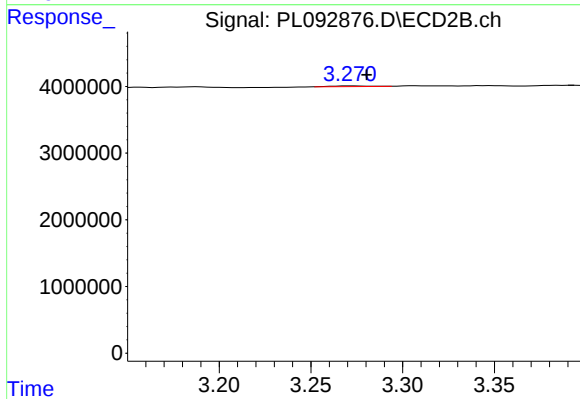

#2 alpha-BHC


R.T.: 3.271 min
Delta R.T.: -0.009 min
Response: 150456
Conc: 0.04 ng/ml

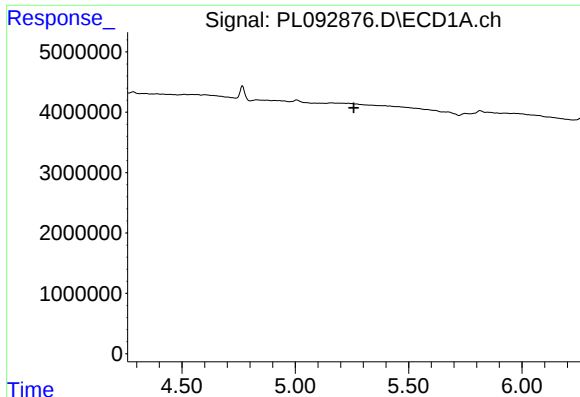

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164707BL

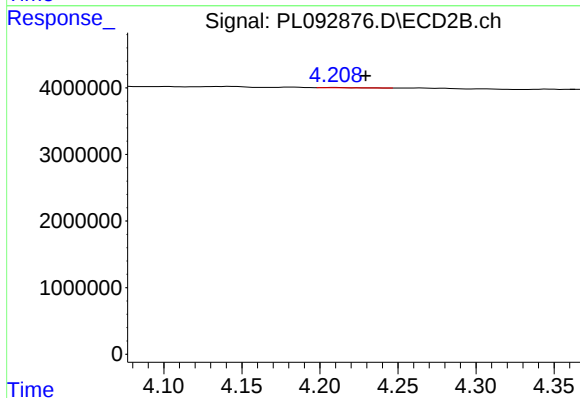


#5 Aldrin

R.T.: 4.210 min
Delta R.T.: -0.020 min
Response: 55989
Conc: 0.02 ng/ml

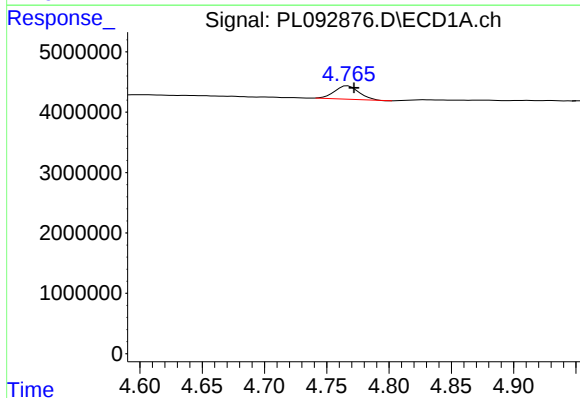


#7 delta-BHC

R.T.: 4.767 min
Delta R.T.: -0.005 min
Response: 3020173
Conc: 0.96 ng/ml

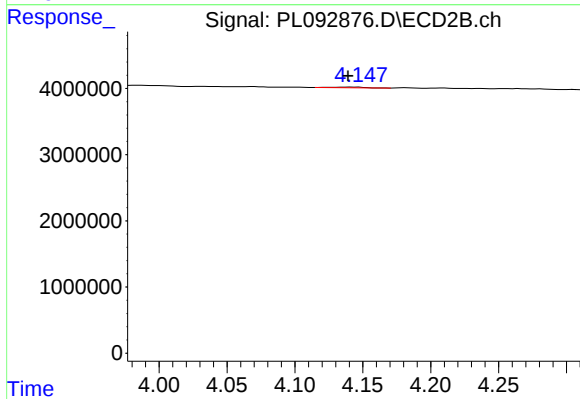

#7 delta-BHC


R.T.: 4.143 min
Delta R.T.: 0.004 min
Response: 161986
Conc: 0.04 ng/ml

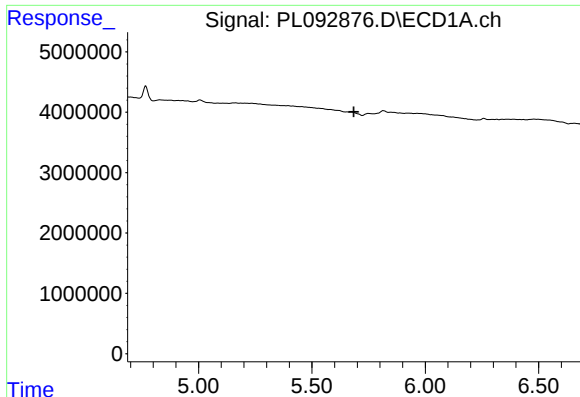

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.684 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164707BL

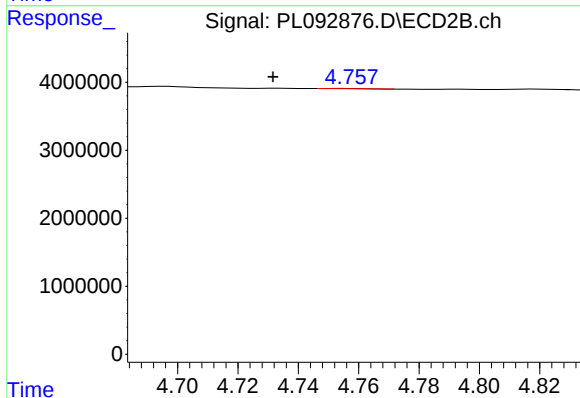


#8 Heptachlor epoxide

R.T.: 4.755 min
Delta R.T.: 0.023 min
Response: 20102
Conc: 0.01 ng/ml

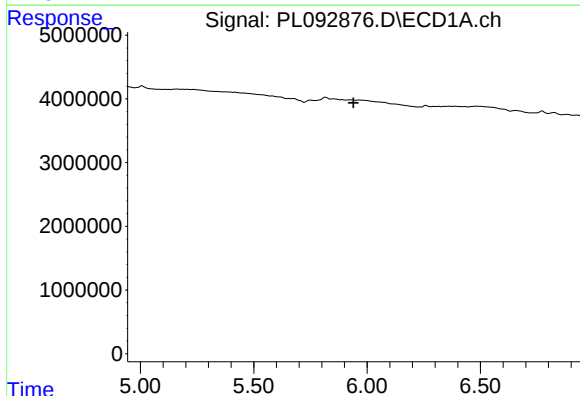


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

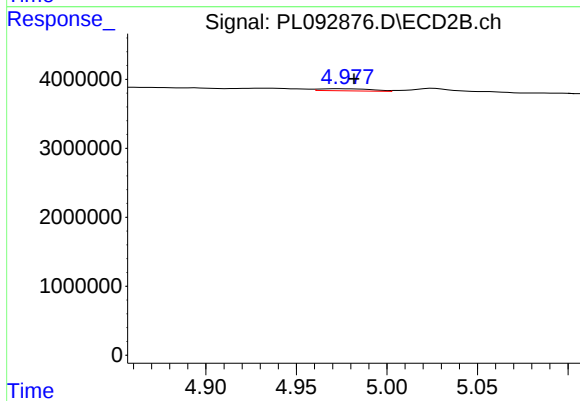

#10 gamma-Chlordane


R.T.: 4.973 min
Delta R.T.: -0.009 min
Response: 599288
Conc: 0.18 ng/ml

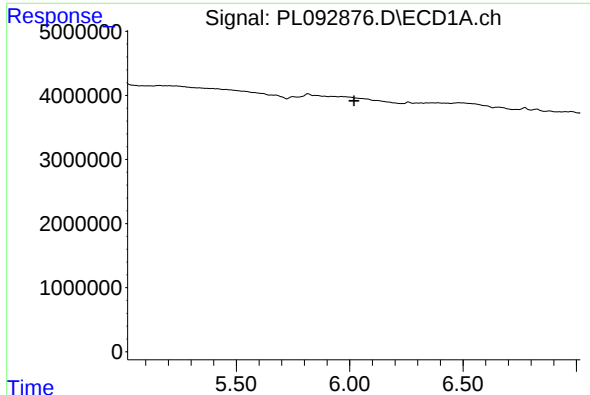

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.019 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164707BL

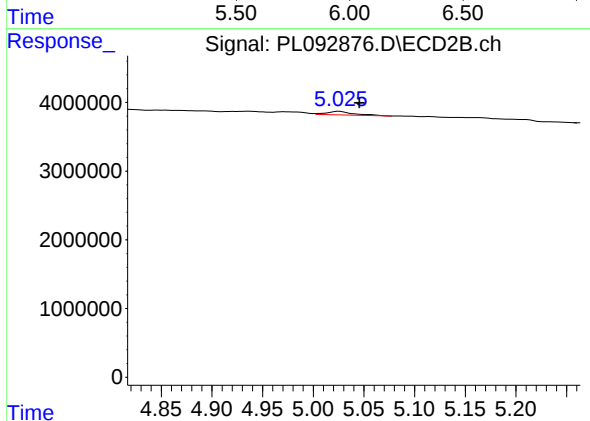


#11 alpha-Chlordane

R.T.: 5.026 min
Delta R.T.: -0.020 min
Response: 980534
Conc: 0.29 ng/ml

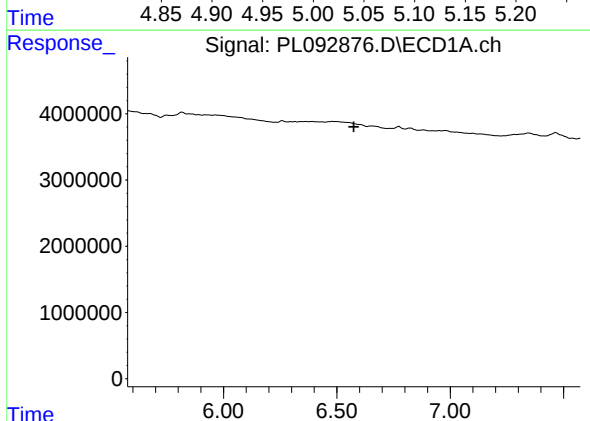


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

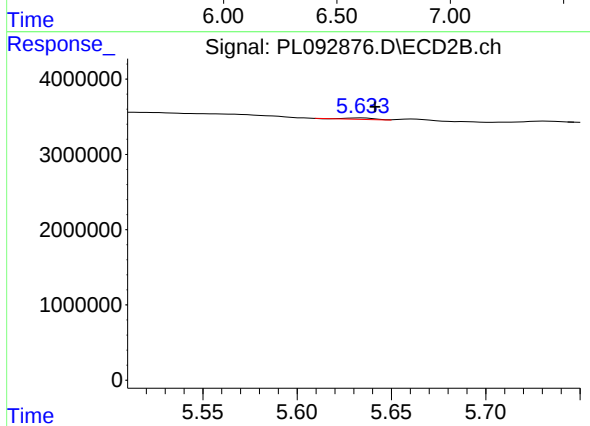

#14 Endrin


R.T.: 5.635 min
Delta R.T.: -0.007 min
Response: 195764
Conc: 0.07 ng/ml

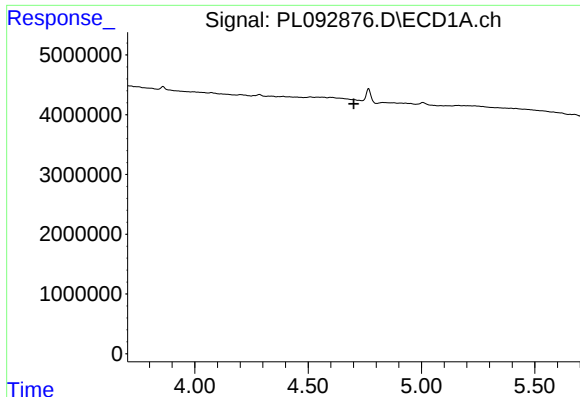

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.702 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164707BL

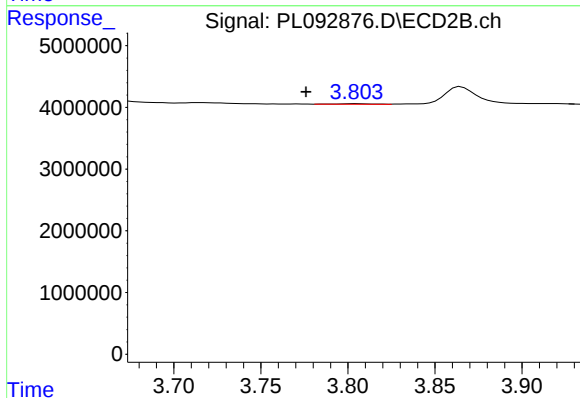


#23 Chlordane-1

R.T.: 3.804 min
Delta R.T.: 0.029 min
Response: 150058
Conc: 1.41 ng/ml

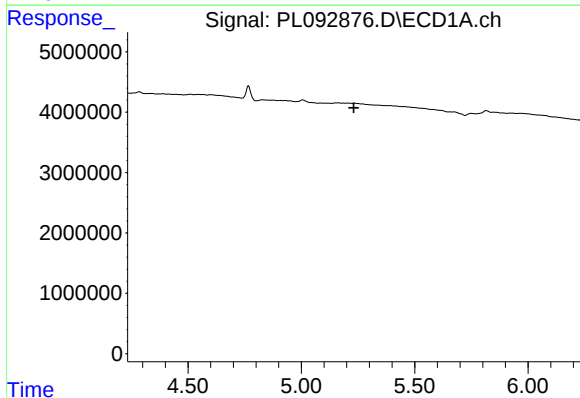


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.231 min
Response: 0
Conc: N.D.

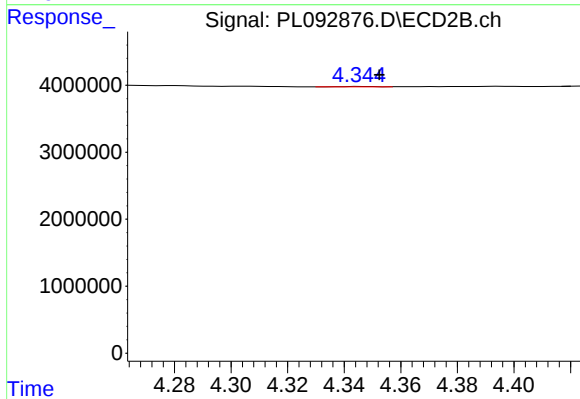

#24 Chlordane-2


R.T.: 4.346 min
Delta R.T.: -0.006 min
Response: 38758
Conc: 0.31 ng/ml

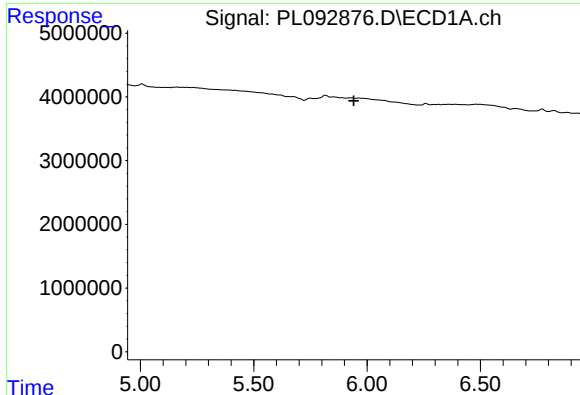

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164707BL

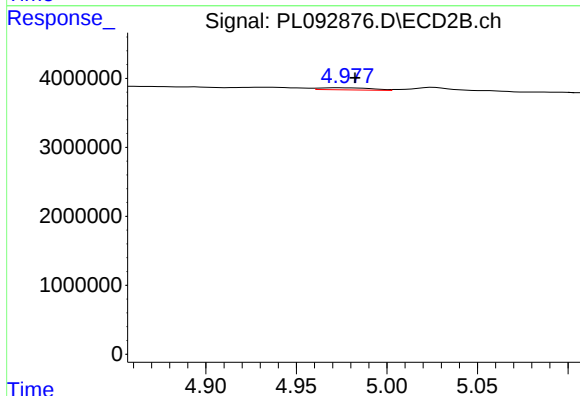


#25 Chlordane-3

R.T.: 4.973 min
Delta R.T.: -0.009 min
Response: 599288
Conc: 1.65 ng/ml

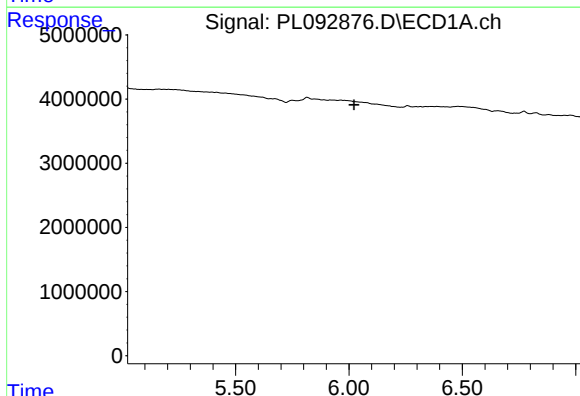


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

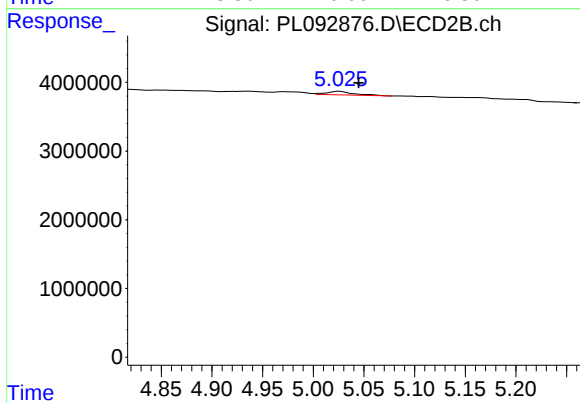

#26 Chlordane-4


R.T.: 5.026 min
Delta R.T.: -0.019 min
Response: 980534
Conc: 2.80 ng/ml

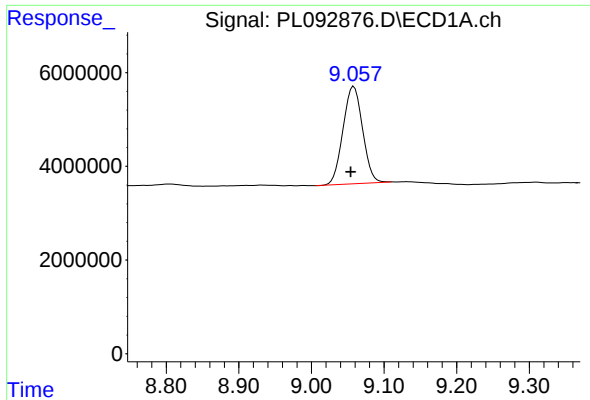

#28 Decachlorobiphenyl

R.T.: 9.058 min
Delta R.T.: 0.004 min
Response: 38990617
Conc: 20.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB164707BL

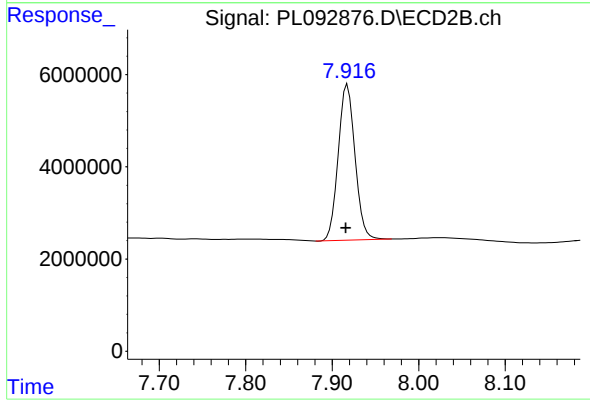

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: 0.002 min
Response: 45263923
Conc: 16.58 ng/ml