

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110624\
 Data File : PL092874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 14:05
 Operator : AR\AJ
 Sample : P4719-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BAYAVE-STOCKPILE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/07/2024
 Supervised By :Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:03:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.778	37139114	39248137	15.157	14.423
28) SA Decachlor...	9.059	7.918	28749571	31768003	14.938	11.640
Target Compounds						
12) B 4,4'-DDE	6.189	5.233	946312	1288635	0.399m	0.400m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110624\
Data File : PL092874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 14:05
Operator : AR\AJ
Sample : P4719-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BAYAVE-STOCKPILE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/07/2024
Supervised By : Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:03:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

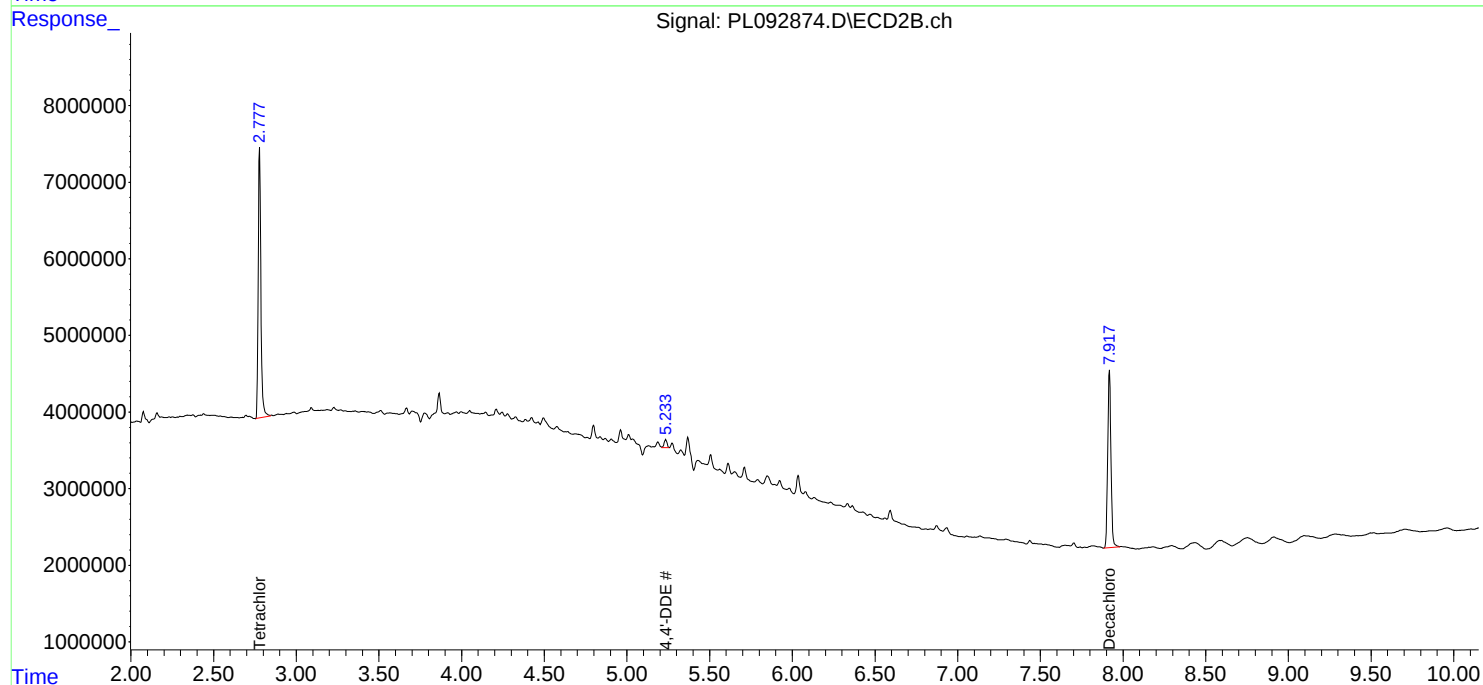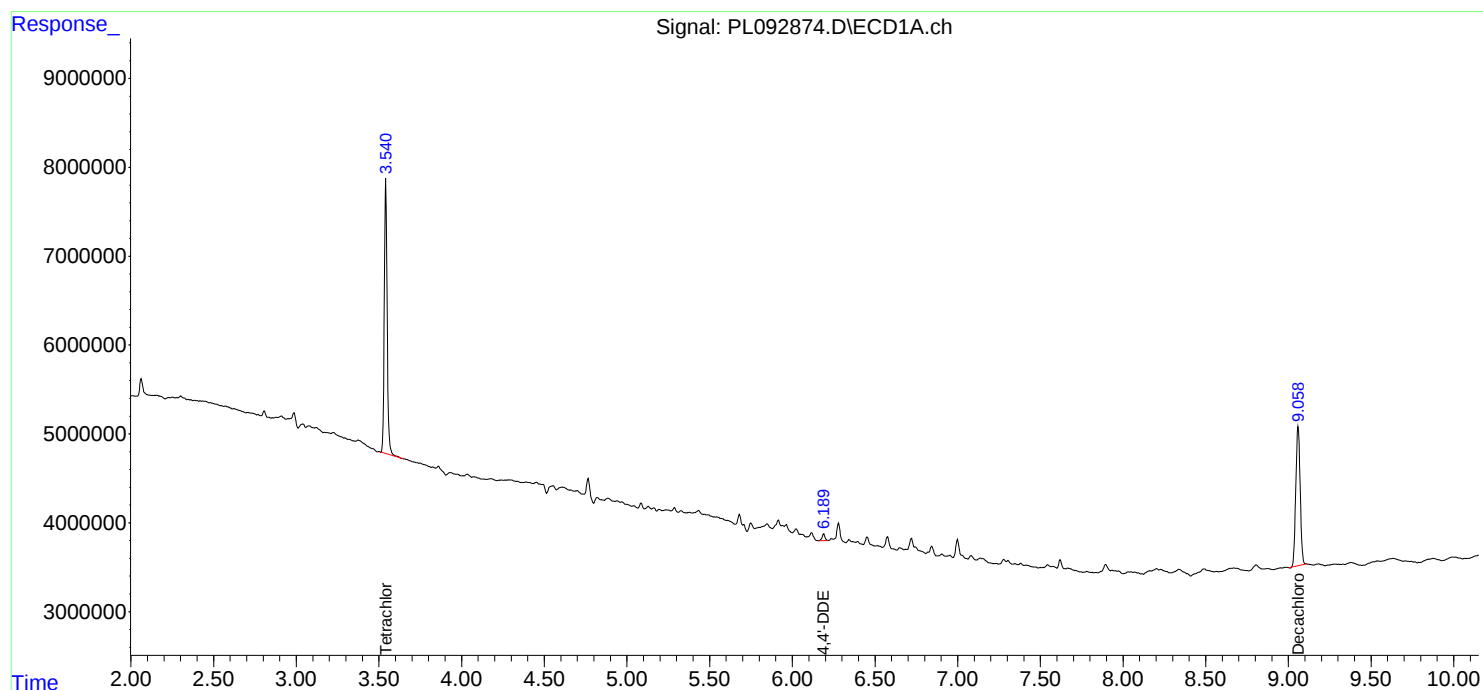

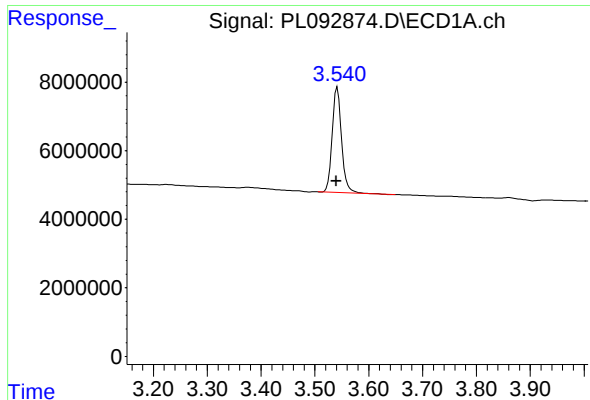

#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: 0.002 min
Response: 37139114
Conc: 15.16 ng/ml

Instrument :

ECD_L


ClientSampleId :

BAYAVE-STOCKPILE

Manual Integrations


APPROVED

Reviewed By :Abdul Mirza 11/07/2024
Supervised By :Ankita Jodhani 11/07/2024

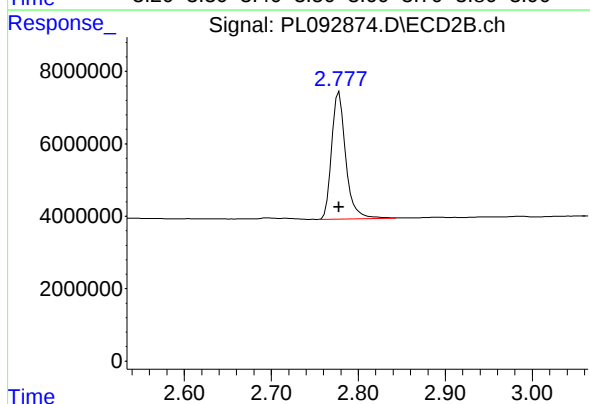


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 39248137
Conc: 14.42 ng/ml

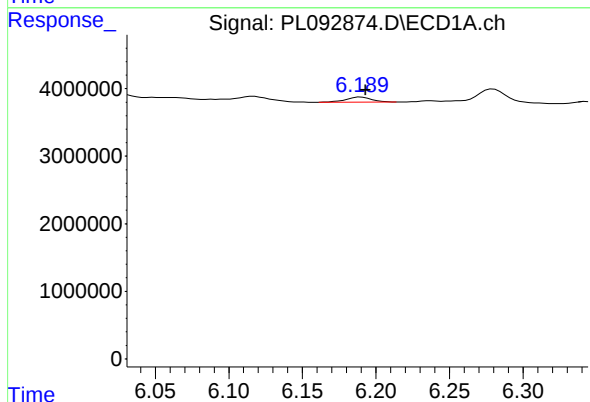


#12 4,4'-DDE

R.T.: 6.189 min
Delta R.T.: -0.004 min
Response: 946312
Conc: 0.40 ng/ml m

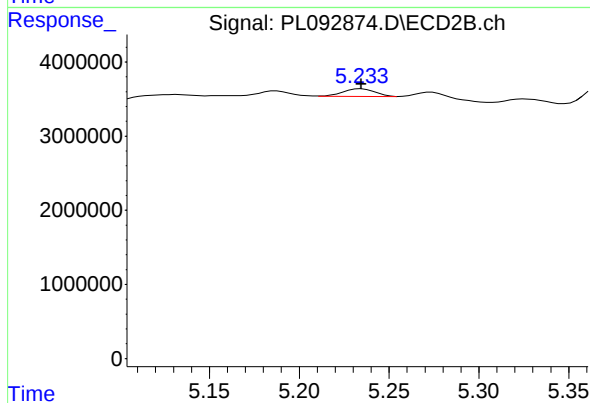

#12 4,4'-DDE

R.T.: 5.233 min
Delta R.T.: -0.001 min
Response: 1288635
Conc: 0.40 ng/ml m

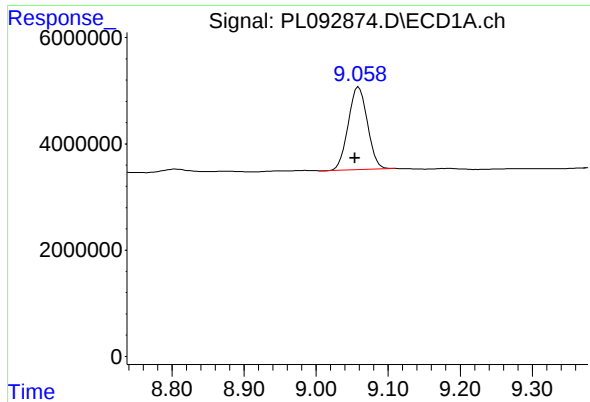


#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: 0.005 min
Response: 28749571
Conc: 14.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAYAVE-STOCKPILE

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/07/2024
Supervised By :Ankita Jodhani 11/07/2024

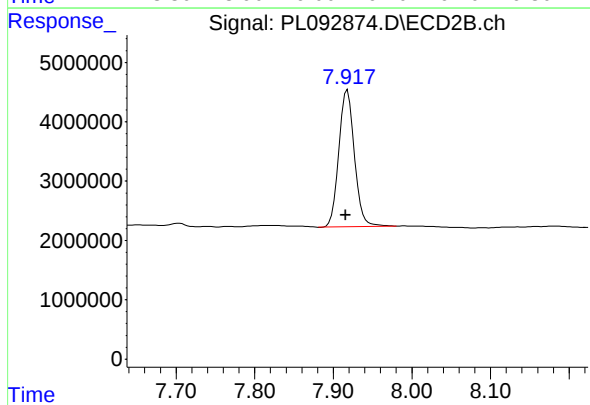

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: 0.002 min
Response: 31768003
Conc: 11.64 ng/ml