

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110624\
 Data File : PL092880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 15:42
 Operator : AR\AJ
 Sample : P4707-01 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-02-110424

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/07/2024
 Supervised By :Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:09:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.546	2.777	10943610	11145368	4.466m	4.096m
28) SA Decachlor...	9.063	7.920	8814181	10765603	4.580m	3.945

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110624\
Data File : PL092880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 15:42
Operator : AR\AJ
Sample : P4707-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HD-02-110424


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/07/2024
Supervised By : Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:09:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

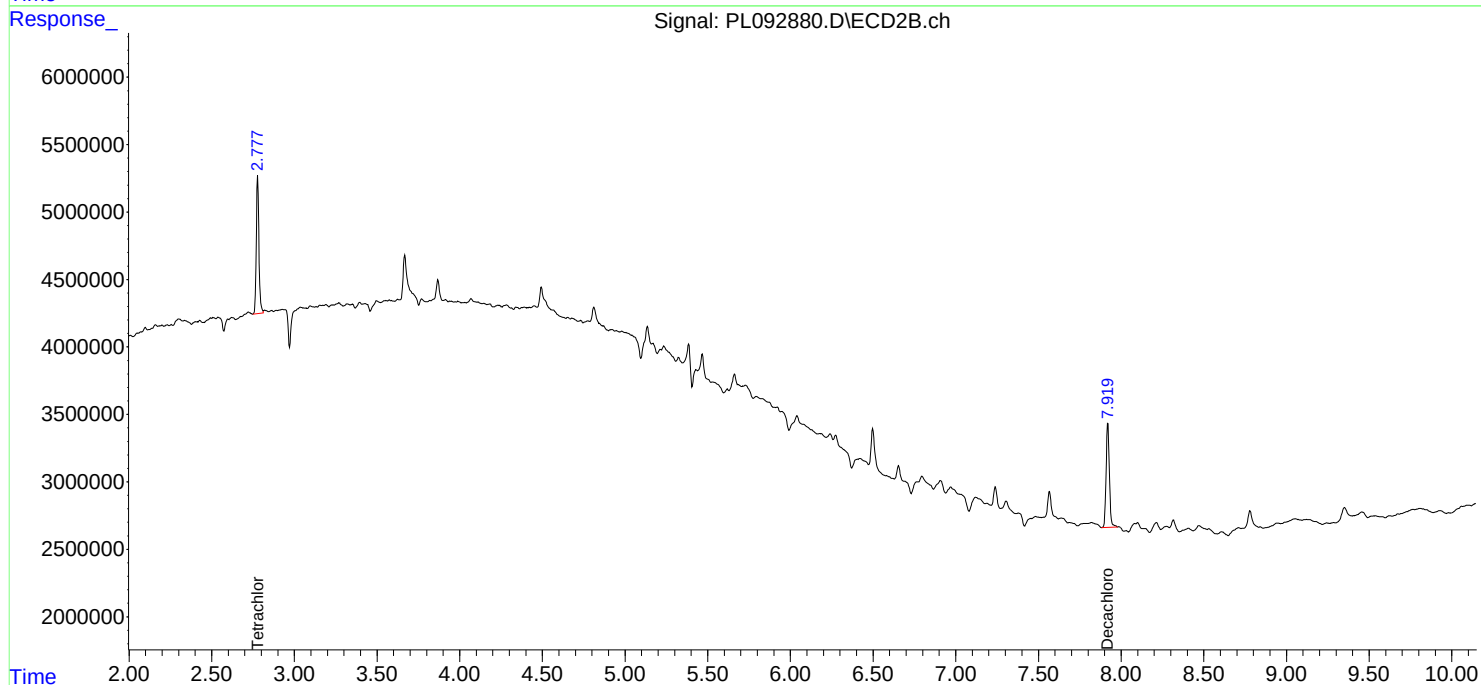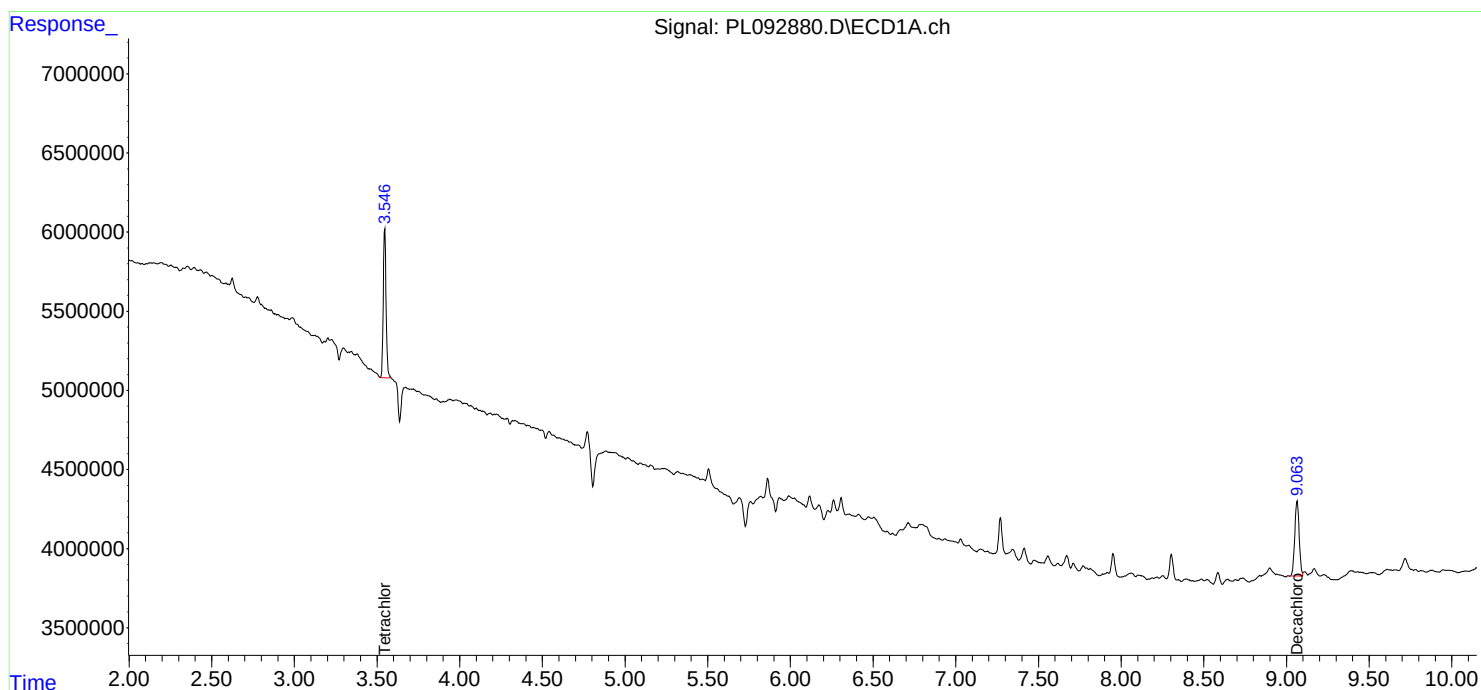

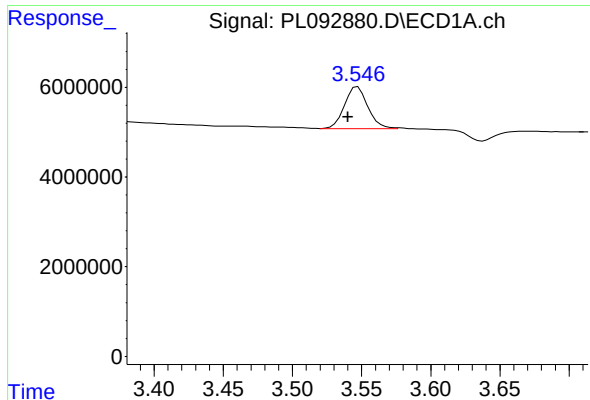


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: 0.006 min
Response: 10943610
Conc: 4.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-110424


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/07/2024
Supervised By :Ankita Jodhani 11/07/2024

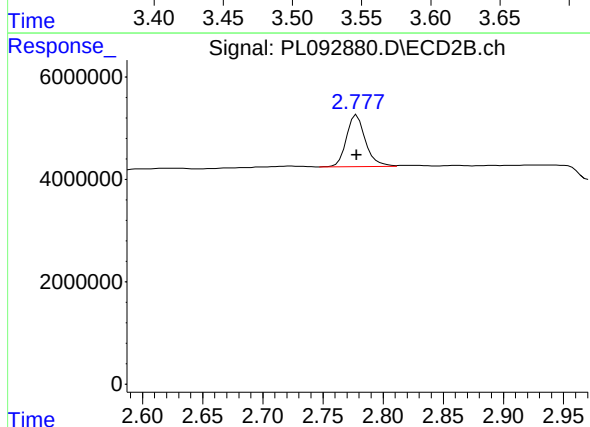


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: -0.001 min
Response: 11145368
Conc: 4.10 ng/ml m

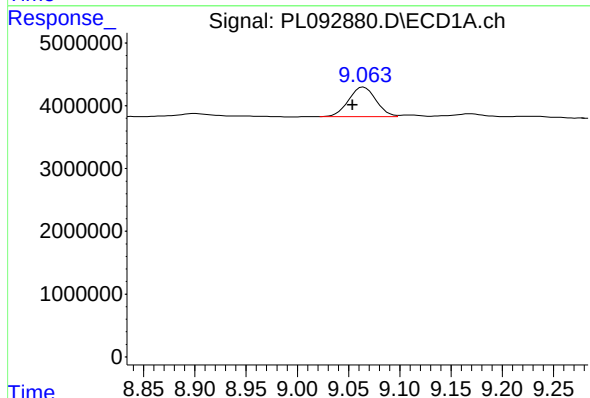

#28 Decachlorobiphenyl

R.T.: 9.063 min
Delta R.T.: 0.009 min
Response: 8814181
Conc: 4.58 ng/ml m

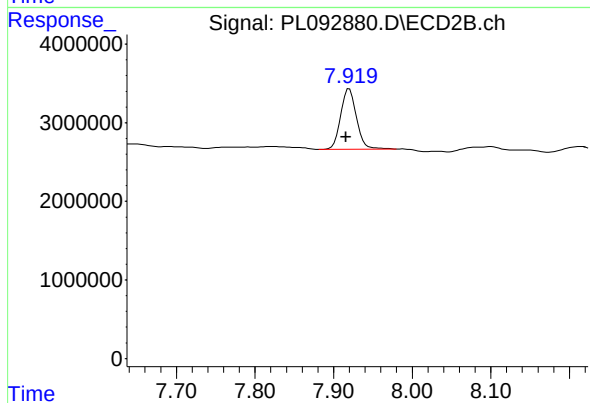

#28 Decachlorobiphenyl

R.T.: 7.920 min
Delta R.T.: 0.004 min
Response: 10765603
Conc: 3.94 ng/ml