

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110718\
 Data File : PL041940.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2018 16:24
 Operator : AJ\SJ
 Sample : J5762-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 08:58:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.104	83354124	41807972	13.085	13.573
28)	SA Decachlor...	8.215	9.237	71311193	28448945	10.766	11.104
Target Compounds							
2)	A alpha-BHC	3.865f	0.000	157425	0	0.016	N.D. #
6)	B beta-BHC	4.408f	0.000	5083094	0	1.349	N.D. #
9)	A Endosulfan I	0.000	6.413f	0	1650577	N.D.	0.531 #
10)	B gamma-Chl...	5.407	0.000	681525	0	0.084	N.D. #
11)	B alpha-Chl...	5.407f	0.000	681525	0	0.084	N.D. #
12)	B 4,4'-DDE	5.634	6.463	15136202	6240582	2.115	1.907
16)	A 4,4'-DDD	6.147	6.956	4829713	3281467	0.831	1.318 #
17)	MA 4,4'-DDT	6.386	7.256	5410719	2807808	0.889	1.117 #
23)	Chlordane-1	4.408	0.000	5083094	0	17.927	N.D. #
24)	Chlordane-2	4.903	0.000	1207743	0	4.101	N.D. #
25)	Chlordane-3	5.407	0.000	681525	0	0.765	N.D. #
26)	Chlordane-4	5.407	0.000	681525	0	0.870	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110718\
Data File : PL041940.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2018 16:24
Operator : AJ\SJ
Sample : J5762-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 08:58:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

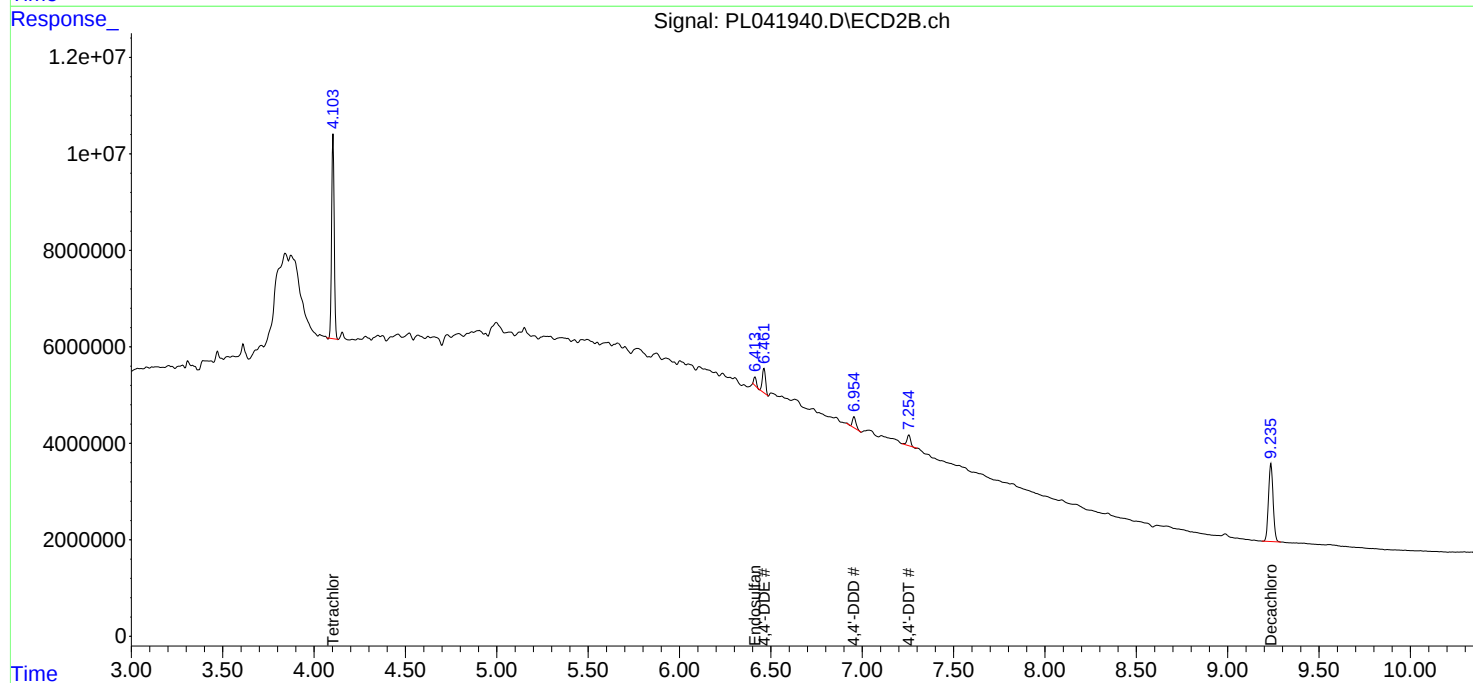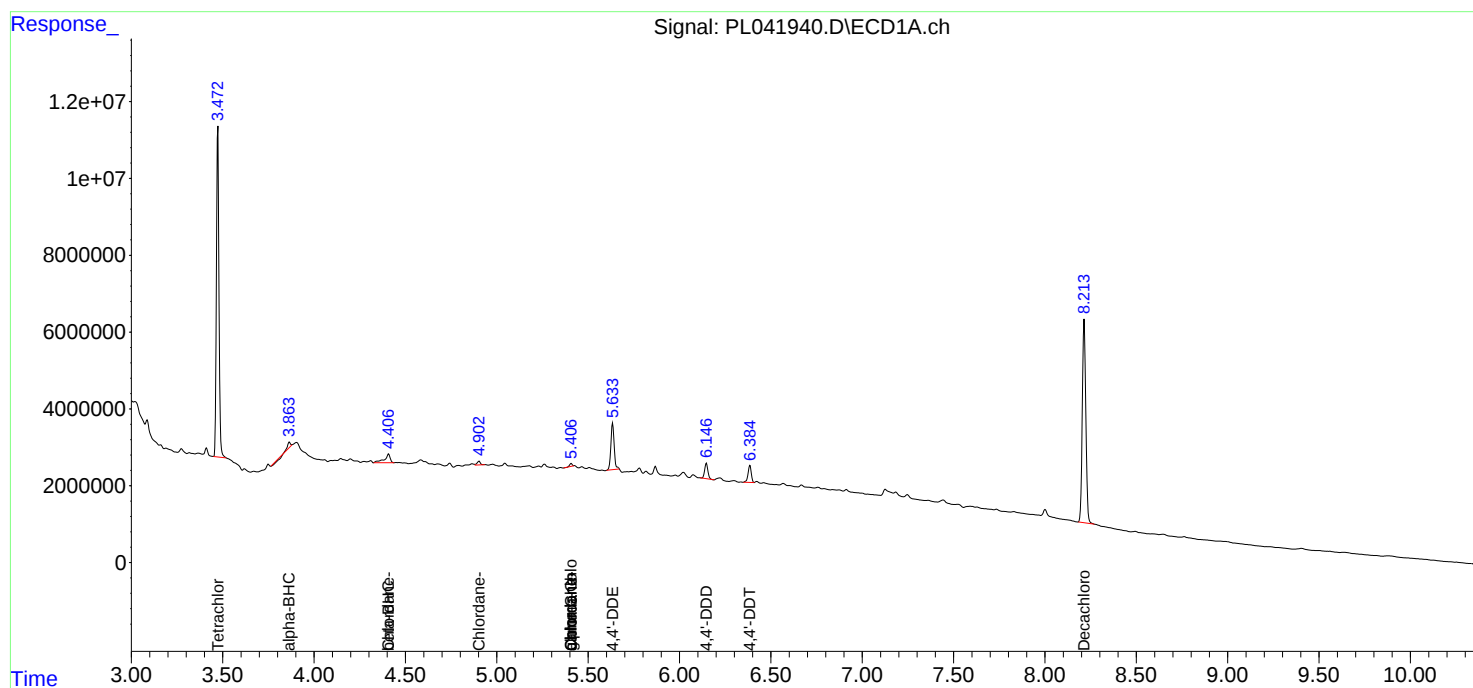


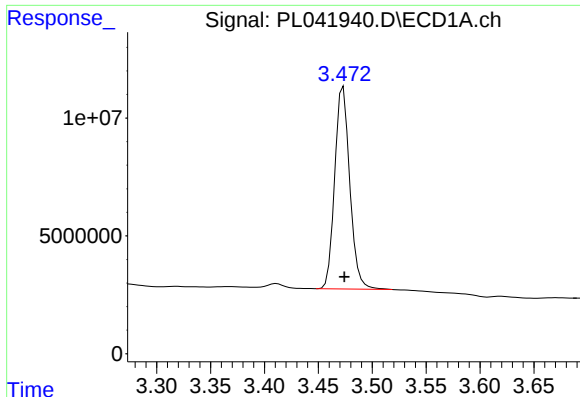

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: 0.000 min
Response: 83354124
Conc: 13.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

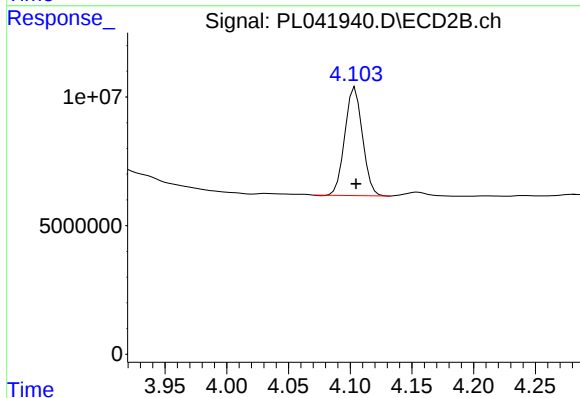


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 41807972
Conc: 13.57 ng/ml

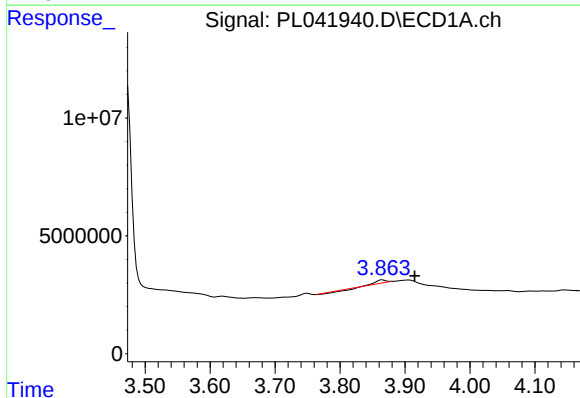


#2 alpha-BHC

R.T.: 3.865 min
Delta R.T.: -0.050 min
Response: 157425
Conc: 0.02 ng/ml

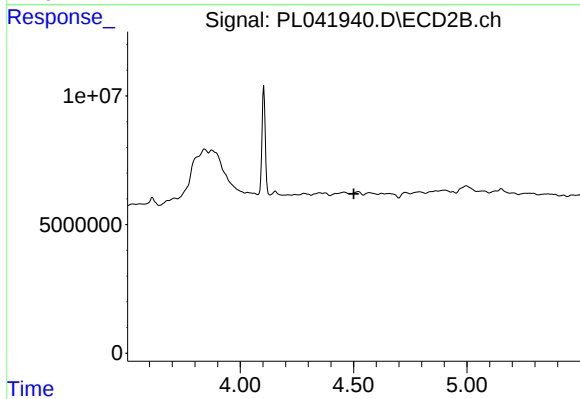

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.501 min
Response: 0
Conc: N.D.

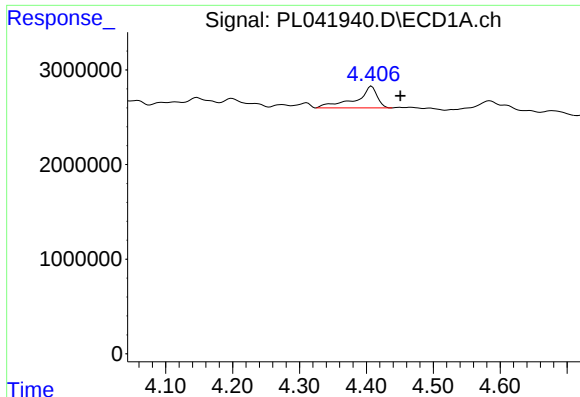

#6 beta-BHC


R.T.: 4.408 min
Delta R.T.: -0.043 min
Response: 5083094
Conc: 1.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

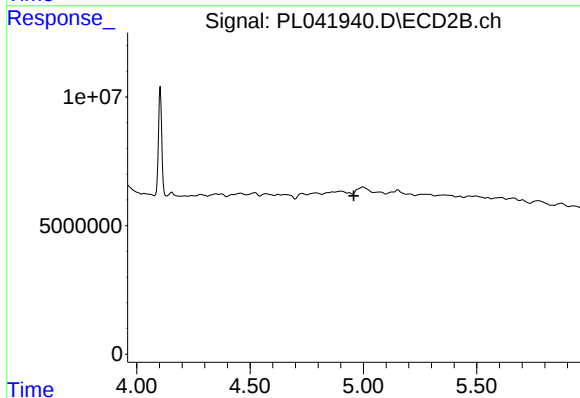


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

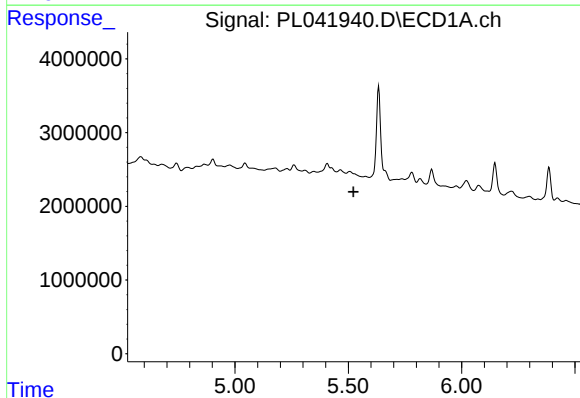


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

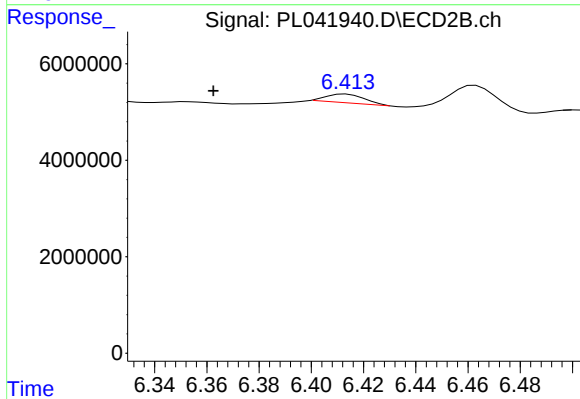

#9 Endosulfan I


R.T.: 6.413 min
Delta R.T.: 0.051 min
Response: 1650577
Conc: 0.53 ng/ml

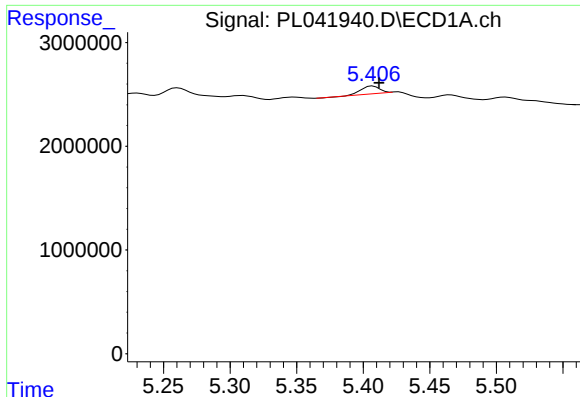

#10 gamma-Chlordane


R.T.: 5.407 min
Delta R.T.: -0.005 min
Response: 681525
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

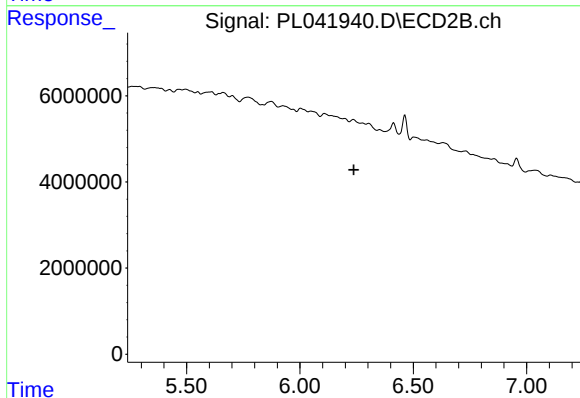


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

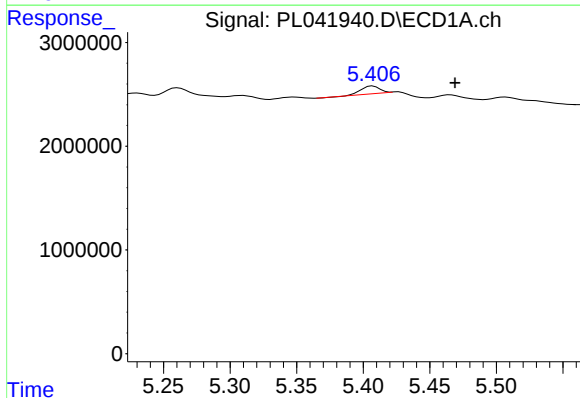


#11 alpha-Chlordane

R.T.: 5.407 min
Delta R.T.: -0.062 min
Response: 681525
Conc: 0.08 ng/ml

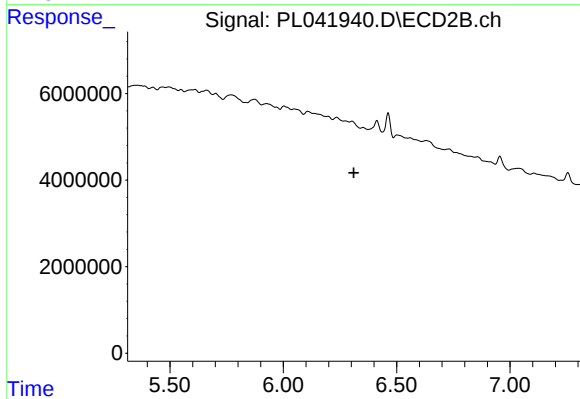

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

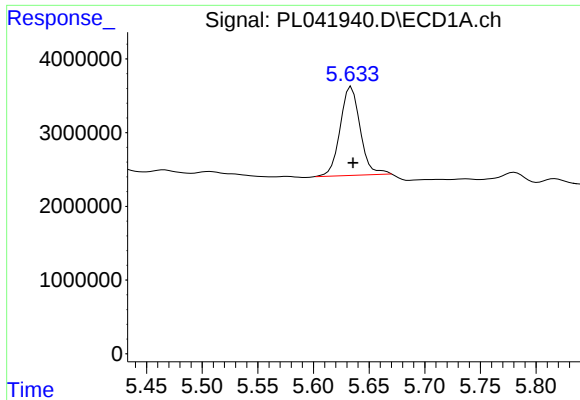

#12 4,4'-DDE


R.T.: 5.634 min
Delta R.T.: -0.001 min
Response: 15136202
Conc: 2.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

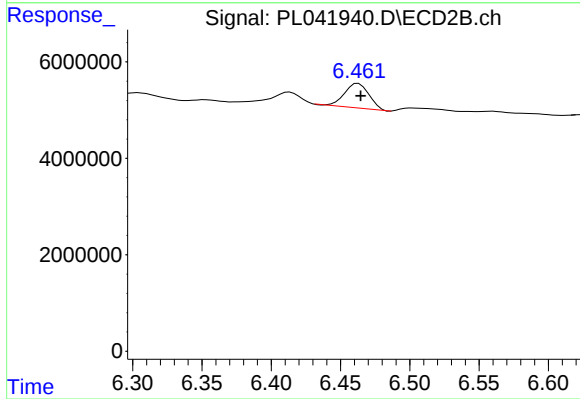


#12 4,4'-DDE

R.T.: 6.463 min
Delta R.T.: -0.002 min
Response: 6240582
Conc: 1.91 ng/ml

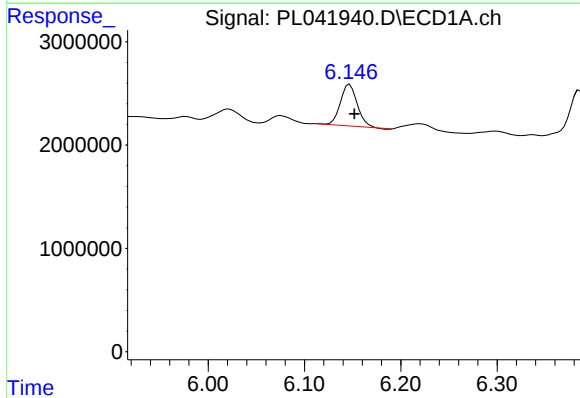


#16 4,4'-DDD

R.T.: 6.147 min
Delta R.T.: -0.005 min
Response: 4829713
Conc: 0.83 ng/ml

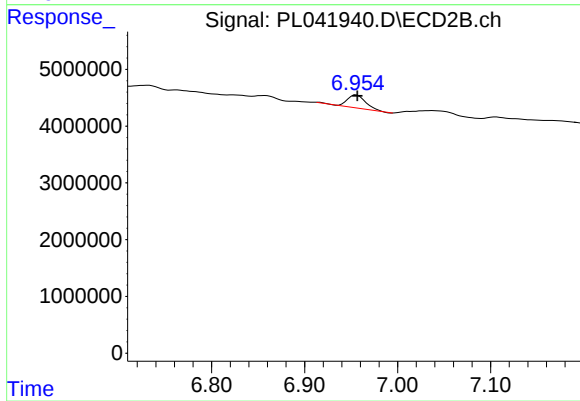

#16 4,4'-DDD


R.T.: 6.956 min
Delta R.T.: -0.001 min
Response: 3281467
Conc: 1.32 ng/ml

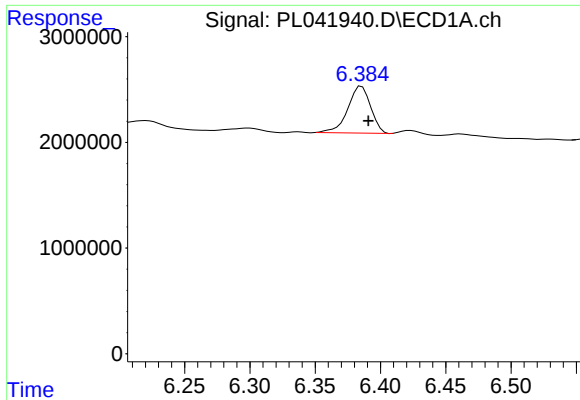

#17 4,4'-DDT


R.T.: 6.386 min
Delta R.T.: -0.005 min
Response: 5410719
Conc: 0.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

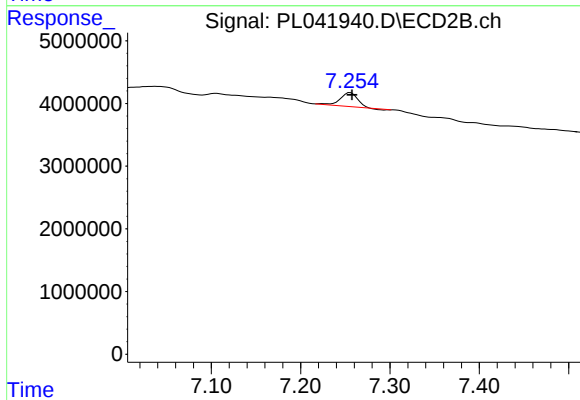


#17 4,4'-DDT

R.T.: 7.256 min
Delta R.T.: -0.002 min
Response: 2807808
Conc: 1.12 ng/ml

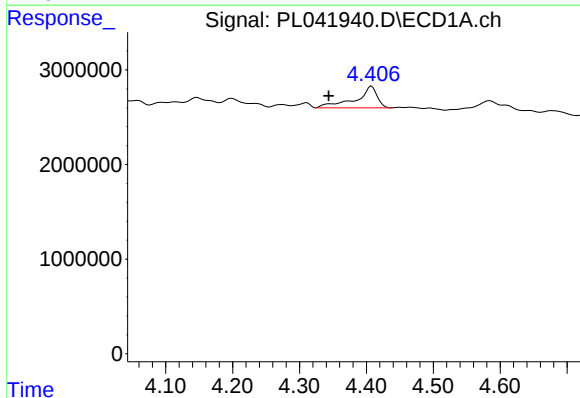


#23 Chlordane-1

R.T.: 4.408 min
Delta R.T.: 0.064 min
Response: 5083094
Conc: 17.93 ng/ml

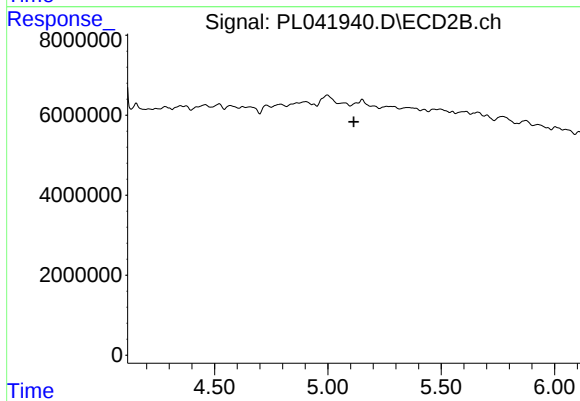

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.115 min
Response: 0
Conc: N.D.

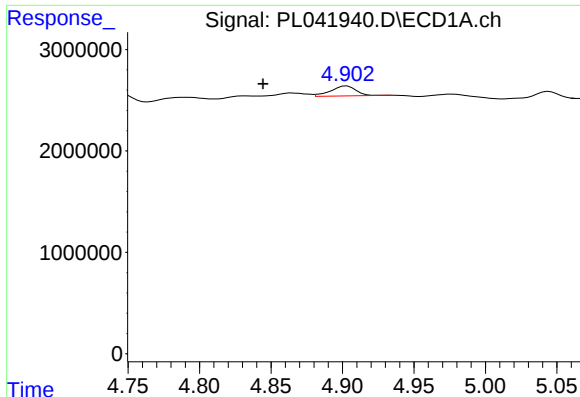

#24 Chlordane-2


R.T.: 4.903 min
Delta R.T.: 0.059 min
Response: 1207743
Conc: 4.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

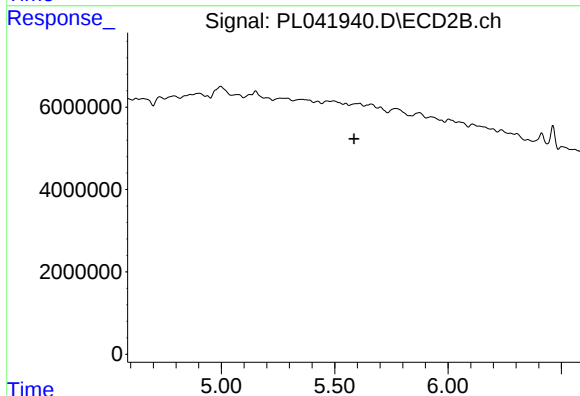


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.586 min
Response: 0
Conc: N.D.

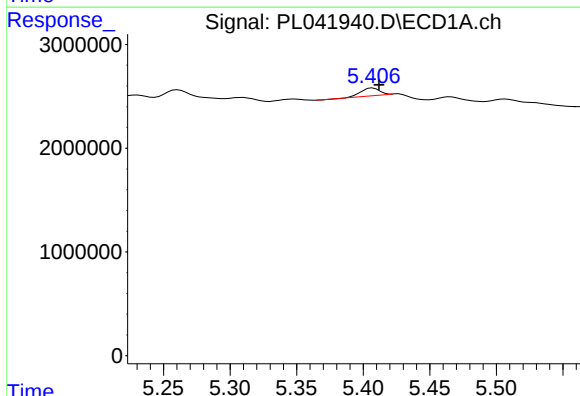


#25 Chlordane-3

R.T.: 5.407 min
Delta R.T.: -0.005 min
Response: 681525
Conc: 0.76 ng/ml

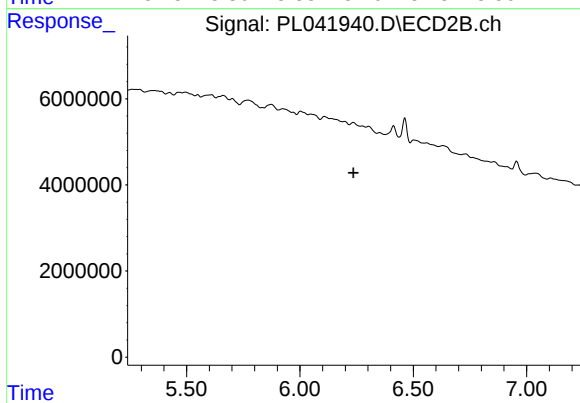

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

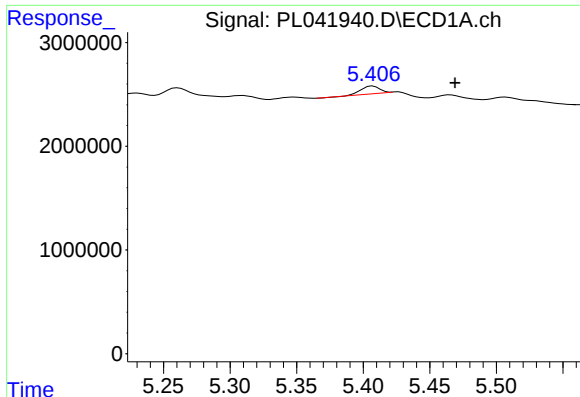

#26 Chlordane-4


R.T.: 5.407 min
Delta R.T.: -0.062 min
Response: 681525
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

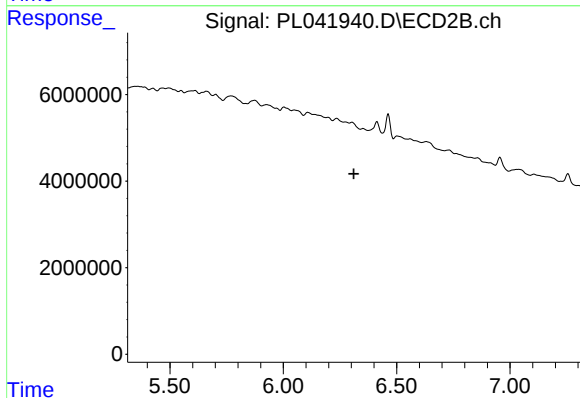


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

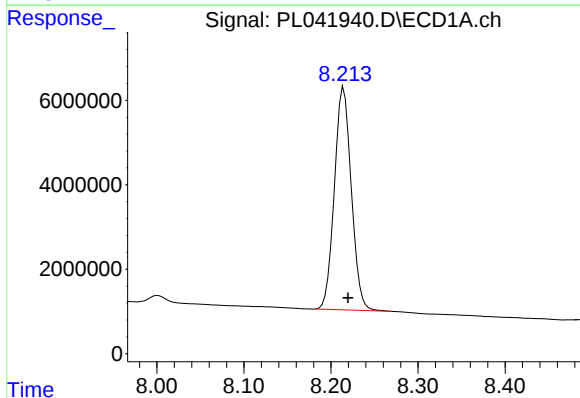

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.005 min
Response: 71311193
Conc: 10.77 ng/ml

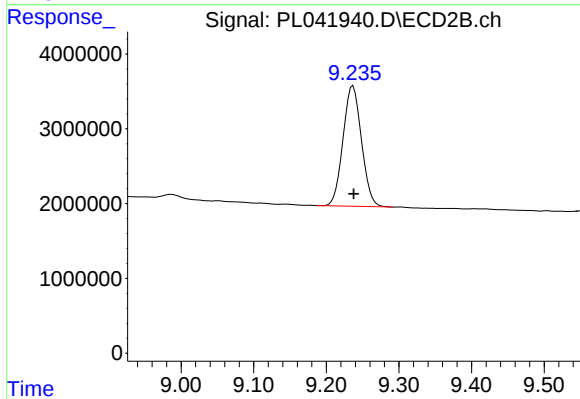

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.000 min
Response: 28448945
Conc: 11.10 ng/ml