

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110718\
 Data File : PL041942.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2018 16:52
 Operator : AJ\SJ
 Sample : J5839-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 08:59:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.471	4.105	80836134	37667286	12.690	12.229
28)	SA Decachlor...	8.213	9.237	73055024	28706770	11.029	11.204
Target Compounds							
6)	B beta-BHC	4.406f	0.000	7594420	0	2.015	N.D. #
10)	B gamma-Chl...	0.000	6.245	0	2503795	N.D.	0.742 #
11)	B alpha-Chl...	0.000	6.245f	0	2503795	N.D.	0.740 #
23)	Chlordane-1	4.351	0.000	3082734	0	10.872	N.D. #
25)	Chlordane-3	0.000	6.245	0	2503795	N.D.	5.564 #
26)	Chlordane-4	0.000	6.245	0	2503795	N.D.	4.789 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110718\
Data File : PL041942.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2018 16:52
Operator : AJ\SJ
Sample : J5839-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 08:59:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

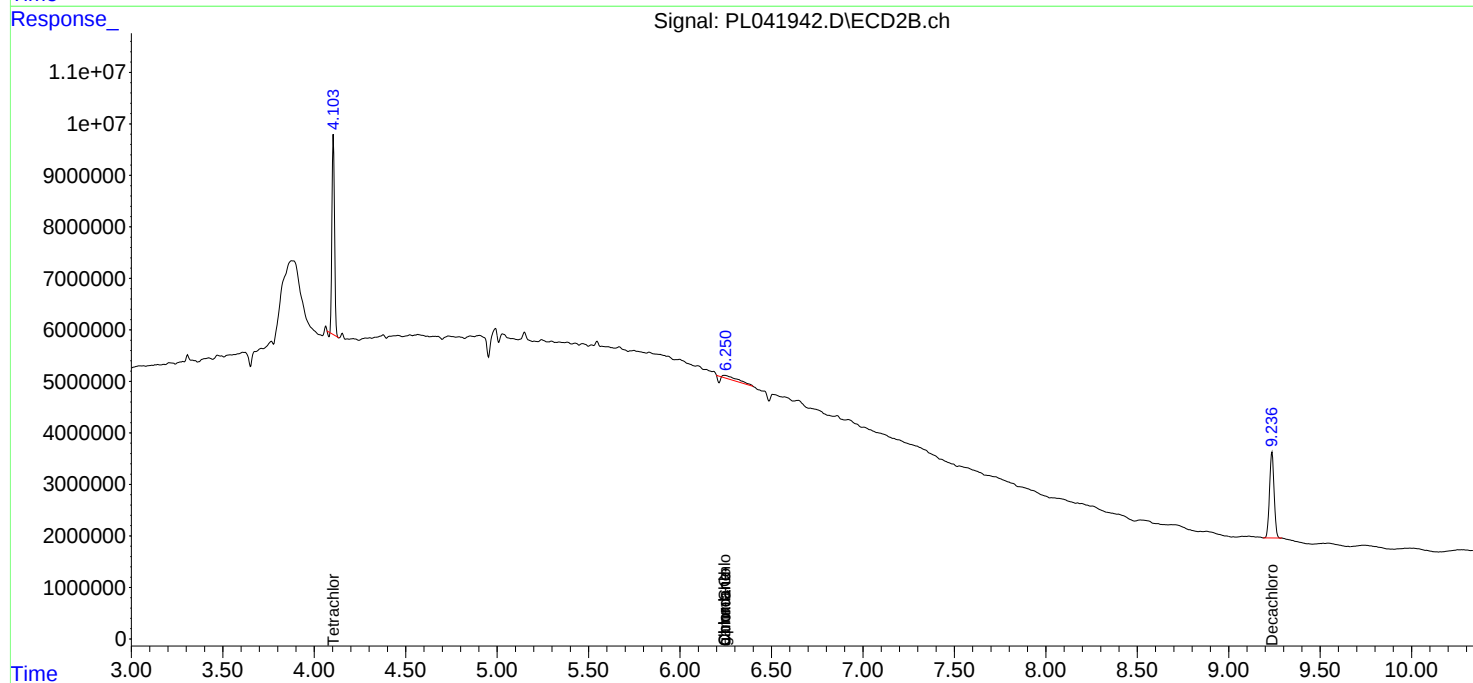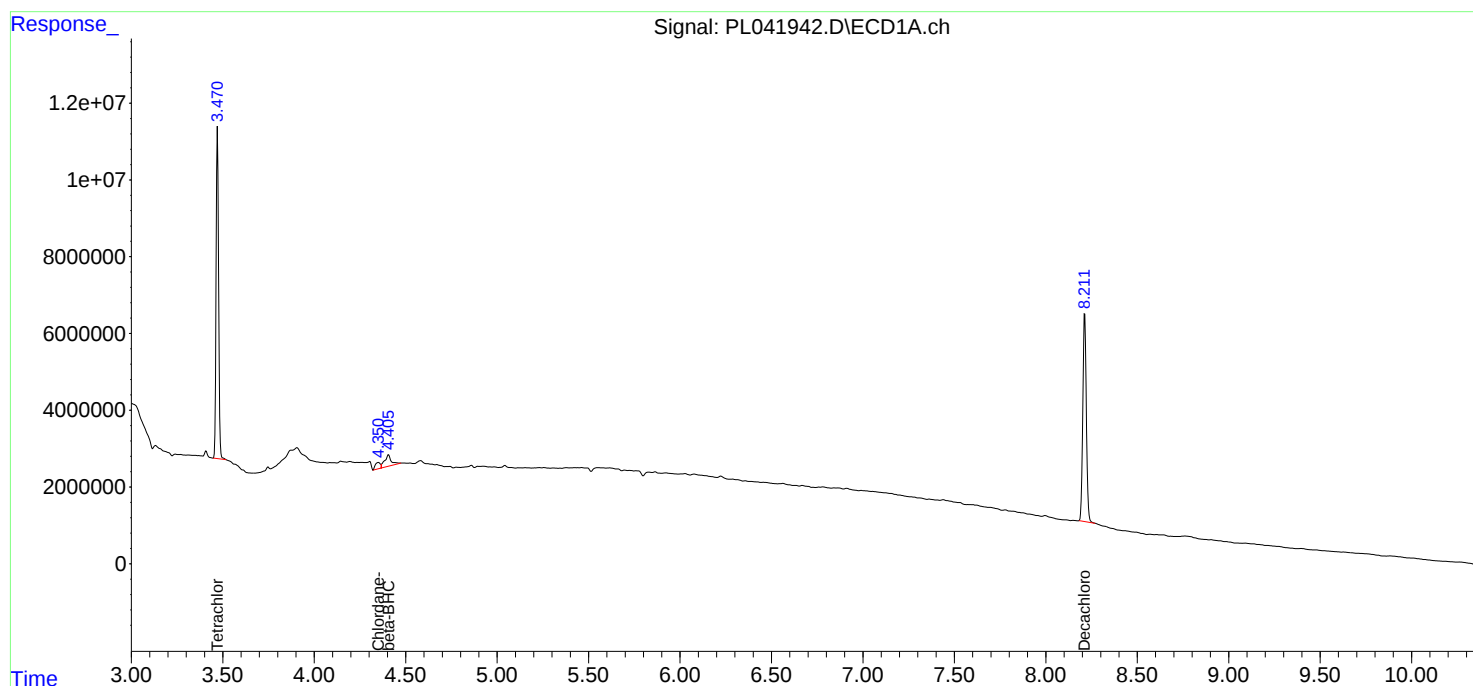


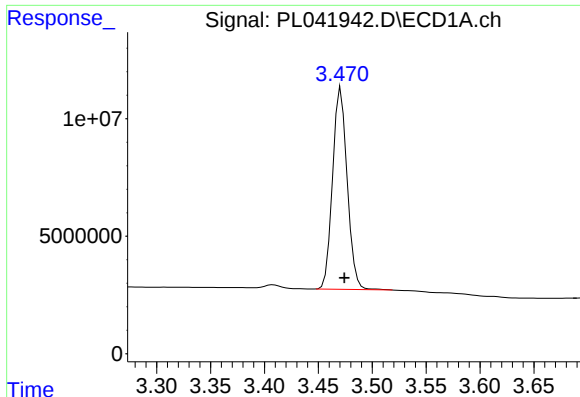

#1 Tetrachloro-m-xylene


R.T.: 3.471 min
Delta R.T.: -0.003 min
Response: 80836134
Conc: 12.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

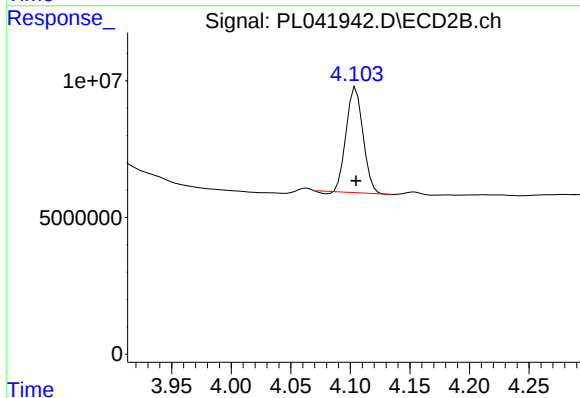


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 37667286
Conc: 12.23 ng/ml

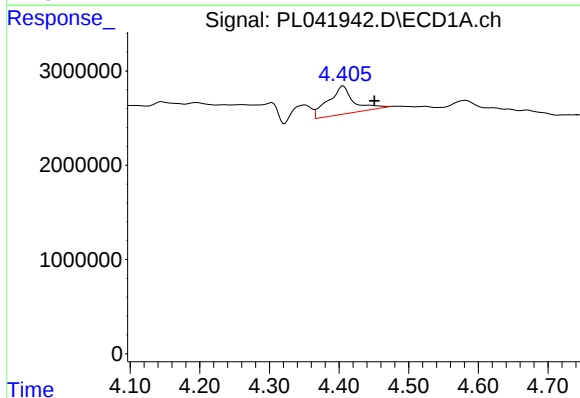


#6 beta-BHC

R.T.: 4.406 min
Delta R.T.: -0.045 min
Response: 7594420
Conc: 2.01 ng/ml

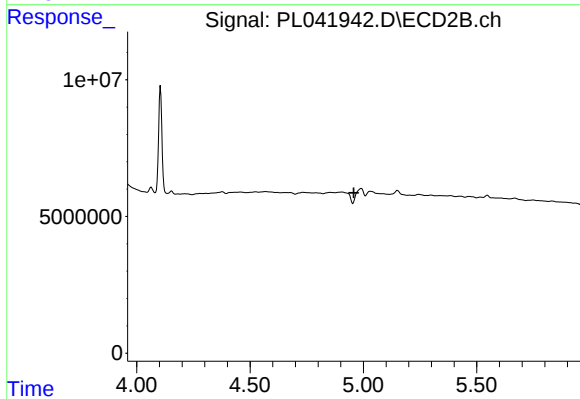

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

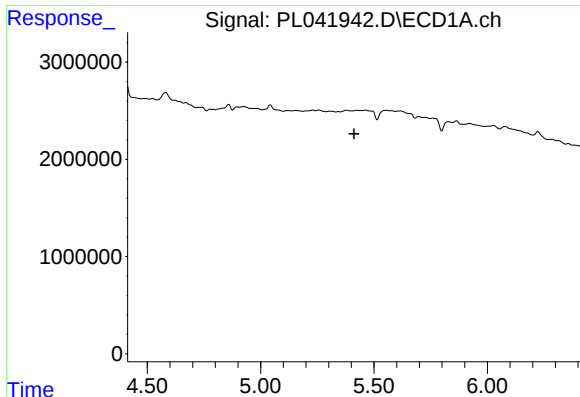

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

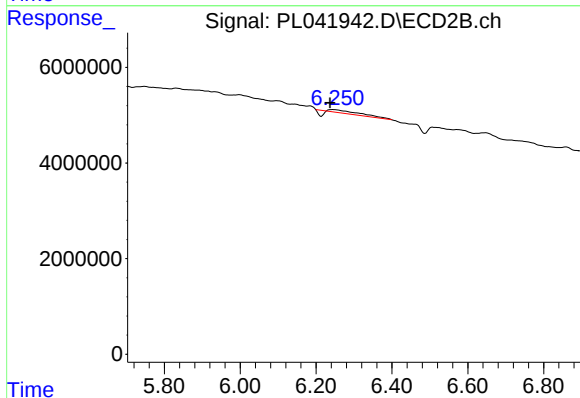


#10 gamma-Chlordane

R.T.: 6.245 min
Delta R.T.: 0.007 min
Response: 2503795
Conc: 0.74 ng/ml

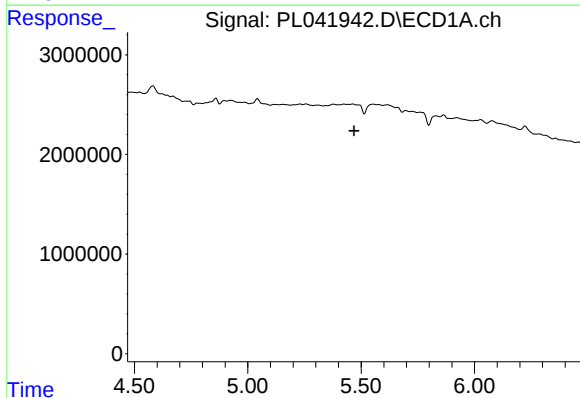


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.469 min
Response: 0
Conc: N.D.

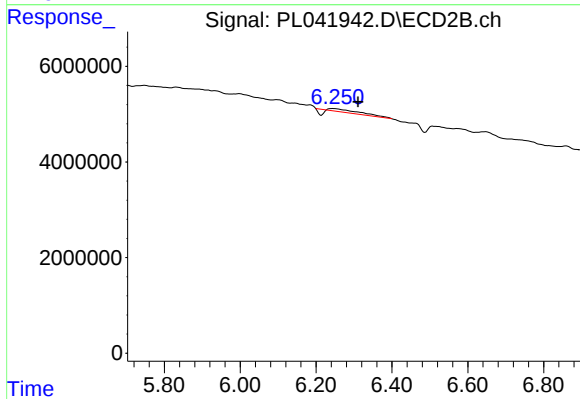

#11 alpha-Chlordane


R.T.: 6.245 min
Delta R.T.: -0.066 min
Response: 2503795
Conc: 0.74 ng/ml

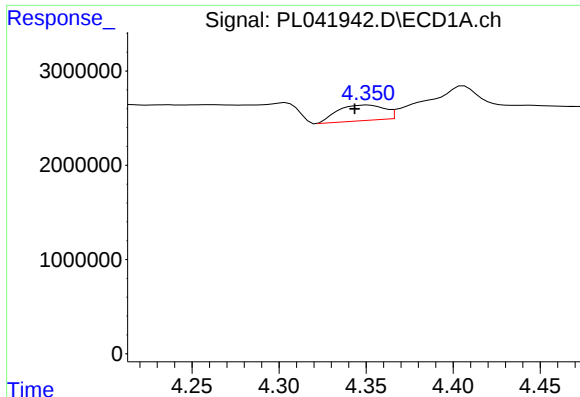

#23 Chlordane-1


R.T.: 4.351 min
Delta R.T.: 0.008 min
Response: 3082734
Conc: 10.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

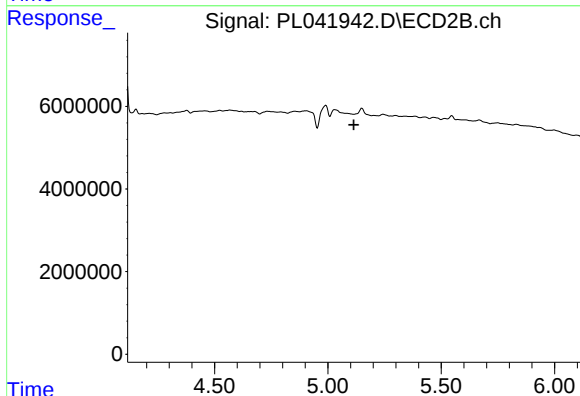


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

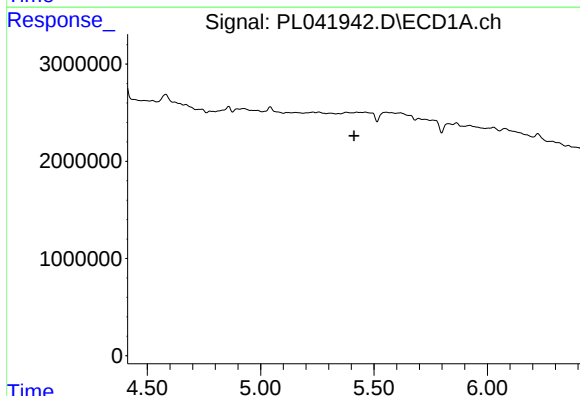


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.412 min
Response: 0
Conc: N.D.

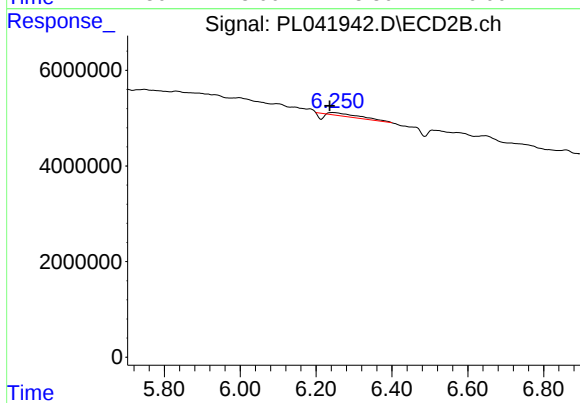

#25 Chlordane-3


R.T.: 6.245 min
Delta R.T.: 0.008 min
Response: 2503795
Conc: 5.56 ng/ml

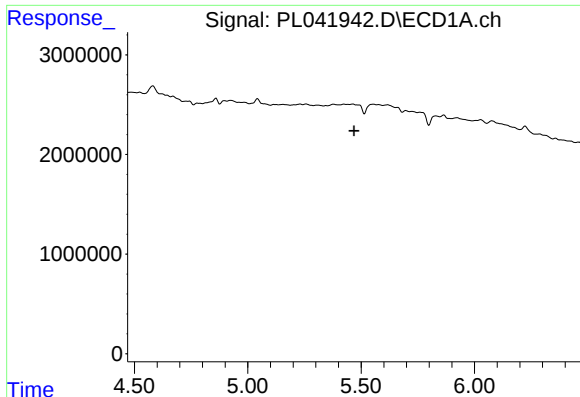

#26 Chlorodane-4


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

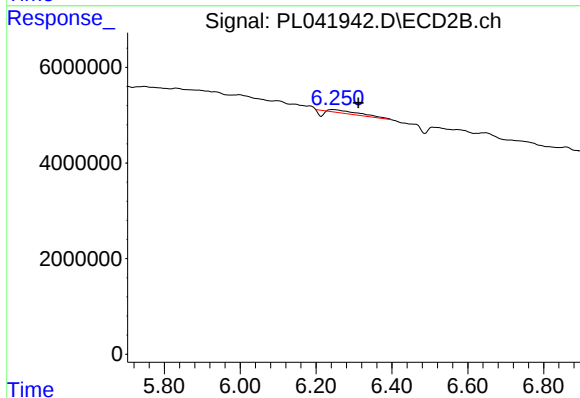


#26 Chlorodane-4

R.T.: 6.245 min
Delta R.T.: -0.067 min
Response: 2503795
Conc: 4.79 ng/ml

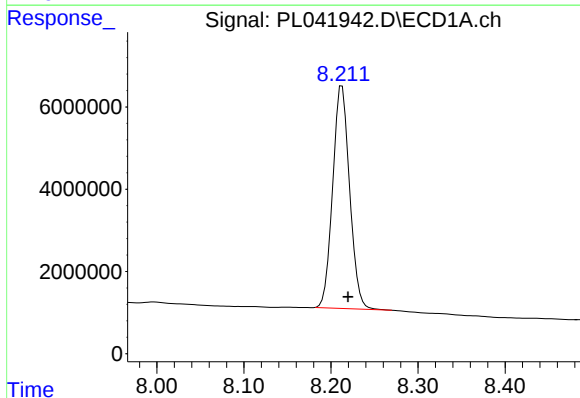

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.007 min
Response: 73055024
Conc: 11.03 ng/ml

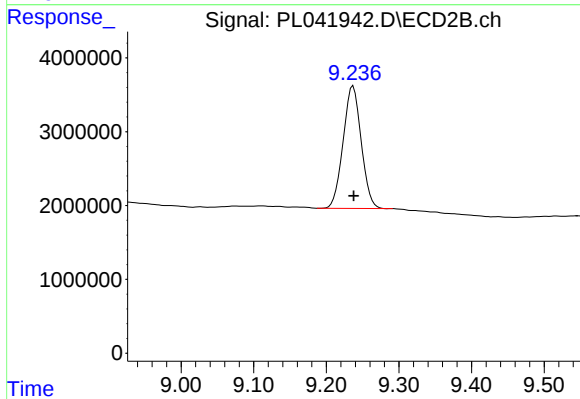

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.000 min
Response: 28706770
Conc: 11.20 ng/ml