

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110718\
 Data File : PL041944.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2018 17:21
 Operator : AJ\SJ
 Sample : J5839-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 08:59:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.471	4.105	106.2E6	52883022	16.666	17.169
28)	SA Decachlor...	8.212	9.236	87874571	35003431	13.266	13.662
Target Compounds							
3)	MA gamma-BHC...	4.201	0.000	1590453	0	0.178	N.D. #
6)	B beta-BHC	4.407f	0.000	3900677	0	1.035	N.D. #
7)	B delta-BHC	0.000	5.151f	0	1701508	N.D.	0.421 #
23)	Chlordane-1	4.346	5.151	2848800	1701508	10.047	12.251



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110718\
Data File : PL041944.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2018 17:21
Operator : AJ\SJ
Sample : J5839-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 08:59:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

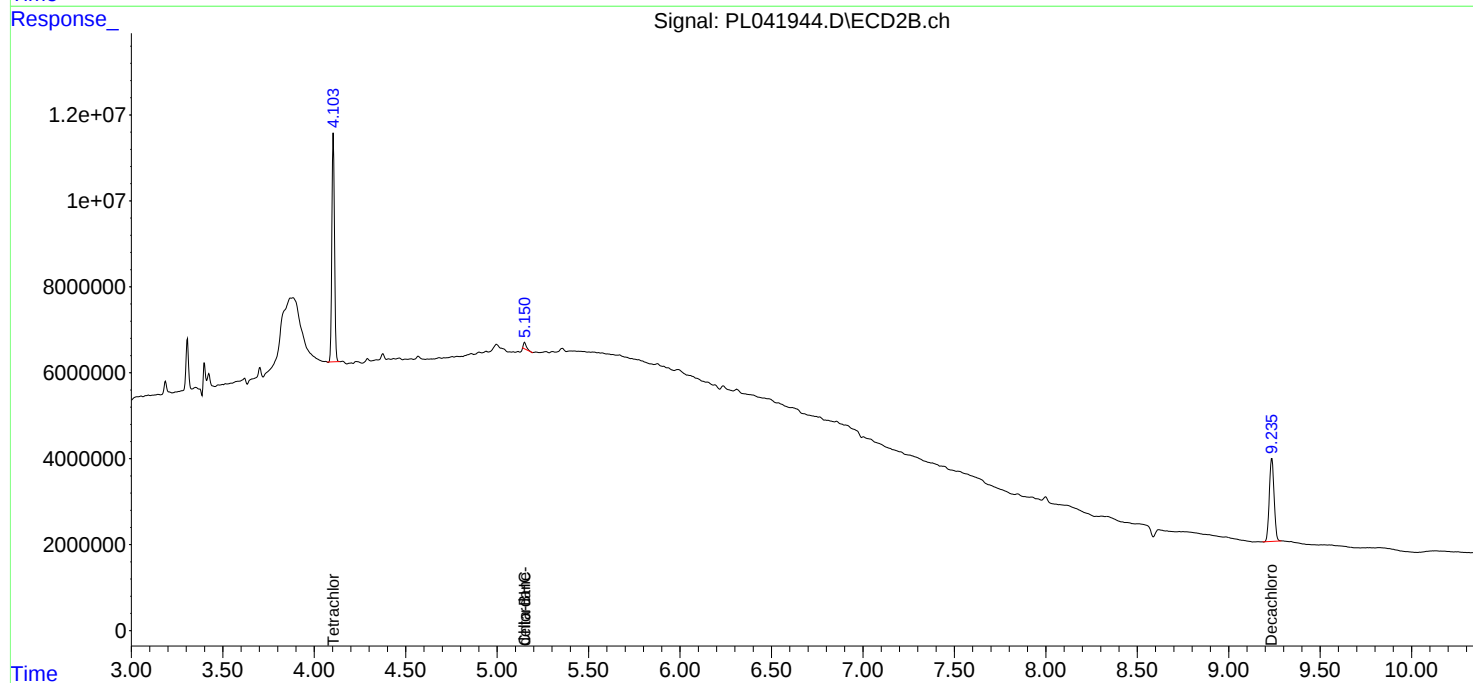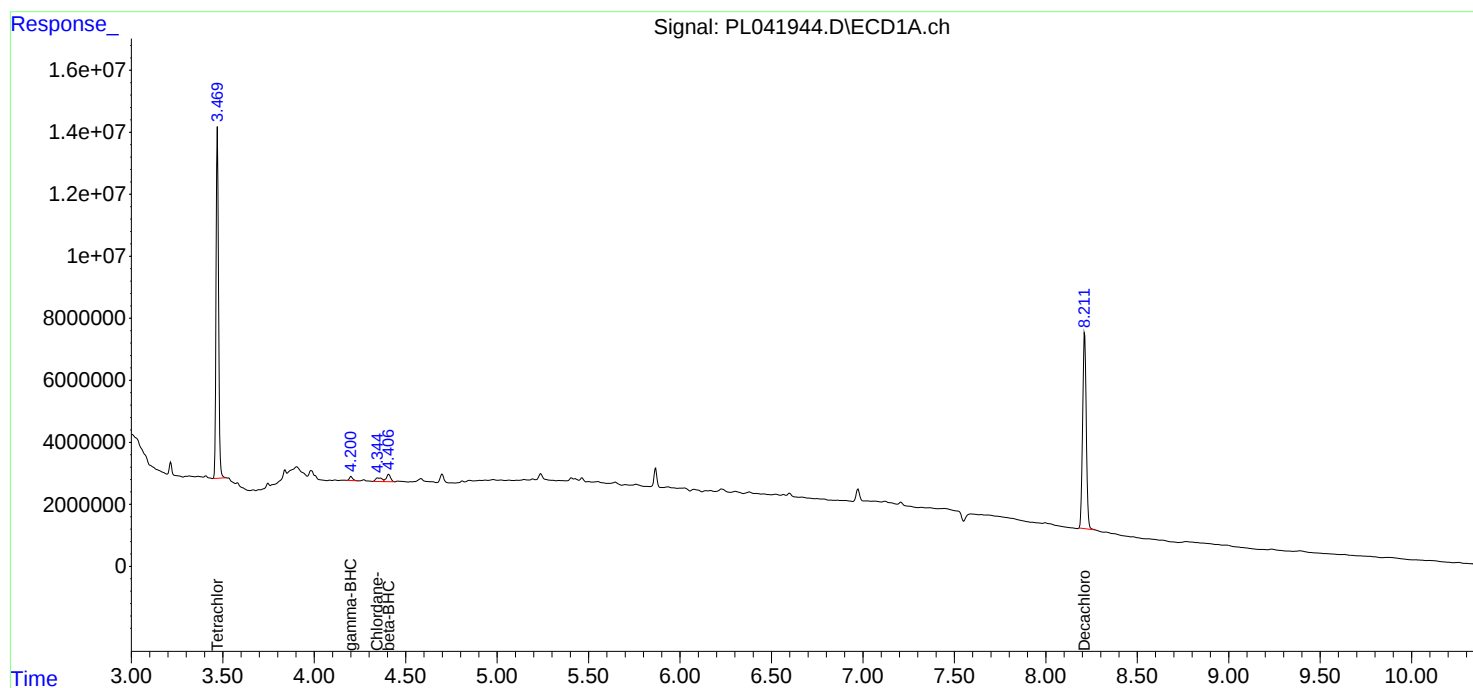


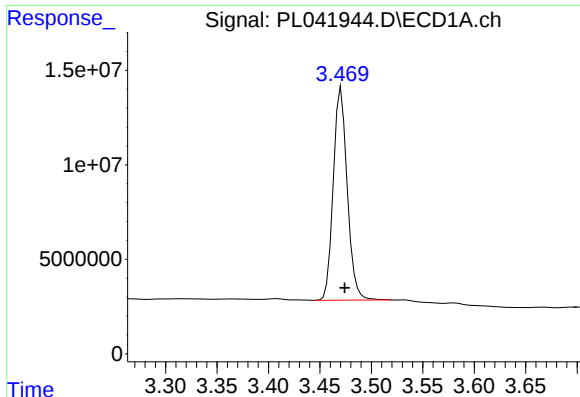

#1 Tetrachloro-m-xylene


R.T.: 3.471 min
Delta R.T.: -0.003 min
Response: 106168042
Conc: 16.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

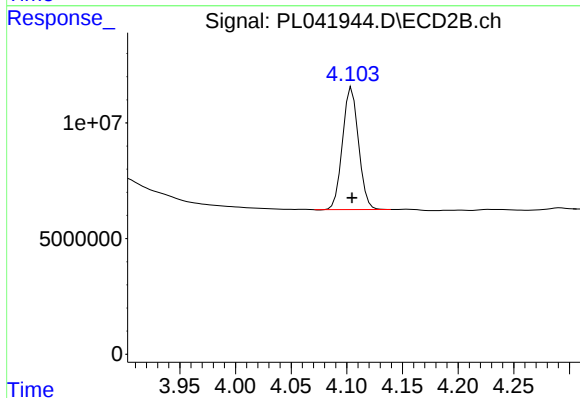


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 52883022
Conc: 17.17 ng/ml

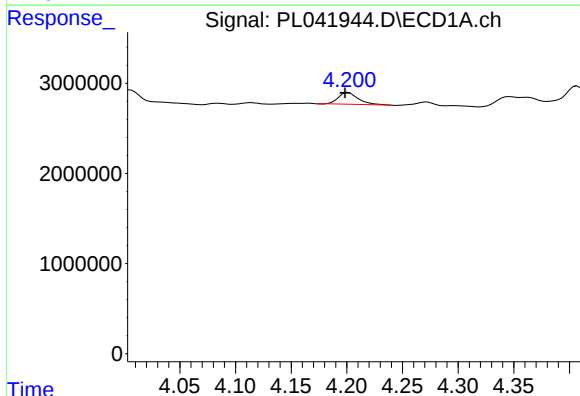


#3 gamma-BHC (Lindane)

R.T.: 4.201 min
Delta R.T.: 0.003 min
Response: 1590453
Conc: 0.18 ng/ml

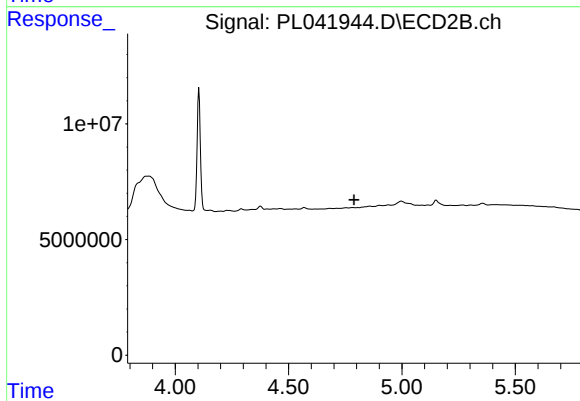

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.789 min
Response: 0
Conc: N.D.

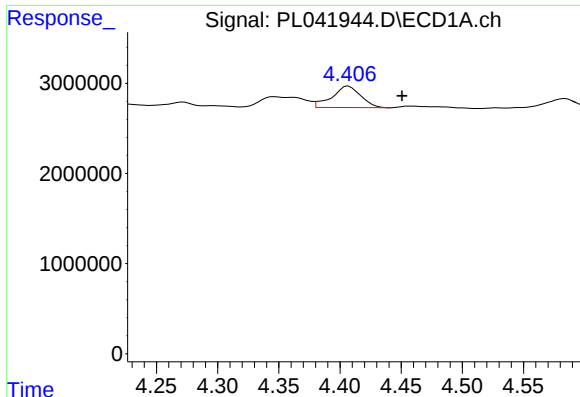

#6 beta-BHC


R.T.: 4.407 min
Delta R.T.: -0.044 min
Response: 3900677
Conc: 1.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

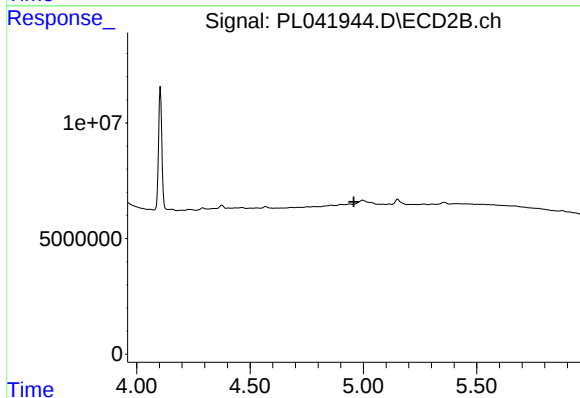


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

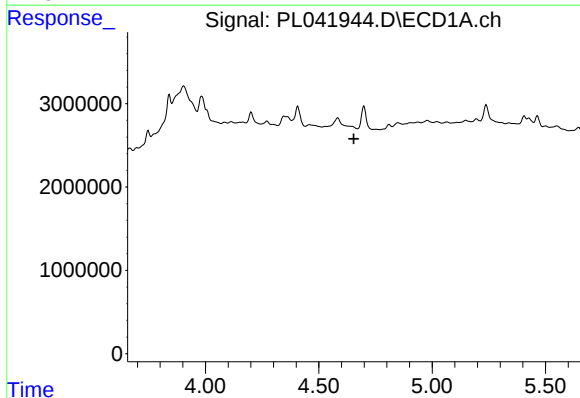


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.654 min
Response: 0
Conc: N.D.

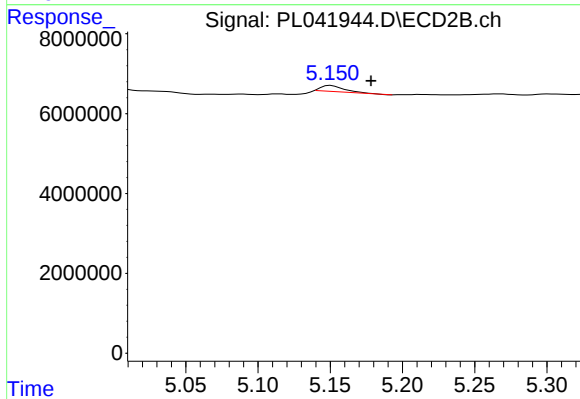

#7 delta-BHC


R.T.: 5.151 min
Delta R.T.: -0.028 min
Response: 1701508
Conc: 0.42 ng/ml

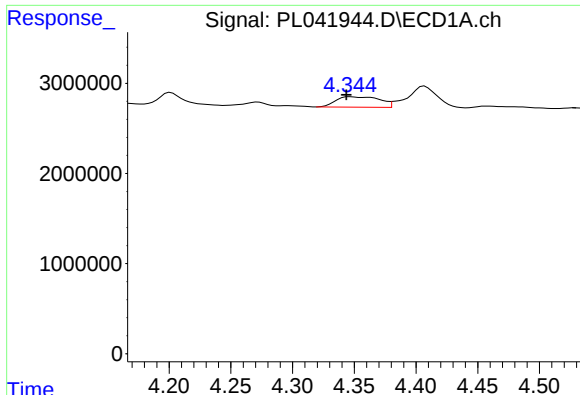

#23 Chlordane-1


R.T.: 4.346 min
Delta R.T.: 0.003 min
Response: 2848800
Conc: 10.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

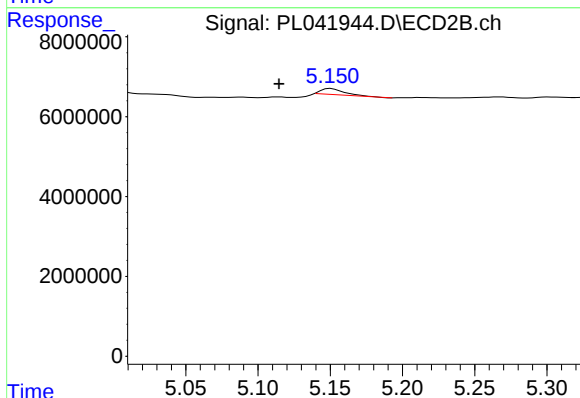


#23 Chlordane-1

R.T.: 5.151 min
Delta R.T.: 0.036 min
Response: 1701508
Conc: 12.25 ng/ml

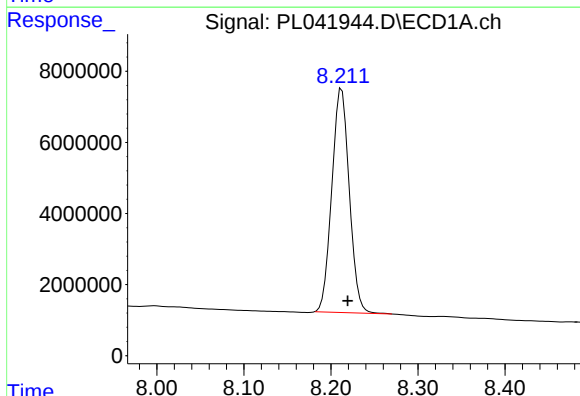

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: -0.007 min
Response: 87874571
Conc: 13.27 ng/ml

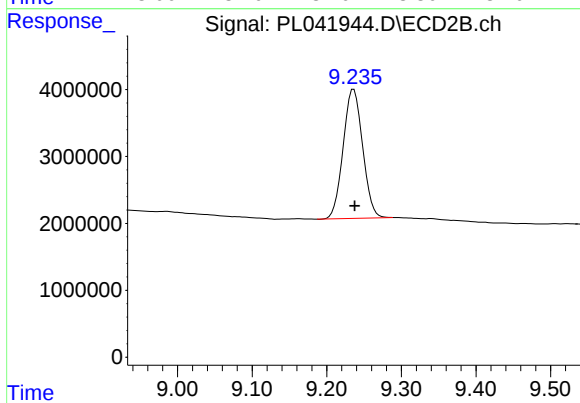

#28 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: -0.002 min
Response: 35003431
Conc: 13.66 ng/ml