

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110719\
 Data File : PL054060.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2019 12:47
 Operator : SG\AJ
 Sample : K5668-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-01-110619

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 00:16:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	4.043	140.7E6	32373951	12.978	12.937
28)	SA Decachlor...	8.325	9.121	105.9E6	31666352	10.789	11.245
Target Compounds							
2)	A alpha-BHC	0.000	4.460f	0	1146752	N.D.	0.332 #
10)	B gamma-Chl...	0.000	6.159	0	2793500	N.D.	0.957 #
11)	B alpha-Chl...	0.000	6.229	0	8408691	N.D.	2.880 #
12)	B 4,4'-DDE	5.723	6.381	4516746	6870531	0.380	2.440 #
17)	MA 4,4'-DDT	0.000	7.171	0	1011977	N.D.	0.438 #
23)	Chlordane-1	4.423	5.040	6199842	835252	17.481	9.959 #
25)	Chlordane-3	0.000	6.159	0	2793500	N.D.	7.649 #
26)	Chlordane-4	0.000	6.229	0	8408691	N.D.	18.730 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110719\
Data File : PL054060.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2019 12:47
Operator : SG\AJ
Sample : K5668-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HD-01-110619

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 00:16:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

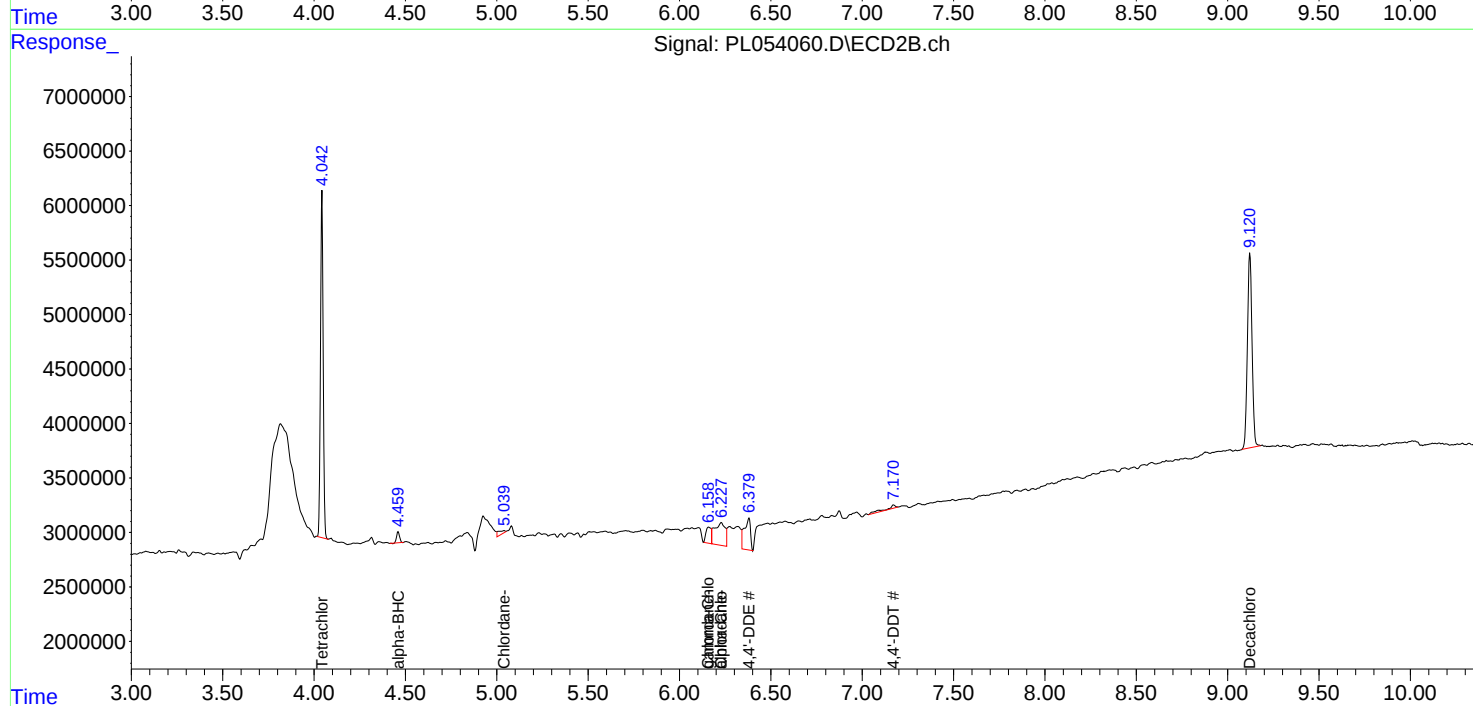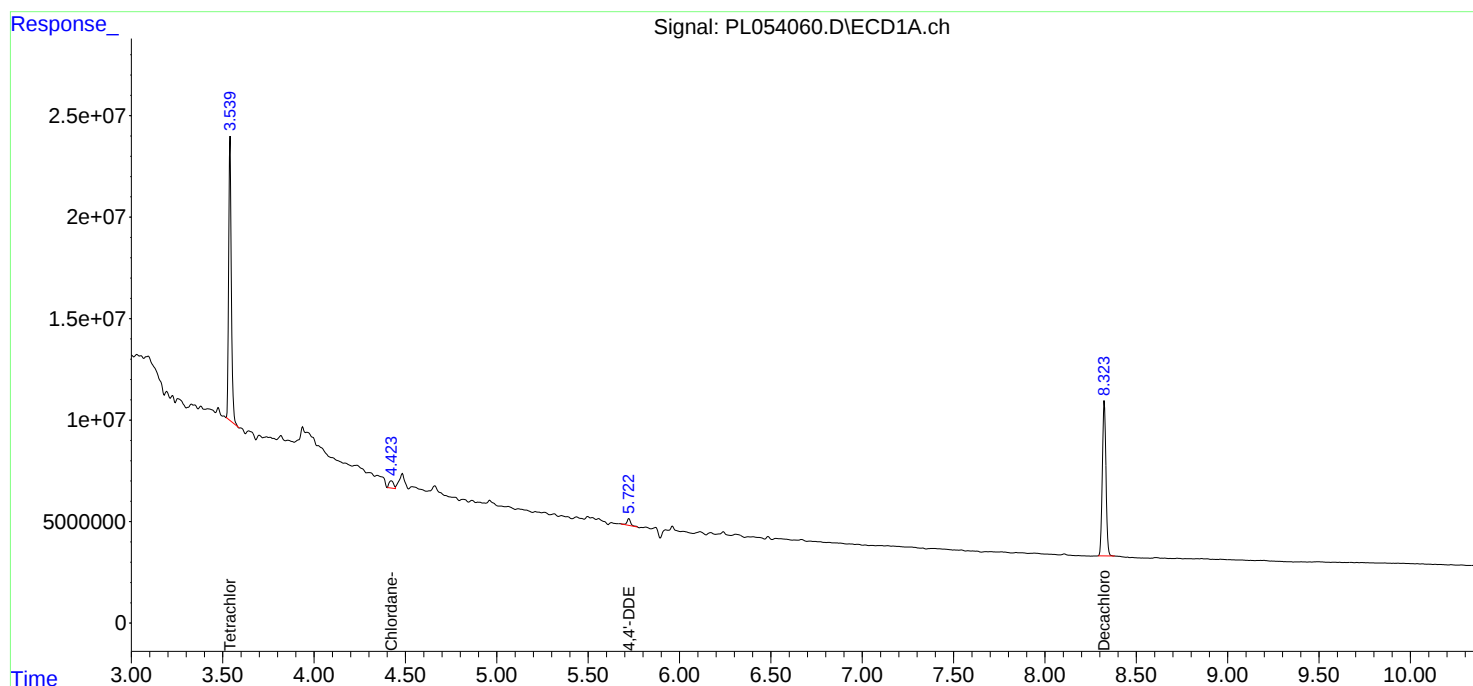


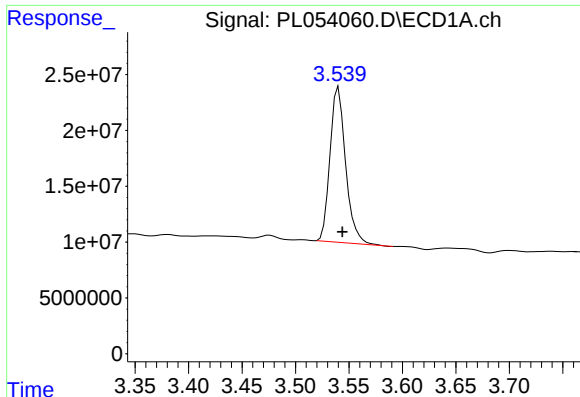

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 140675321
Conc: 12.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-110619

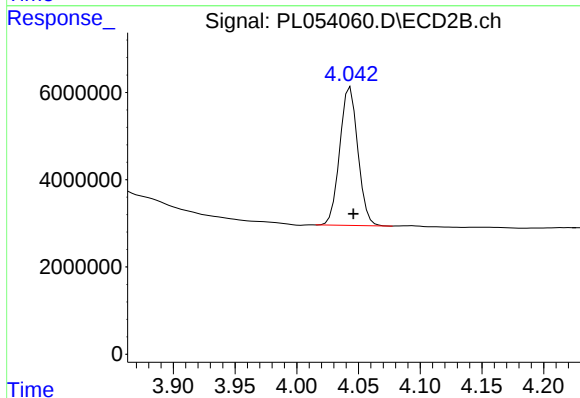


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.002 min
Response: 32373951
Conc: 12.94 ng/ml

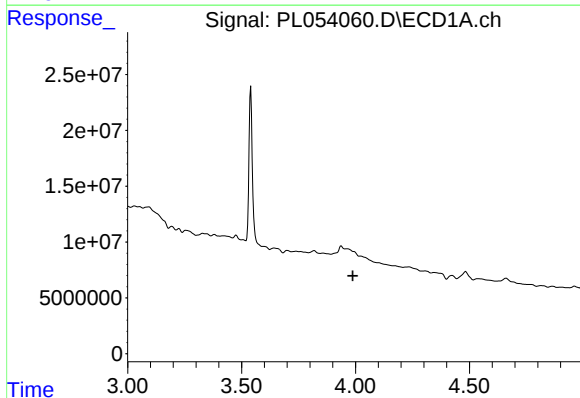


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.988 min
Response: 0
Conc: N.D.

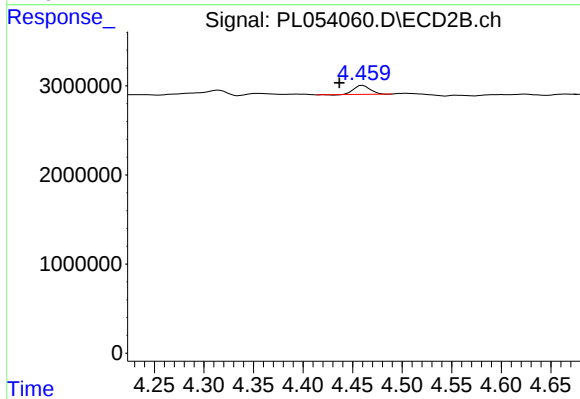

#2 alpha-BHC


R.T.: 4.460 min
Delta R.T.: 0.023 min
Response: 1146752
Conc: 0.33 ng/ml

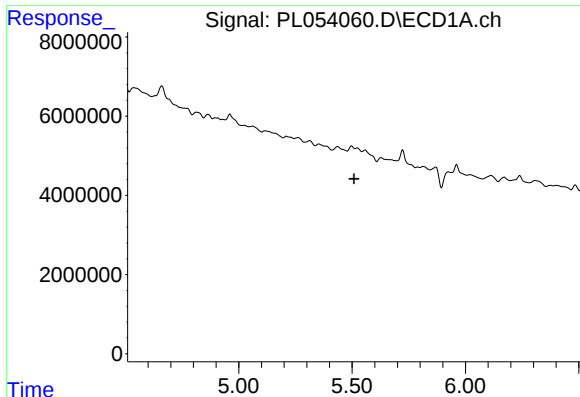

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HD-01-110619

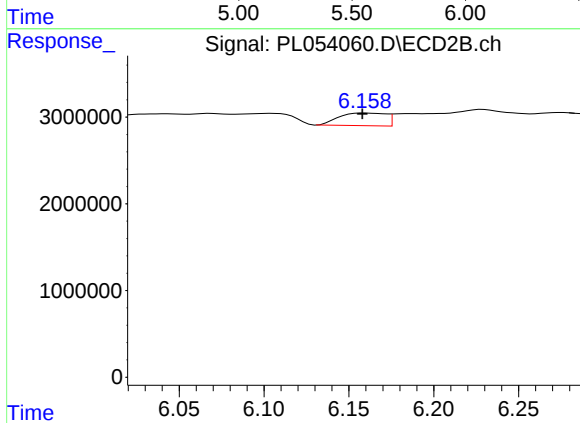


#10 gamma-Chlordane

R.T.: 6.159 min
Delta R.T.: 0.001 min
Response: 2793500
Conc: 0.96 ng/ml

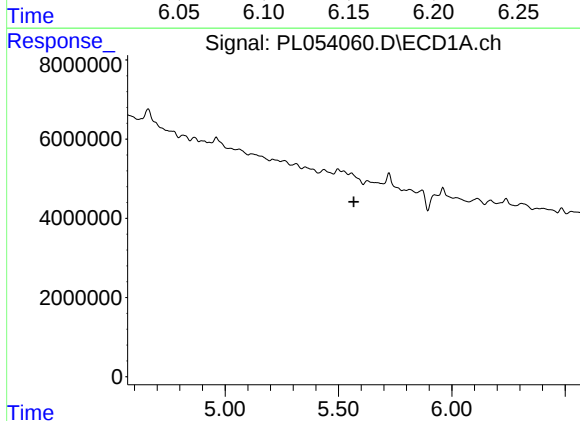


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.568 min
Response: 0
Conc: N.D.

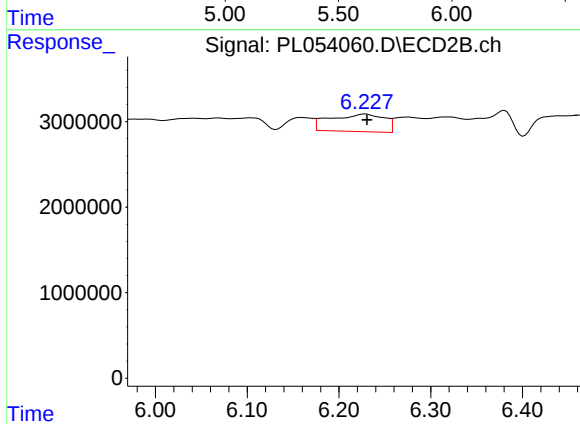

#11 alpha-Chlordane


R.T.: 6.229 min
Delta R.T.: -0.002 min
Response: 8408691
Conc: 2.88 ng/ml

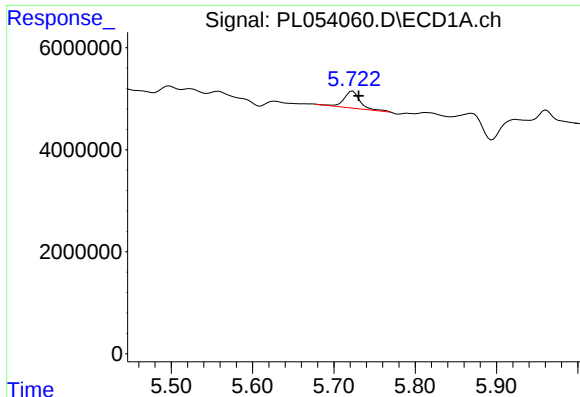

#12 4,4'-DDE


R.T.: 5.723 min
Delta R.T.: -0.008 min
Response: 4516746
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-110619

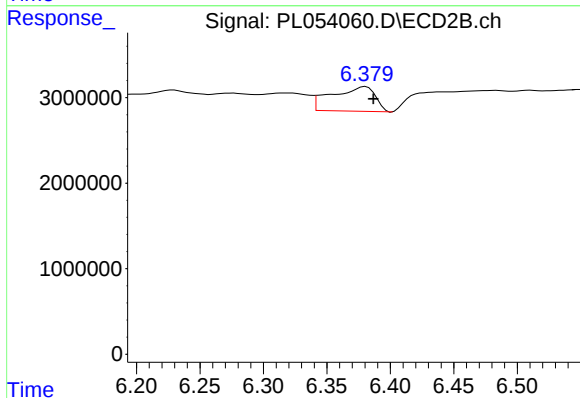


#12 4,4'-DDE

R.T.: 6.381 min
Delta R.T.: -0.006 min
Response: 6870531
Conc: 2.44 ng/ml

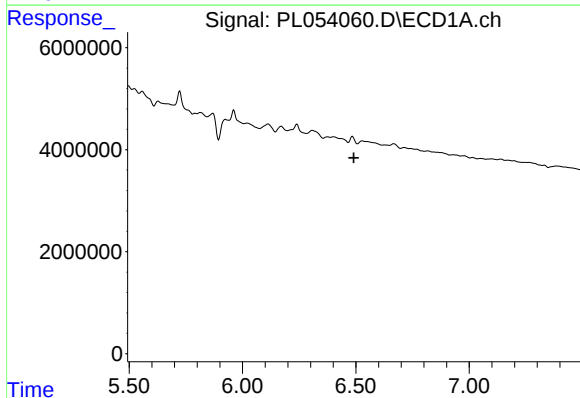


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.491 min
Response: 0
Conc: N.D.

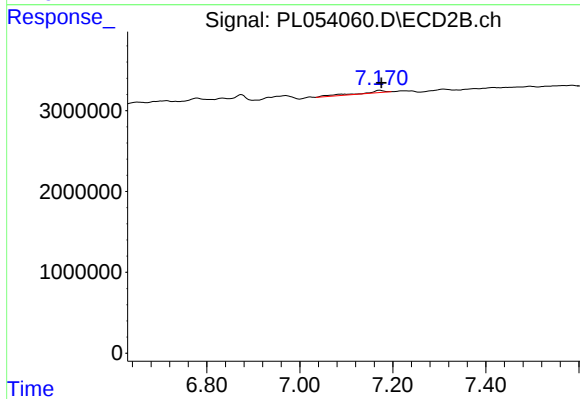

#17 4,4'-DDT


R.T.: 7.171 min
Delta R.T.: -0.004 min
Response: 1011977
Conc: 0.44 ng/ml

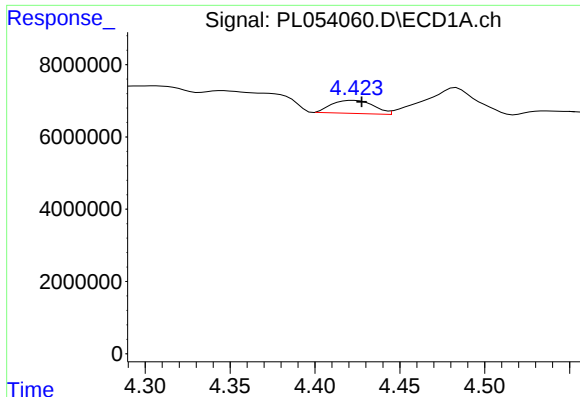

#23 Chlordane-1


R.T.: 4.423 min
Delta R.T.: -0.005 min
Response: 6199842
Conc: 17.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-110619

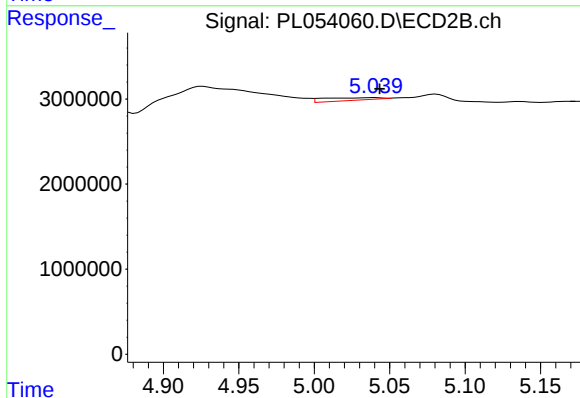


#23 Chlordane-1

R.T.: 5.040 min
Delta R.T.: -0.003 min
Response: 835252
Conc: 9.96 ng/ml

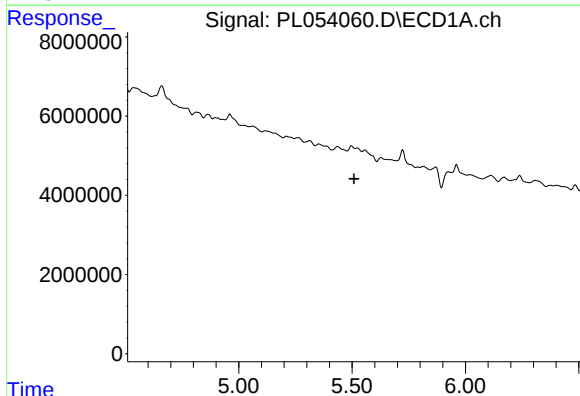


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.509 min
Response: 0
Conc: N.D.

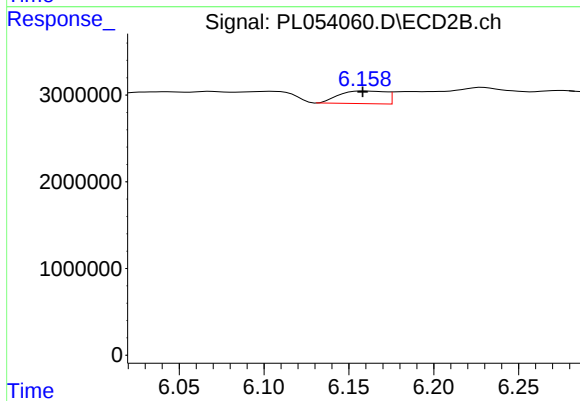

#25 Chlordane-3


R.T.: 6.159 min
Delta R.T.: 0.001 min
Response: 2793500
Conc: 7.65 ng/ml

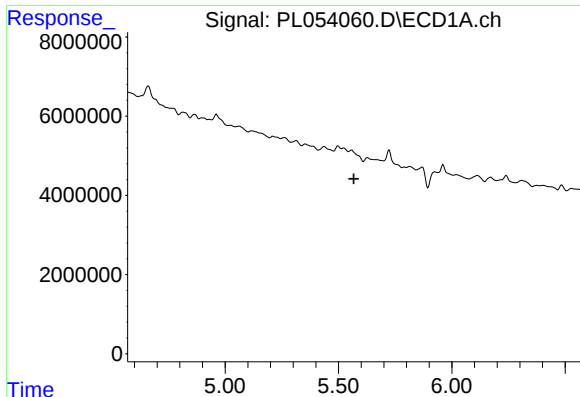

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.568 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HD-01-110619

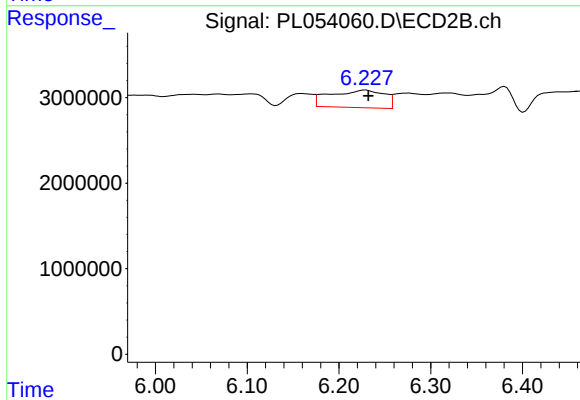


#26 Chlordane-4

R.T.: 6.229 min
Delta R.T.: -0.003 min
Response: 8408691
Conc: 18.73 ng/ml

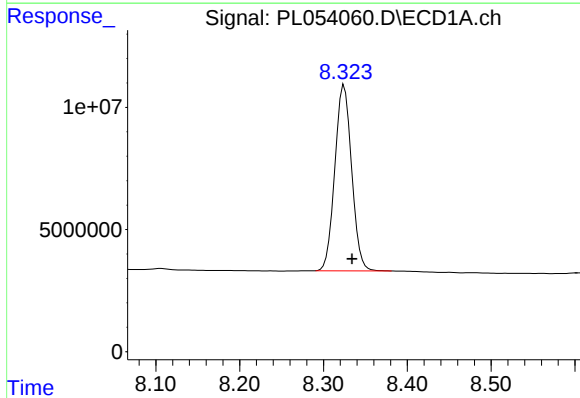

#28 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.009 min
Response: 105857698
Conc: 10.79 ng/ml

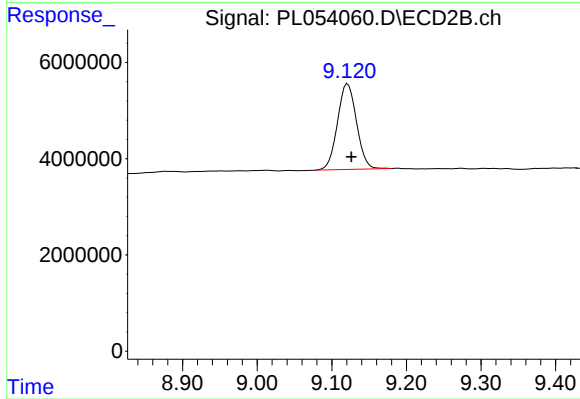

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.005 min
Response: 31666352
Conc: 11.25 ng/ml