

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110719\
 Data File : PL054061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2019 13:01
 Operator : SG\AJ
 Sample : K5710-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP- 31-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 00:17:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	4.043	137.1E6	33251736	12.653	13.288
28)	SA Decachlor...	8.325	9.122	111.4E6	32053784	11.352	11.383
Target Compounds							
17)	MA 4,4'-DDT	0.000	7.147f	0	2879855	N.D.	1.245 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110719\
Data File : PL054061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2019 13:01
Operator : SG\AJ
Sample : K5710-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP- 31-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 00:17:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

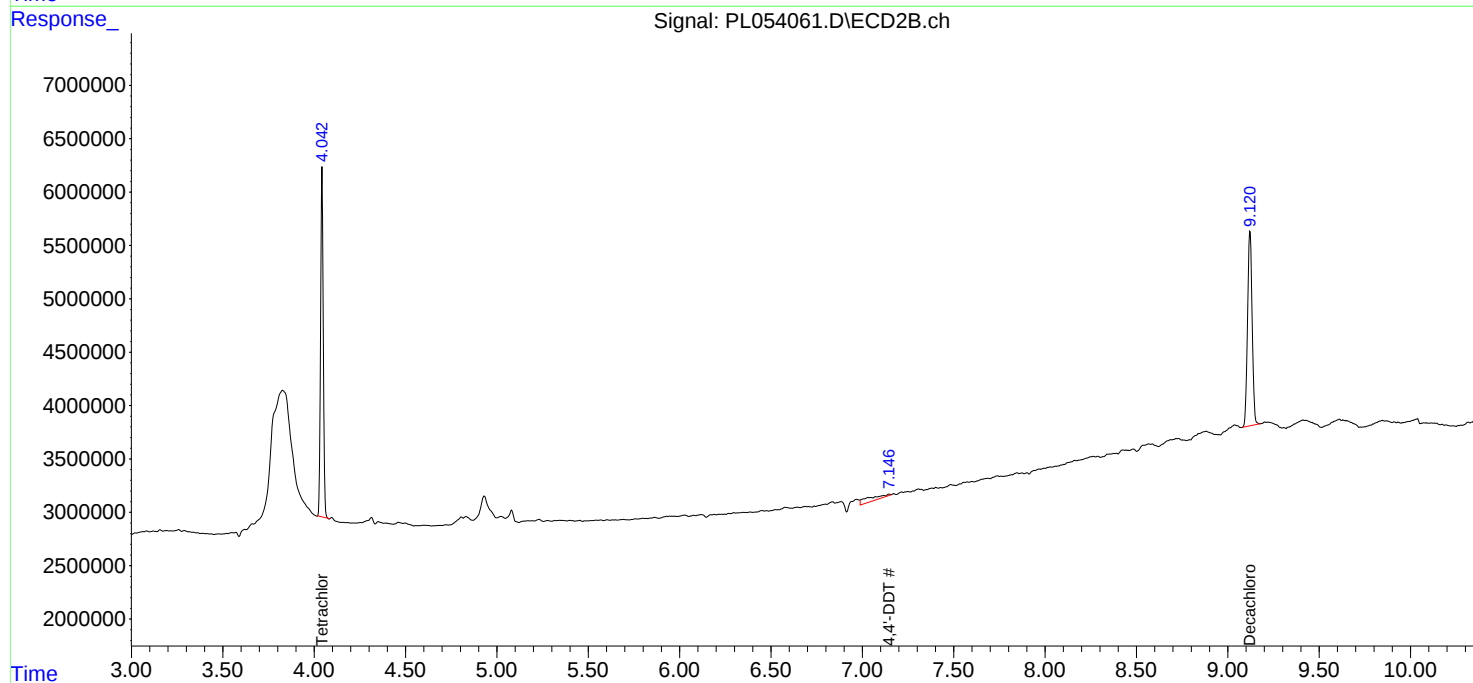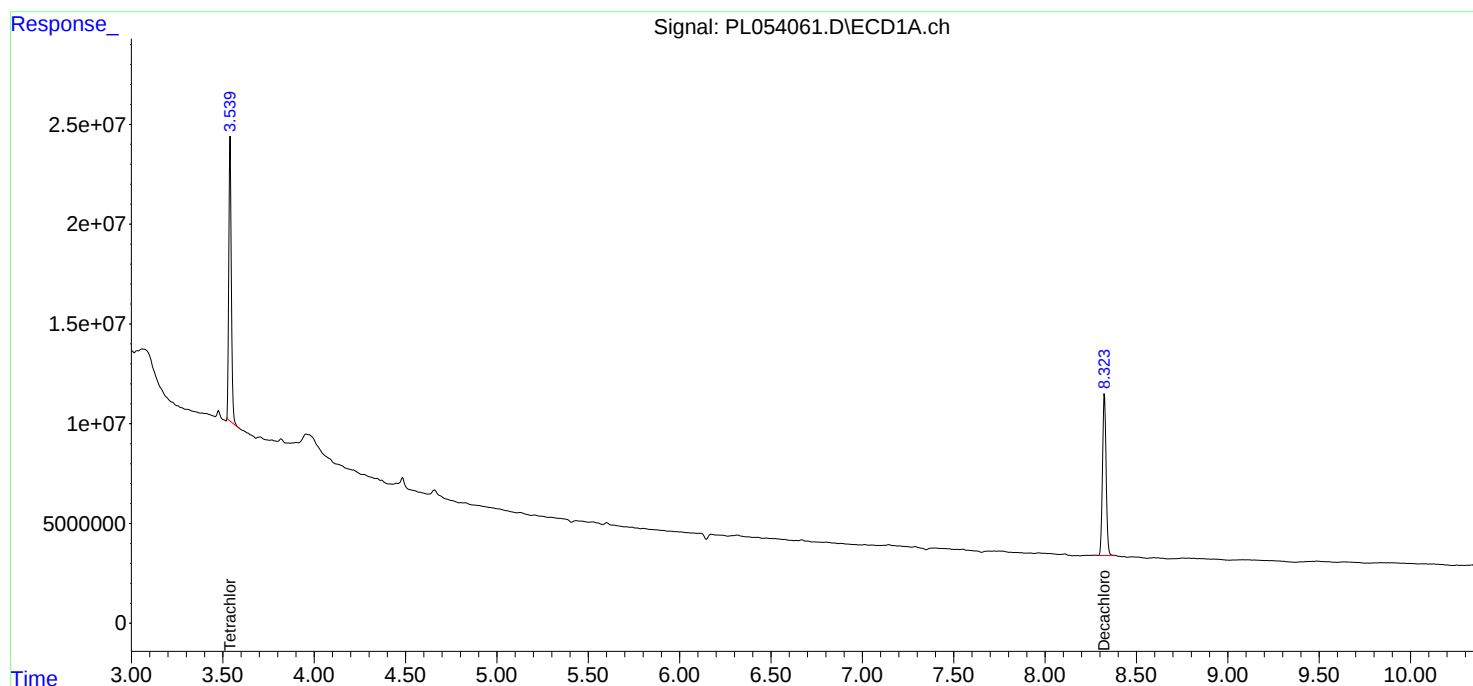


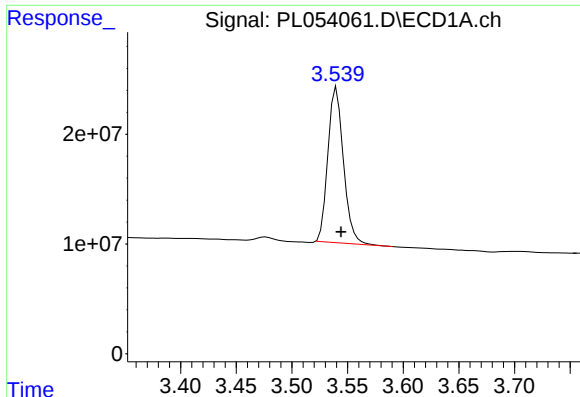

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 137146723
Conc: 12.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP- 31-S

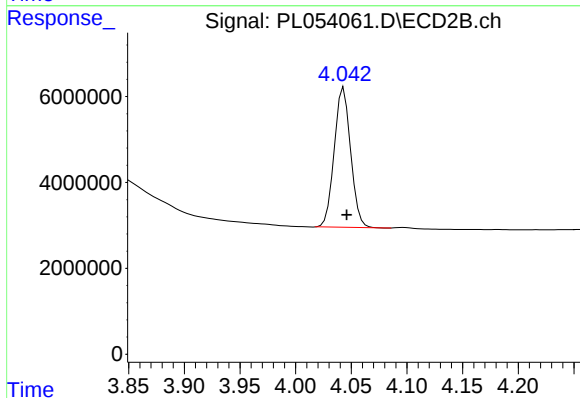


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.003 min
Response: 33251736
Conc: 13.29 ng/ml

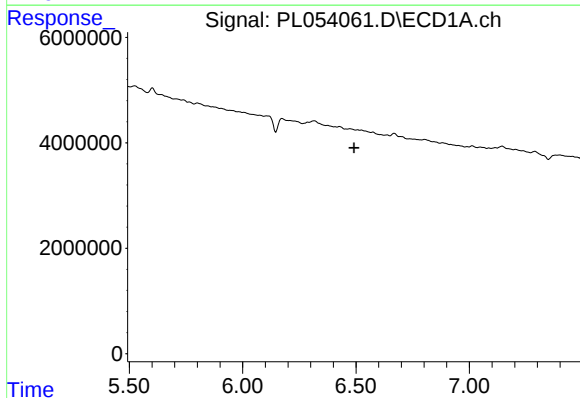


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.491 min
Response: 0
Conc: N.D.

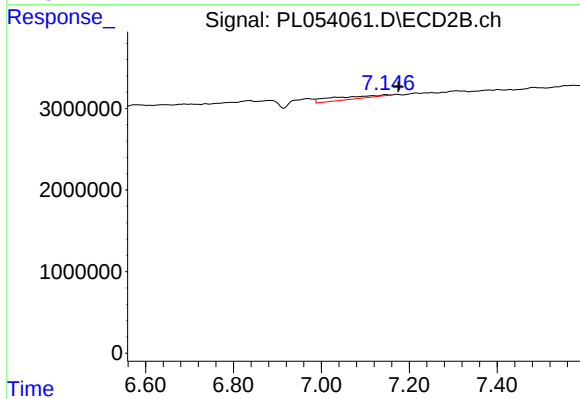

#17 4,4'-DDT


R.T.: 7.147 min
Delta R.T.: -0.029 min
Response: 2879855
Conc: 1.25 ng/ml

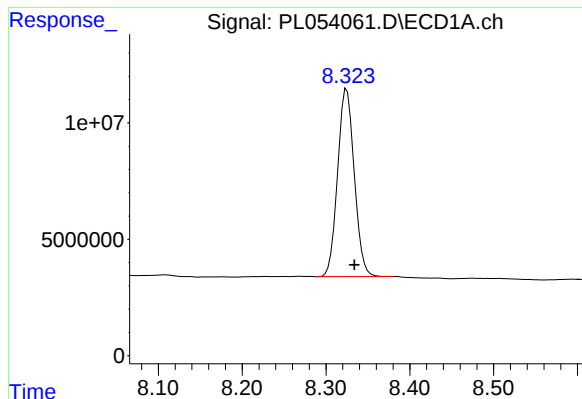

#28 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.009 min
Response: 111383060
Conc: 11.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP- 31-S

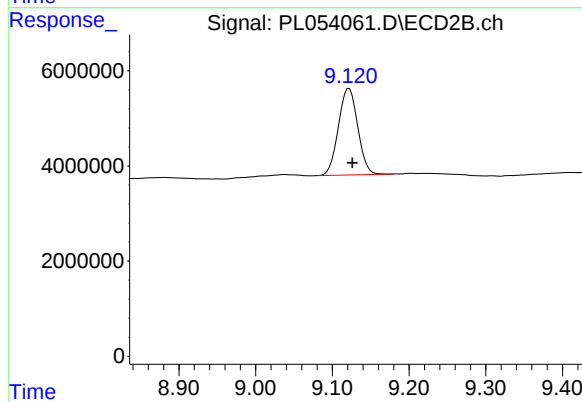

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.004 min
Response: 32053784
Conc: 11.38 ng/ml