

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110719\
 Data File : PL054088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2019 19:19
 Operator : SG\AJ
 Sample : K5671-05
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-110519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 00:22:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	4.044	213.7E6	52489449	19.717	20.976
28)	SA Decachlor...	8.325	9.122	166.9E6	50657905	17.009	17.989
Target Compounds							
7)	B delta-BHC	0.000	5.080f	0	2238823	N.D.	0.741 #
8)	B Heptachlo...	0.000	5.901f	0	4051074	N.D.	1.389 #
10)	B gamma-Chl...	5.480f	0.000	9769061	0	0.716	N.D. #
15)	B Endosulfa...	0.000	6.967	0	7584921	N.D.	2.969 #
16)	A 4,4'-DDD	6.241	0.000	6469321	0	0.727	N.D. #
23)	Chlordane-1	4.453f	0.000	11153731	0	31.448	N.D. #
25)	Chlordane-3	5.480f	0.000	9769061	0	8.475	N.D. #
27)	Chlordane-5	0.000	7.049	0	4714248	N.D.	61.666 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110719\
Data File : PL054088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2019 19:19
Operator : SG\AJ
Sample : K5671-05
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-02-110519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 00:22:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

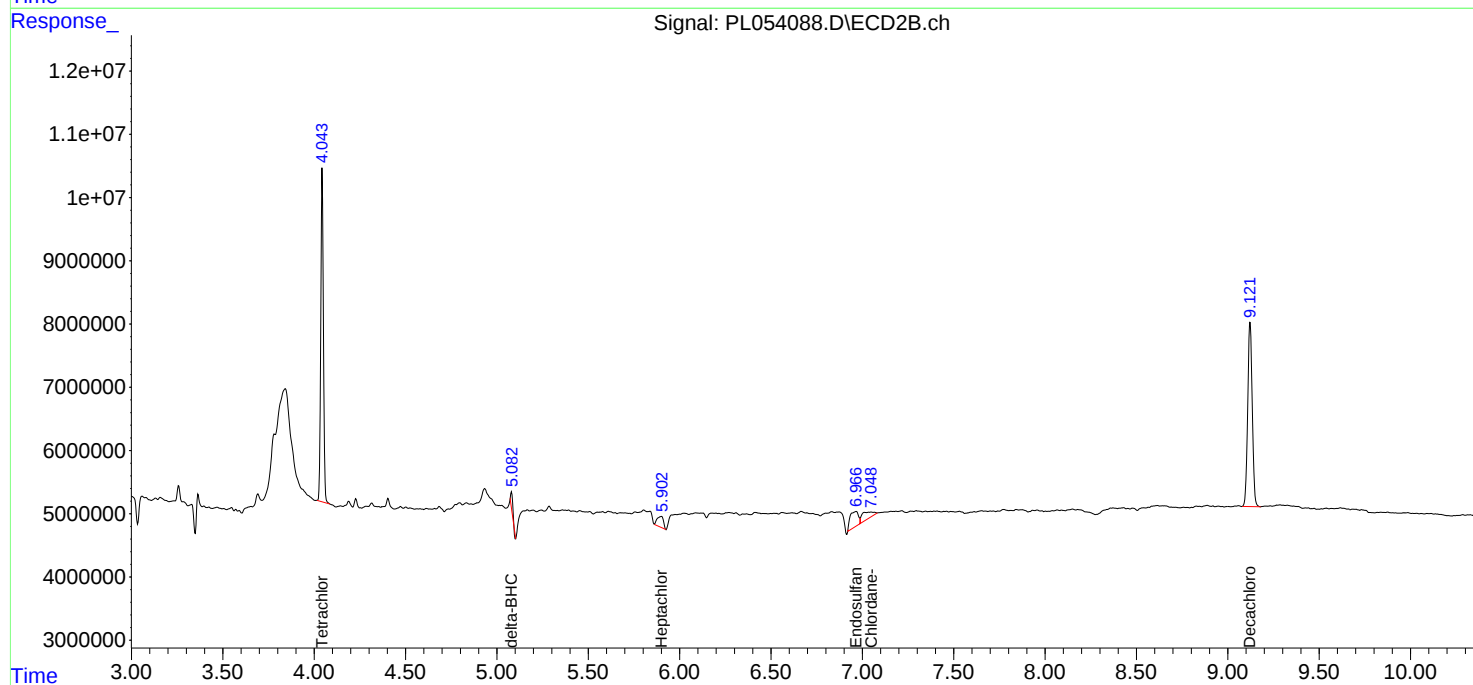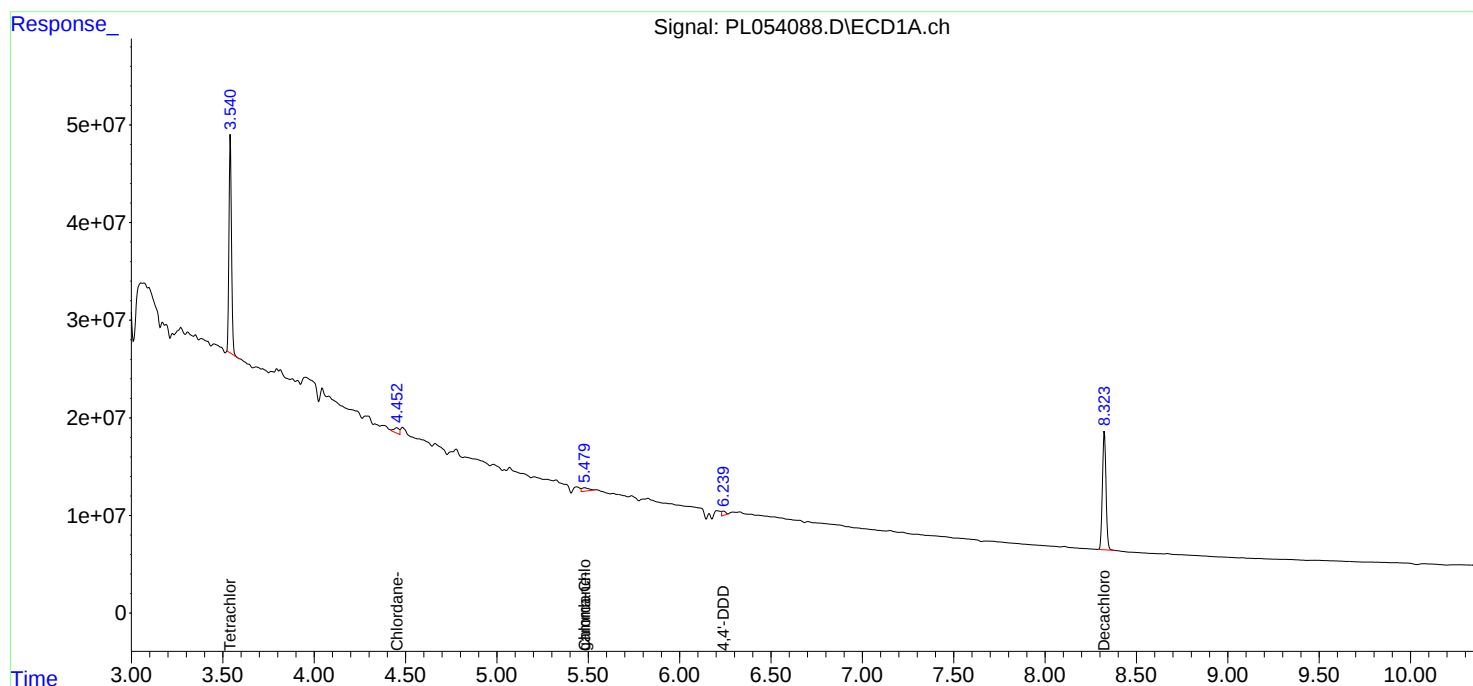


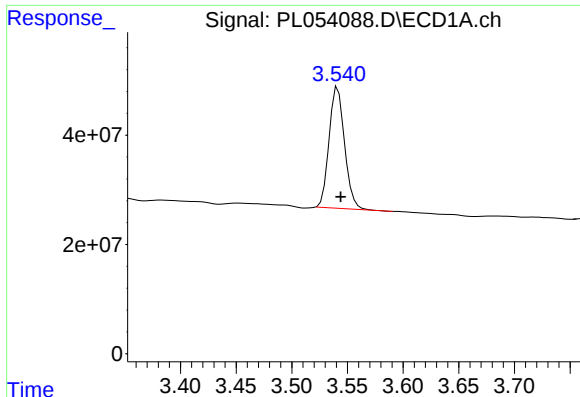

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: -0.003 min
Response: 213717769
Conc: 19.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-110519

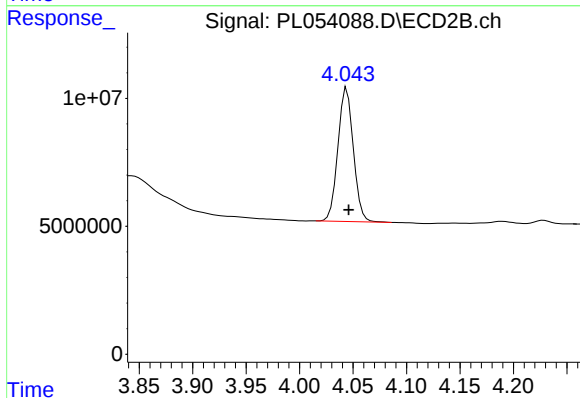


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 52489449
Conc: 20.98 ng/ml

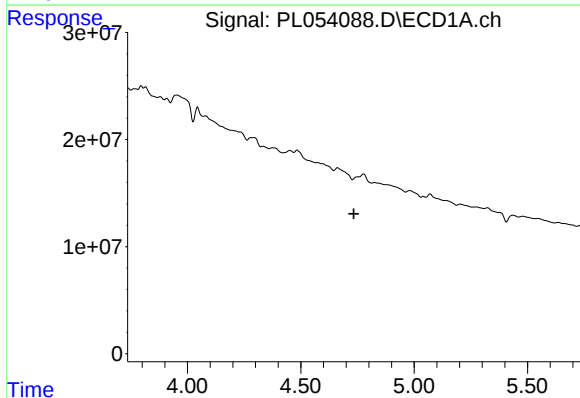


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

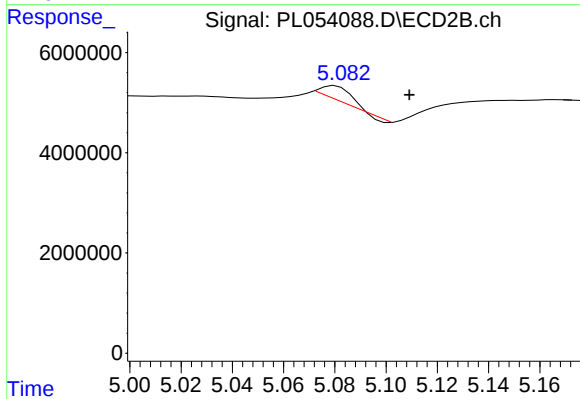

#7 delta-BHC


R.T.: 5.080 min
Delta R.T.: -0.029 min
Response: 2238823
Conc: 0.74 ng/ml

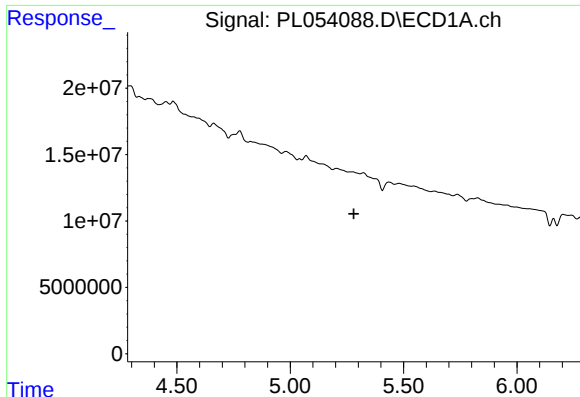

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.280 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-02-110519

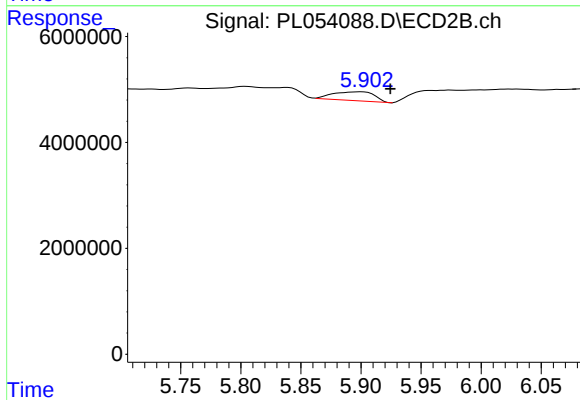


#8 Heptachlor epoxide

R.T.: 5.901 min
Delta R.T.: -0.024 min
Response: 4051074
Conc: 1.39 ng/ml

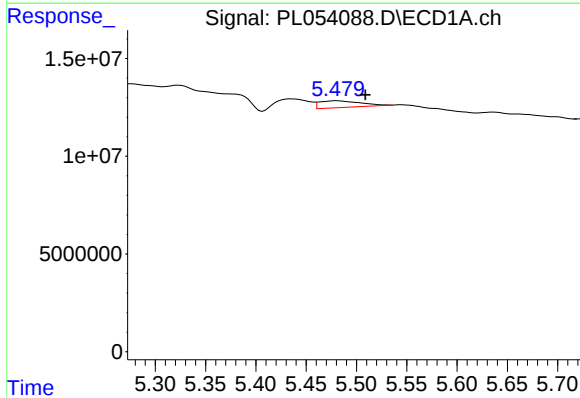


#10 gamma-Chlordane

R.T.: 5.480 min
Delta R.T.: -0.028 min
Response: 9769061
Conc: 0.72 ng/ml

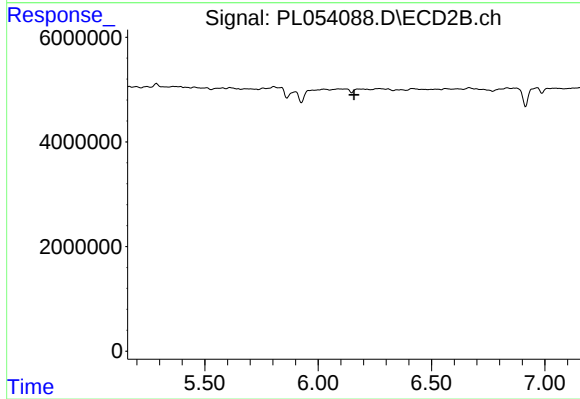

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

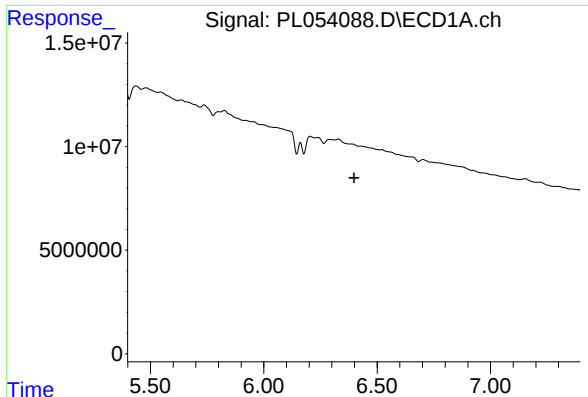

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.399 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-02-110519

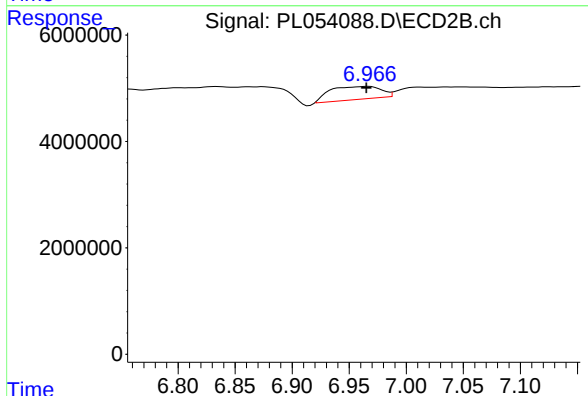


#15 Endosulfan II

R.T.: 6.967 min
Delta R.T.: 0.002 min
Response: 7584921
Conc: 2.97 ng/ml

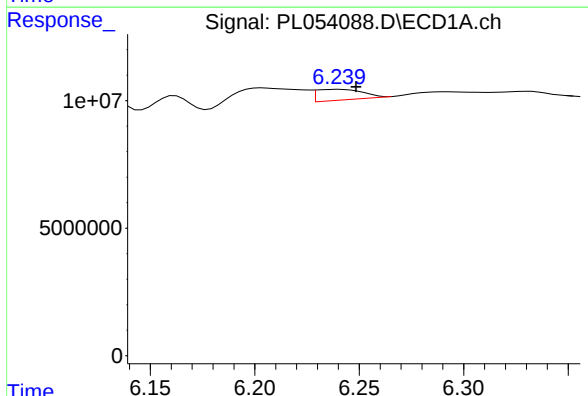


#16 4,4'-DDD

R.T.: 6.241 min
Delta R.T.: -0.008 min
Response: 6469321
Conc: 0.73 ng/ml

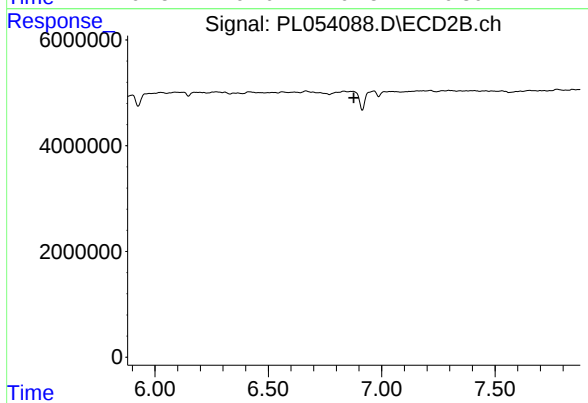

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.877 min
Response: 0
Conc: N.D.

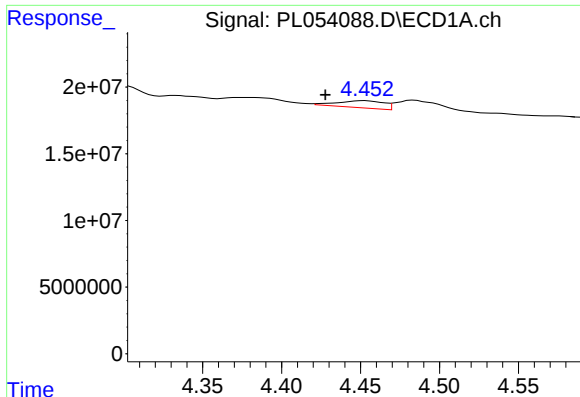

#23 Chlordane-1


R.T.: 4.453 min
Delta R.T.: 0.025 min
Response: 11153731
Conc: 31.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-110519

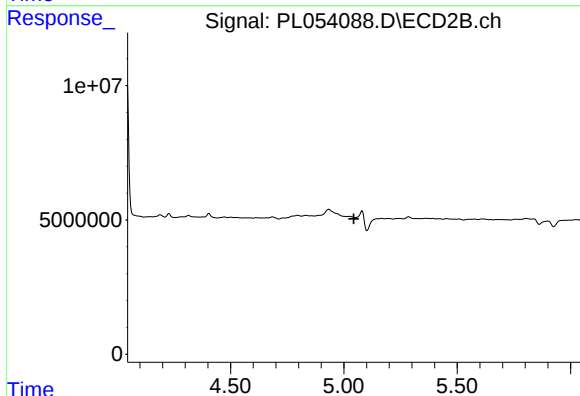


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.043 min
Response: 0
Conc: N.D.

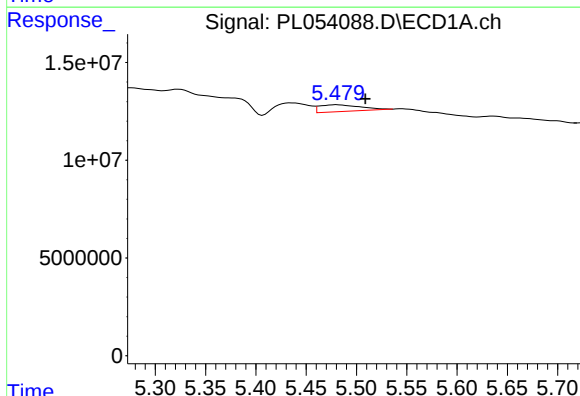


#25 Chlordane-3

R.T.: 5.480 min
Delta R.T.: -0.028 min
Response: 9769061
Conc: 8.48 ng/ml

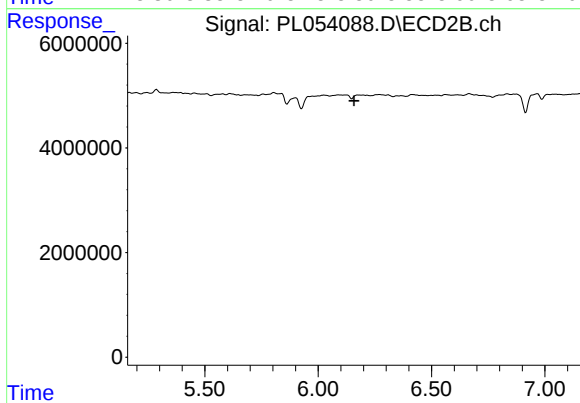

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

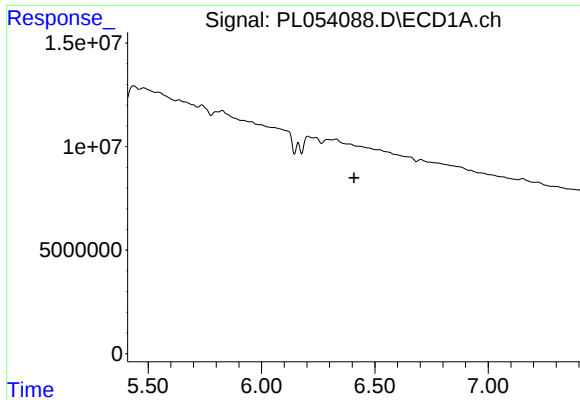

#27 Chlorodane-5


R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-02-110519

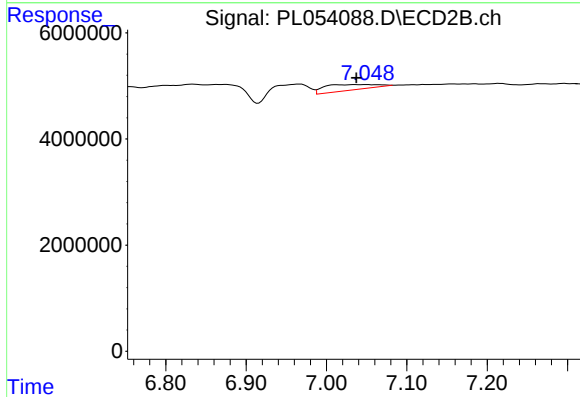


#27 Chlorodane-5

R.T.: 7.049 min
Delta R.T.: 0.012 min
Response: 4714248
Conc: 61.67 ng/ml

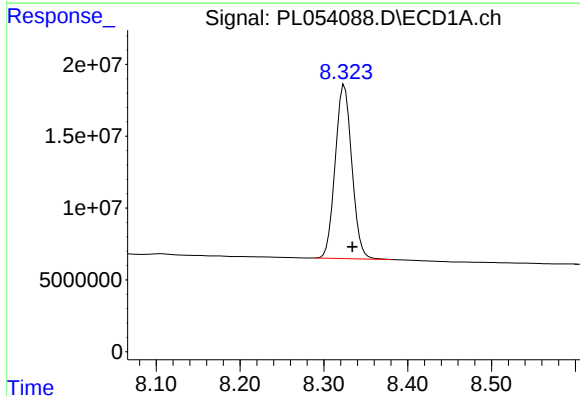

#28 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.009 min
Response: 166888542
Conc: 17.01 ng/ml

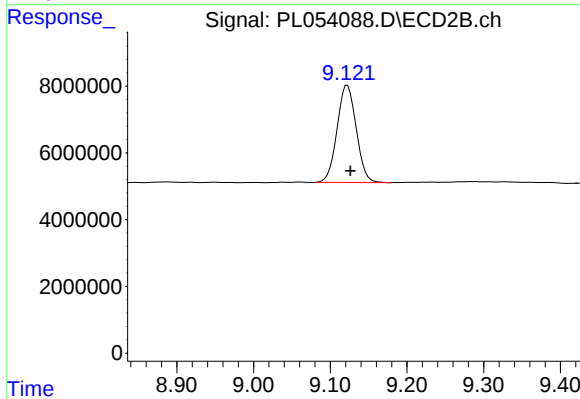

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.004 min
Response: 50657905
Conc: 17.99 ng/ml