

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110719\
 Data File : PL054070.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2019 15:07
 Operator : SG\AJ
 Sample : K5723-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 8-B

Manual Integrations
 APPROVED

Ankita
 11/8/2019 8:46:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 00:18:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	4.043	205.8E6	46791942	18.990	18.699
28) SA Decachlor...	8.323	9.121	164.4E6	51332272	16.756m	18.229m
Target Compounds						
12) B 4,4'-DDE	5.724	6.381	36508584	6345293	3.073	2.253m#
17) MA 4,4'-DDT	6.482	7.173	52631616	8133261	5.313	3.517 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110719\
Data File : PL054070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2019 15:07
Operator : SG\AJ
Sample : K5723-05
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
8-B


Manual Integrations
APPROVED

Ankita
11/8/2019 8:46:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 00:18:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

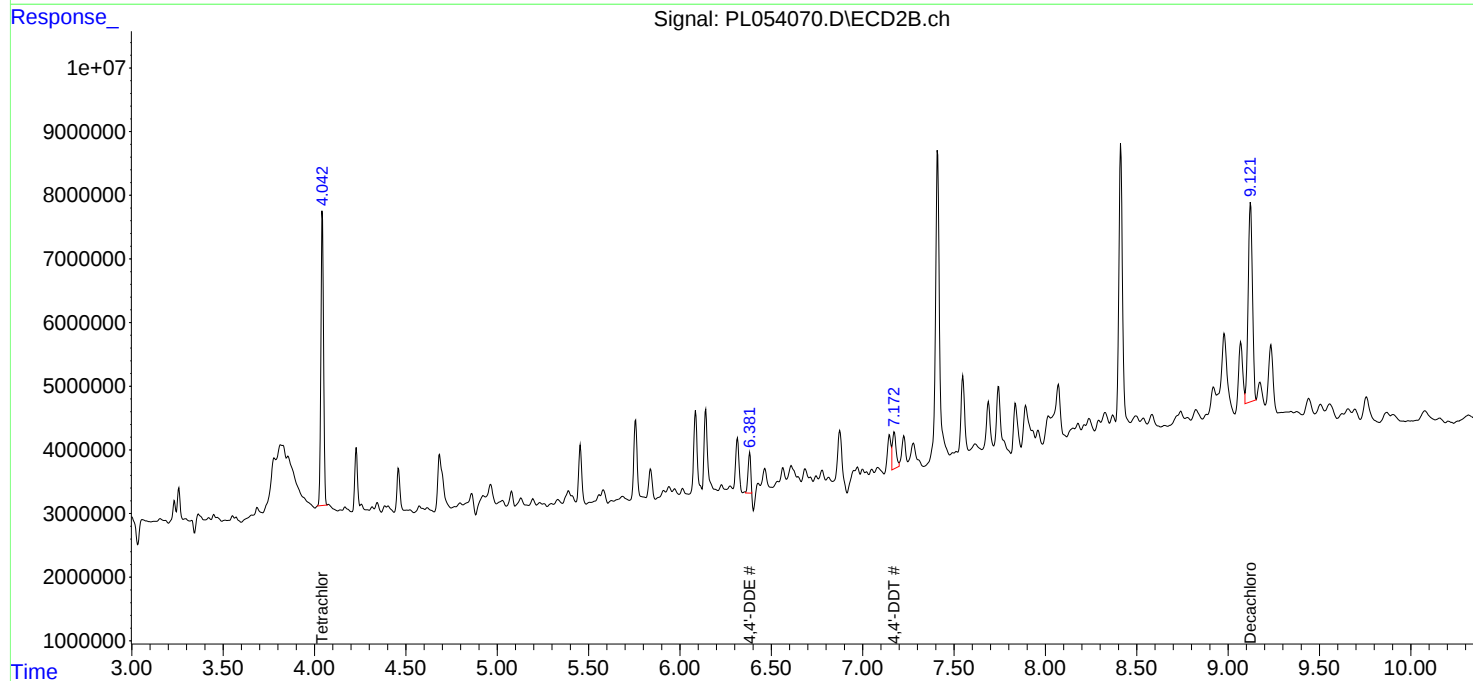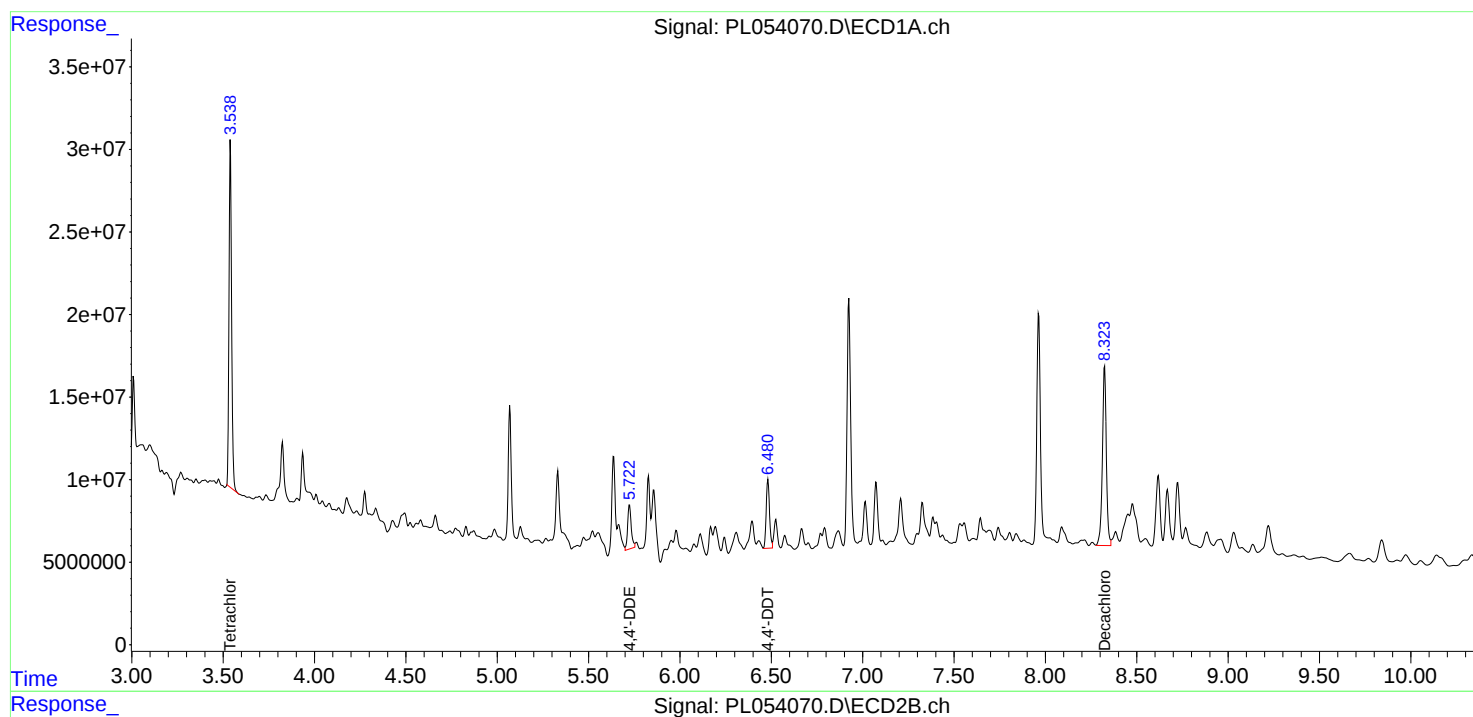

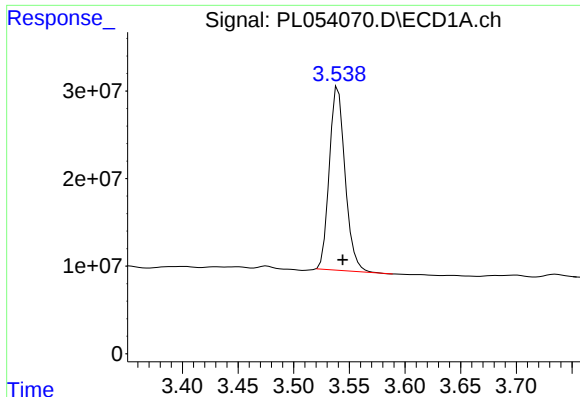


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 205834391
Conc: 18.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
8-B


Manual Integrations
APPROVED

Ankita
11/8/2019 8:46:51 AM

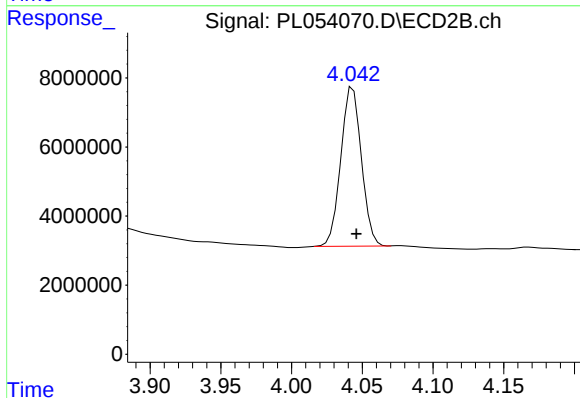


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.002 min
Response: 46791942
Conc: 18.70 ng/ml

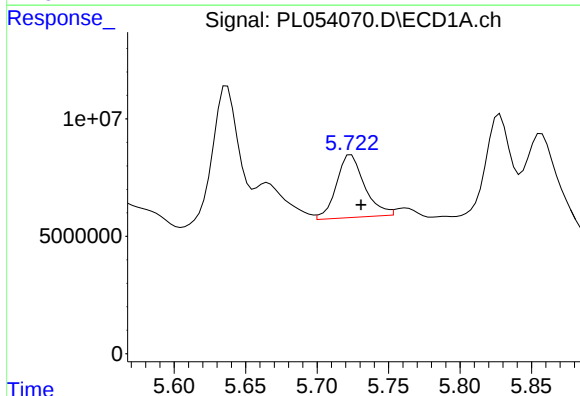


#12 4,4'-DDE

R.T.: 5.724 min
Delta R.T.: -0.007 min
Response: 36508584
Conc: 3.07 ng/ml

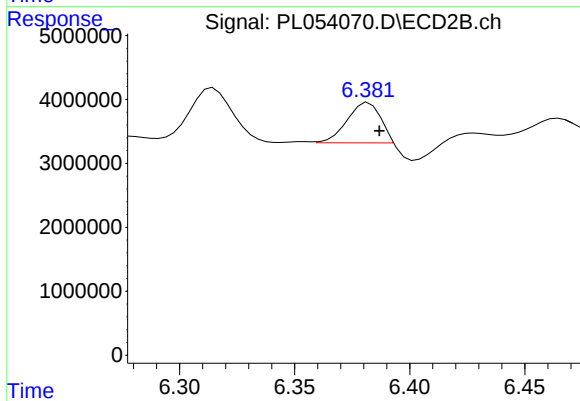

#12 4,4'-DDE

R.T.: 6.381 min
Delta R.T.: -0.006 min
Response: 6345293
Conc: 2.25 ng/ml m

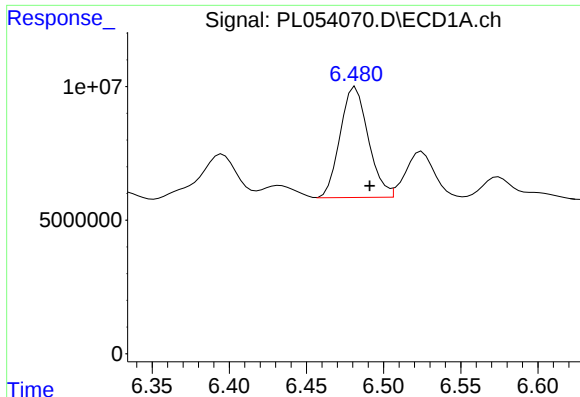


#17 4,4'-DDT

R.T.: 6.482 min
Delta R.T.: -0.009 min
Response: 52631616
Conc: 5.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
8-B


Manual Integrations
APPROVED

Ankita
11/8/2019 8:46:51 AM

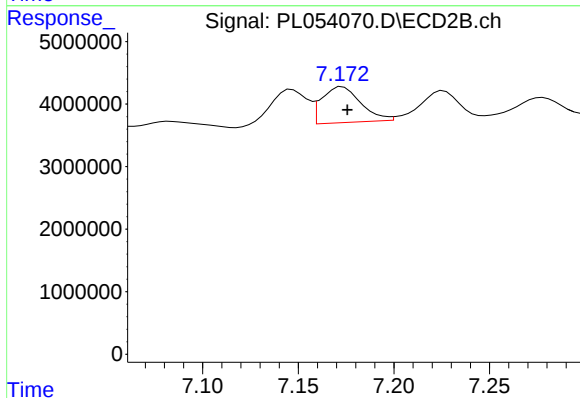


#17 4,4'-DDT

R.T.: 7.173 min
Delta R.T.: -0.003 min
Response: 8133261
Conc: 3.52 ng/ml

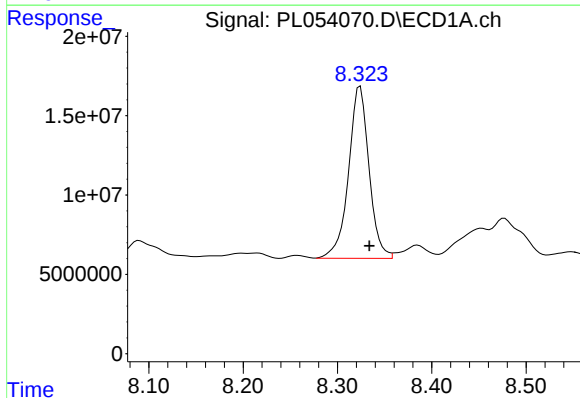

#28 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: -0.011 min
Response: 164406476
Conc: 16.76 ng/ml m

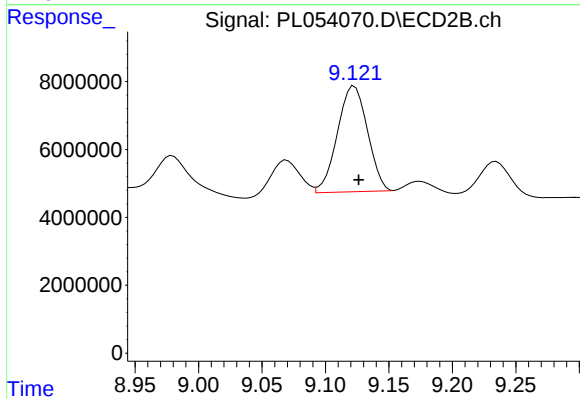

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.005 min
Response: 51332272
Conc: 18.23 ng/ml m