

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
 Data File : PL078858.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2022 15:17
 Operator : AR\AJ
 Sample : N5436-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 250FERRYBLVD-TFS-06

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/08/2022
 Supervised By :Ankita Jodhani 11/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 17:24:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	2.570	43706729	27451279	22.919	10.752 #
2)	SA Decachlor...	8.774	7.638	238.8E6	299.4E6	158.724	158.064
Target Compounds							
13)	MA Dieldrin	6.118	5.106	172.2E6	90274705	79.847	30.466m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
Data File : PL078858.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2022 15:17
Operator : AR\AJ
Sample : N5436-06
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-06


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/08/2022
Supervised By : Ankita Jodhani 11/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 17:24:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

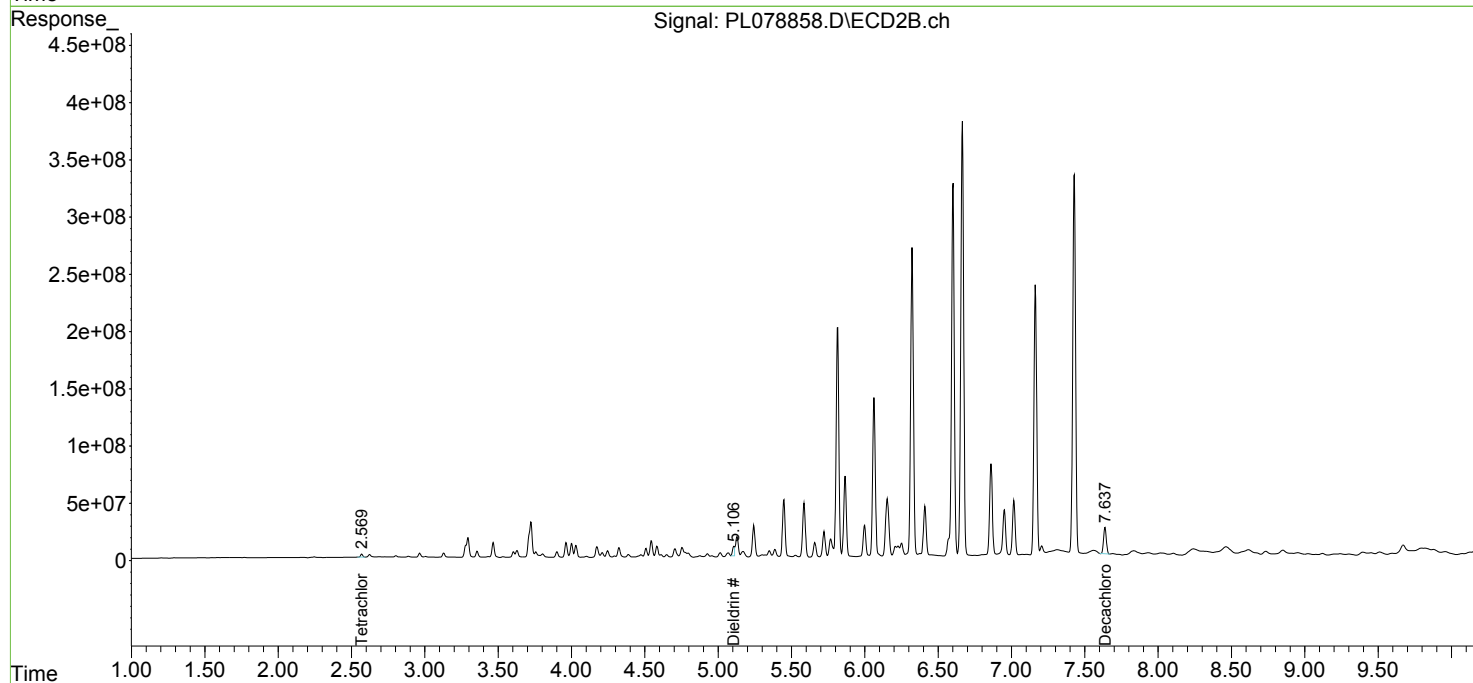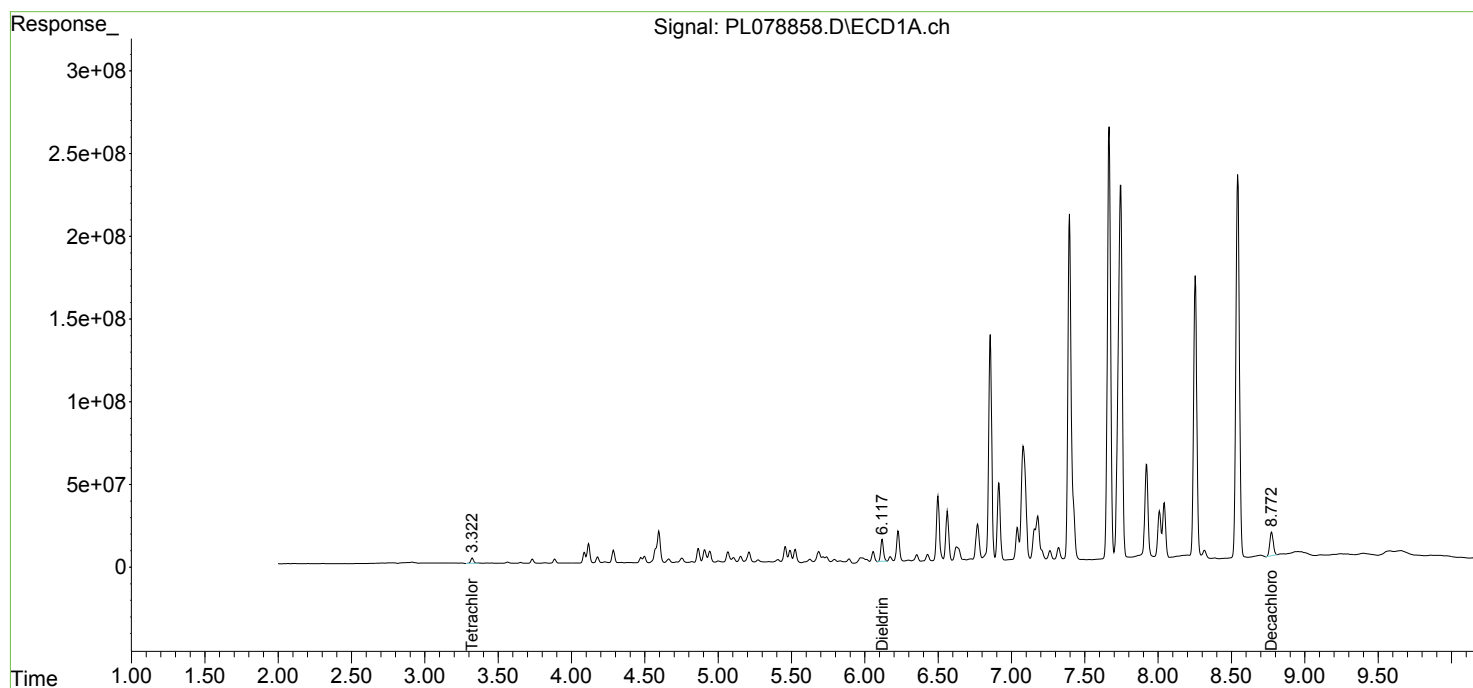

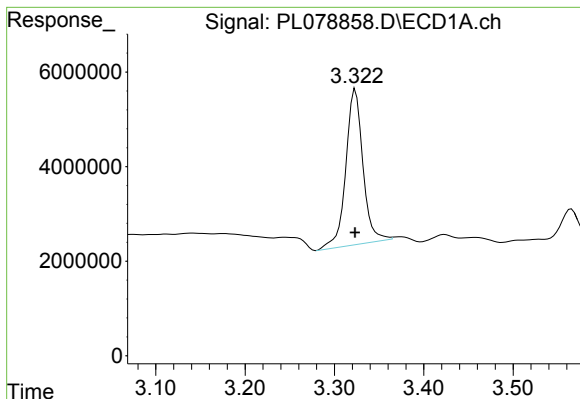


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 43706729
Conc: 22.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-06


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/08/2022
Supervised By :Ankita Jodhani 11/10/2022

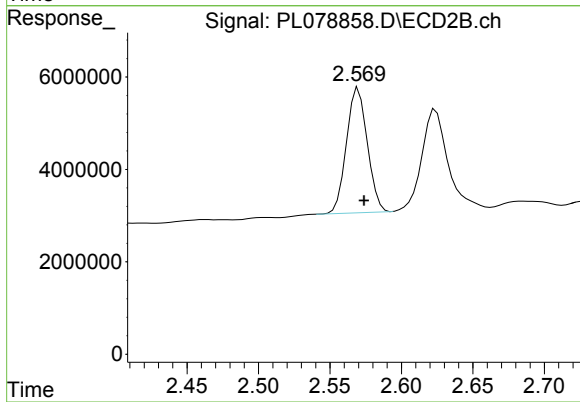


#1 Tetrachloro-m-xylene

R.T.: 2.570 min
Delta R.T.: -0.004 min
Response: 27451279
Conc: 10.75 ng/ml

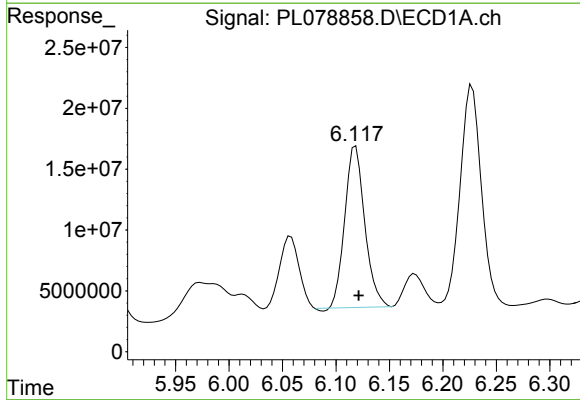


#13 Dieldrin

R.T.: 6.118 min
Delta R.T.: -0.003 min
Response: 172190474
Conc: 79.85 ng/ml

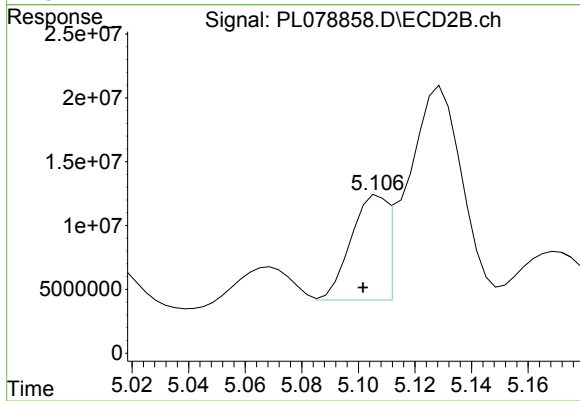

#13 Dieldrin

R.T.: 5.106 min
Delta R.T.: 0.004 min
Response: 90274705
Conc: 30.47 ng/ml m

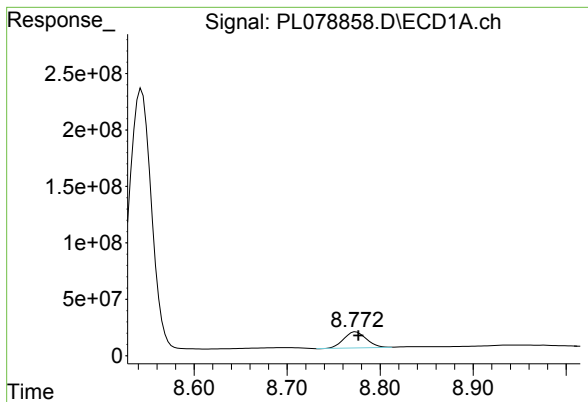

#28 Decachlorobiphenyl

R.T.: 8.774 min

Delta R.T.: -0.003 min


Response: 238777738

Conc: 158.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-06

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/08/2022
Supervised By :Ankita Jodhani 11/10/2022

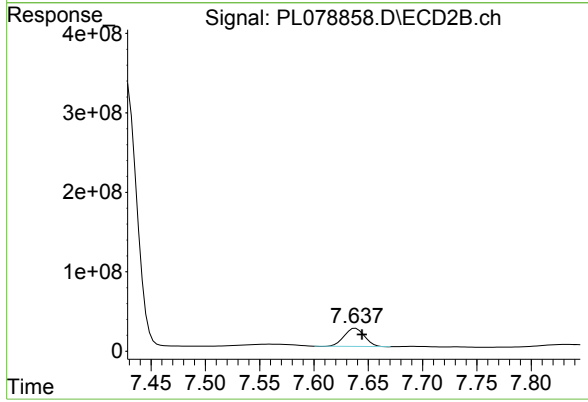

#28 Decachlorobiphenyl

R.T.: 7.638 min

Delta R.T.: -0.006 min

Response: 299389235

Conc: 158.06 ng/ml