

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
 Data File : PL078863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2022 16:45
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 02:10:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	2.565	96567373	148.8E6	50.638	58.265
28)	SA Decachlor...	8.780	7.637	61686760	88968883	41.005	46.972
Target Compounds							
23)	Chlordane-1	4.478	3.531	39829008	48967396	508.332	485.523
24)	Chlordane-2	5.010	4.098	39569335	53764489	478.215	505.180
25)	Chlordane-3	5.720	4.718	169.0E6	153.2E6	505.866	502.771
26)	Chlordane-4	5.798	4.778	204.7E6	163.4E6	498.605	499.938
27)	Chlordane-5	6.654	5.439	30573323	40411535	467.550	495.505



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
Data File : PL078863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2022 16:45
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 02:10:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

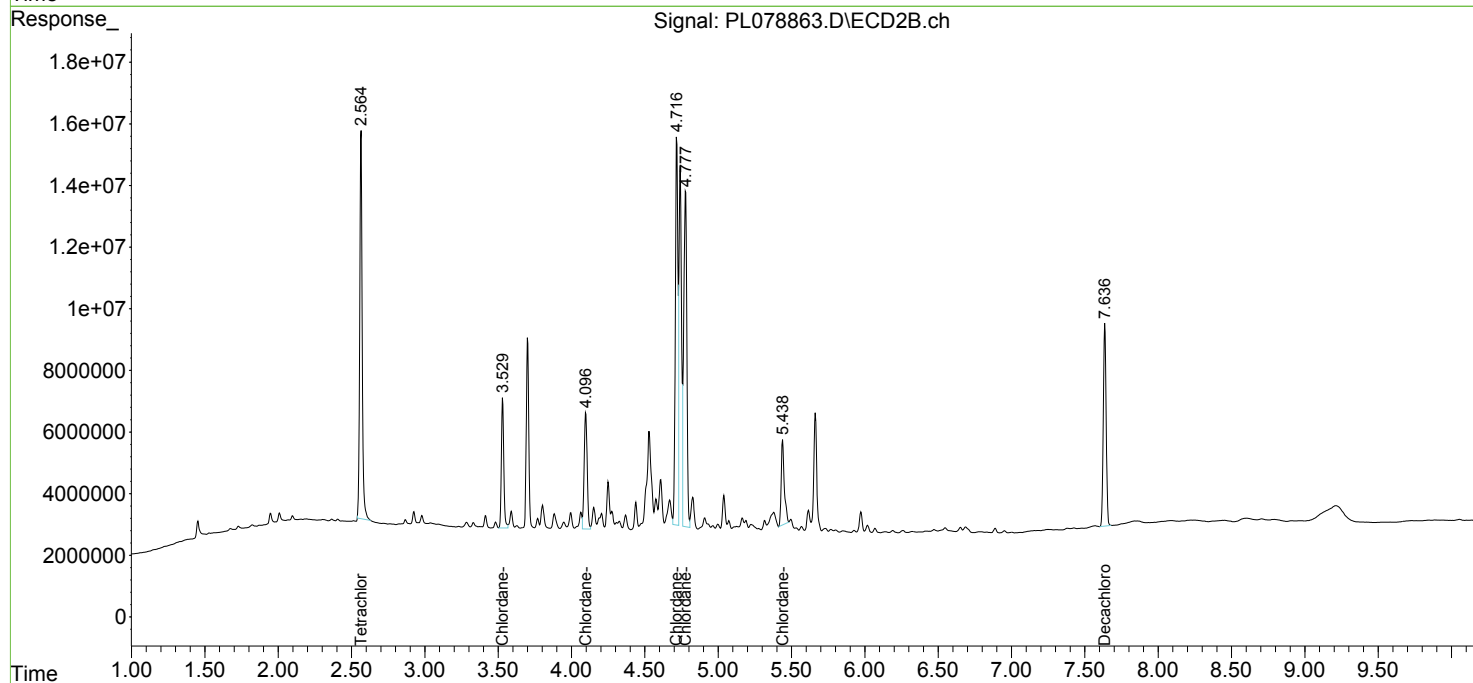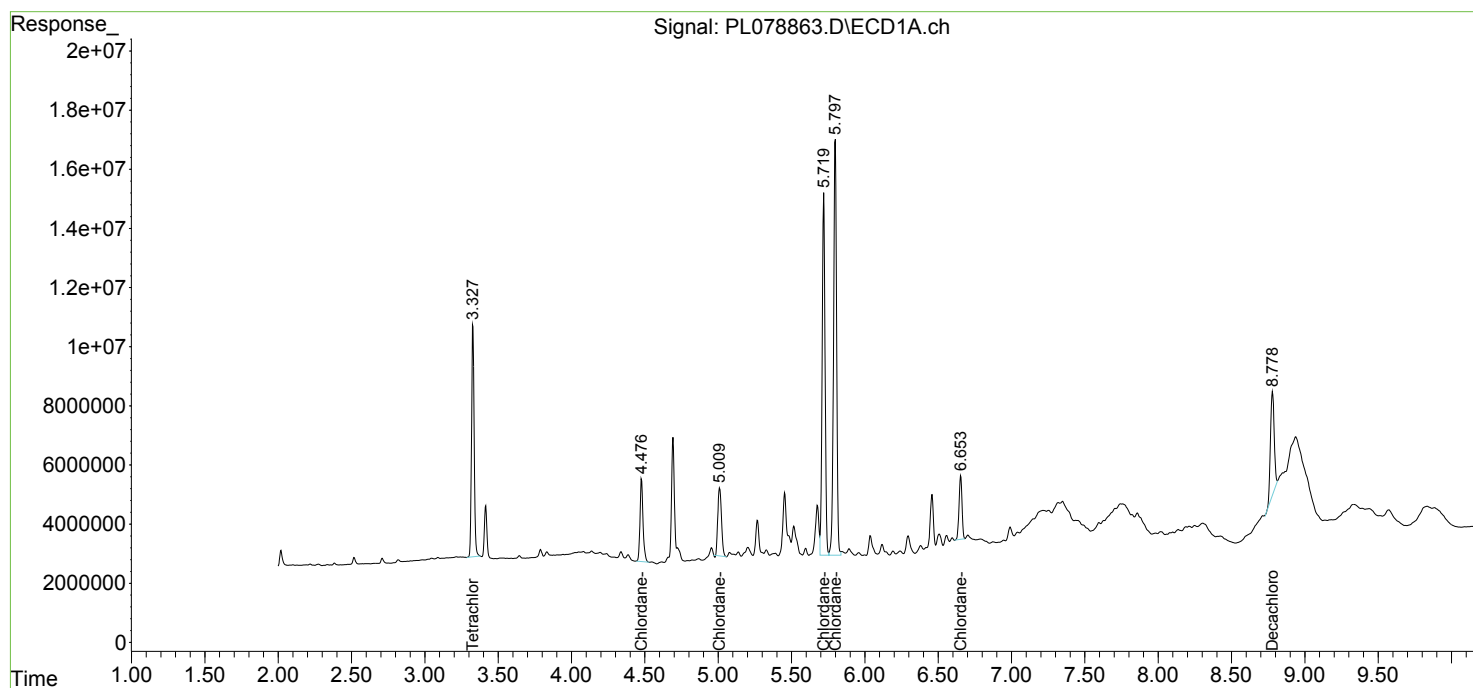


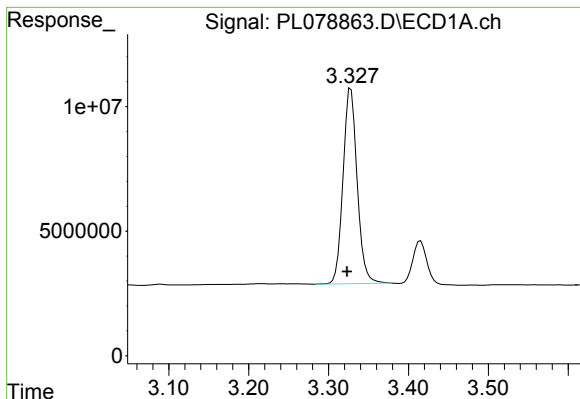

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.005 min
Response: 96567373
Conc: 50.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

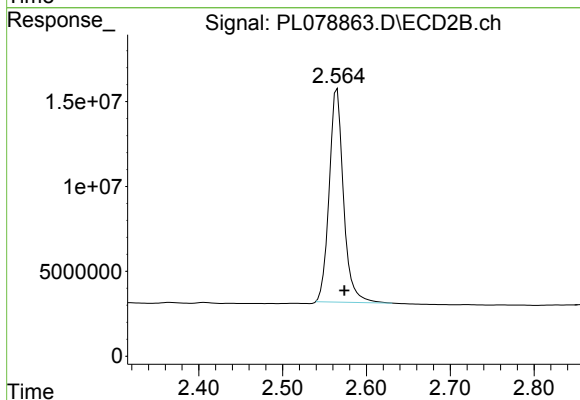


#1 Tetrachloro-m-xylene

R.T.: 2.565 min
Delta R.T.: -0.009 min
Response: 148763012
Conc: 58.27 ng/ml

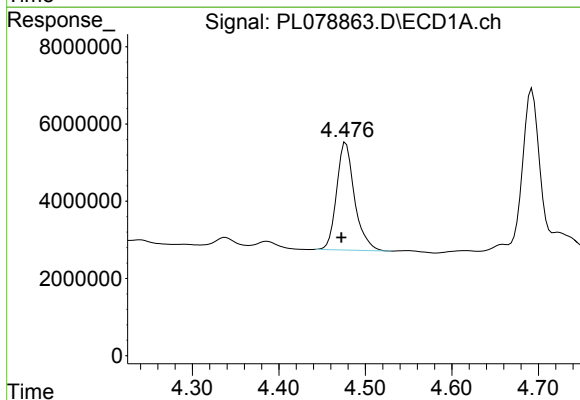


#23 Chlordane-1

R.T.: 4.478 min
Delta R.T.: 0.005 min
Response: 39829008
Conc: 508.33 ng/ml

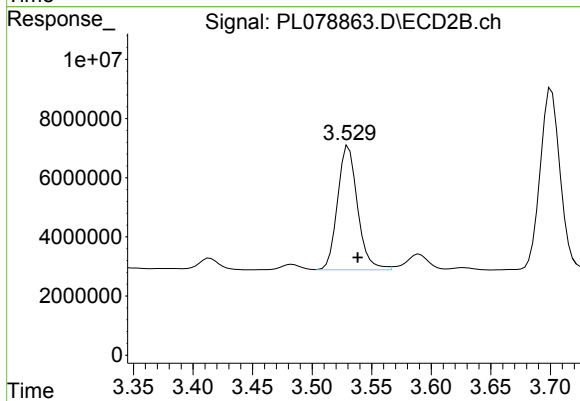

#23 Chlordane-1


R.T.: 3.531 min
Delta R.T.: -0.008 min
Response: 48967396
Conc: 485.52 ng/ml

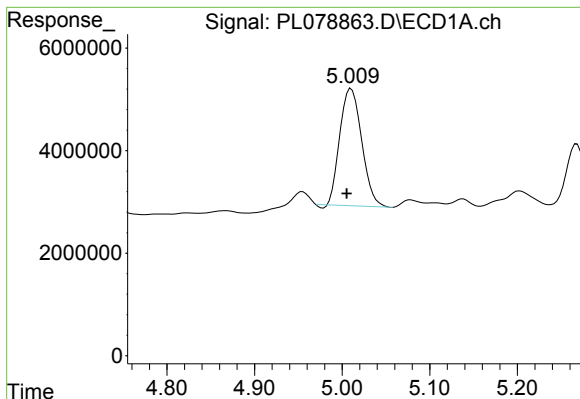

#24 Chlordane-2


R.T.: 5.010 min
Delta R.T.: 0.005 min
Response: 39569335
Conc: 478.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

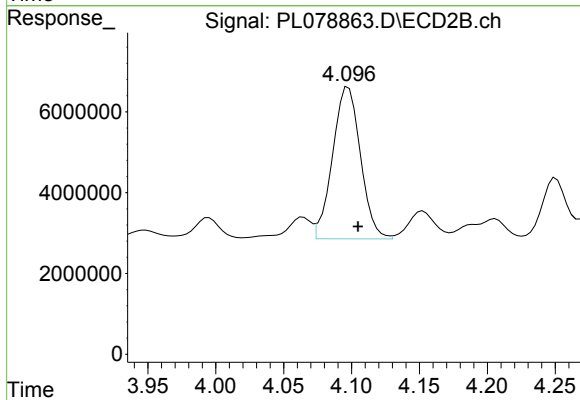


#24 Chlordane-2

R.T.: 4.098 min
Delta R.T.: -0.007 min
Response: 53764489
Conc: 505.18 ng/ml

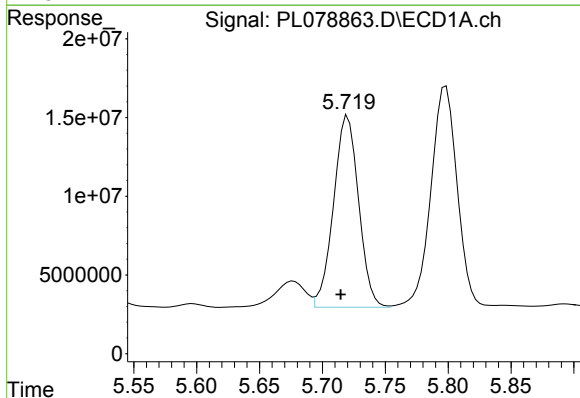


#25 Chlordane-3

R.T.: 5.720 min
Delta R.T.: 0.006 min
Response: 168981257
Conc: 505.87 ng/ml

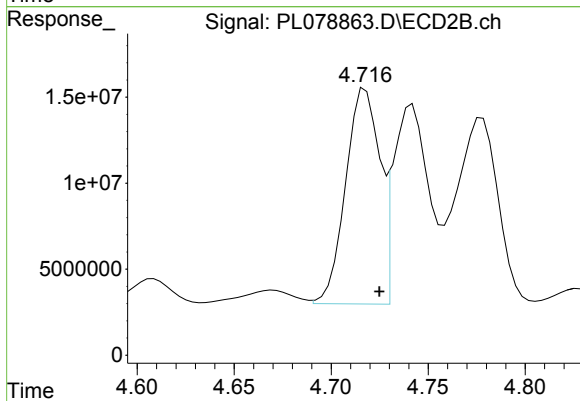

#25 Chlordane-3


R.T.: 4.718 min
Delta R.T.: -0.007 min
Response: 153236866
Conc: 502.77 ng/ml

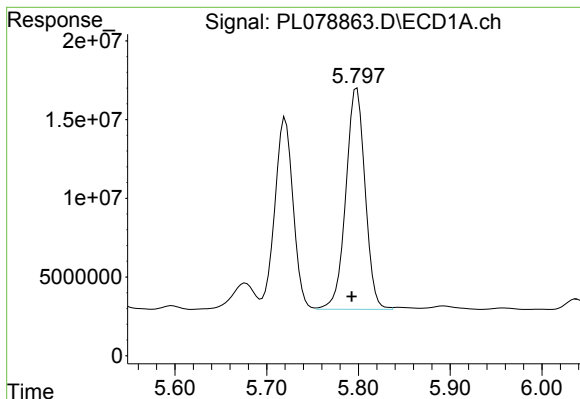

#26 Chlordane-4


R.T.: 5.798 min
Delta R.T.: 0.006 min
Response: 204697301
Conc: 498.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

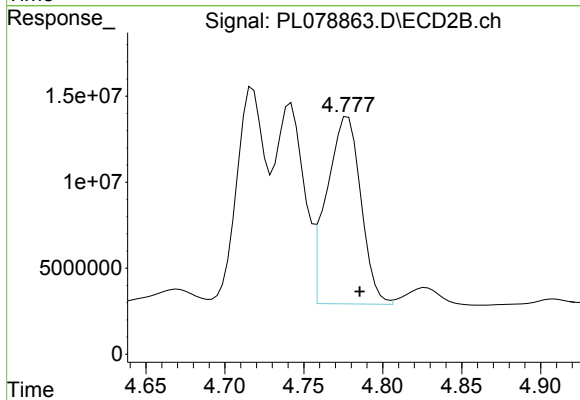


#26 Chlordane-4

R.T.: 4.778 min
Delta R.T.: -0.008 min
Response: 163361477
Conc: 499.94 ng/ml

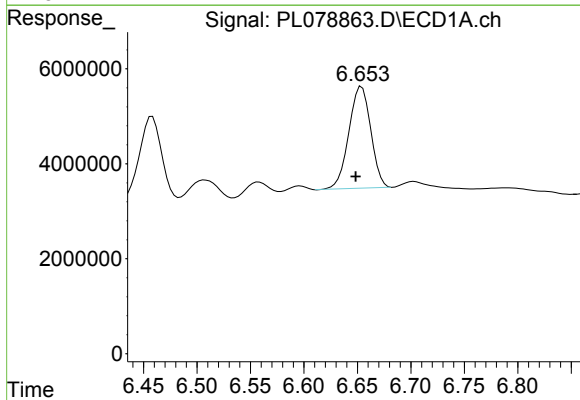


#27 Chlordane-5

R.T.: 6.654 min
Delta R.T.: 0.005 min
Response: 30573323
Conc: 467.55 ng/ml

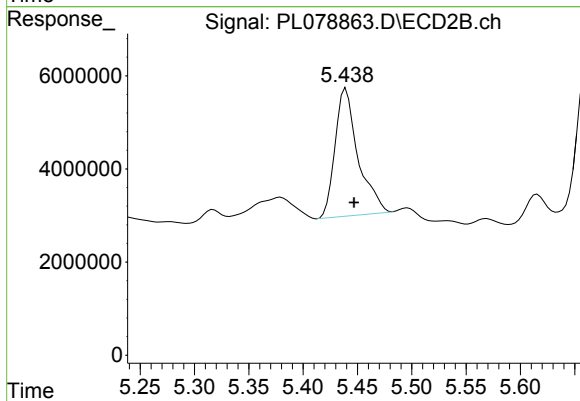

#27 Chlordane-5


R.T.: 5.439 min
Delta R.T.: -0.008 min
Response: 40411535
Conc: 495.51 ng/ml

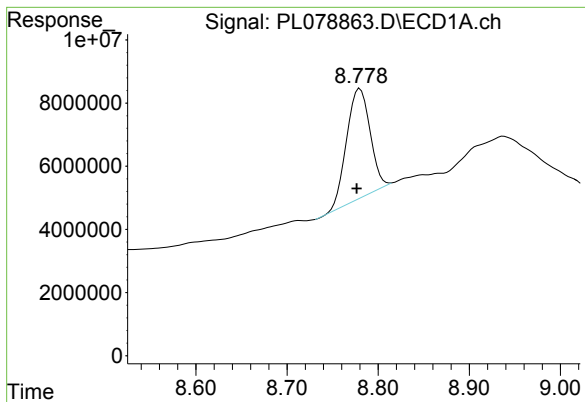

#28 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: 0.004 min
Response: 61686760
Conc: 41.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

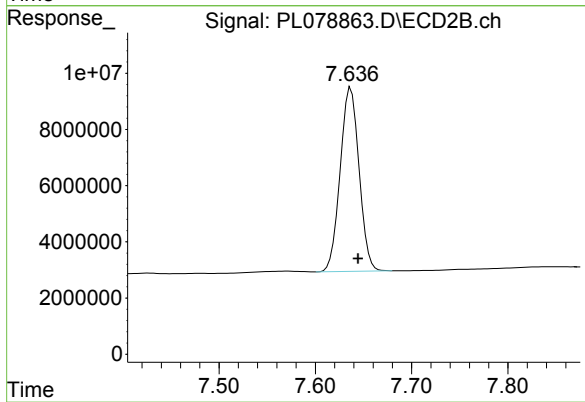

#28 Decachlorobiphenyl

R.T.: 7.637 min
Delta R.T.: -0.007 min
Response: 88968883
Conc: 46.97 ng/ml