

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
 Data File : PL078866.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2022 17:29
 Operator : AR\AJ
 Sample : N5436-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 250FERRYBLVD-TFS-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 17:39:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	2.568	40512488	26374245	21.244	10.330 #
28)	SA Decachlor...	8.770	7.635	311.1E6	348.0E6	206.816	183.706
Target Compounds							
13)	MA Dieldrin	6.117	5.103	222.7E6	74646834	103.261	25.192m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
Data File : PL078866.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2022 17:29
Operator : AR\AJ
Sample : N5436-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 17:39:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

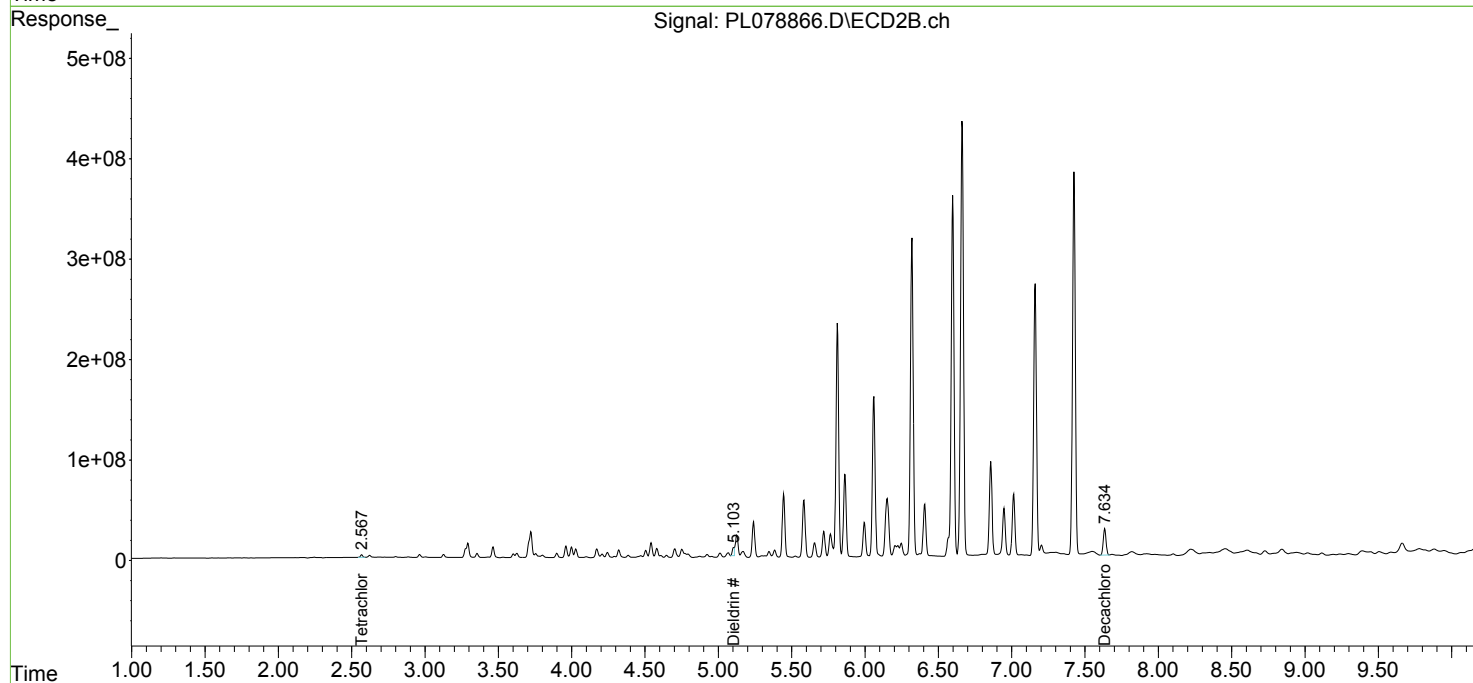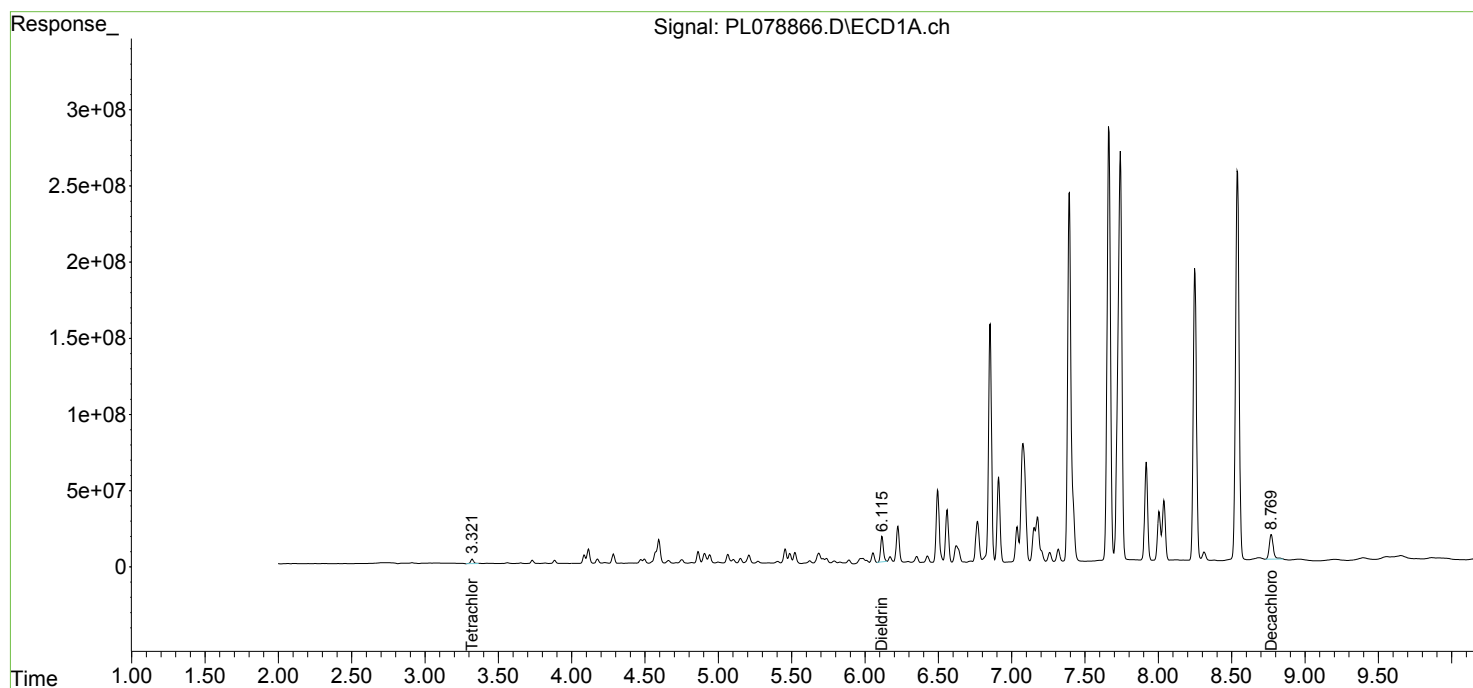


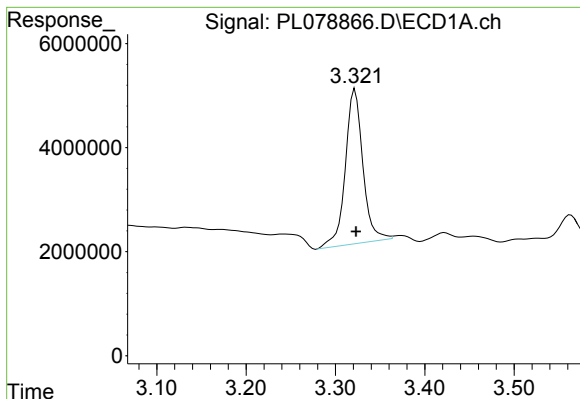

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.001 min
Response: 40512488
Conc: 21.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-10

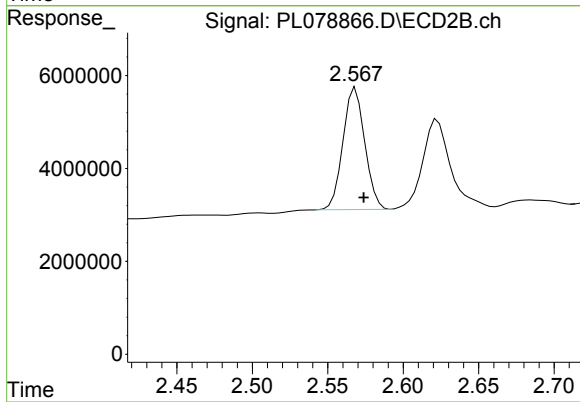


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.005 min
Response: 26374245
Conc: 10.33 ng/ml

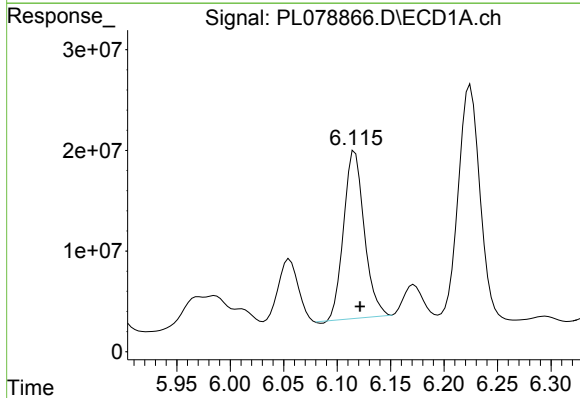


#13 Dieldrin

R.T.: 6.117 min
Delta R.T.: -0.005 min
Response: 222683117
Conc: 103.26 ng/ml

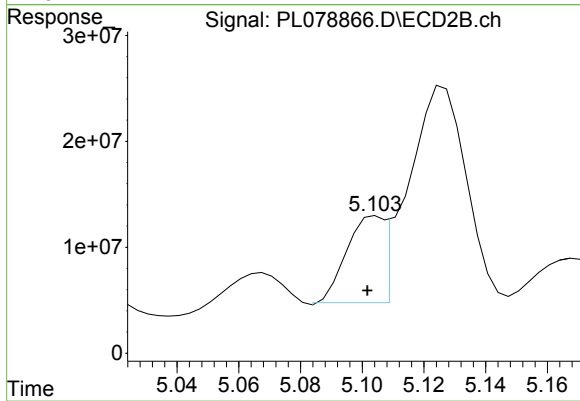

#13 Dieldrin

R.T.: 5.103 min
Delta R.T.: 0.002 min
Response: 74646834
Conc: 25.19 ng/ml m

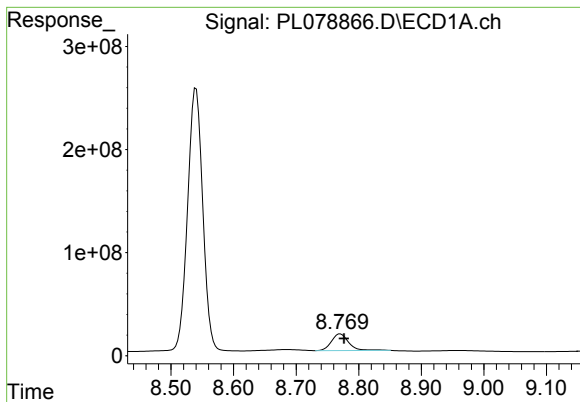

#28 Decachlorobiphenyl


R.T.: 8.770 min

Delta R.T.: -0.006 min

Response: 311125636

Conc: 206.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-10

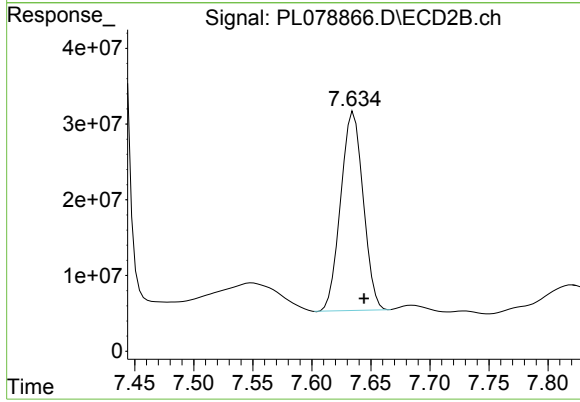

#28 Decachlorobiphenyl

R.T.: 7.635 min

Delta R.T.: -0.009 min

Response: 347958806

Conc: 183.71 ng/ml