

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
 Data File : PL078867.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2022 17:43
 Operator : AR\AJ
 Sample : N5436-11
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 250FERRYBLVD-TFS-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 17:48:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	2.568	29807575	22973375	15.630	8.998 #
28)	SA Decachlor...	8.771	7.635	276.1E6	293.7E6	183.539	155.080
Target Compounds							
13)	MA Dieldrin	6.116	5.106	155.2E6	30758892	71.948	10.381m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
Data File : PL078867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2022 17:43
Operator : AR\AJ
Sample : N5436-11
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 17:48:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

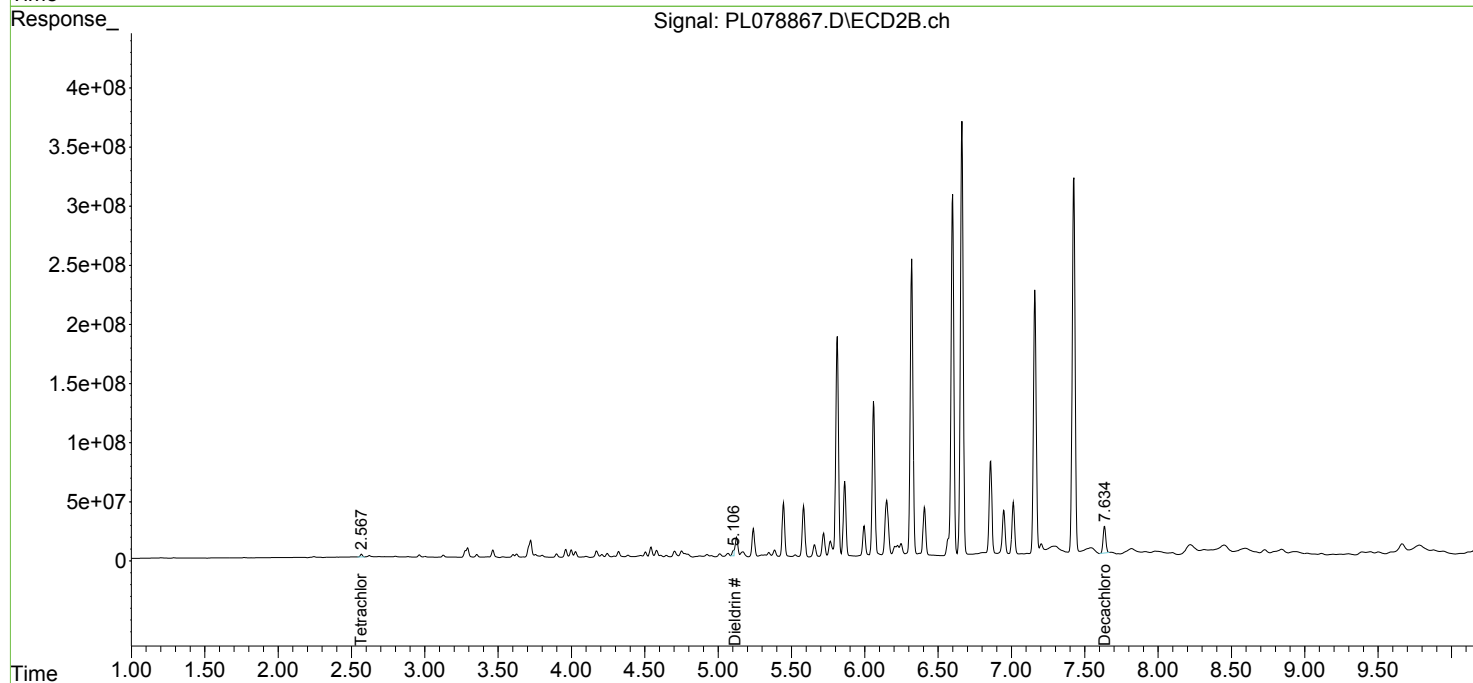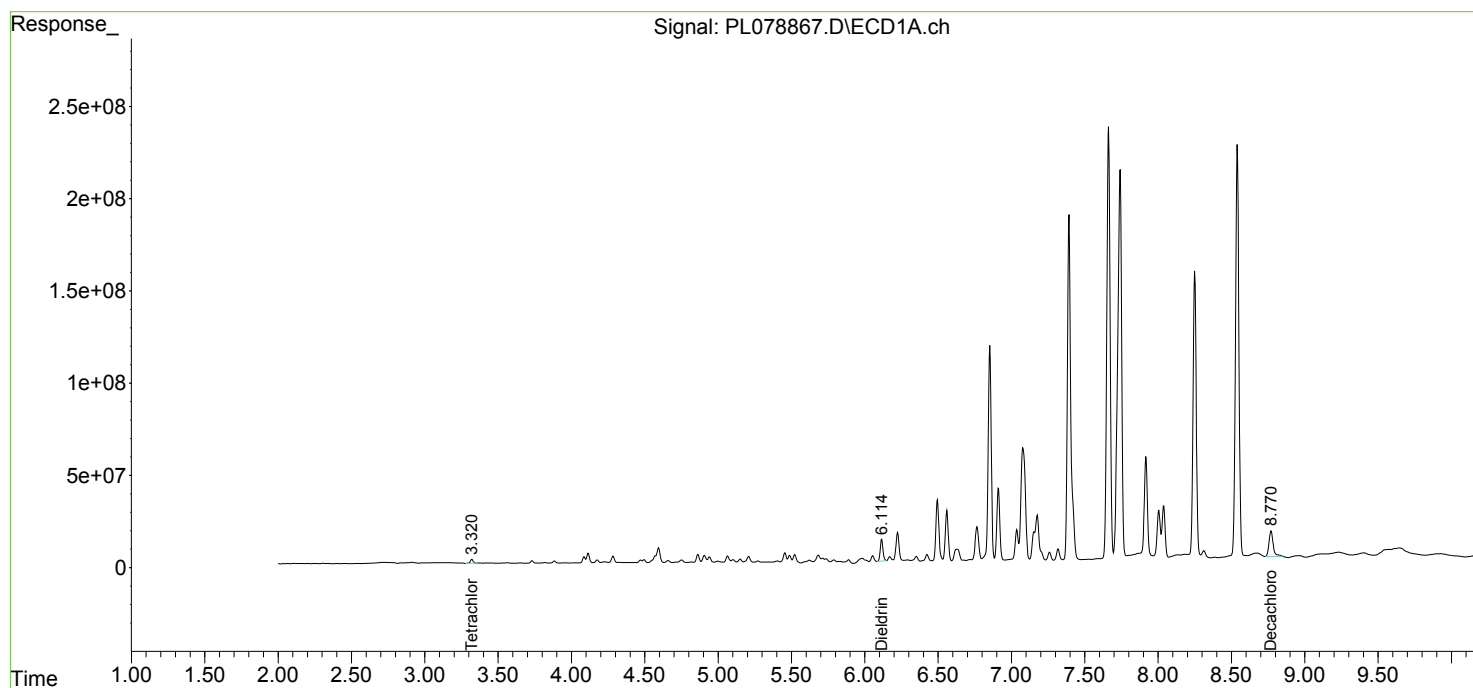


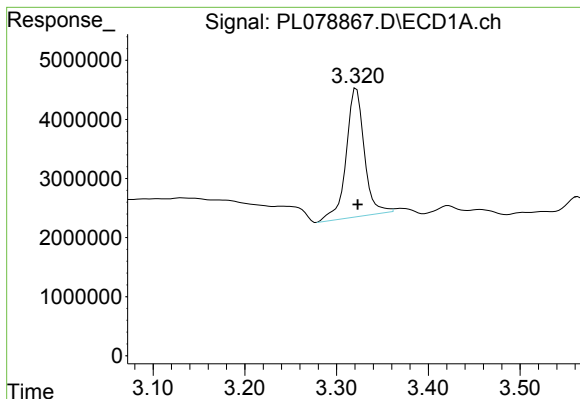

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.001 min
Response: 29807575
Conc: 15.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-11

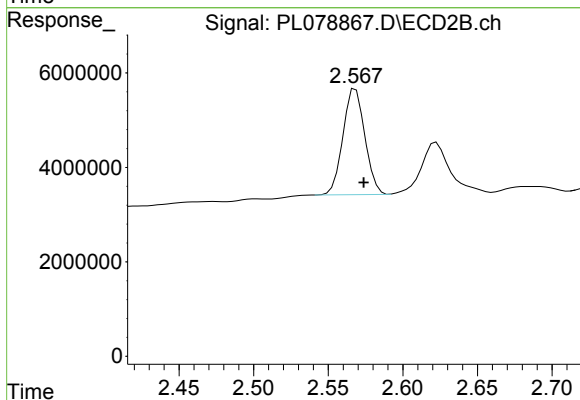


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.005 min
Response: 22973375
Conc: 9.00 ng/ml

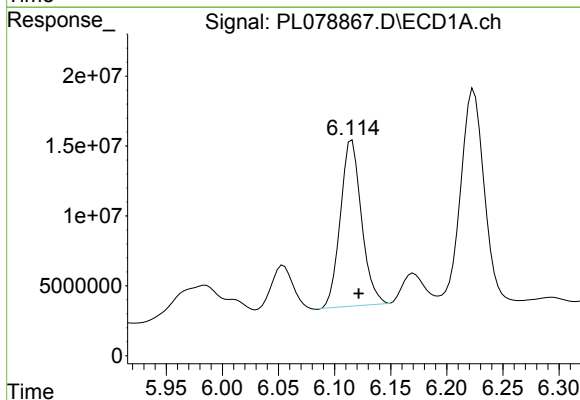


#13 Dieldrin

R.T.: 6.116 min
Delta R.T.: -0.006 min
Response: 155156311
Conc: 71.95 ng/ml

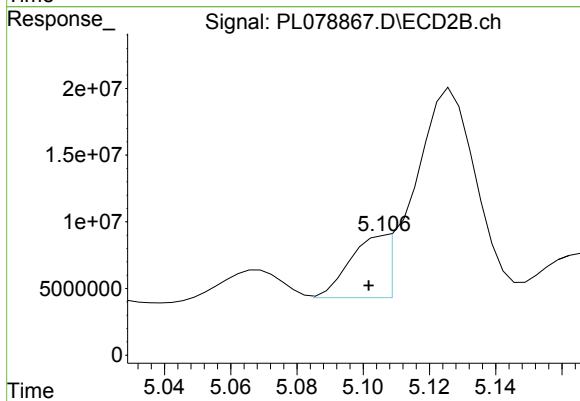

#13 Dieldrin

R.T.: 5.106 min
Delta R.T.: 0.004 min
Response: 30758892
Conc: 10.38 ng/ml m

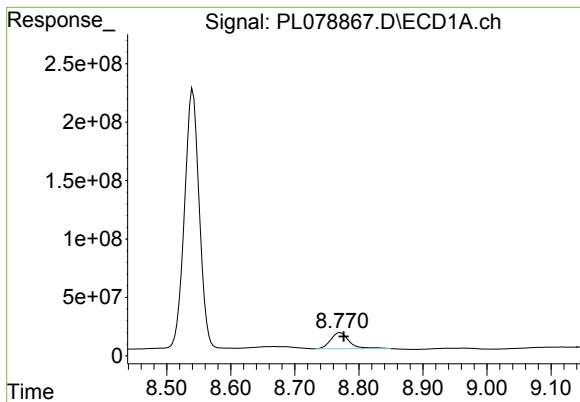

#28 Decachlorobiphenyl


R.T.: 8.771 min

Delta R.T.: -0.006 min

Response: 276108510

Conc: 183.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-11

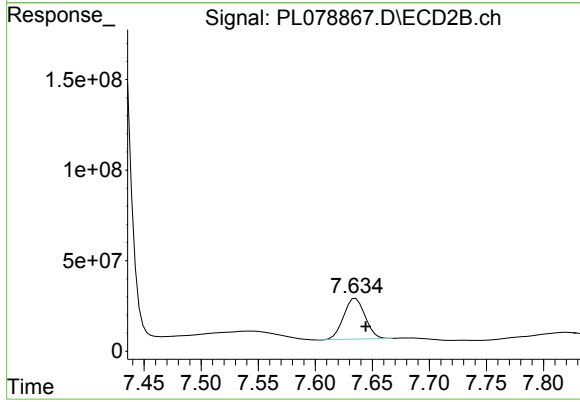

#28 Decachlorobiphenyl

R.T.: 7.635 min

Delta R.T.: -0.009 min

Response: 293738157

Conc: 155.08 ng/ml