

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
 Data File : PL078868.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2022 17:56
 Operator : AR\AJ
 Sample : N5436-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 250FERRYBLVD-TFS-12

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 17:47:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	2.568	35599848	22907406	18.668	8.972 #
28)	SA Decachlor...	8.769	7.635	221.3E6	281.6E6	147.118	148.671
Target Compounds							
13)	MA Dieldrin	6.115	5.103	150.2E6	66834579	69.669	22.556m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
Data File : PL078868.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2022 17:56
Operator : AR\AJ
Sample : N5436-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-12

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 17:47:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

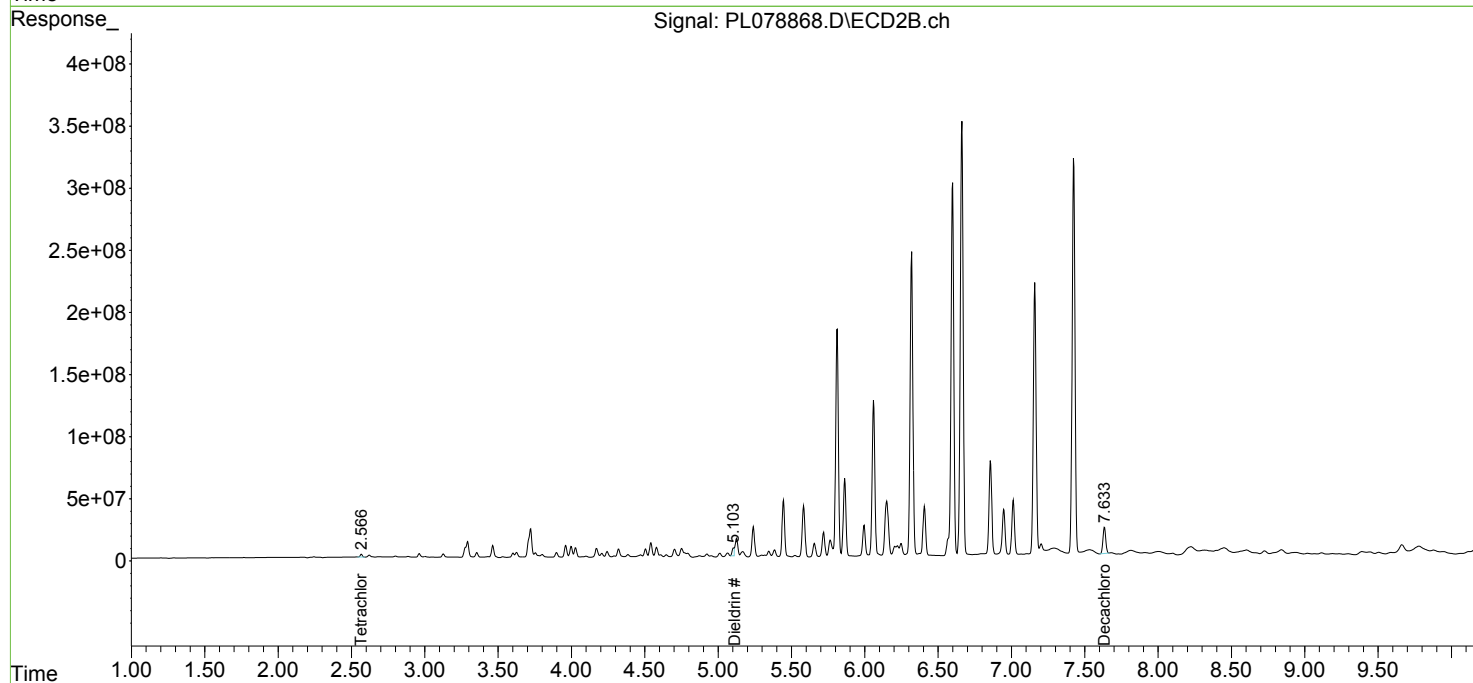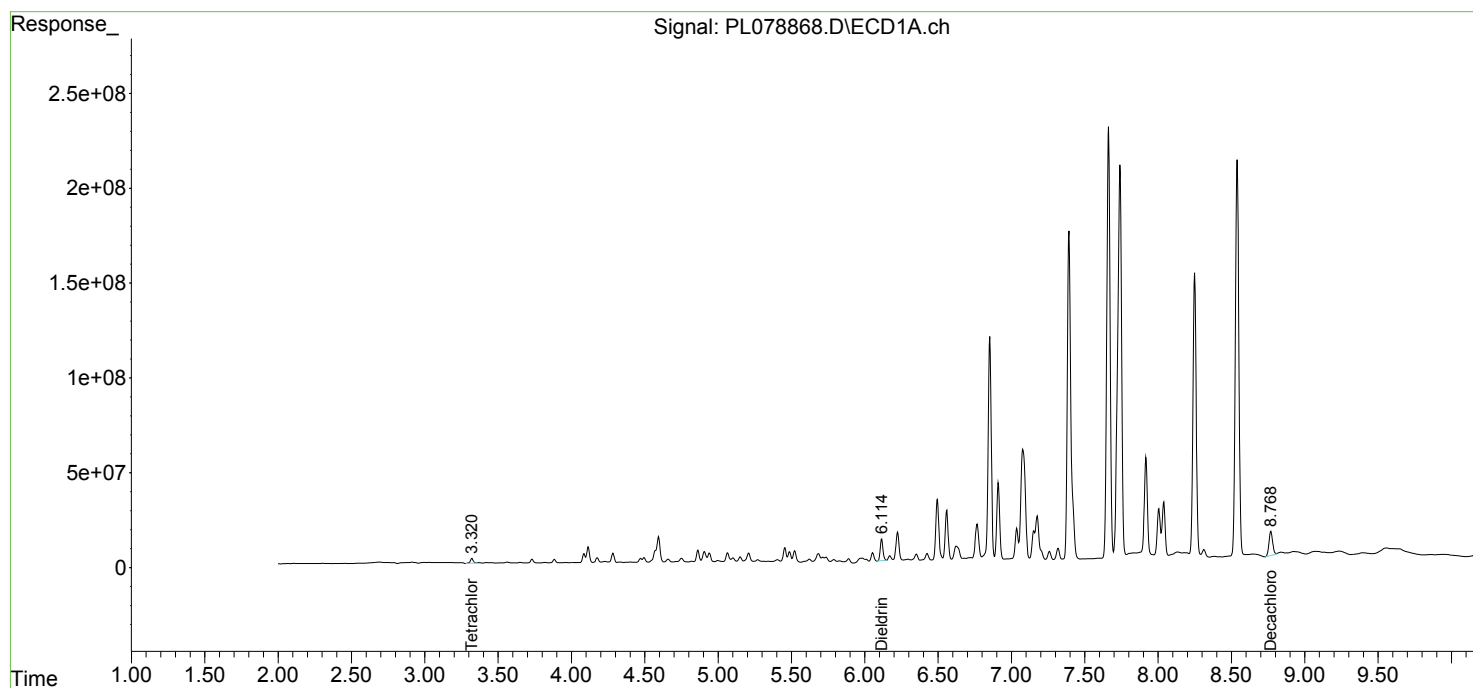


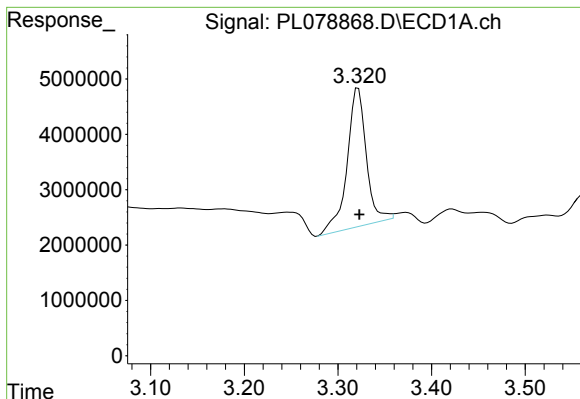

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.001 min
Response: 35599848
Conc: 18.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-12

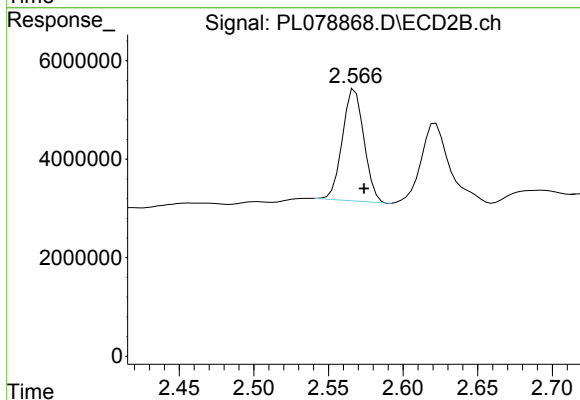


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.006 min
Response: 22907406
Conc: 8.97 ng/ml

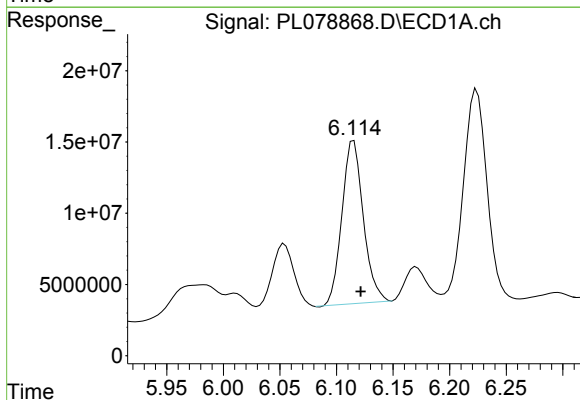


#13 Dieldrin

R.T.: 6.115 min
Delta R.T.: -0.006 min
Response: 150241018
Conc: 69.67 ng/ml

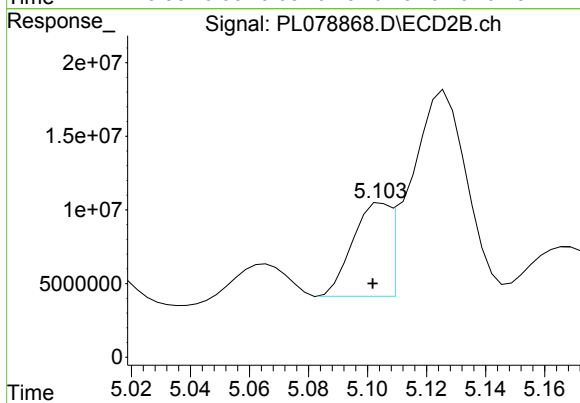

#13 Dieldrin


R.T.: 5.103 min
Delta R.T.: 0.002 min
Response: 66834579
Conc: 22.56 ng/ml m

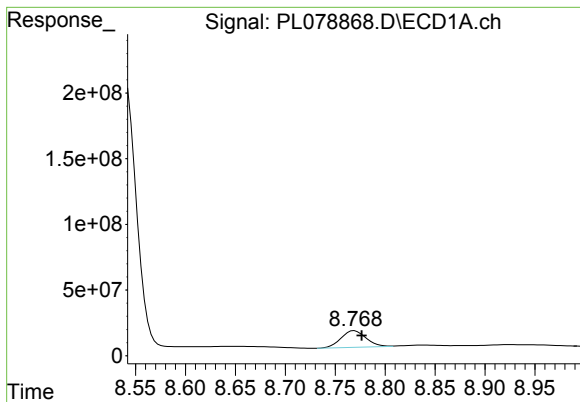

#28 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: -0.007 min
Response: 221318395
Conc: 147.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-12

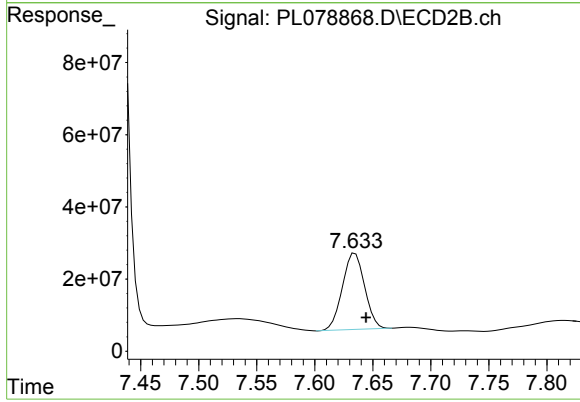

#28 Decachlorobiphenyl

R.T.: 7.635 min
Delta R.T.: -0.010 min
Response: 281598635
Conc: 148.67 ng/ml