

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
 Data File : PL078869.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2022 18:10
 Operator : AR\AJ
 Sample : N5436-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 250FERRYBLVD-TFS-13

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 17:52:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	2.568	38482685	25846714	20.180	10.123 #
28)	SA Decachlor...	8.770	7.634	320.9E6	395.6E6	213.327	208.877
Target Compounds							
13)	MA Dieldrin	6.115	5.103	194.1E6	58014174	90.024	19.579m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
Data File : PL078869.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2022 18:10
Operator : AR\AJ
Sample : N5436-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-13

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 17:52:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

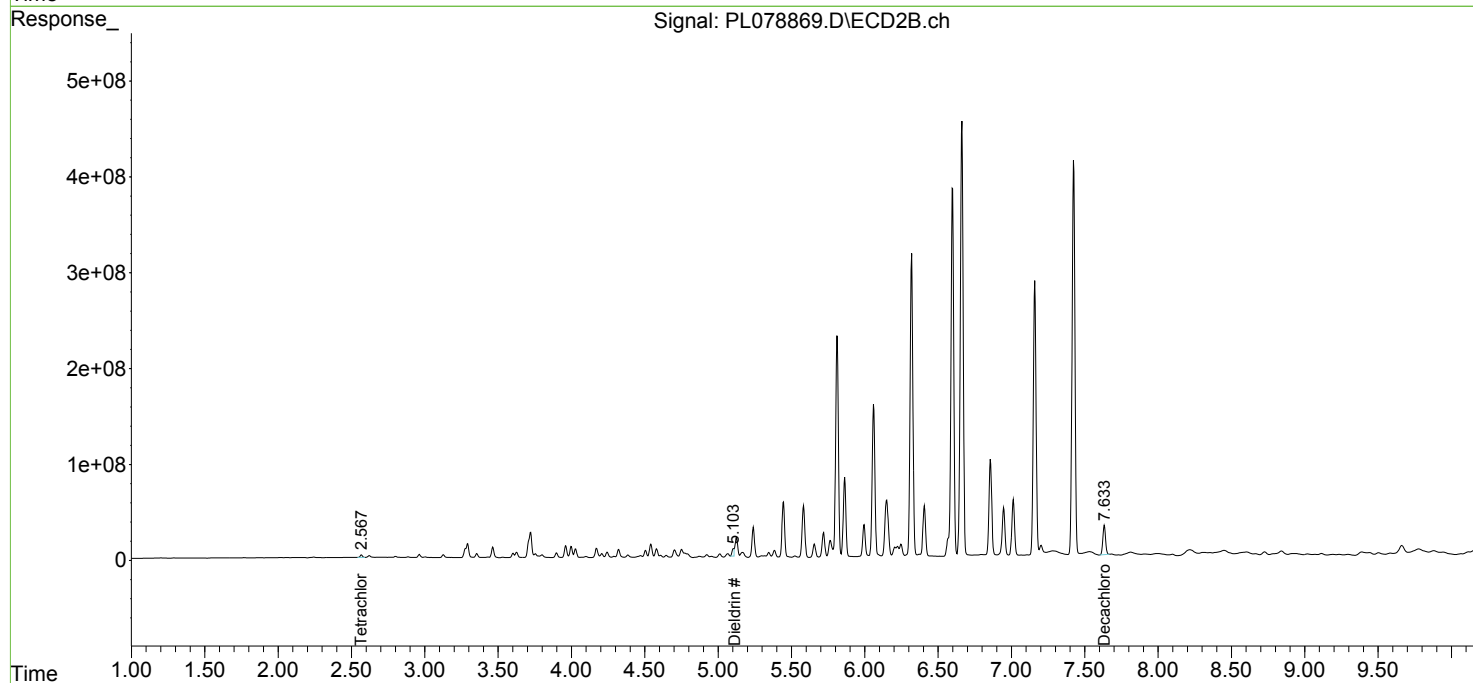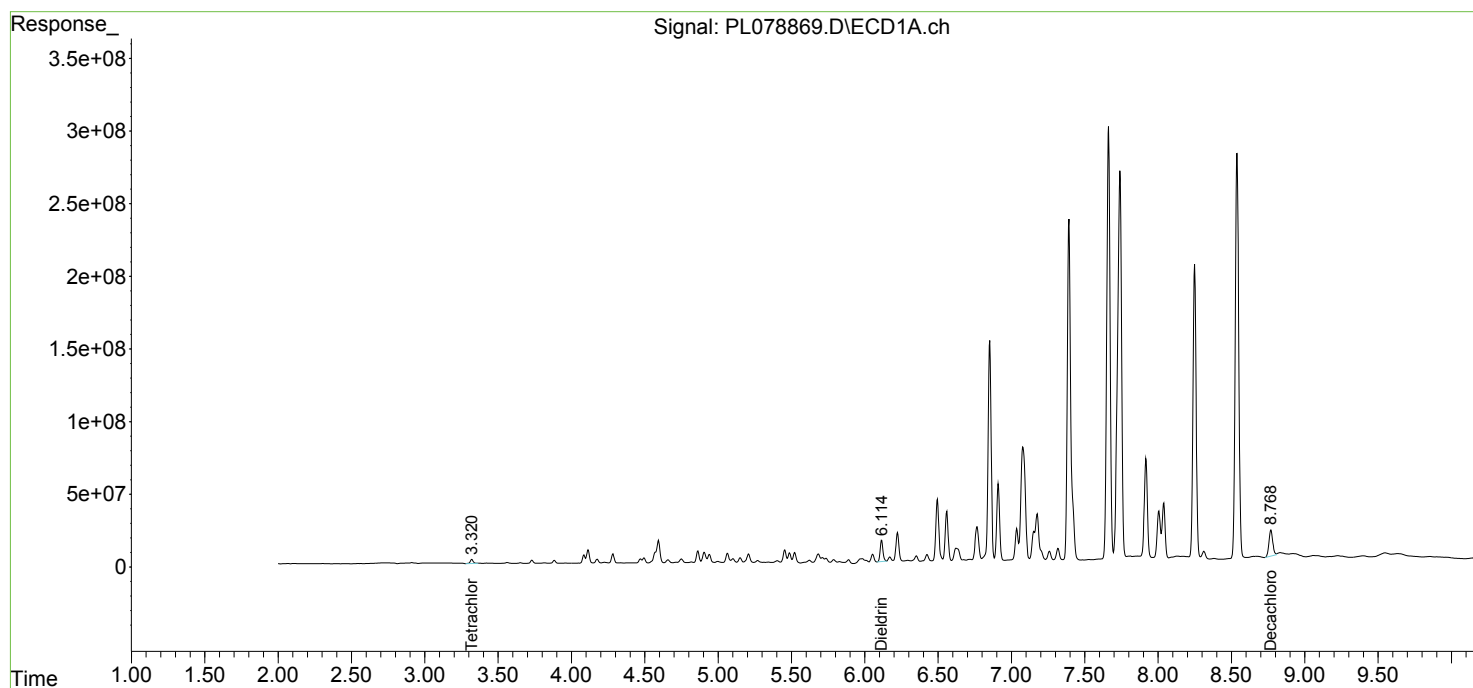


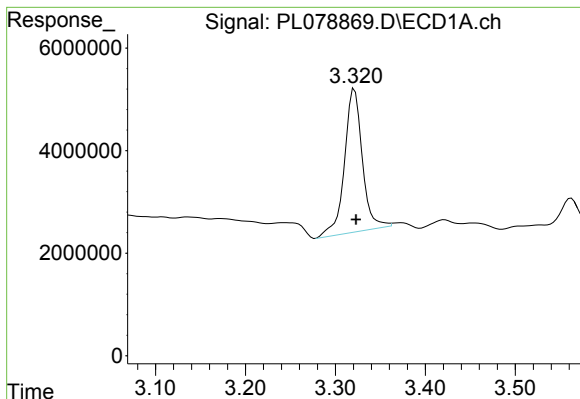

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: -0.002 min
Response: 38482685
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-13

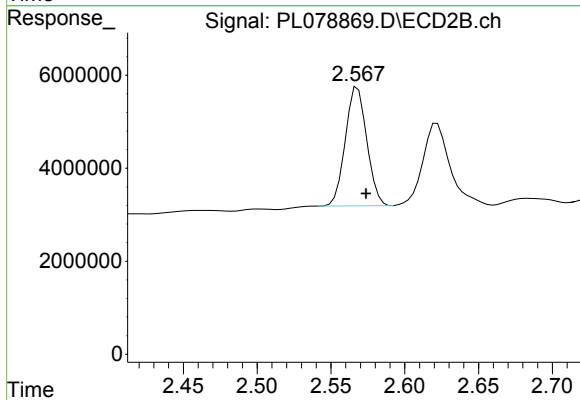


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.006 min
Response: 25846714
Conc: 10.12 ng/ml

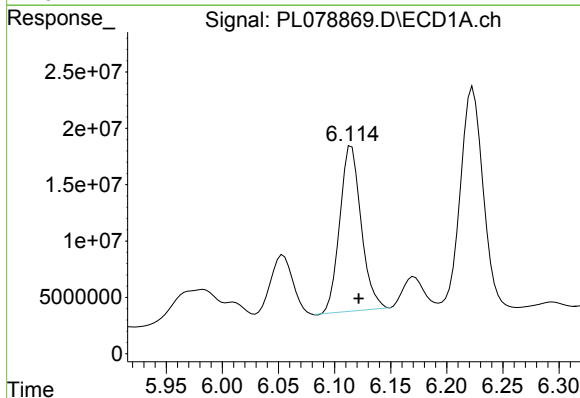


#13 Dieldrin

R.T.: 6.115 min
Delta R.T.: -0.006 min
Response: 194136800
Conc: 90.02 ng/ml

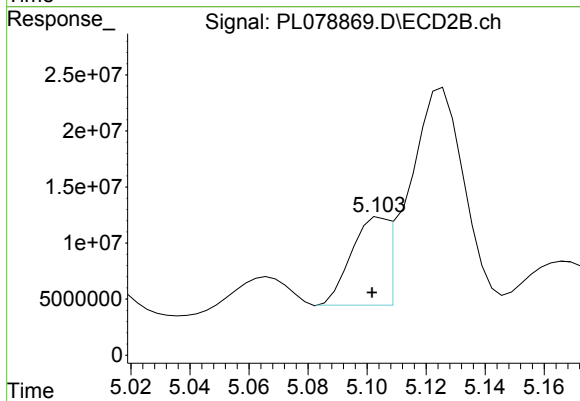

#13 Dieldrin


R.T.: 5.103 min
Delta R.T.: 0.002 min
Response: 58014174
Conc: 19.58 ng/ml m

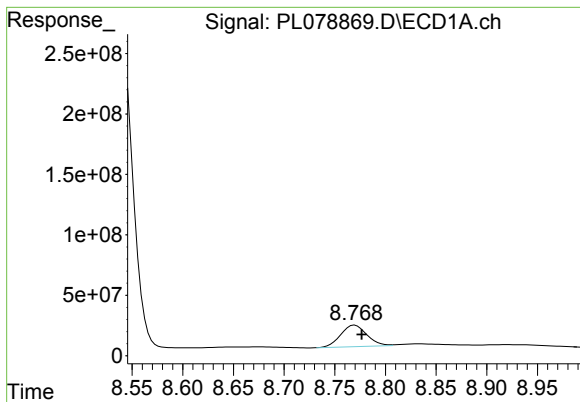

#28 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.007 min
Response: 320920293
Conc: 213.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-13

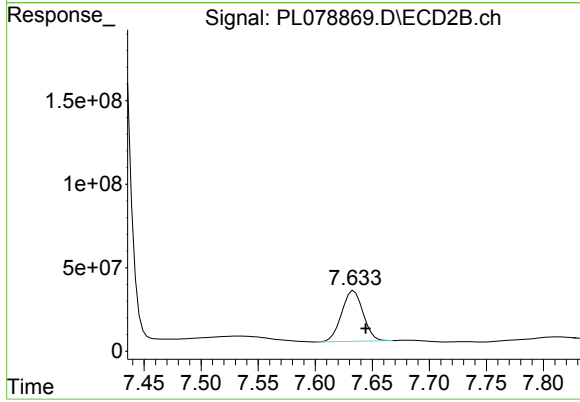

#28 Decachlorobiphenyl

R.T.: 7.634 min
Delta R.T.: -0.010 min
Response: 395634000
Conc: 208.88 ng/ml