

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
 Data File : PL078875.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2022 20:15
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 02:13:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	2.567	96046538	151.6E6	50.365	59.389
28)	SA Decachlor...	8.770	7.635	67808762	95639967	45.075	50.494
Target Compounds							
23)	Chlordane-1	4.470	3.532	40370389	50341916	515.242	499.152
24)	Chlordane-2	5.002	4.098	42685156	57457019	515.871	539.876
25)	Chlordane-3	5.712	4.718	170.9E6	160.8E6	511.708	527.457
26)	Chlordane-4	5.790	4.778	205.8E6	170.7E6	501.236	522.345
27)	Chlordane-5	6.645	5.439	31452484	44031634	480.995	539.893



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110722\
Data File : PL078875.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2022 20:15
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 02:13:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

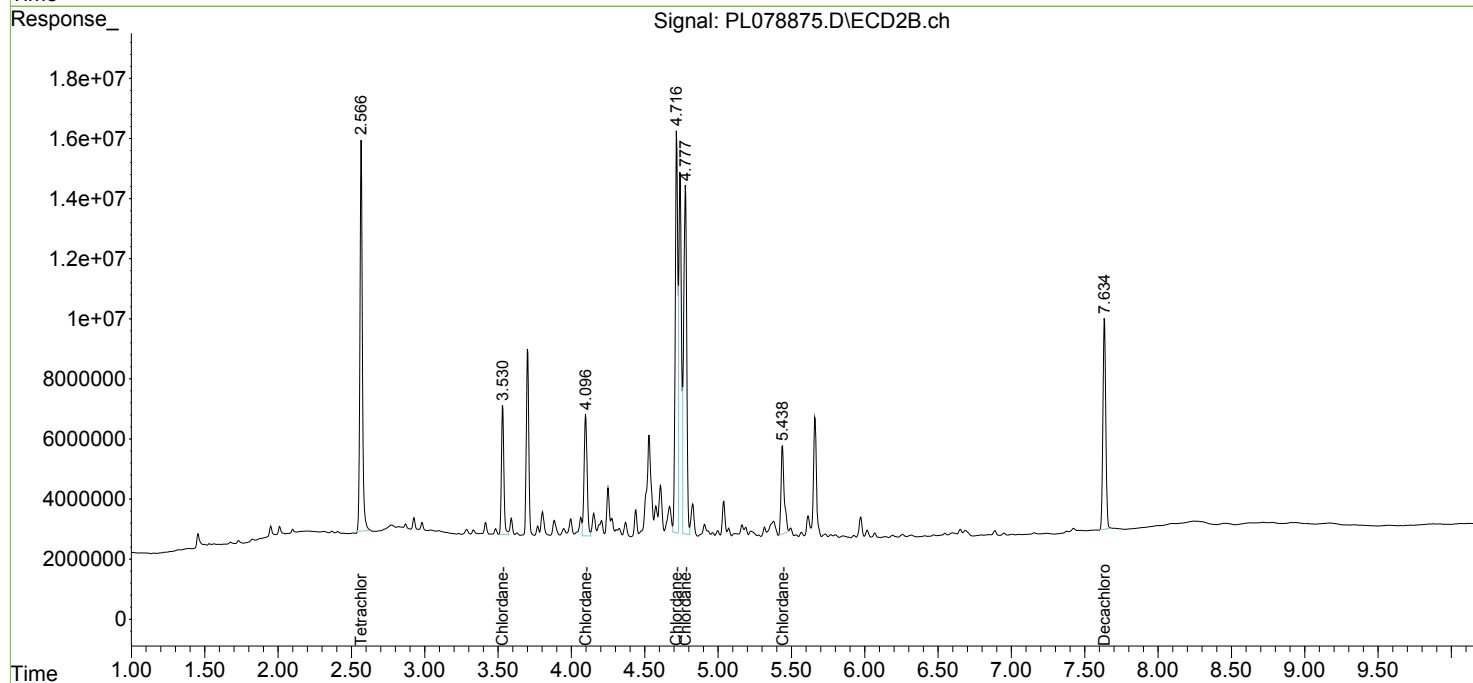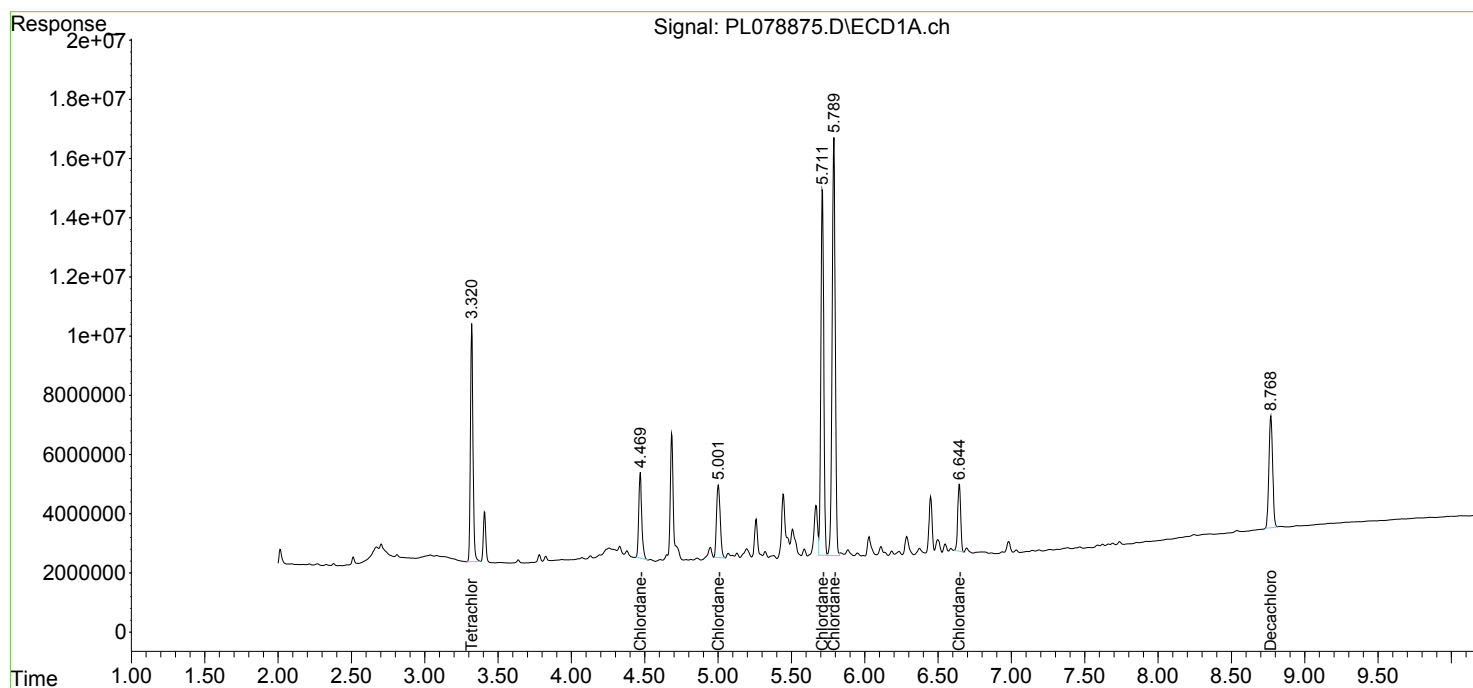


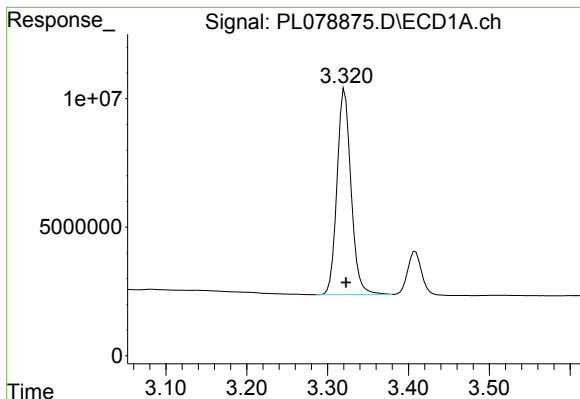

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: -0.002 min
Response: 96046538
Conc: 50.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

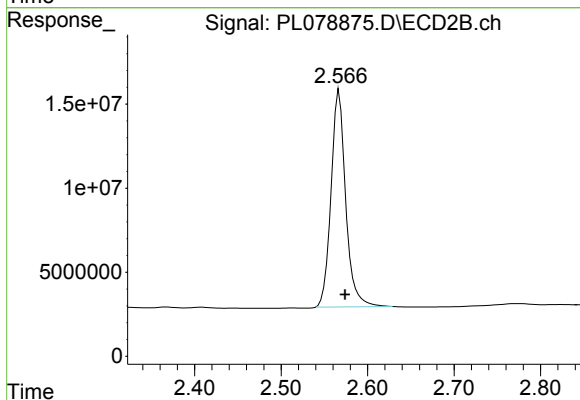


#1 Tetrachloro-m-xylene

R.T.: 2.567 min
Delta R.T.: -0.007 min
Response: 151630614
Conc: 59.39 ng/ml

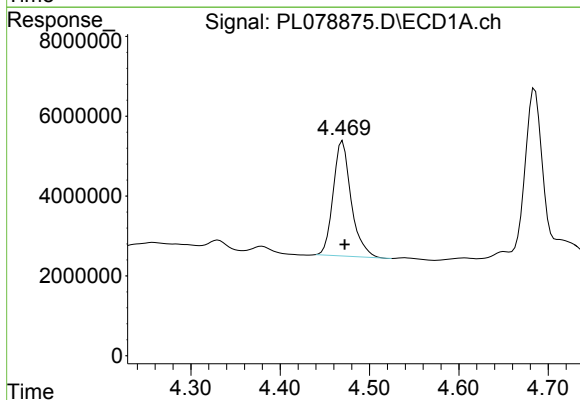


#23 Chlordane-1

R.T.: 4.470 min
Delta R.T.: -0.002 min
Response: 40370389
Conc: 515.24 ng/ml

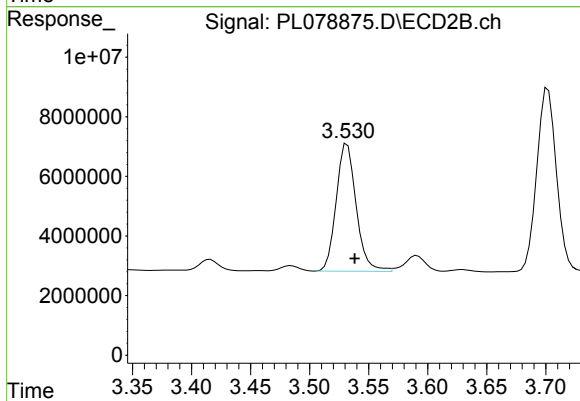

#23 Chlordane-1


R.T.: 3.532 min
Delta R.T.: -0.006 min
Response: 50341916
Conc: 499.15 ng/ml

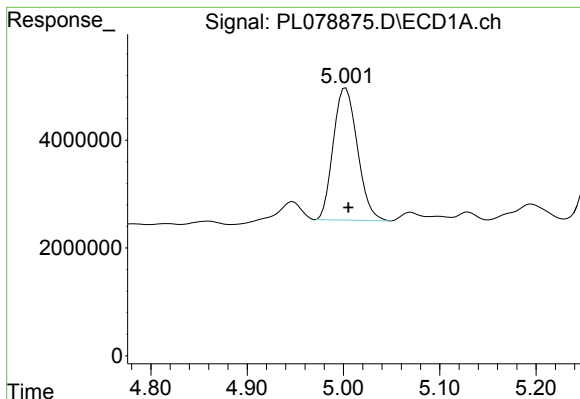

#24 Chlordane-2


R.T.: 5.002 min
Delta R.T.: -0.003 min
Response: 42685156
Conc: 515.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

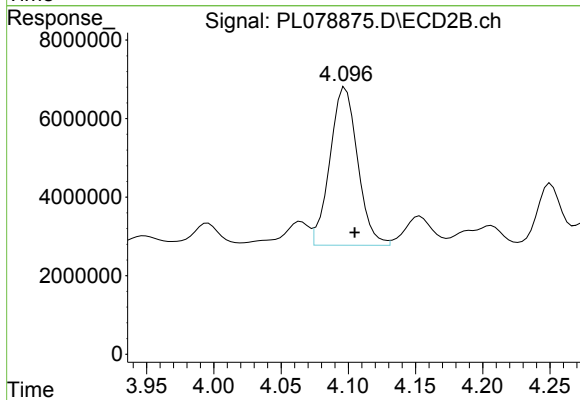


#24 Chlordane-2

R.T.: 4.098 min
Delta R.T.: -0.007 min
Response: 57457019
Conc: 539.88 ng/ml

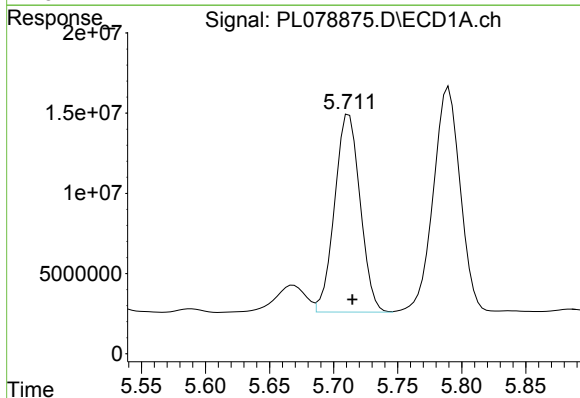


#25 Chlordane-3

R.T.: 5.712 min
Delta R.T.: -0.002 min
Response: 170932935
Conc: 511.71 ng/ml

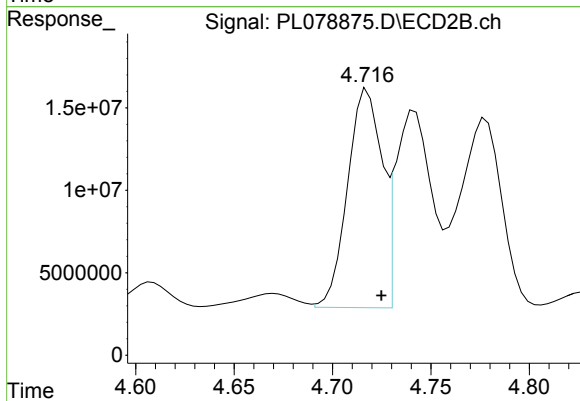

#25 Chlordane-3


R.T.: 4.718 min
Delta R.T.: -0.007 min
Response: 160760873
Conc: 527.46 ng/ml

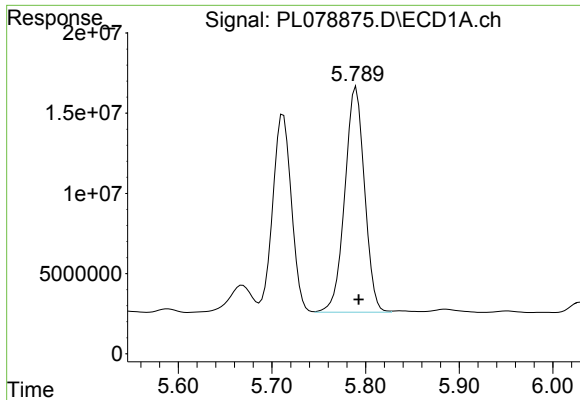

#26 Chlordane-4


R.T.: 5.790 min
Delta R.T.: -0.003 min
Response: 205777393
Conc: 501.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

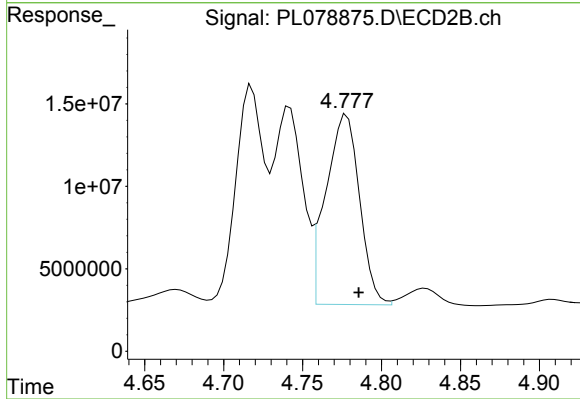


#26 Chlordane-4

R.T.: 4.778 min
Delta R.T.: -0.008 min
Response: 170683432
Conc: 522.35 ng/ml

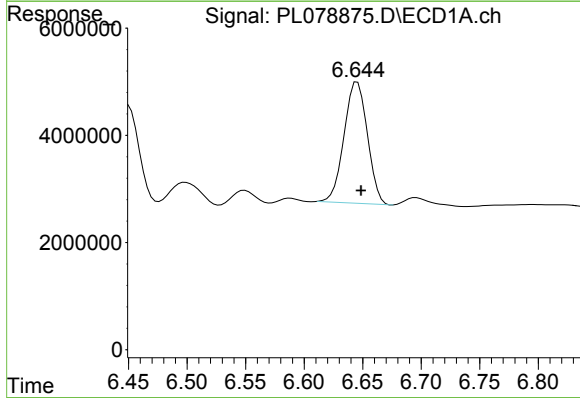


#27 Chlordane-5

R.T.: 6.645 min
Delta R.T.: -0.003 min
Response: 31452484
Conc: 480.99 ng/ml

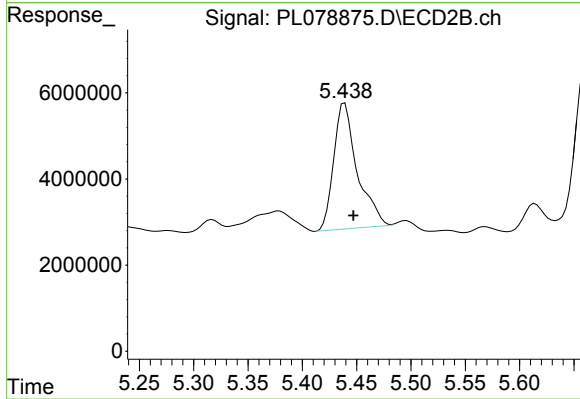

#27 Chlordane-5


R.T.: 5.439 min
Delta R.T.: -0.008 min
Response: 44031634
Conc: 539.89 ng/ml

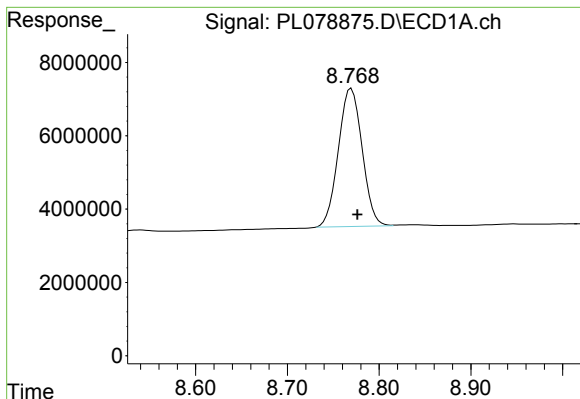

#28 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.007 min
Response: 67808762
Conc: 45.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

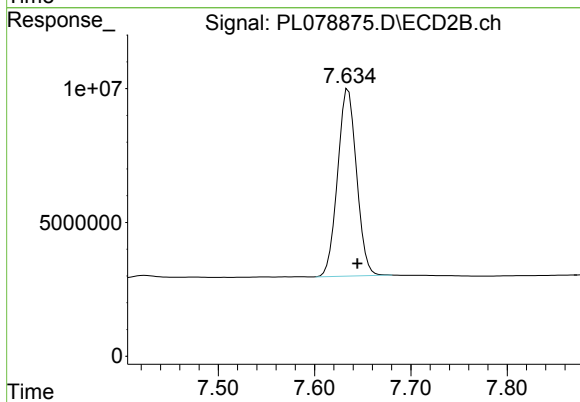

#28 Decachlorobiphenyl

R.T.: 7.635 min
Delta R.T.: -0.009 min
Response: 95639967
Conc: 50.49 ng/ml