

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110819\
 Data File : PL054139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2019 13:25
 Operator : SG\AJ
 Sample : K5730-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HILTON-STOCKPILE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 22:05:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	4.043	117.5E6	27485946	10.844	10.984
28)	SA Decachlor...	8.324	9.123	71235739	21067332	7.260	7.481
Target Compounds							
10)	B gamma-Chl...	5.495	0.000	63524437	0	4.656	N.D. #
12)	B 4,4'-DDE	5.723	6.384	334.5E6	73009155	28.150	25.923
13)	MA Dieldrin	5.874	0.000	16006925	0	1.228	N.D. #
16)	A 4,4'-DDD	6.240	6.874	51781258	15471403	5.818	7.424 #
17)	MA 4,4'-DDT	6.482	7.173	9593323	3105189	0.968	1.343 #
23)	Chlordane-1	4.423	0.000	5347889	0	15.078	N.D. #
25)	Chlordane-3	5.495	0.000	63524437	0	55.110	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110819\
Data File : PL054139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2019 13:25
Operator : SG\AJ
Sample : K5730-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HILTON-STOCKPILE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 22:05:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

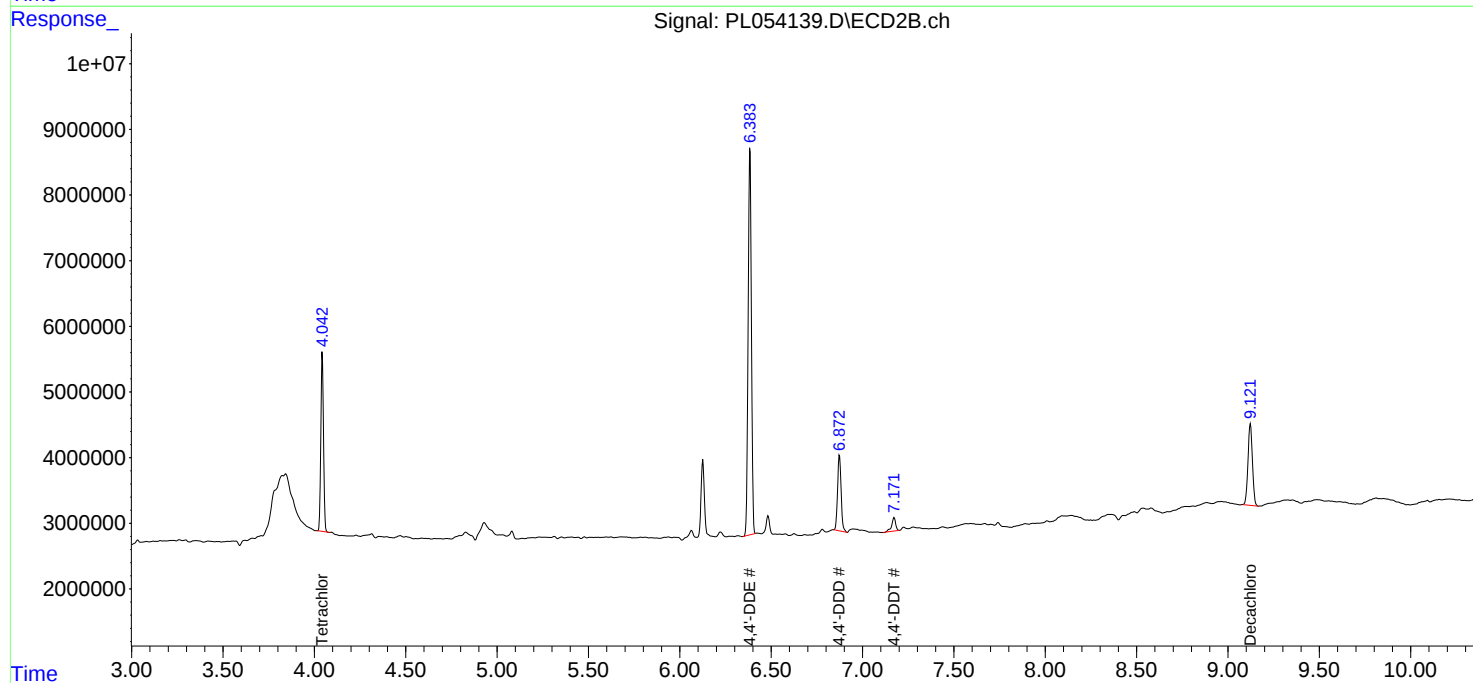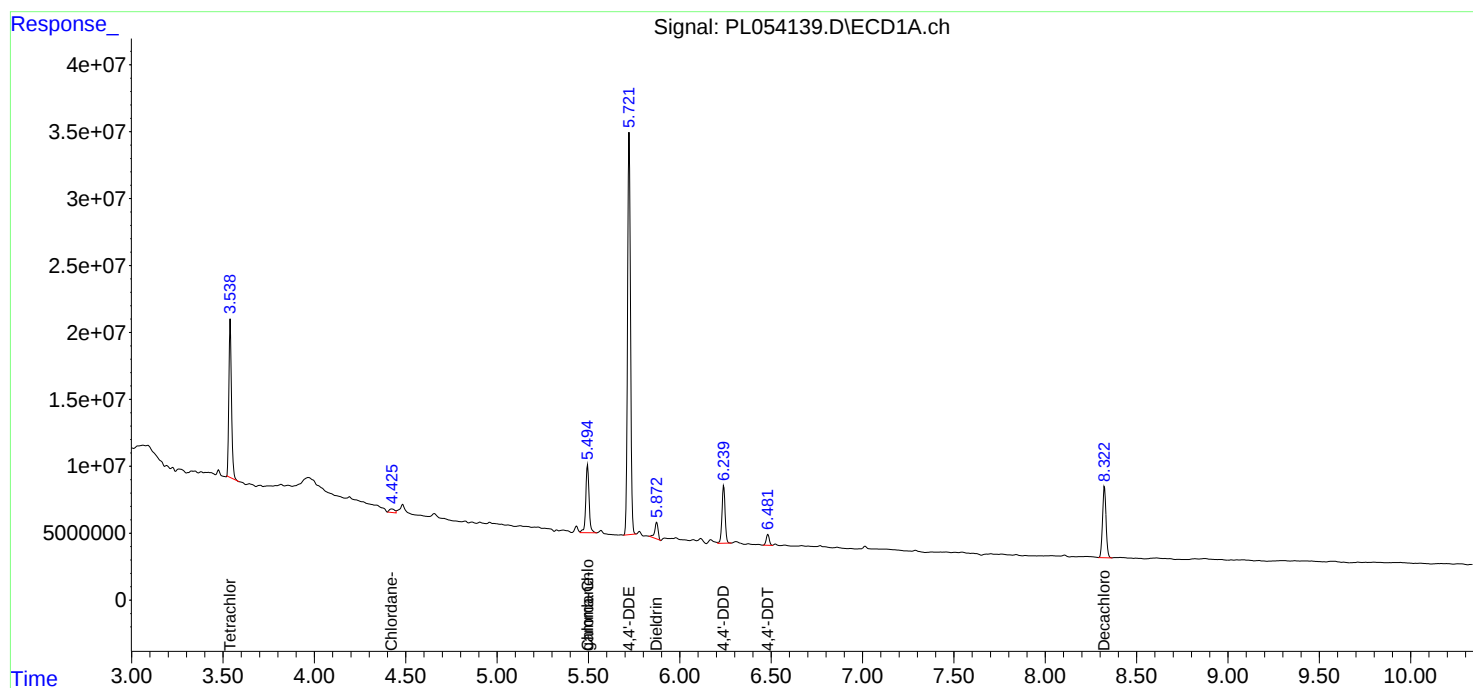


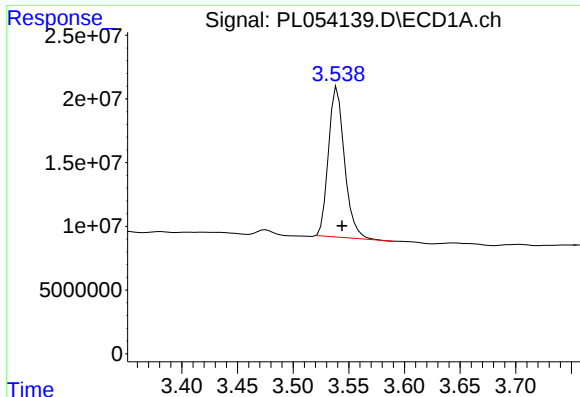

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 117538954
Conc: 10.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
HILTON-STOCKPILE

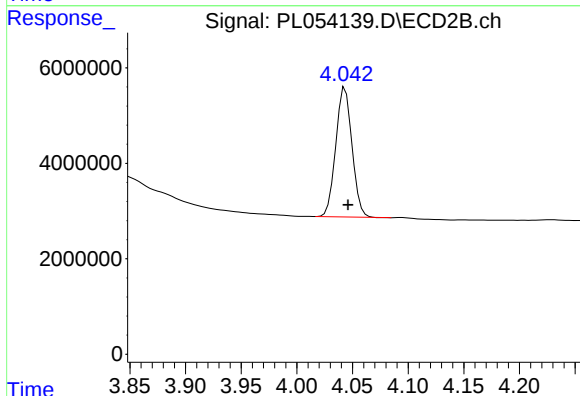


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.002 min
Response: 27485946
Conc: 10.98 ng/ml

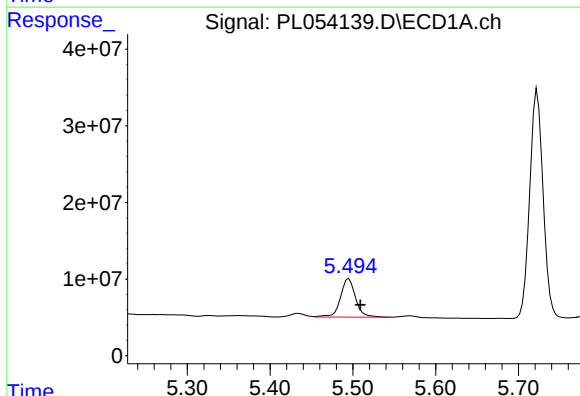


#10 gamma-Chlordane

R.T.: 5.495 min
Delta R.T.: -0.014 min
Response: 63524437
Conc: 4.66 ng/ml

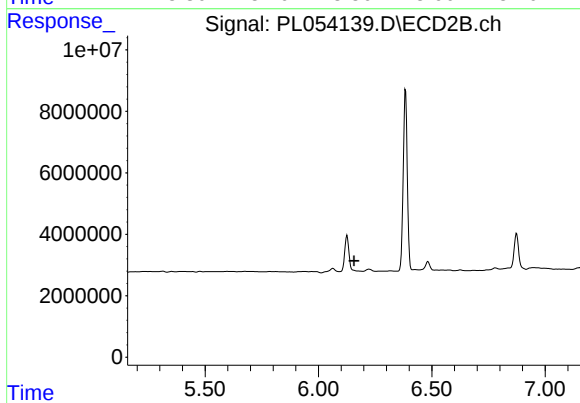

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

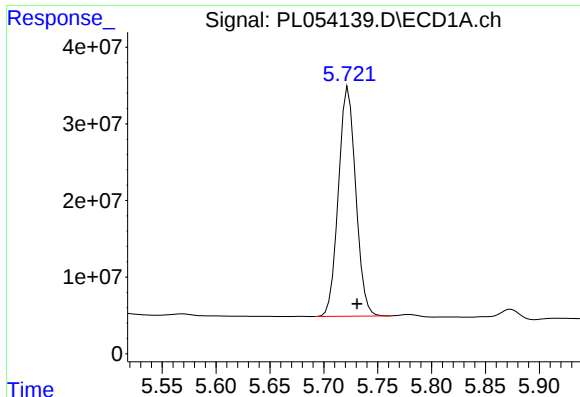

#12 4,4'-DDE


R.T.: 5.723 min
Delta R.T.: -0.008 min
Response: 334482911
Conc: 28.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
HILTON-STOCKPILE

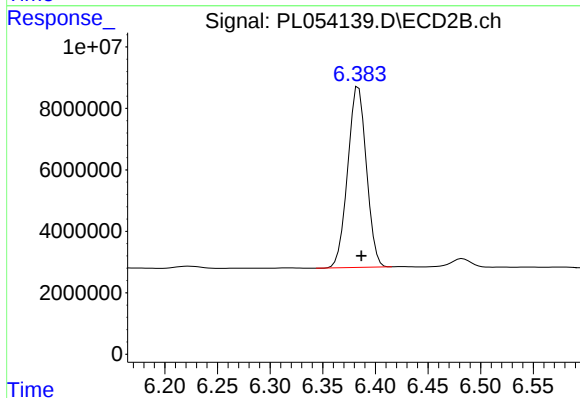


#12 4,4'-DDE

R.T.: 6.384 min
Delta R.T.: -0.003 min
Response: 73009155
Conc: 25.92 ng/ml

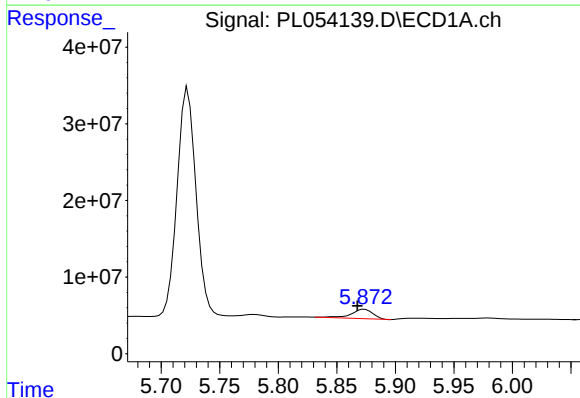


#13 Dieldrin

R.T.: 5.874 min
Delta R.T.: 0.006 min
Response: 16006925
Conc: 1.23 ng/ml

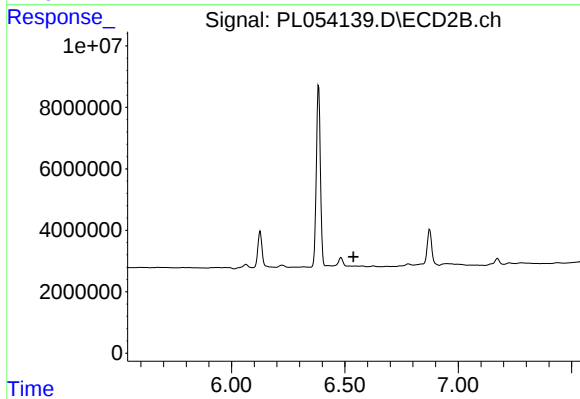

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.538 min
Response: 0
Conc: N.D.

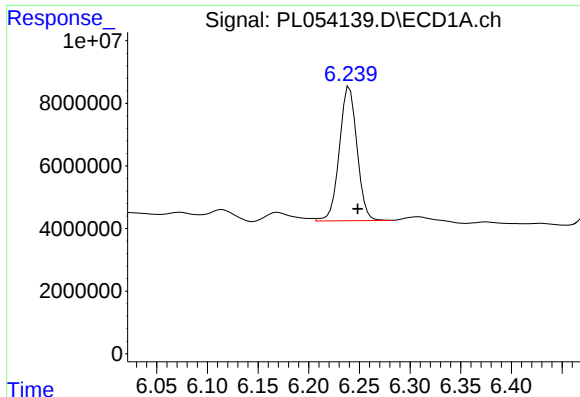

#16 4,4'-DDD


R.T.: 6.240 min
Delta R.T.: -0.008 min
Response: 51781258
Conc: 5.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
HILTON-STOCKPILE

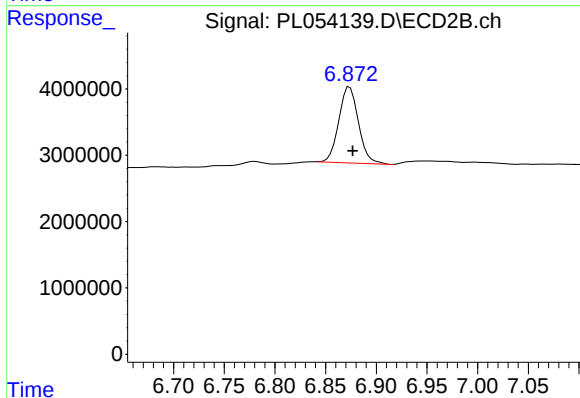


#16 4,4'-DDD

R.T.: 6.874 min
Delta R.T.: -0.003 min
Response: 15471403
Conc: 7.42 ng/ml

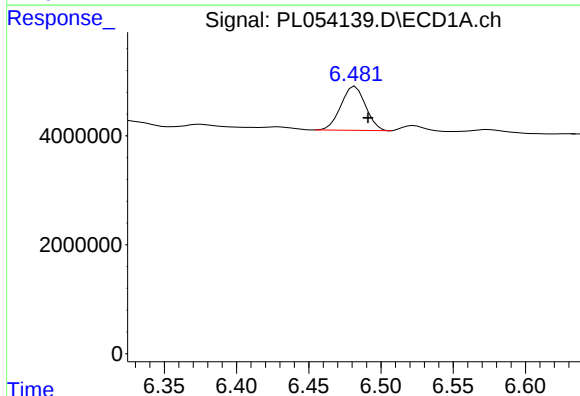


#17 4,4'-DDT

R.T.: 6.482 min
Delta R.T.: -0.009 min
Response: 9593323
Conc: 0.97 ng/ml

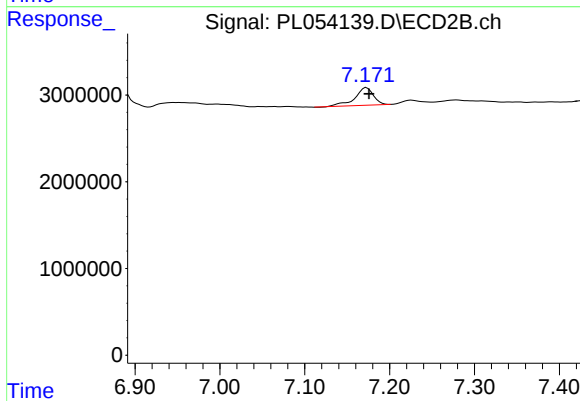

#17 4,4'-DDT


R.T.: 7.173 min
Delta R.T.: -0.003 min
Response: 3105189
Conc: 1.34 ng/ml

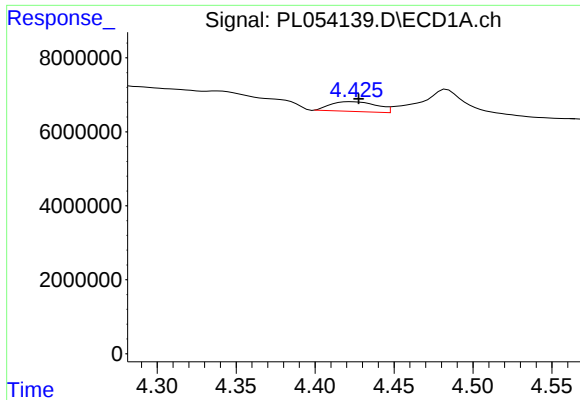

#23 Chlordane-1


R.T.: 4.423 min
Delta R.T.: -0.005 min
Response: 5347889
Conc: 15.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
HILTON-STOCKPILE

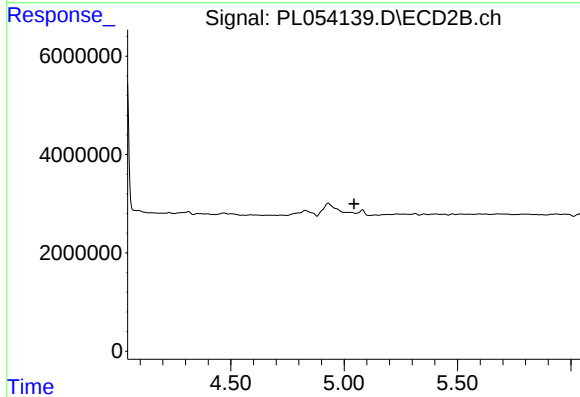


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.043 min
Response: 0
Conc: N.D.

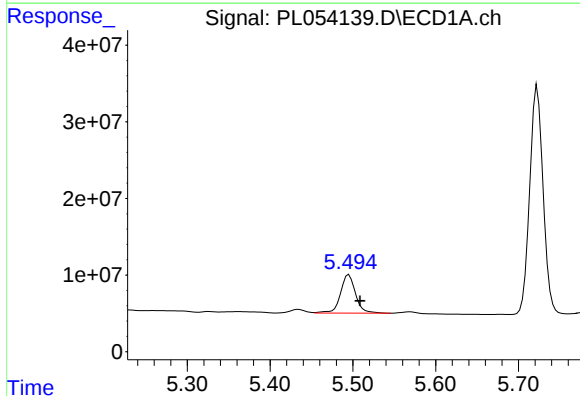


#25 Chlordane-3

R.T.: 5.495 min
Delta R.T.: -0.014 min
Response: 63524437
Conc: 55.11 ng/ml

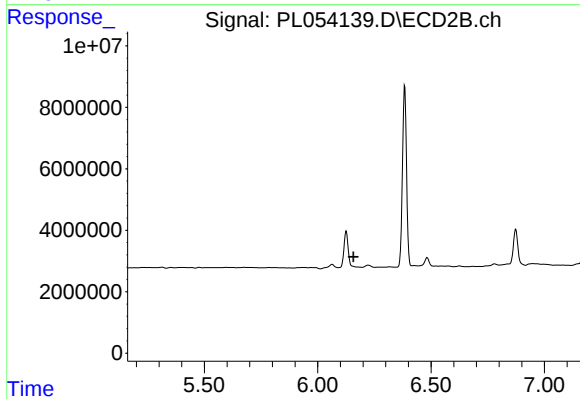

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

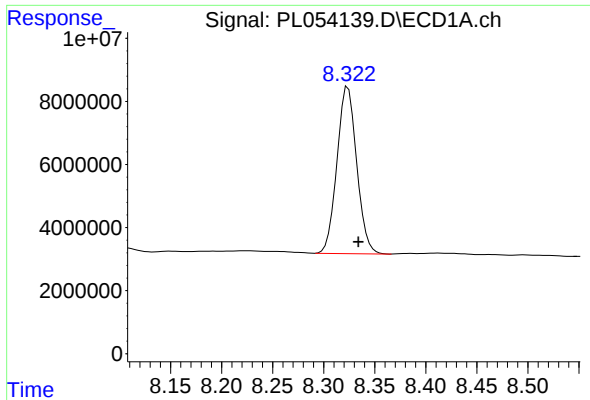

#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.010 min
Response: 71235739
Conc: 7.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
HILTON-STOCKPILE

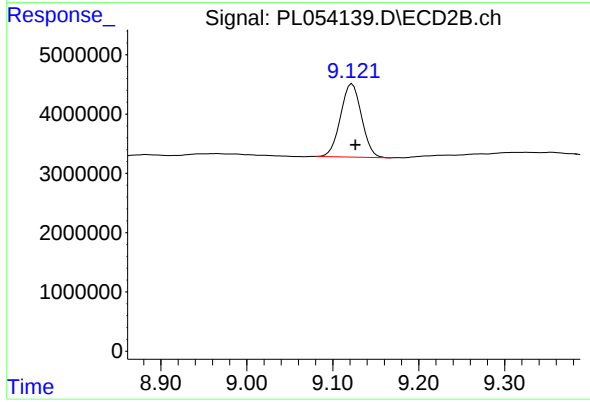

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.004 min
Response: 21067332
Conc: 7.48 ng/ml