

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110819\
 Data File : PL054138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2019 13:11
 Operator : SG\AJ
 Sample : K5728-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CS-001-4

Manual Integrations
 APPROVED

Ankita
 11/11/2019 1:18:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 22:04:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	4.044	223.1E6	49277005	20.580	19.692
28)	SA Decachlor...	8.324	9.122	156.1E6	49301886	15.909	17.508
Target Compounds							
10)	B gamma-Chl...	5.501	6.155	7180130	2263740	0.526m	0.776 #
11)	B alpha-Chl...	5.559	6.229	7552670	3652034	0.568m	1.251 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110819\
Data File : PL054138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2019 13:11
Operator : SG\AJ
Sample : K5728-11
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CS-001-4


Manual Integrations
APPROVED

Ankita
11/11/2019 1:18:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 22:04:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

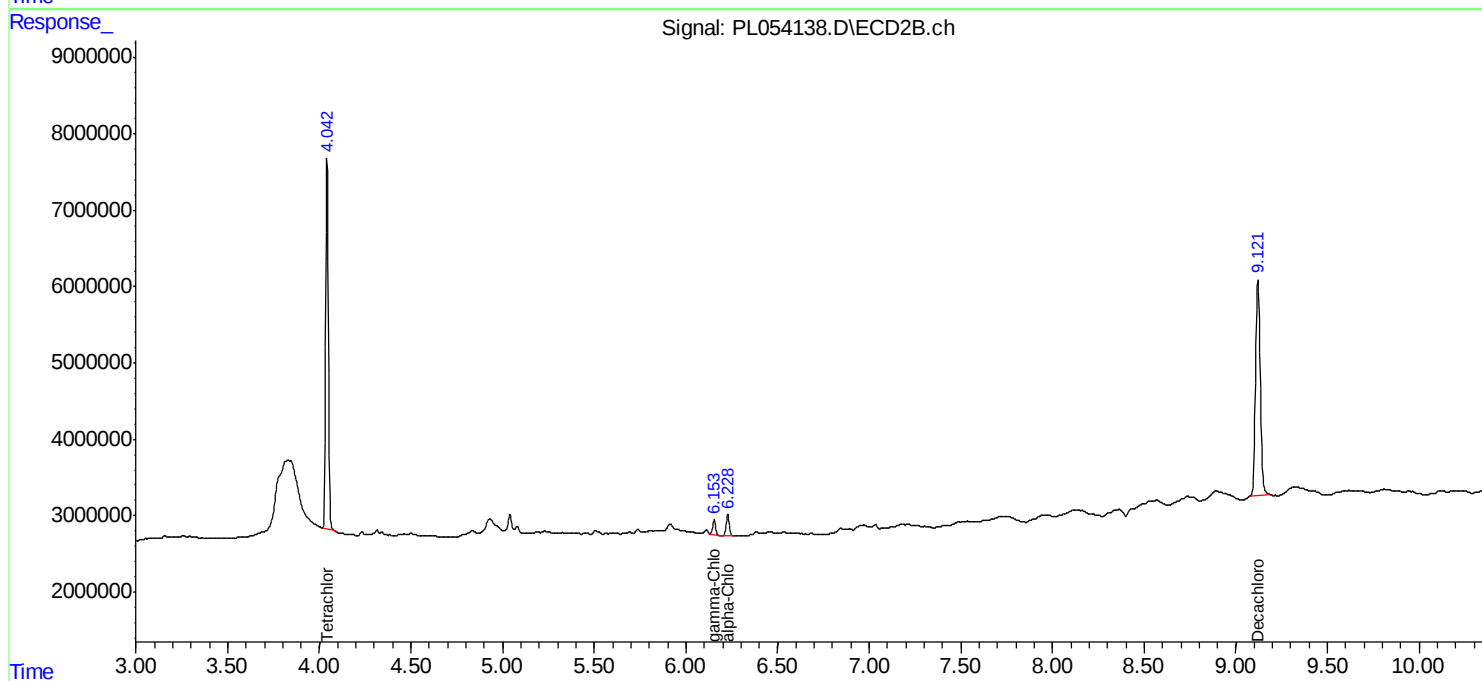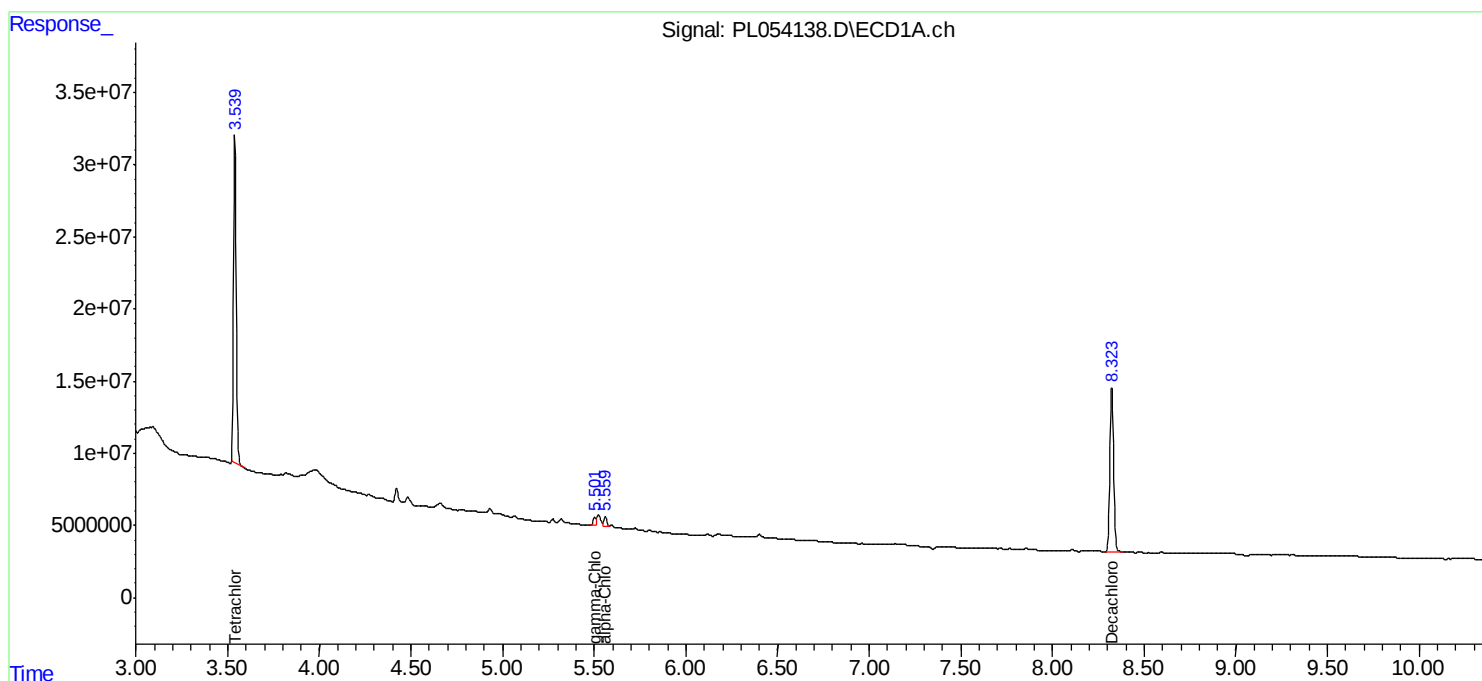

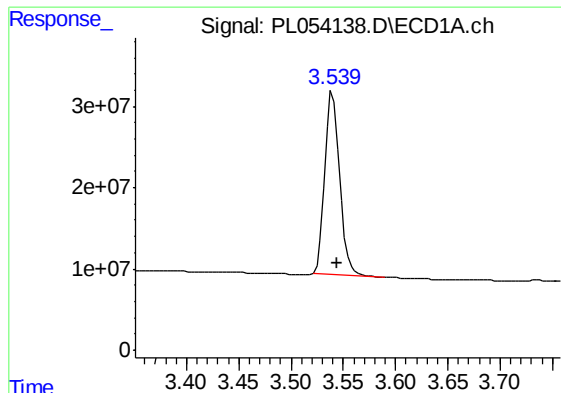


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 223072079
Conc: 20.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-001-4


Manual Integrations
APPROVED

Ankita
11/11/2019 1:18:55 PM

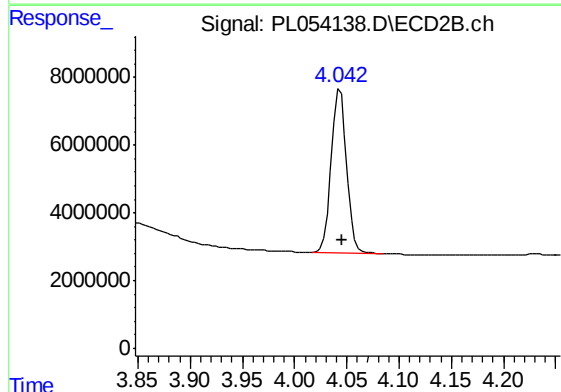


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 49277005
Conc: 19.69 ng/ml

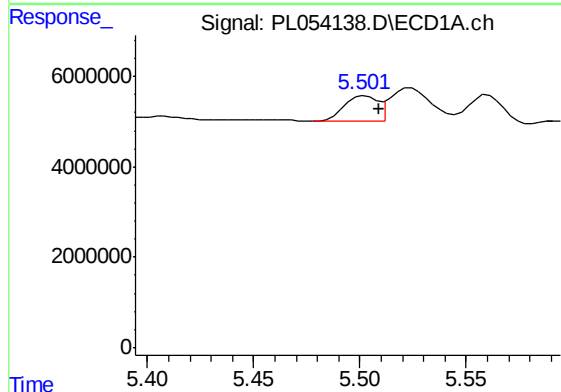


#10 gamma-Chlordane

R.T.: 5.501 min
Delta R.T.: -0.008 min
Response: 7180130
Conc: 0.53 ng/ml m

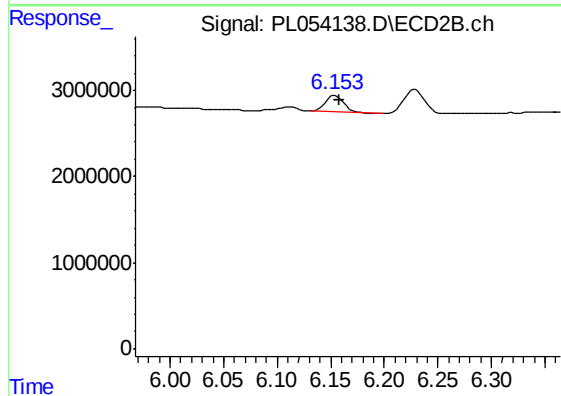

#10 gamma-Chlordane

R.T.: 6.155 min
Delta R.T.: -0.003 min
Response: 2263740
Conc: 0.78 ng/ml

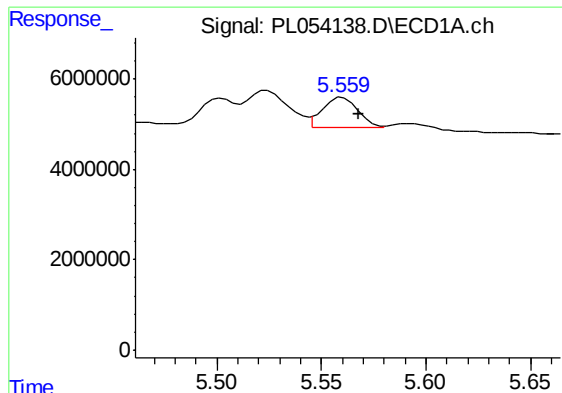


#11 alpha-Chlordane

R.T.: 5.559 min
Delta R.T.: -0.009 min
Response: 7552670
Conc: 0.57 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CS-001-4


Manual Integrations
APPROVED

Ankita
11/11/2019 1:18:55 PM

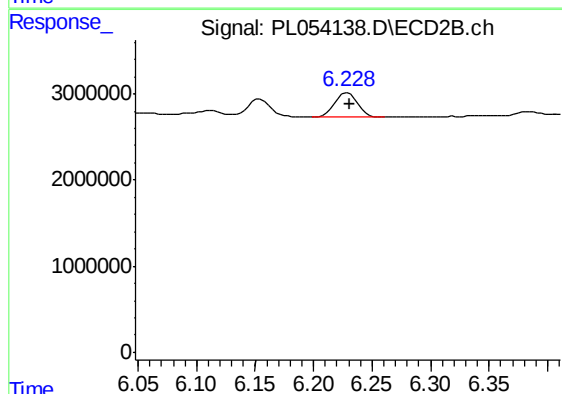


#11 alpha-Chlordane

R.T.: 6.229 min
Delta R.T.: -0.002 min
Response: 3652034
Conc: 1.25 ng/ml

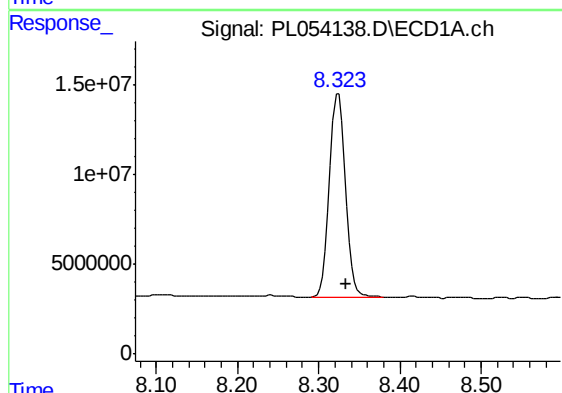

#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.010 min
Response: 156090401
Conc: 15.91 ng/ml

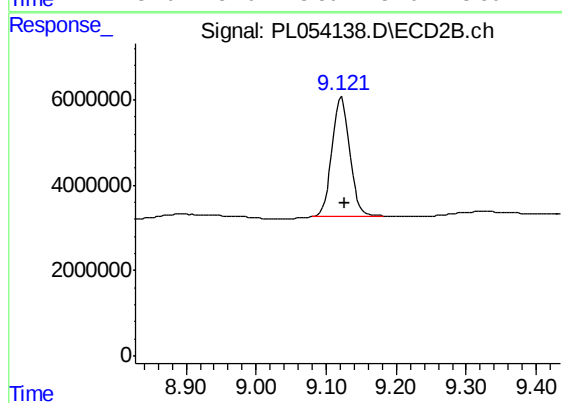

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.004 min
Response: 49301886
Conc: 17.51 ng/ml