

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110821\
 Data File : PL070820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2021 09:35
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 00:44:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
6) B	beta-BHC	0.000	6.757f	0 21614114	N.D.	25.226 #
23)	Chlordane-1	0.000	6.894	0 4987415	N.D.	102.707 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110821\
Data File : PL070820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2021 09:35
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 00:44:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

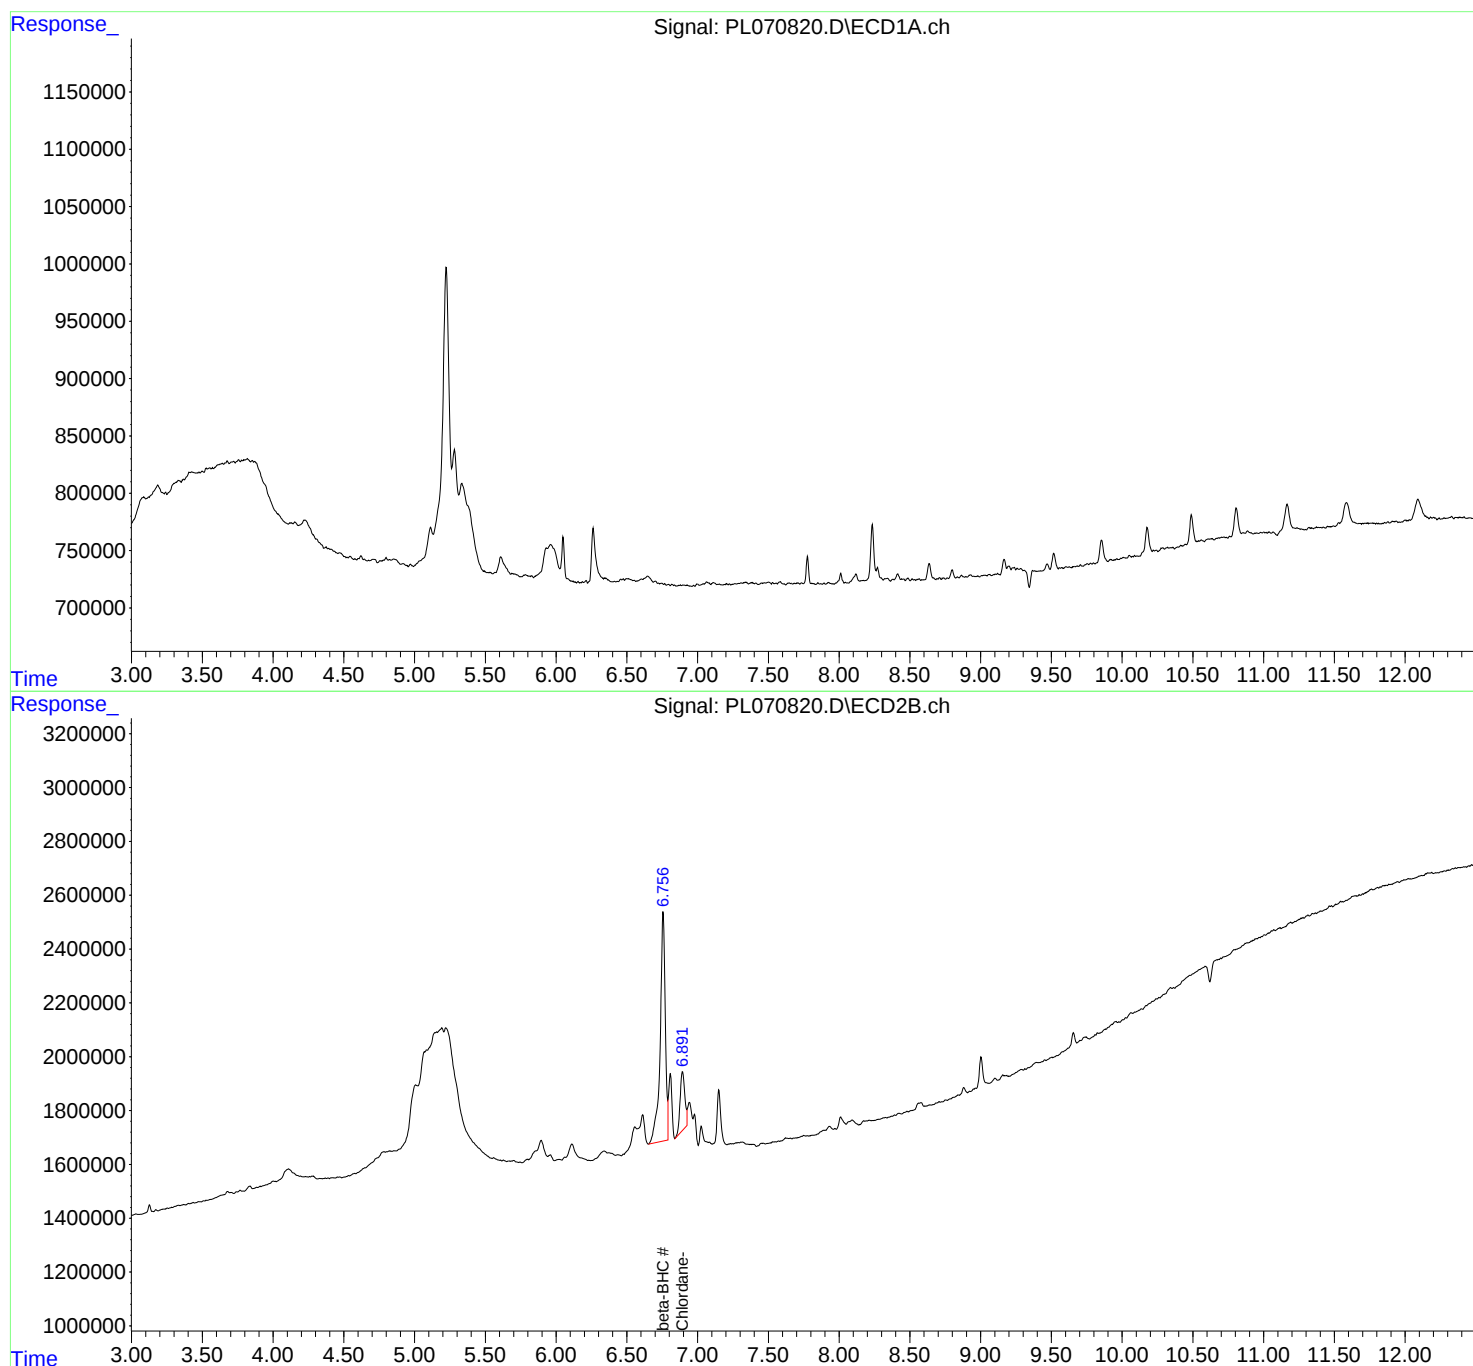

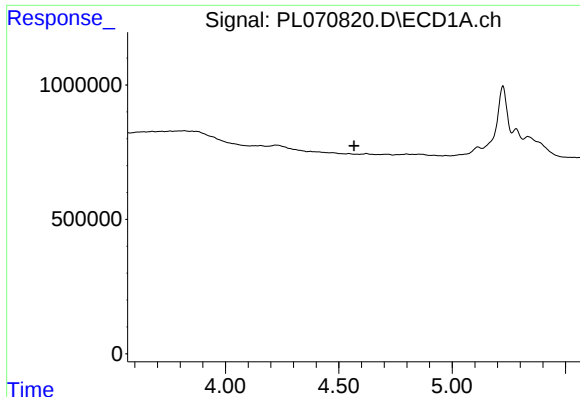


#1 Tetrachloro-m-xylene

```

      R.T.:      0.000 min
Exp R.T.  :      4.568 min
  Response:           0
    Conc:    N.D.


```

Instrument :
ECD_L
ClientSampleId :

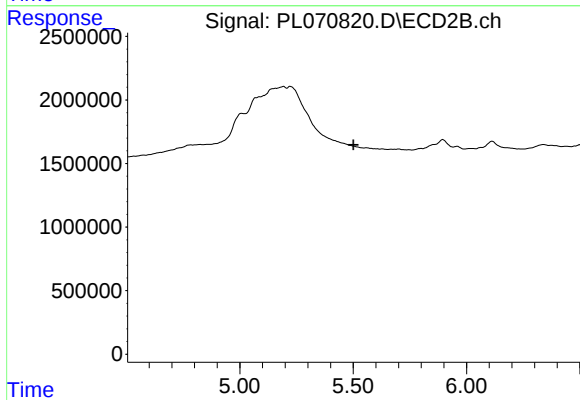

#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

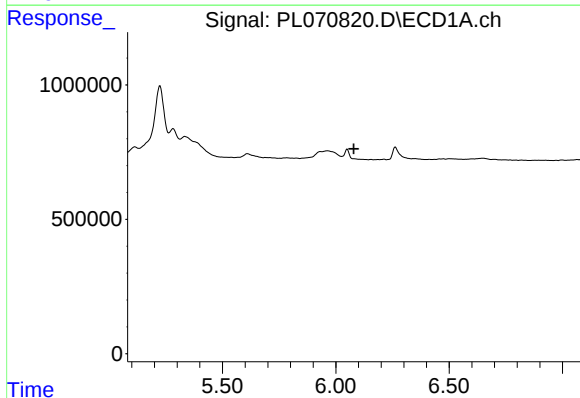


#6 beta-BHC

```

      R.T.:      0.000 min
Exp R.T.  :      6.079 min
  Response:           0
    Conc:    N.D.

```

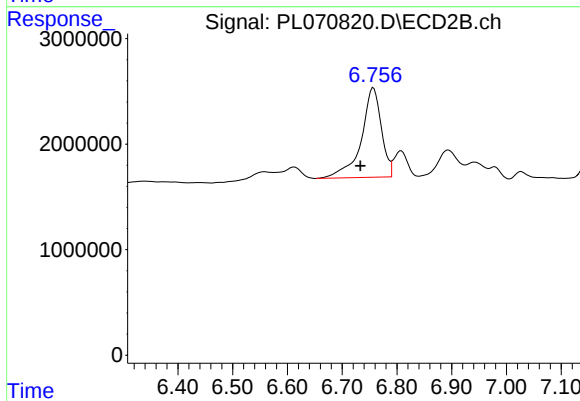


#6 beta-BHC

```

      R.T.:      6.757 min
Delta R.T.:      0.023 min
Response: 21614114
      Conc: 25.23 ng/ml


```

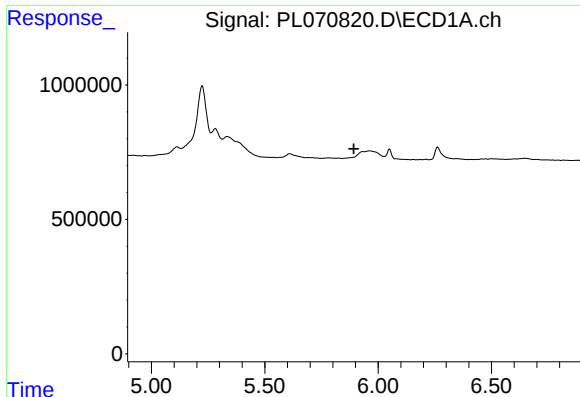

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.893 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

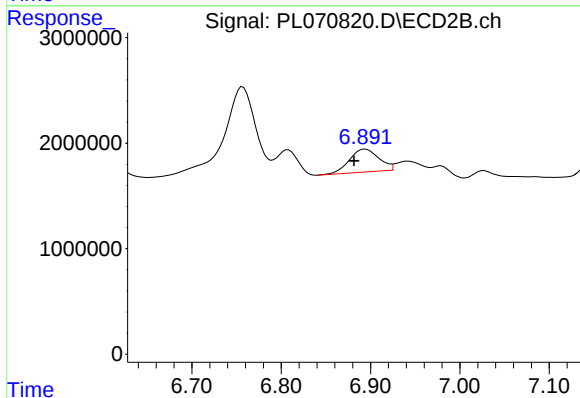


#23 Chlordane-1

R.T.: 6.894 min
Delta R.T.: 0.012 min
Response: 4987415
Conc: 102.71 ng/ml

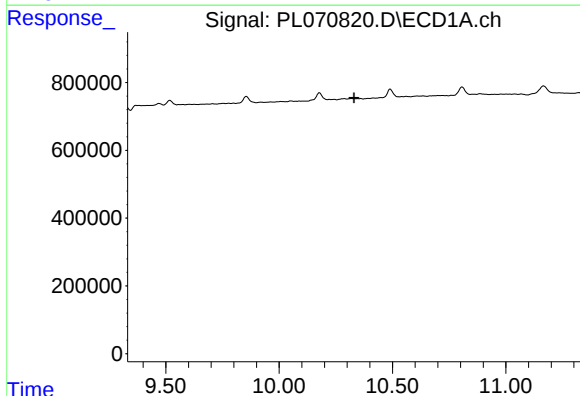

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 10.330 min
Response: 0
Conc: N.D.

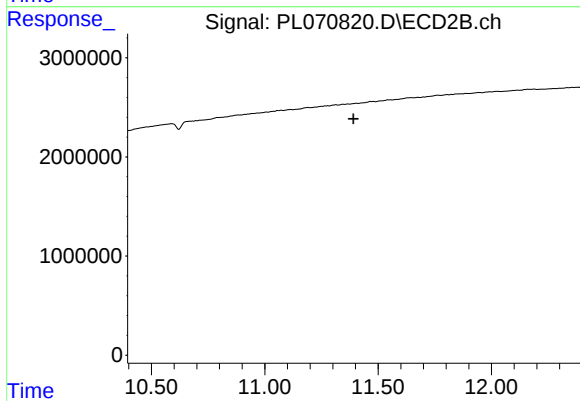

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 11.392 min
Response: 0
Conc: N.D.