

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL110821\  
 Data File : PL070829.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Nov 2021 15:15  
 Operator : AR\AJ  
 Sample : M4497-07  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 09 00:46:30 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL110321.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Nov 04 19:28:07 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1   | RT#2   | Resp#1  | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-----------------|--------|--------|---------|----------|--------|---------|
| -----                       |                 |        |        |         |          |        |         |
| System Monitoring Compounds |                 |        |        |         |          |        |         |
| 1)                          | SA Tetrachlo... | 4.570  | 5.505  | 6804686 | 16935279 | 13.893 | 13.432  |
| 28)                         | SA Decachlor... | 10.335 | 11.399 | 9774844 | 19158501 | 14.305 | 14.325  |
| Target Compounds            |                 |        |        |         |          |        |         |
| 11)                         | B alpha-Chl...  | 0.000  | 8.317  | 0       | 658718   | N.D.   | 0.433 # |
| 16)                         | A 4,4'-DDD      | 0.000  | 9.043  | 0       | 514305   | N.D.   | 0.427 # |
| 17)                         | MA 4,4'-DDT     | 0.000  | 9.361  | 0       | 703134   | N.D.   | 0.557 # |
| 26)                         | Chlordane-4     | 0.000  | 8.317  | 0       | 658718   | N.D.   | 2.714 # |
| -----                       |                 |        |        |         |          |        |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL110821\  
Data File : PL070829.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 08 Nov 2021 15:15  
Operator : AR\AJ  
Sample : M4497-07  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 09 00:46:30 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL110321.M  
Quant Title : GC Extractables  
QLast Update : Thu Nov 04 19:28:07 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

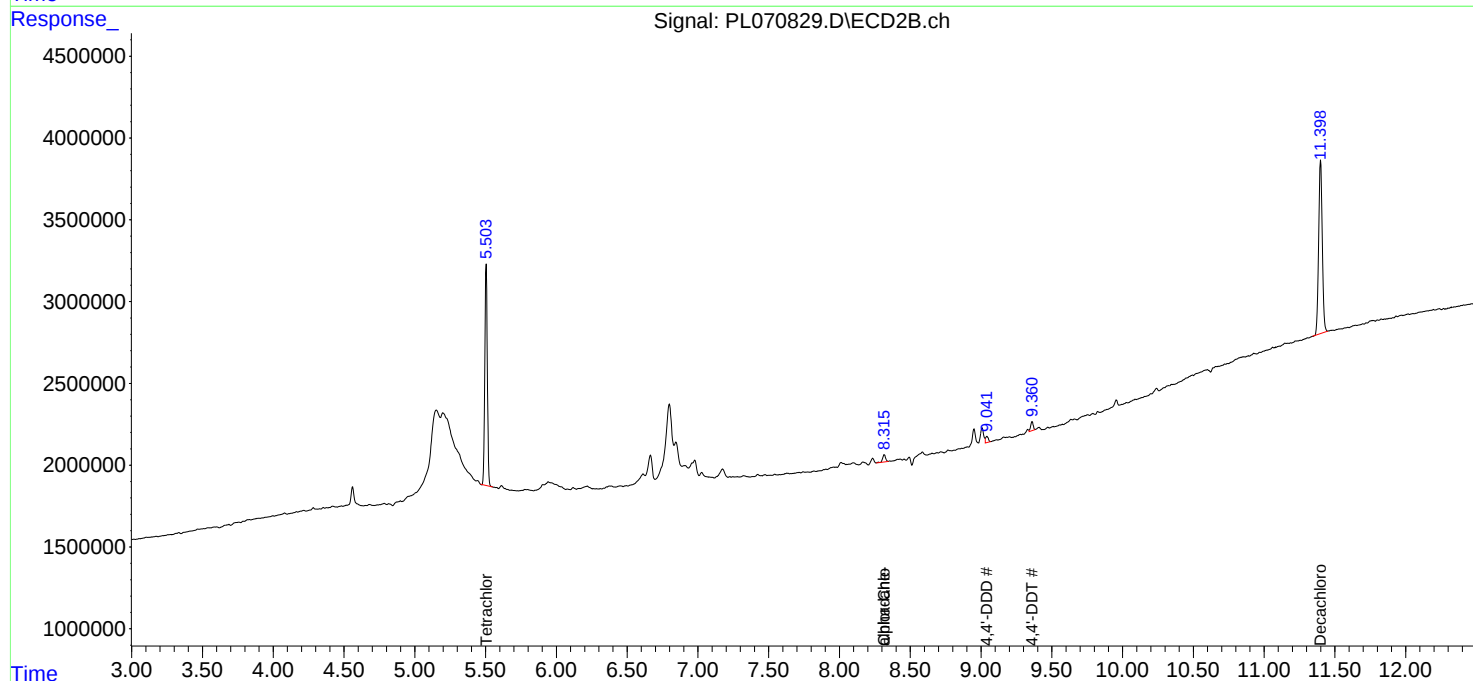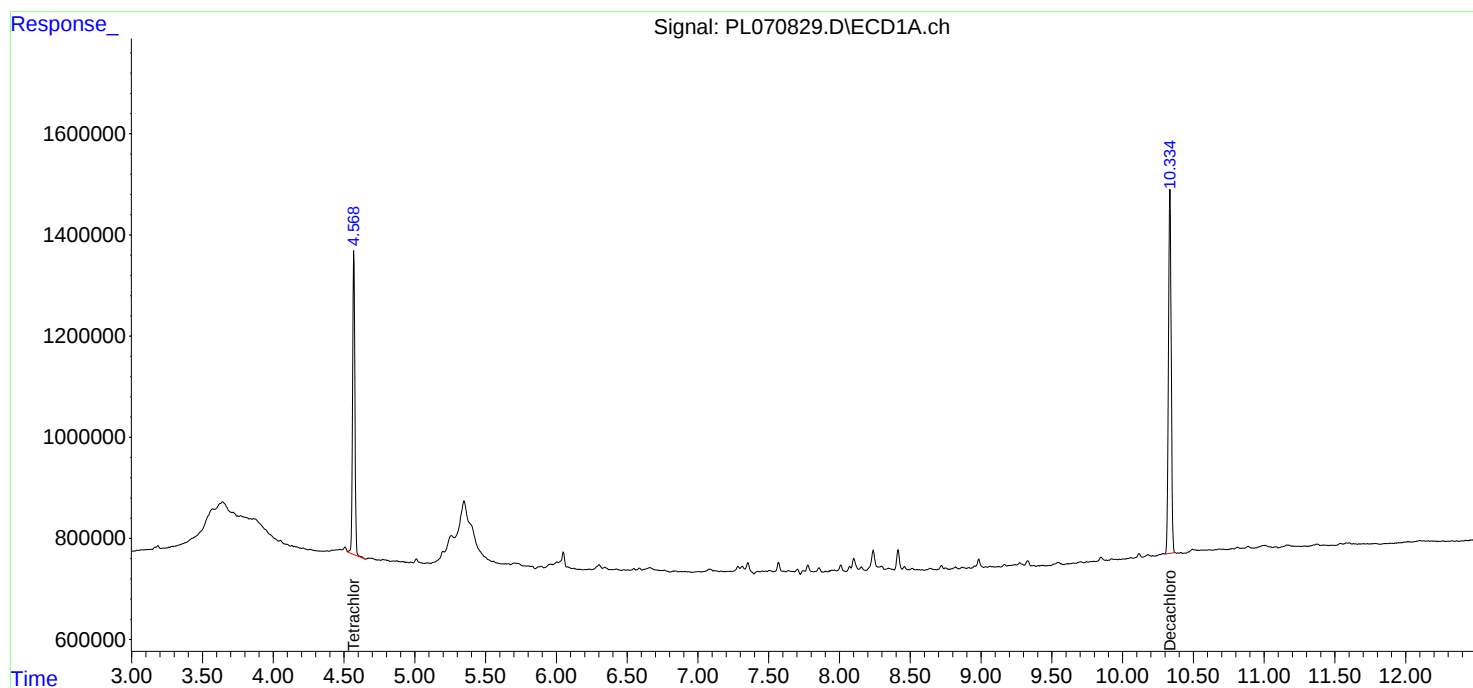


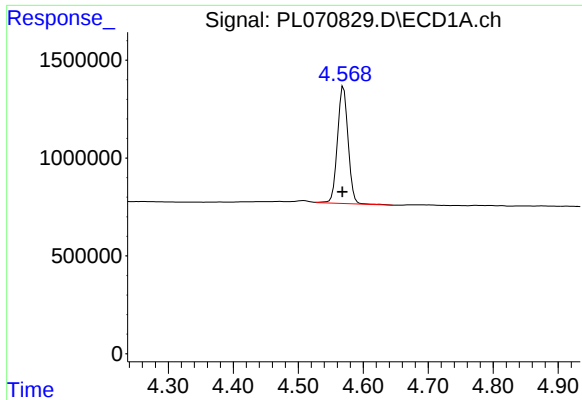

#1 Tetrachloro-m-xylene


R.T.: 4.570 min  
Delta R.T.: 0.002 min  
Response: 6804686  
Conc: 13.89 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

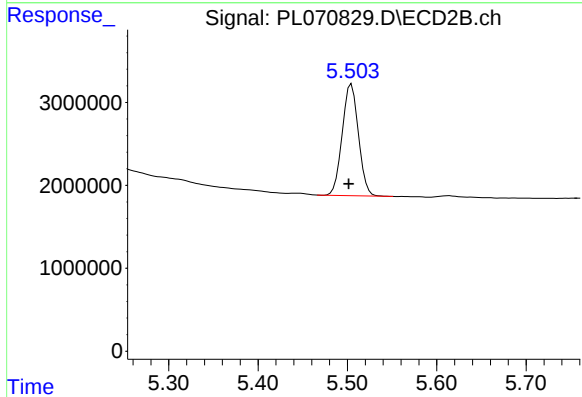


#1 Tetrachloro-m-xylene

R.T.: 5.505 min  
Delta R.T.: 0.003 min  
Response: 16935279  
Conc: 13.43 ng/ml

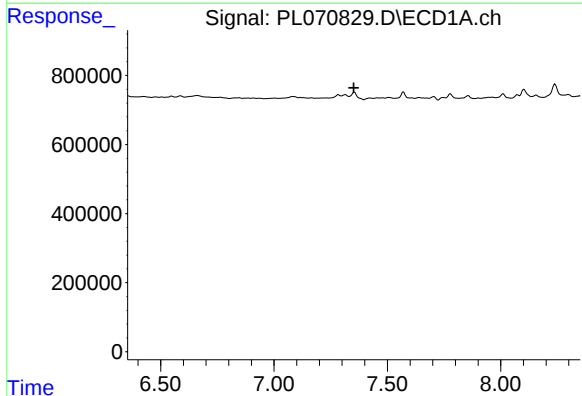


#11 alpha-Chlordane

R.T.: 0.000 min  
Exp R.T. : 7.352 min  
Response: 0  
Conc: N.D.

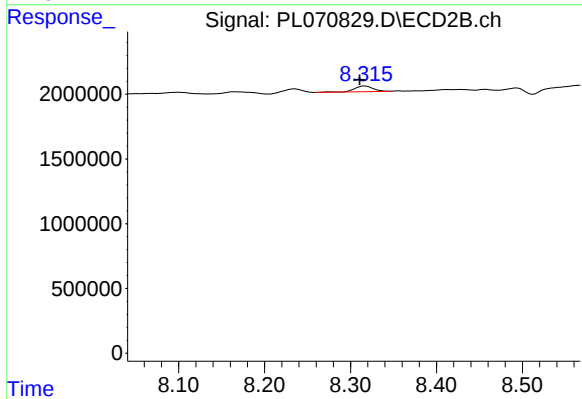

#11 alpha-Chlordane


R.T.: 8.317 min  
Delta R.T.: 0.006 min  
Response: 658718  
Conc: 0.43 ng/ml

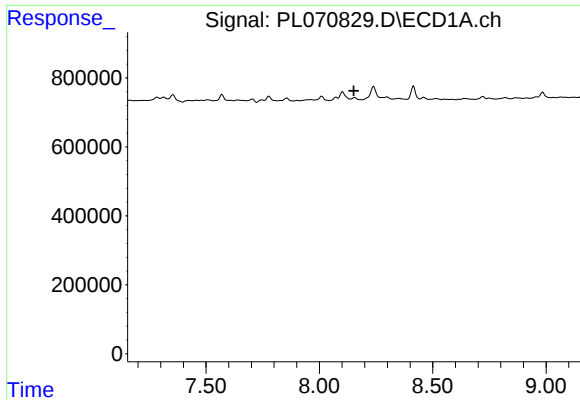

#16 4,4'-DDD


R.T.: 0.000 min  
Exp R.T.: 8.152 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

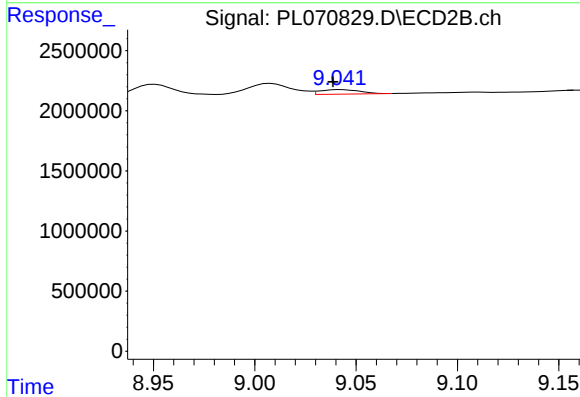


#16 4,4'-DDD

R.T.: 9.043 min  
Delta R.T.: 0.004 min  
Response: 514305  
Conc: 0.43 ng/ml

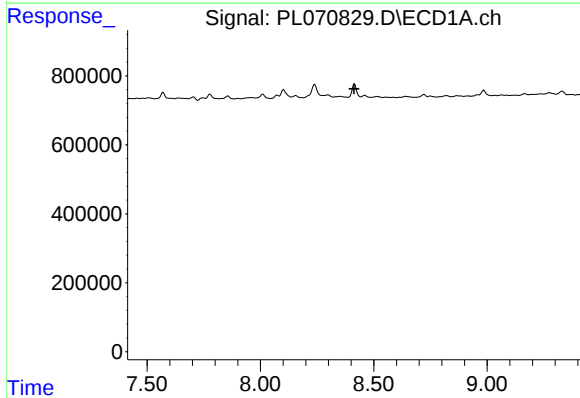


#17 4,4'-DDT

R.T.: 0.000 min  
Exp R.T.: 8.413 min  
Response: 0  
Conc: N.D.

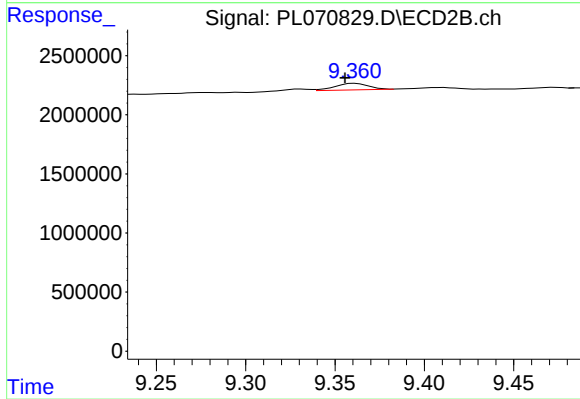

#17 4,4'-DDT


R.T.: 9.361 min  
Delta R.T.: 0.005 min  
Response: 703134  
Conc: 0.56 ng/ml

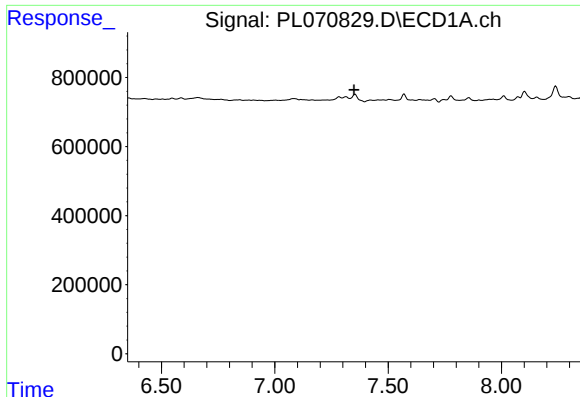

#26 Chlordane-4


R.T.: 0.000 min  
Exp R.T.: 7.350 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

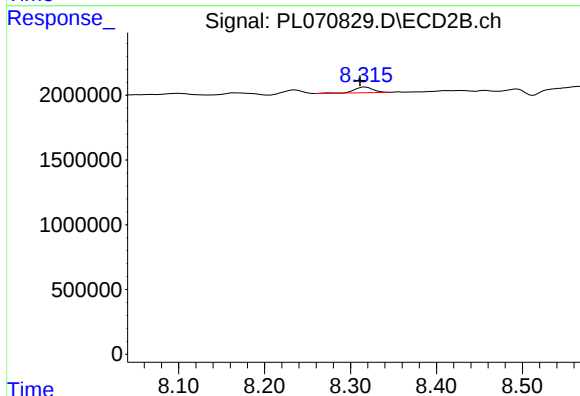


#26 Chlordane-4

R.T.: 8.317 min  
Delta R.T.: 0.006 min  
Response: 658718  
Conc: 2.71 ng/ml

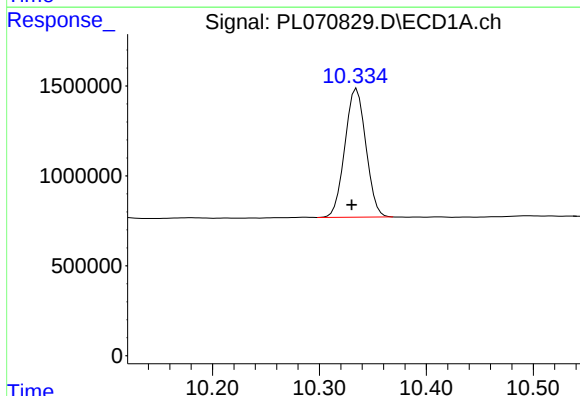

#28 Decachlorobiphenyl

R.T.: 10.335 min  
Delta R.T.: 0.005 min  
Response: 9774844  
Conc: 14.31 ng/ml

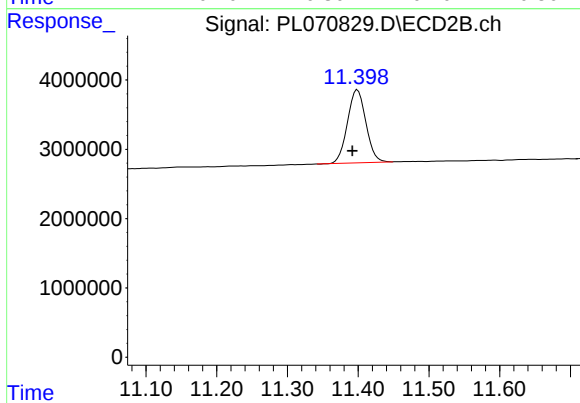

#28 Decachlorobiphenyl

R.T.: 11.399 min  
Delta R.T.: 0.007 min  
Response: 19158501  
Conc: 14.33 ng/ml