

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110821\
 Data File : PL070830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2021 15:32
 Operator : AR\AJ
 Sample : M4541-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 00:46:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.570	5.505	5820967	14800154	11.884	11.738
28)	SA Decachlor...	10.335	11.399	7568076	15296327	11.076	11.438
Target Compounds							
6)	B beta-BHC	0.000	6.740	0	1256610	N.D.	1.467 #
10)	B gamma-Chl...	0.000	8.237	0	1290775	N.D.	0.834 #
11)	B alpha-Chl...	0.000	8.318	0	992759	N.D.	0.653 #
17)	MA 4,4'-DDT	0.000	9.330f	0	1272191	N.D.	1.008 #
25)	Chlordane-3	0.000	8.237	0	1290775	N.D.	6.386 #
26)	Chlordane-4	0.000	8.318	0	992759	N.D.	4.091 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110821\
Data File : PL070830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2021 15:32
Operator : AR\AJ
Sample : M4541-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 00:46:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

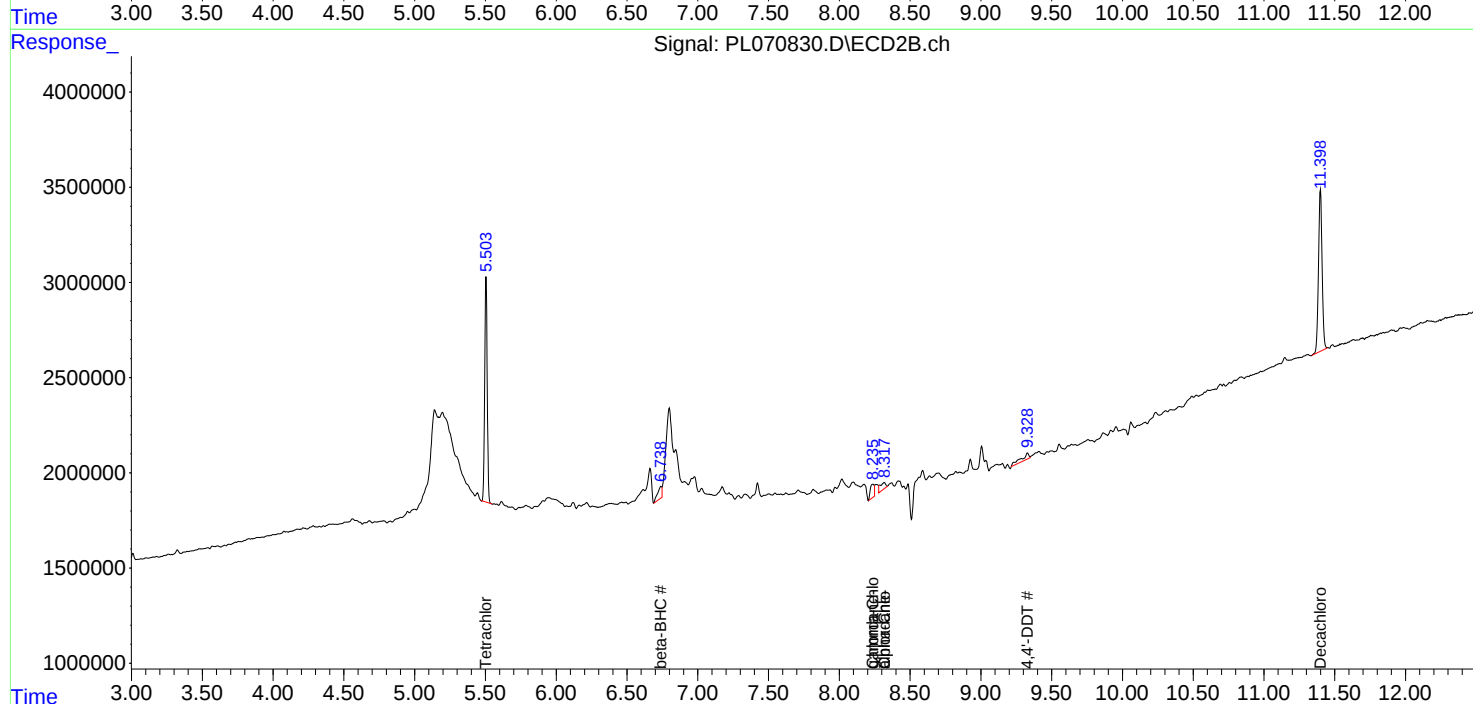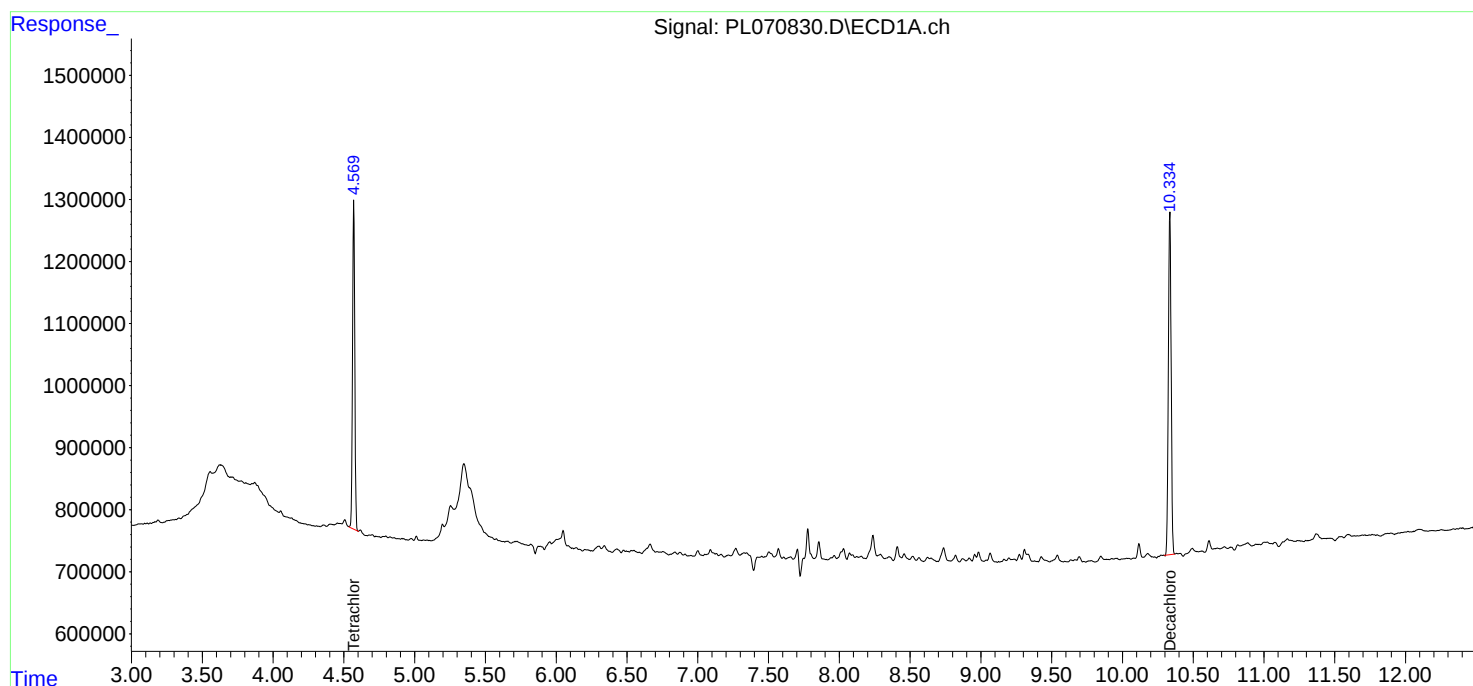


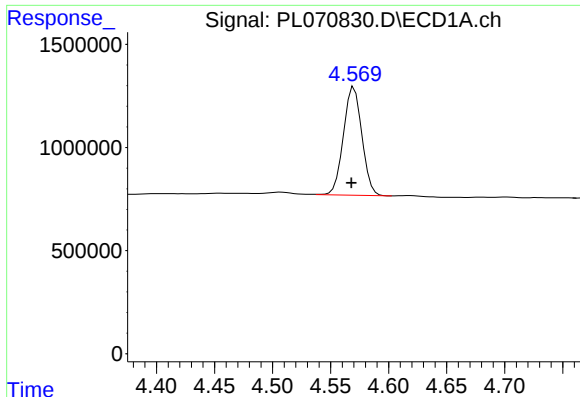

#1 Tetrachloro-m-xylene


R.T.: 4.570 min
Delta R.T.: 0.002 min
Response: 5820967
Conc: 11.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

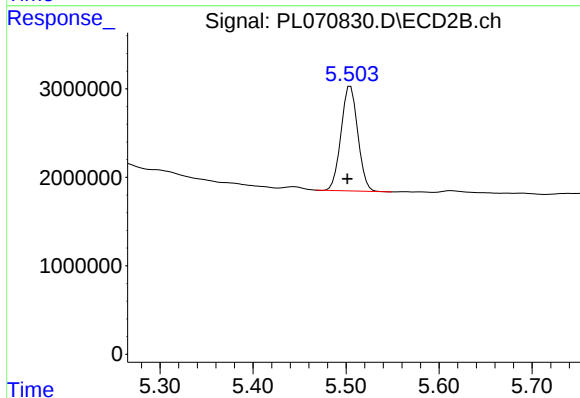


#1 Tetrachloro-m-xylene

R.T.: 5.505 min
Delta R.T.: 0.003 min
Response: 14800154
Conc: 11.74 ng/ml

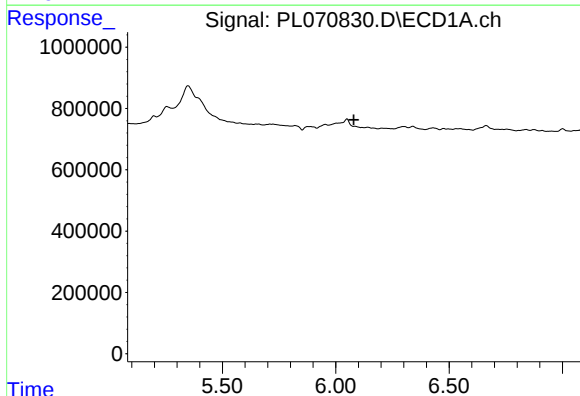


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.079 min
Response: 0
Conc: N.D.

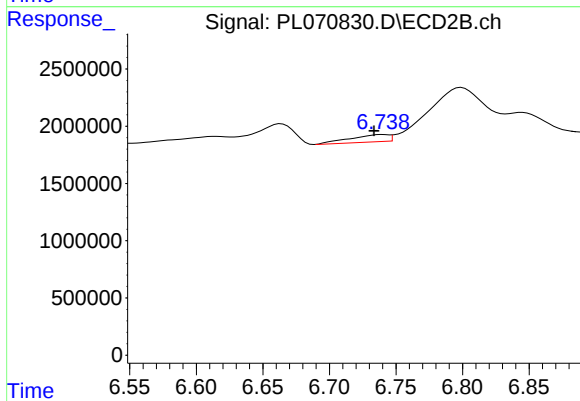

#6 beta-BHC


R.T.: 6.740 min
Delta R.T.: 0.006 min
Response: 1256610
Conc: 1.47 ng/ml

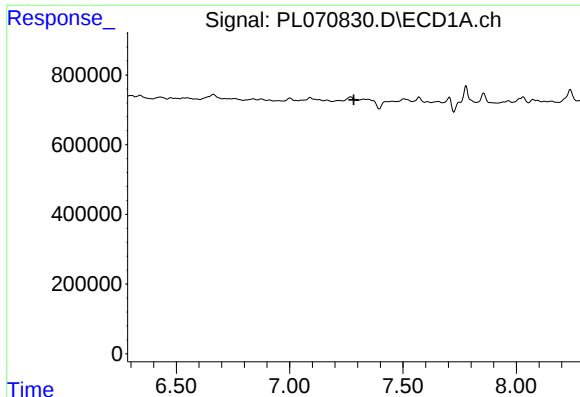

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

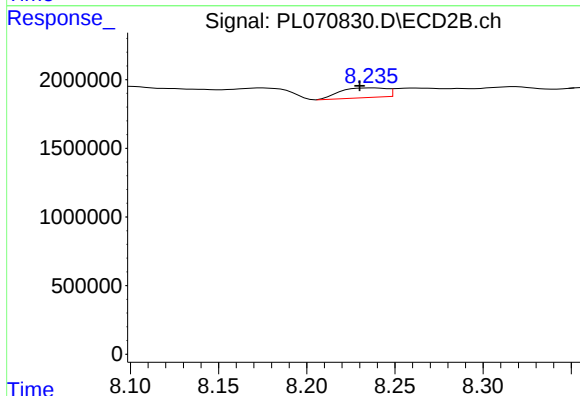


#10 gamma-Chlordane

R.T.: 8.237 min
Delta R.T.: 0.007 min
Response: 1290775
Conc: 0.83 ng/ml

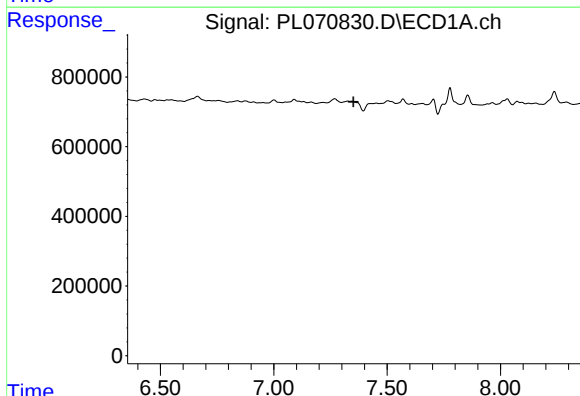


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.352 min
Response: 0
Conc: N.D.

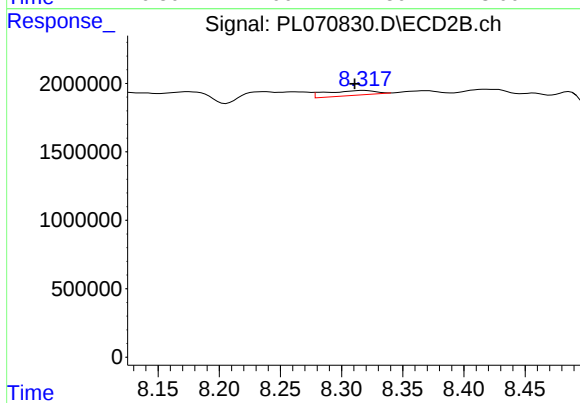

#11 alpha-Chlordane


R.T.: 8.318 min
Delta R.T.: 0.008 min
Response: 992759
Conc: 0.65 ng/ml

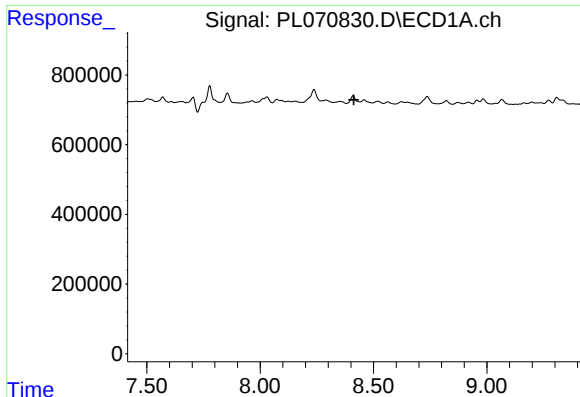

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.413 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

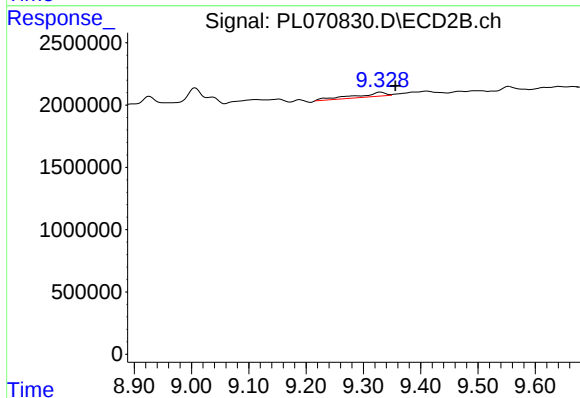


#17 4,4'-DDT

R.T.: 9.330 min
Delta R.T.: -0.026 min
Response: 1272191
Conc: 1.01 ng/ml

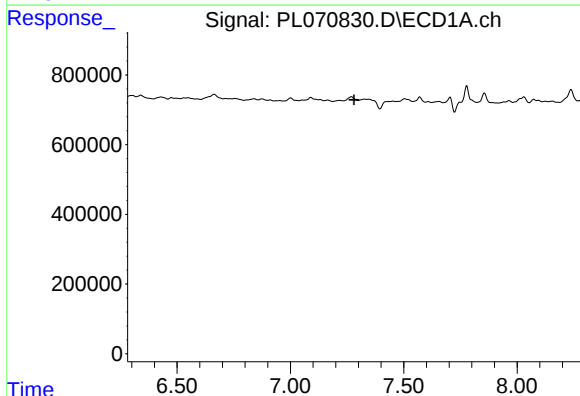


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.281 min
Response: 0
Conc: N.D.

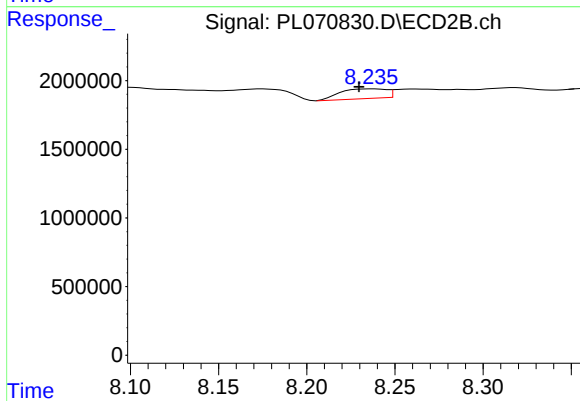

#25 Chlordane-3


R.T.: 8.237 min
Delta R.T.: 0.008 min
Response: 1290775
Conc: 6.39 ng/ml

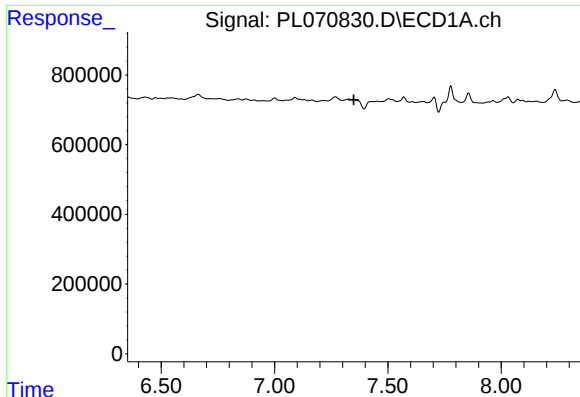

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

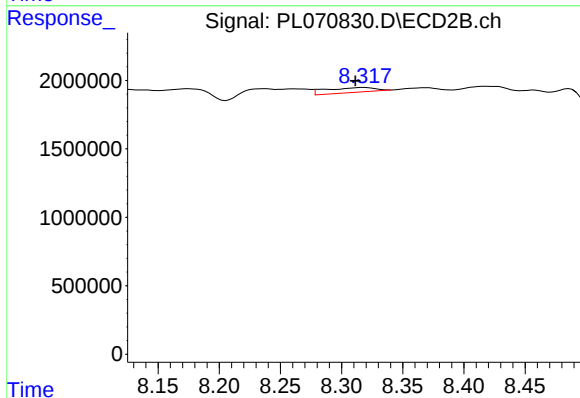


#26 Chlordane-4

R.T.: 8.318 min
Delta R.T.: 0.007 min
Response: 992759
Conc: 4.09 ng/ml

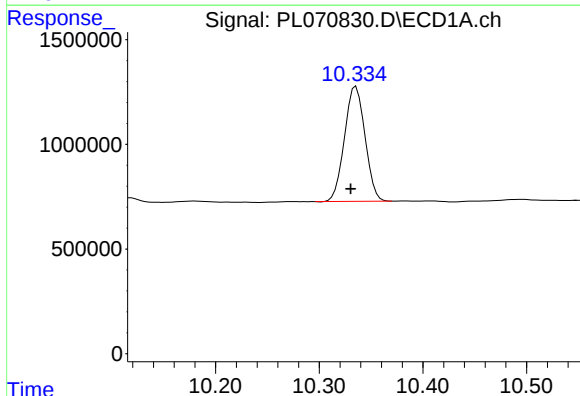

#28 Decachlorobiphenyl

R.T.: 10.335 min
Delta R.T.: 0.005 min
Response: 7568076
Conc: 11.08 ng/ml

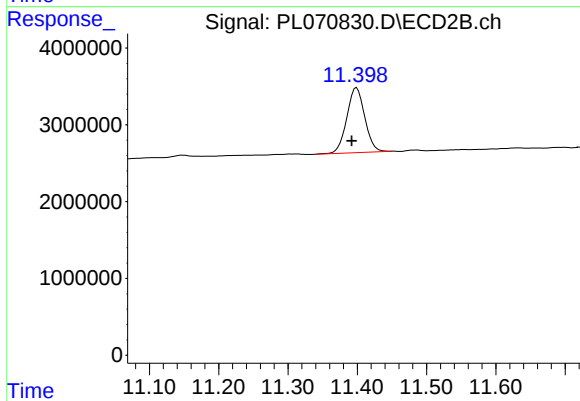

#28 Decachlorobiphenyl

R.T.: 11.399 min
Delta R.T.: 0.007 min
Response: 15296327
Conc: 11.44 ng/ml