

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110821\
 Data File : PL070847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2021 22:58
 Operator : AR\AJ
 Sample : M4574-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 00:50:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.567	5.501	6749960	17781823	13.781	14.103
28)	SA Decachlor...	10.330	11.391	10121143	21471886	14.812	16.055
Target Compounds							
6)	B beta-BHC	0.000	6.731	0	2102271	N.D.	2.454 #
10)	B gamma-Chl...	0.000	8.231	0	1087747	N.D.	0.703 #
11)	B alpha-Chl...	0.000	8.310	0	1096463	N.D.	0.721 #
17)	MA 4,4'-DDT	0.000	9.356	0	1286758	N.D.	1.020 #
21)	B Endrin ke...	0.000	10.004	0	861796	N.D.	0.600 #
22)	Mirex	0.000	10.481f	0	972602	N.D.	0.934 #
25)	Chlordane-3	0.000	8.231	0	1087747	N.D.	5.381 #
26)	Chlordane-4	0.000	8.310	0	1096463	N.D.	4.518 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110821\
Data File : PL070847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2021 22:58
Operator : AR\AJ
Sample : M4574-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 00:50:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

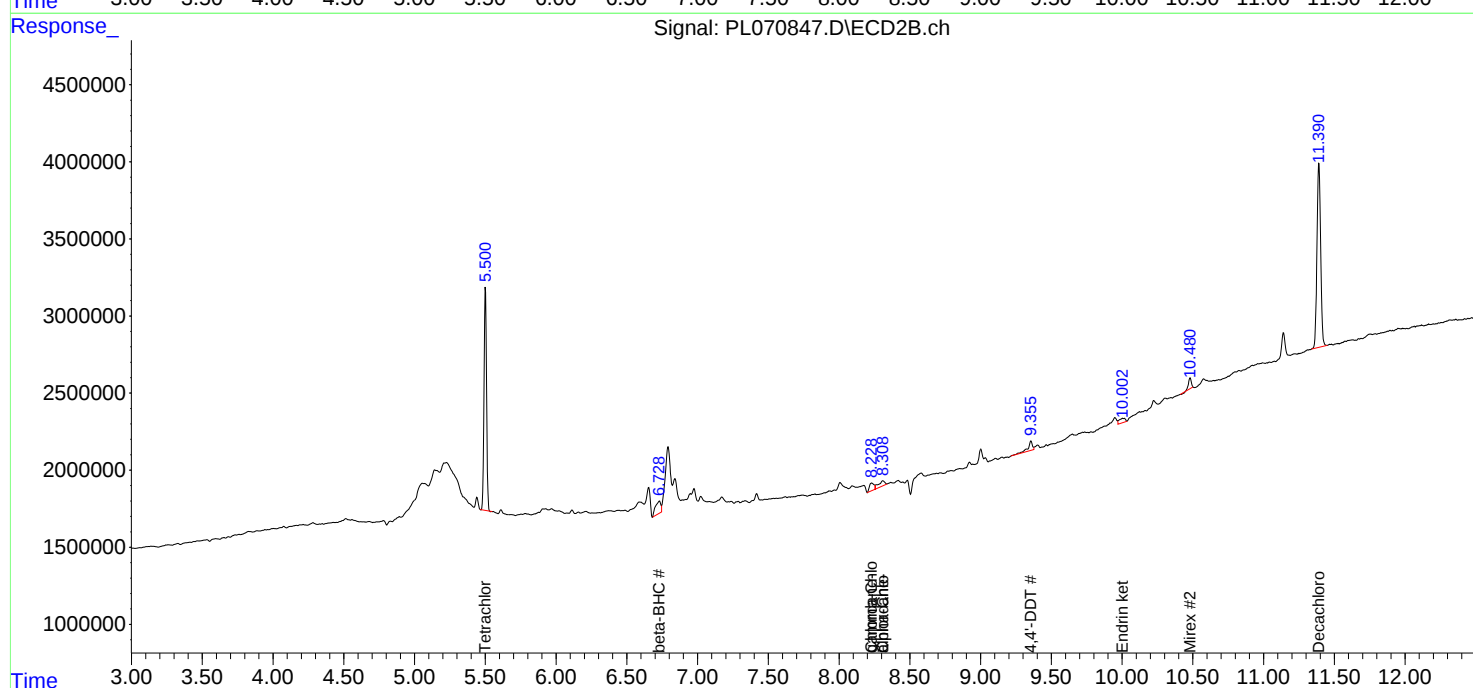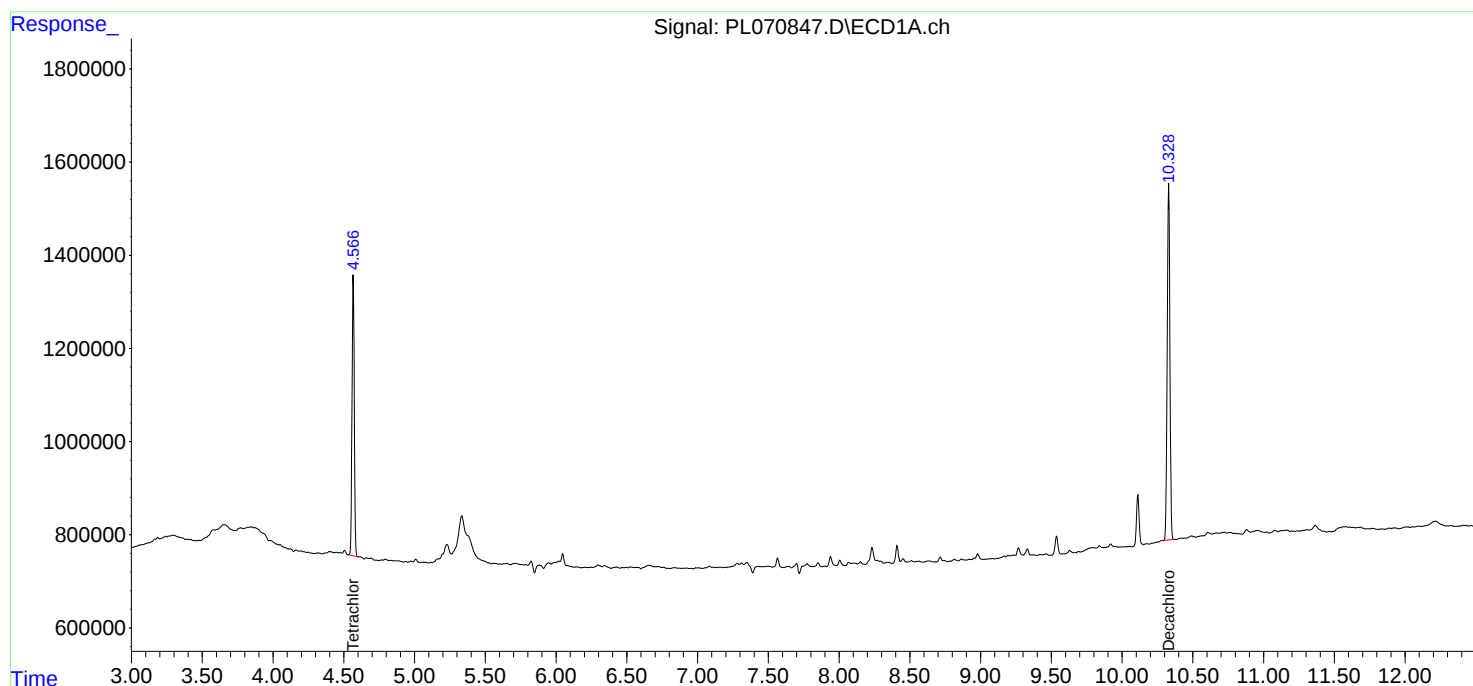


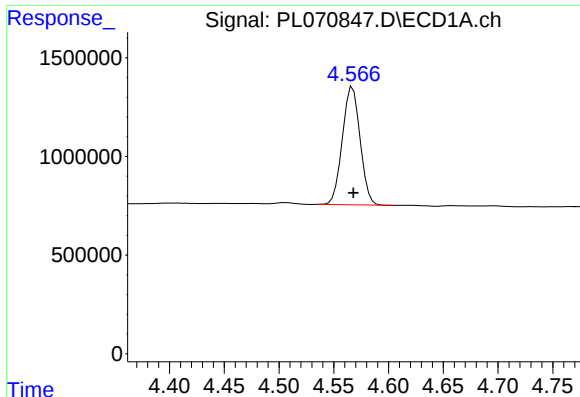

#1 Tetrachloro-m-xylene


R.T.: 4.567 min
Delta R.T.: 0.000 min
Response: 6749960
Conc: 13.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

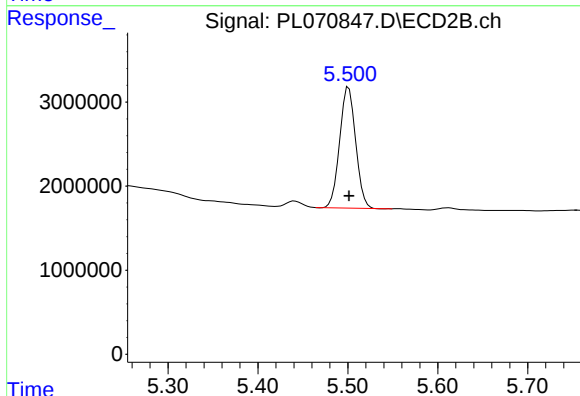


#1 Tetrachloro-m-xylene

R.T.: 5.501 min
Delta R.T.: 0.000 min
Response: 17781823
Conc: 14.10 ng/ml

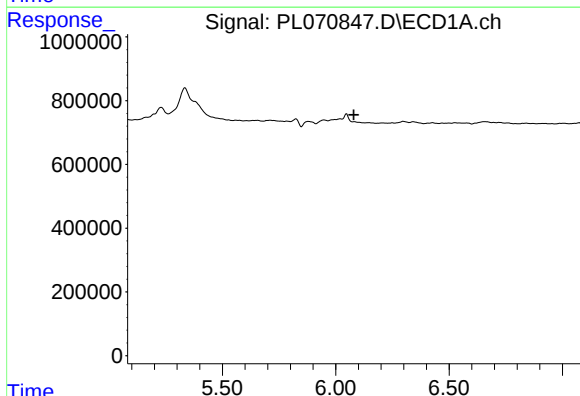


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.079 min
Response: 0
Conc: N.D.

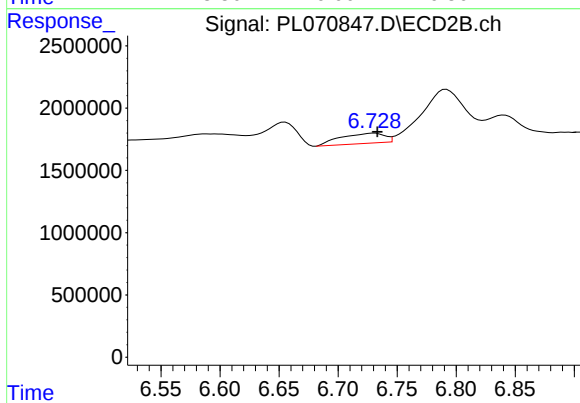

#6 beta-BHC


R.T.: 6.731 min
Delta R.T.: -0.003 min
Response: 2102271
Conc: 2.45 ng/ml

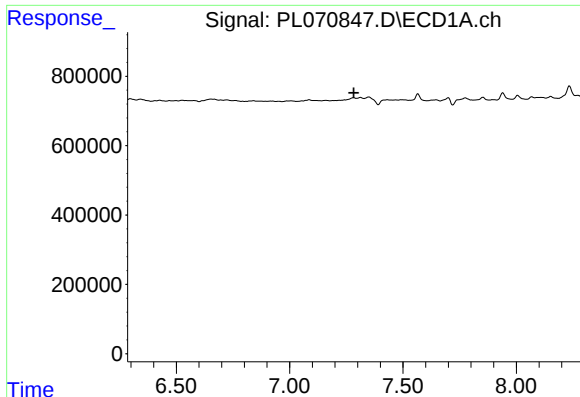

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

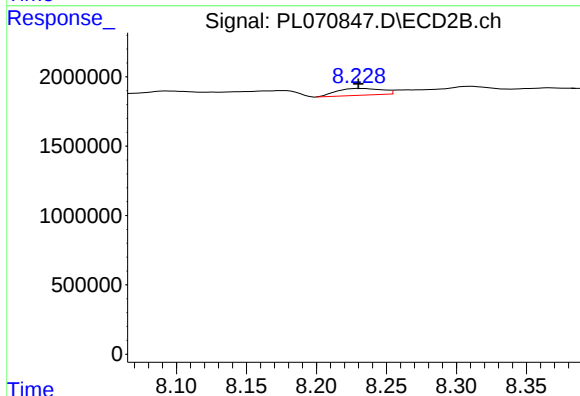


#10 gamma-Chlordane

R.T.: 8.231 min
Delta R.T.: 0.000 min
Response: 1087747
Conc: 0.70 ng/ml

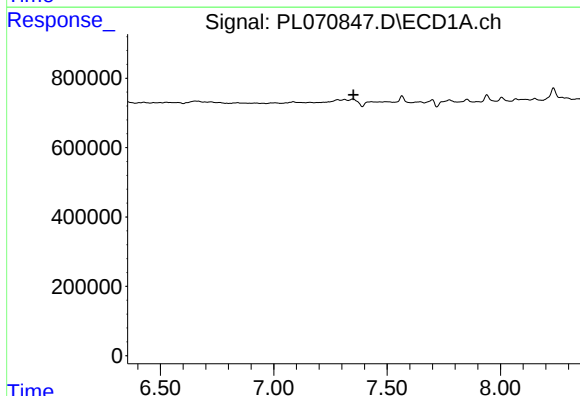


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.352 min
Response: 0
Conc: N.D.

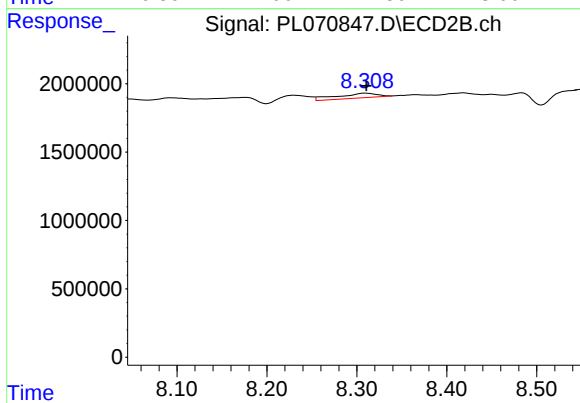

#11 alpha-Chlordane


R.T.: 8.310 min
Delta R.T.: 0.000 min
Response: 1096463
Conc: 0.72 ng/ml

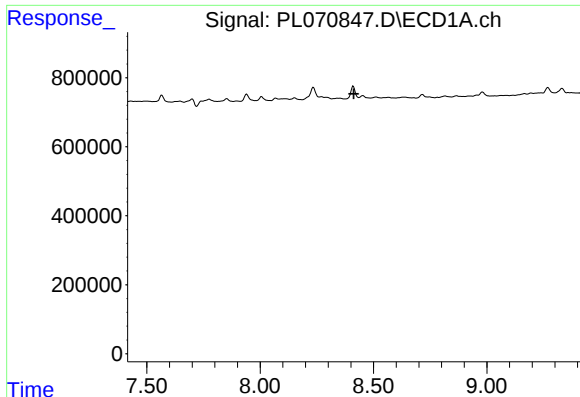

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.413 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

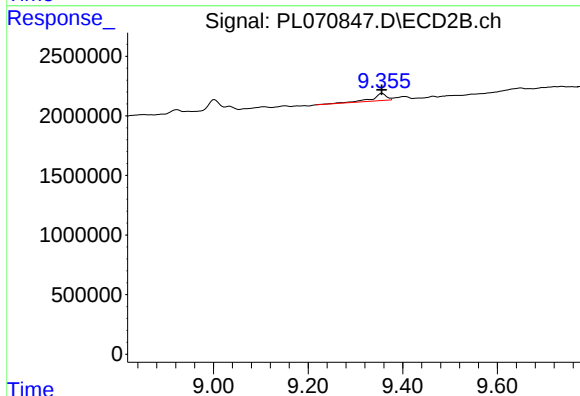


#17 4,4'-DDT

R.T.: 9.356 min
Delta R.T.: 0.000 min
Response: 1286758
Conc: 1.02 ng/ml

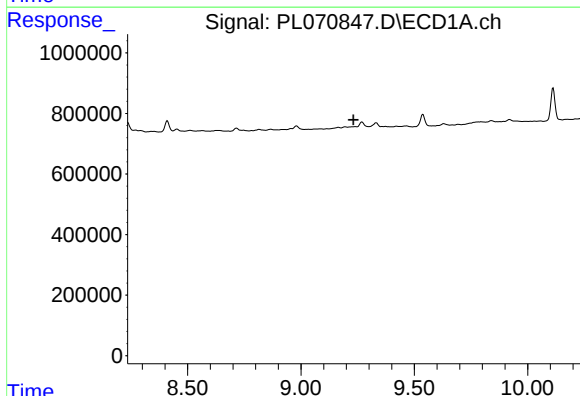


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.232 min
Response: 0
Conc: N.D.

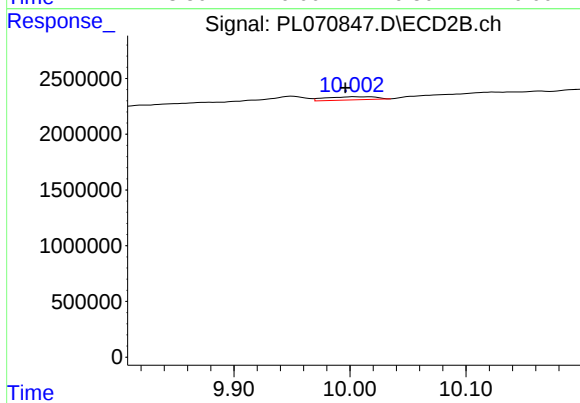

#21 Endrin ketone


R.T.: 10.004 min
Delta R.T.: 0.007 min
Response: 861796
Conc: 0.60 ng/ml

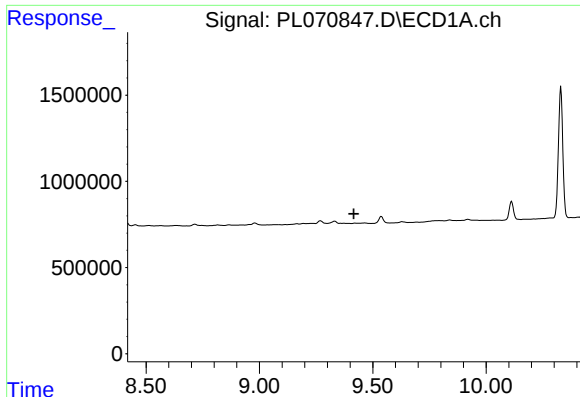

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.417 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

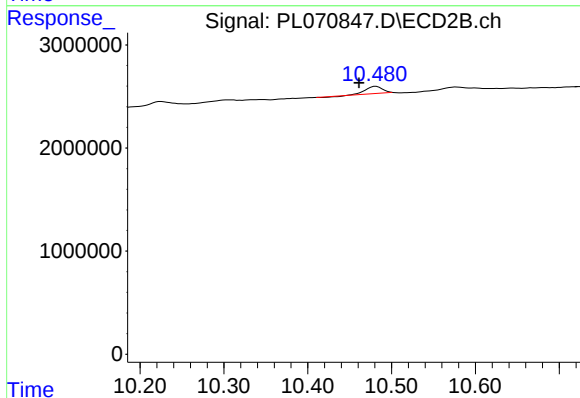


#22 Mirex

R.T.: 10.481 min
Delta R.T.: 0.020 min
Response: 972602
Conc: 0.93 ng/ml

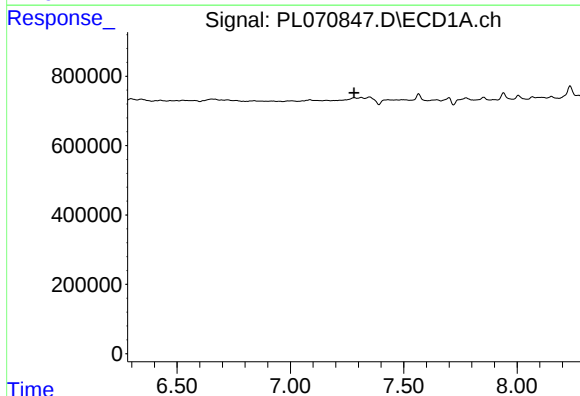


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.281 min
Response: 0
Conc: N.D.

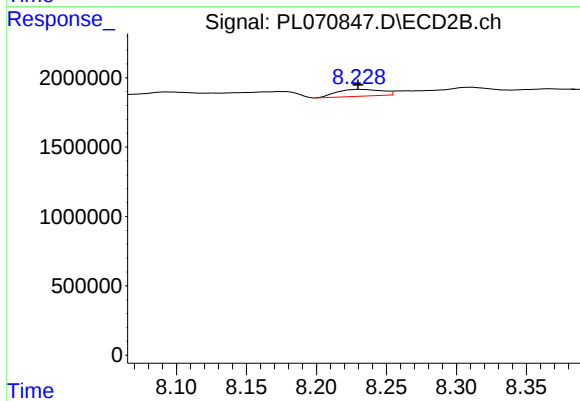

#25 Chlordane-3


R.T.: 8.231 min
Delta R.T.: 0.000 min
Response: 1087747
Conc: 5.38 ng/ml

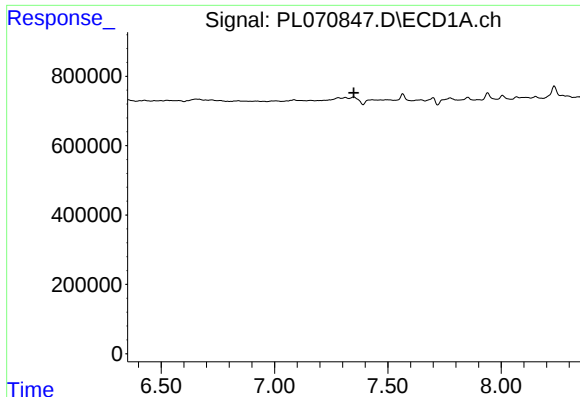

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

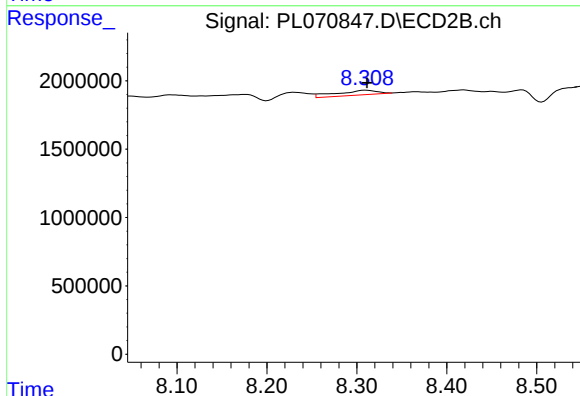


#26 Chlordane-4

R.T.: 8.310 min
Delta R.T.: -0.001 min
Response: 1096463
Conc: 4.52 ng/ml

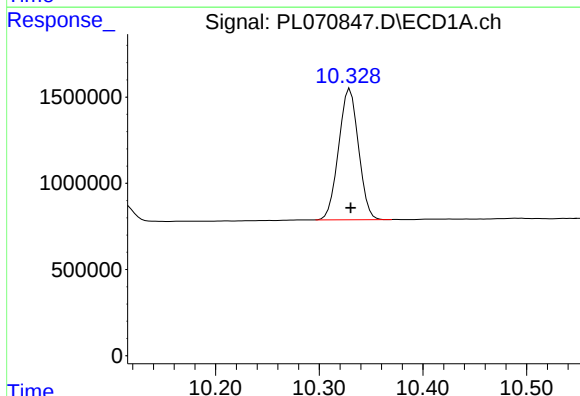

#28 Decachlorobiphenyl

R.T.: 10.330 min
Delta R.T.: 0.000 min
Response: 10121143
Conc: 14.81 ng/ml

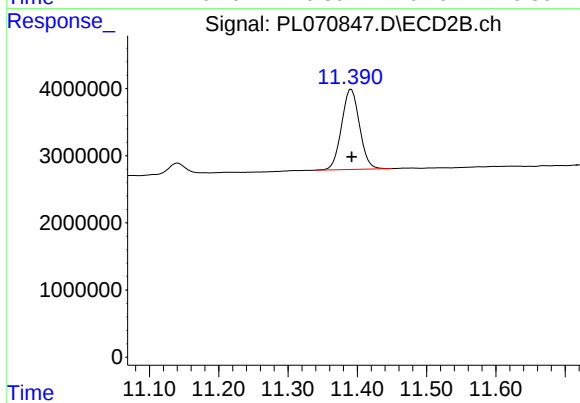

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: 0.000 min
Response: 21471886
Conc: 16.06 ng/ml