

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110821\
 Data File : PL070844.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2021 22:08
 Operator : AR\AJ
 Sample : M4574-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VWE-B6-110521-0-10

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/09/2021
 Supervised By :mohammad ahmed 11/09/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 00:49:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.567	5.501	11076140	29470646	22.613	23.374
28)	SA Decachlor...	10.330	11.391	12681567	26781315	18.559	20.025
Target Compounds							
12)	B 4,4'-DDE	7.566	8.498	795176	1486231	1.365	1.007 #
16)	A 4,4'-DDD	8.151	9.038	181034	1443797	0.356m	1.200 #
17)	MA 4,4'-DDT	8.411	9.356	823969	1506562	1.498	1.194

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110821\
Data File : PL070844.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2021 22:08
Operator : AR\AJ
Sample : M4574-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VWE-B6-110521-0-10


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/09/2021
Supervised By :mohammad ahmed 11/09/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 00:49:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

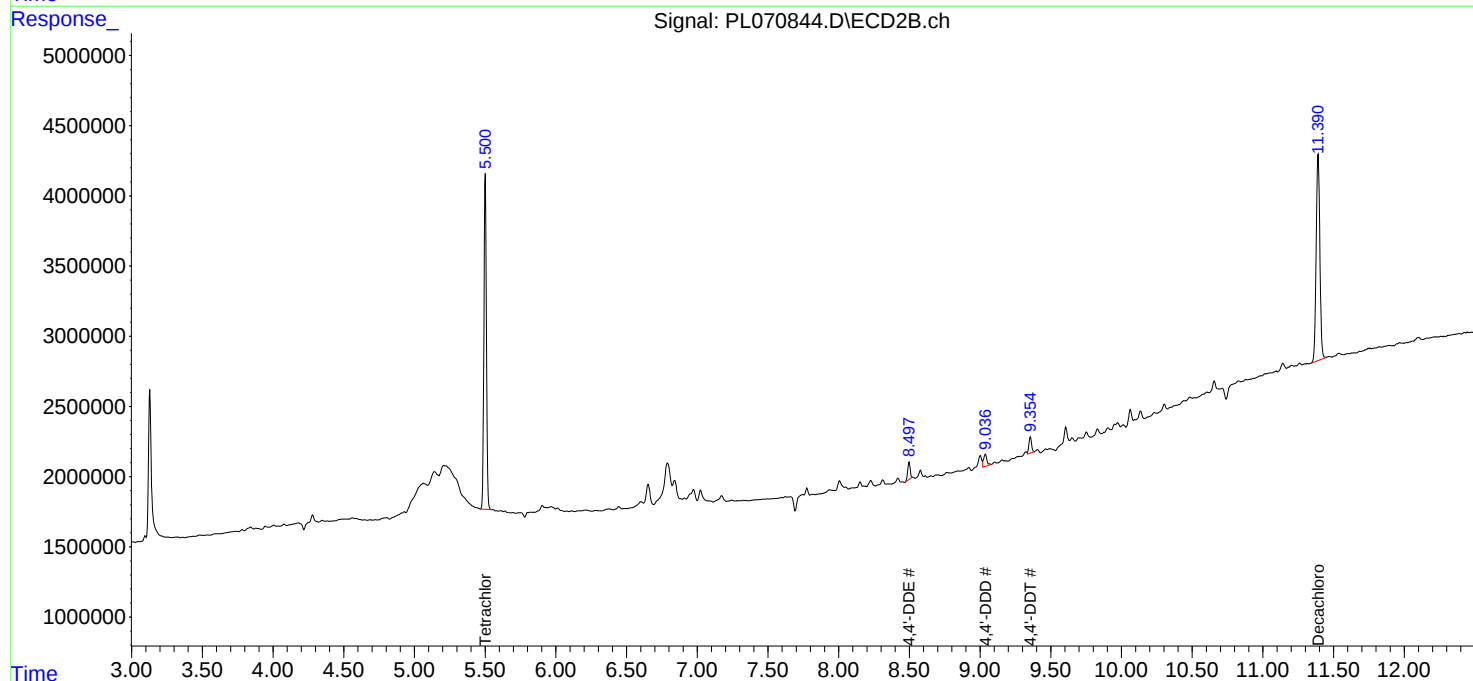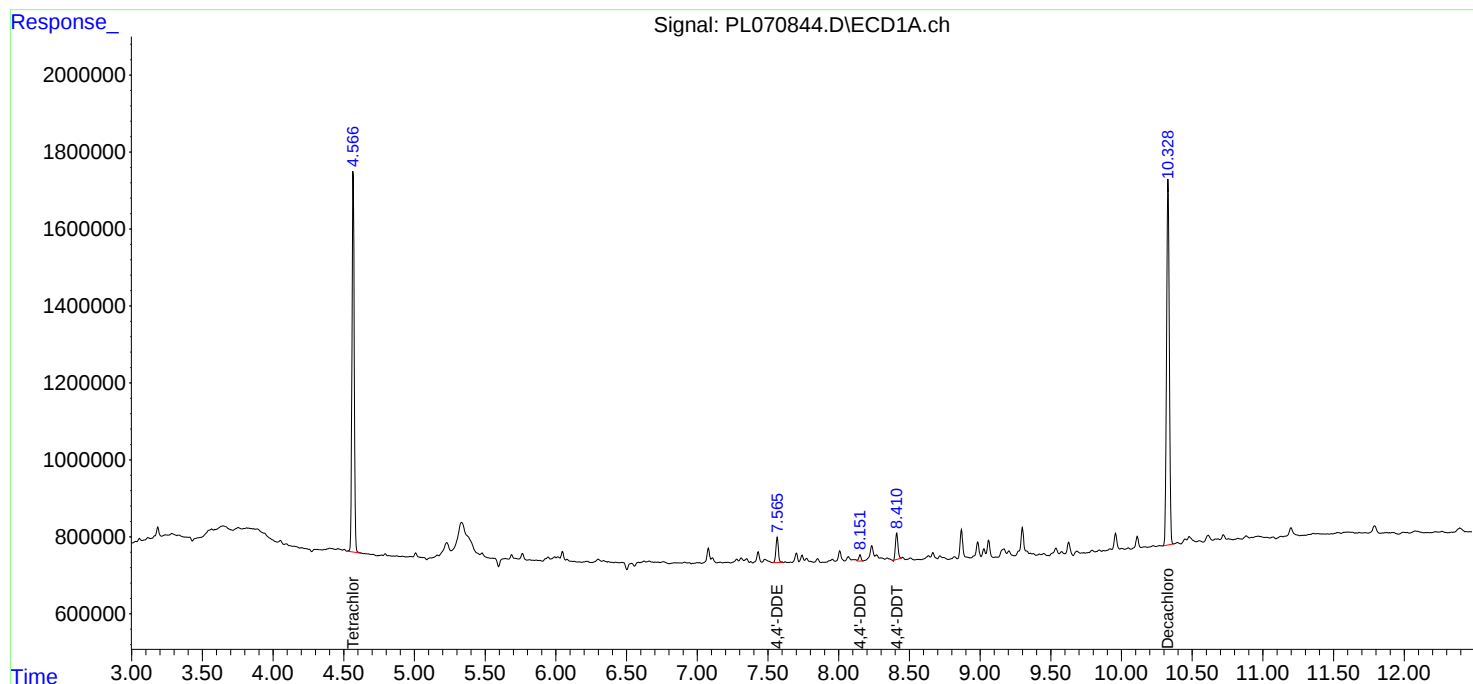

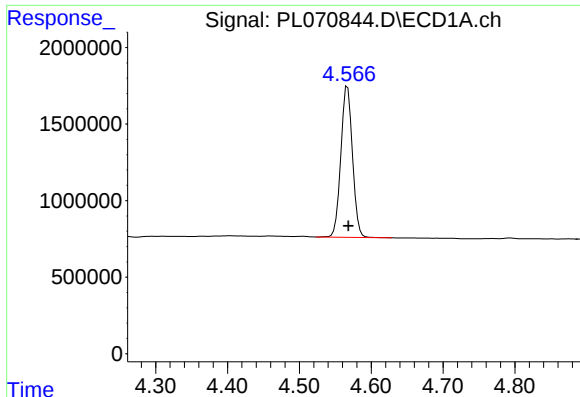


#1 Tetrachloro-m-xylene

R.T.: 4.567 min
Delta R.T.: 0.000 min
Response: 11076140
Conc: 22.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
VWE-B6-110521-0-10


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/09/2021
Supervised By :mohammad ahmed 11/09/2021

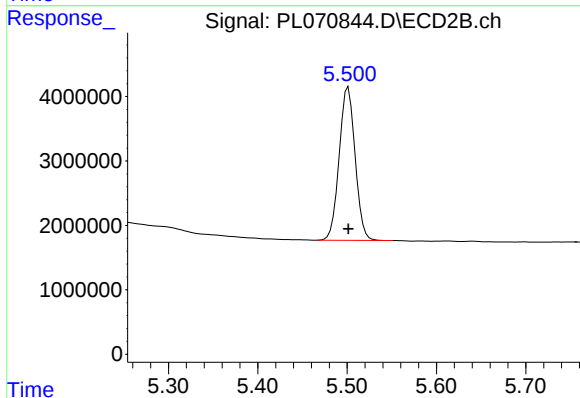


#1 Tetrachloro-m-xylene

R.T.: 5.501 min
Delta R.T.: 0.000 min
Response: 29470646
Conc: 23.37 ng/ml

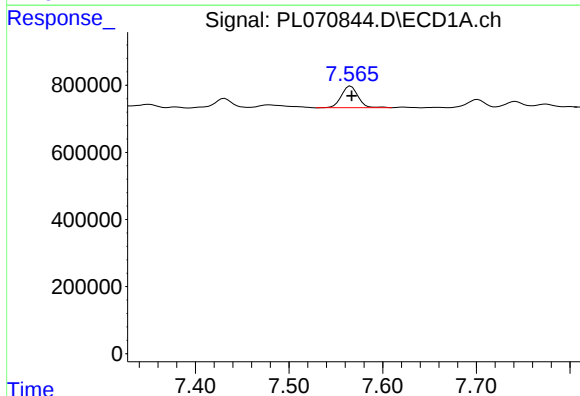


#12 4,4'-DDE

R.T.: 7.566 min
Delta R.T.: -0.001 min
Response: 795176
Conc: 1.36 ng/ml

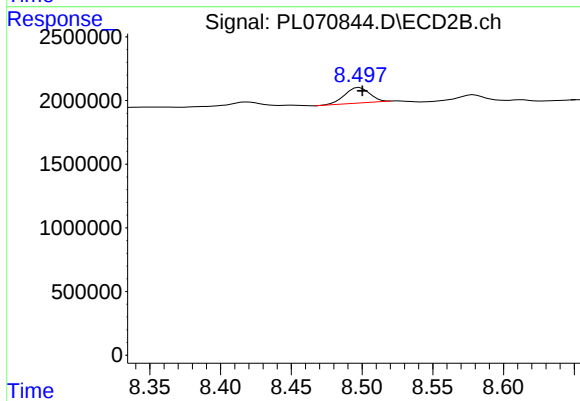

#12 4,4'-DDE

R.T.: 8.498 min
Delta R.T.: -0.002 min
Response: 1486231
Conc: 1.01 ng/ml

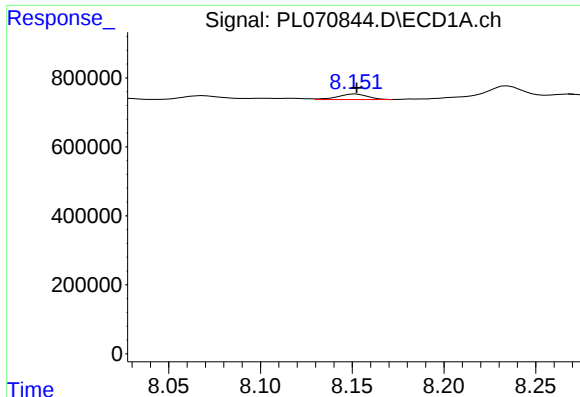


#16 4,4'-DDD

R.T.: 8.151 min
Delta R.T.: -0.002 min
Response: 181034
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
VWE-B6-110521-0-10


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/09/2021
Supervised By :mohammad ahmed 11/09/2021

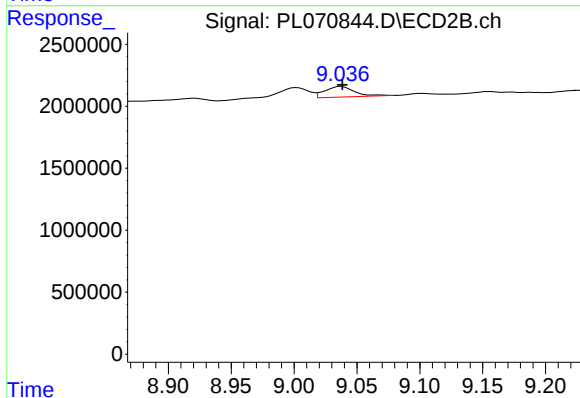


#16 4,4'-DDD

R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 1443797
Conc: 1.20 ng/ml

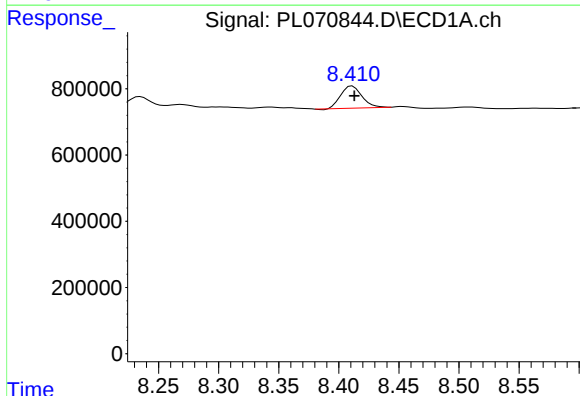


#17 4,4'-DDT

R.T.: 8.411 min
Delta R.T.: -0.002 min
Response: 823969
Conc: 1.50 ng/ml

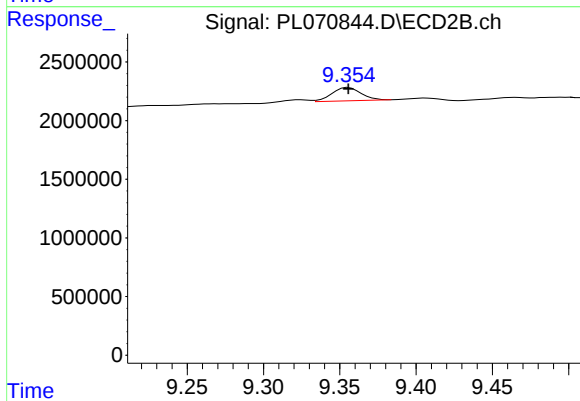

#17 4,4'-DDT

R.T.: 9.356 min
Delta R.T.: 0.000 min
Response: 1506562
Conc: 1.19 ng/ml

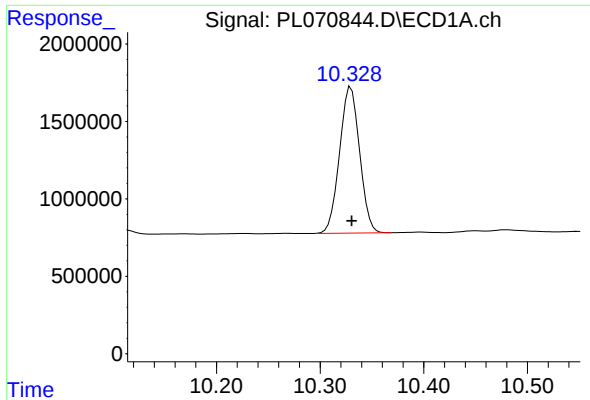


#28 Decachlorobiphenyl

R.T.: 10.330 min
Delta R.T.: 0.000 min
Response: 12681567
Conc: 18.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
VWE-B6-110521-0-10

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/09/2021
Supervised By :mohammad ahmed 11/09/2021

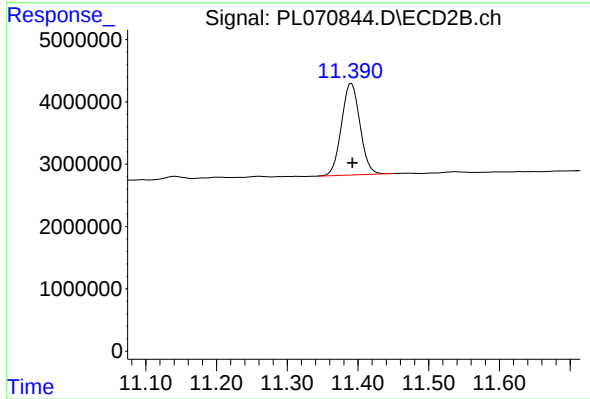

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: 0.000 min
Response: 26781315
Conc: 20.03 ng/ml