

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110821\
 Data File : PL070847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2021 22:58
 Operator : AR\AJ
 Sample : M4574-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VWE-B6-110521-10-20

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/09/2021
 Supervised By :mohammad ahmed 11/09/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 00:50:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.567	5.501	6749960	17781823	13.781	14.103
2)	SA Decachlor...	10.330	11.391	10121143	21471886	14.812	16.055
Target Compounds							
17)	MA 4,4'-DDT	8.409	9.355	522676	602888	0.950m	0.478m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110821\
Data File : PL070847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2021 22:58
Operator : AR\AJ
Sample : M4574-02
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VWE-B6-110521-10-20


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/09/2021
Supervised By :mohammad ahmed 11/09/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 00:50:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

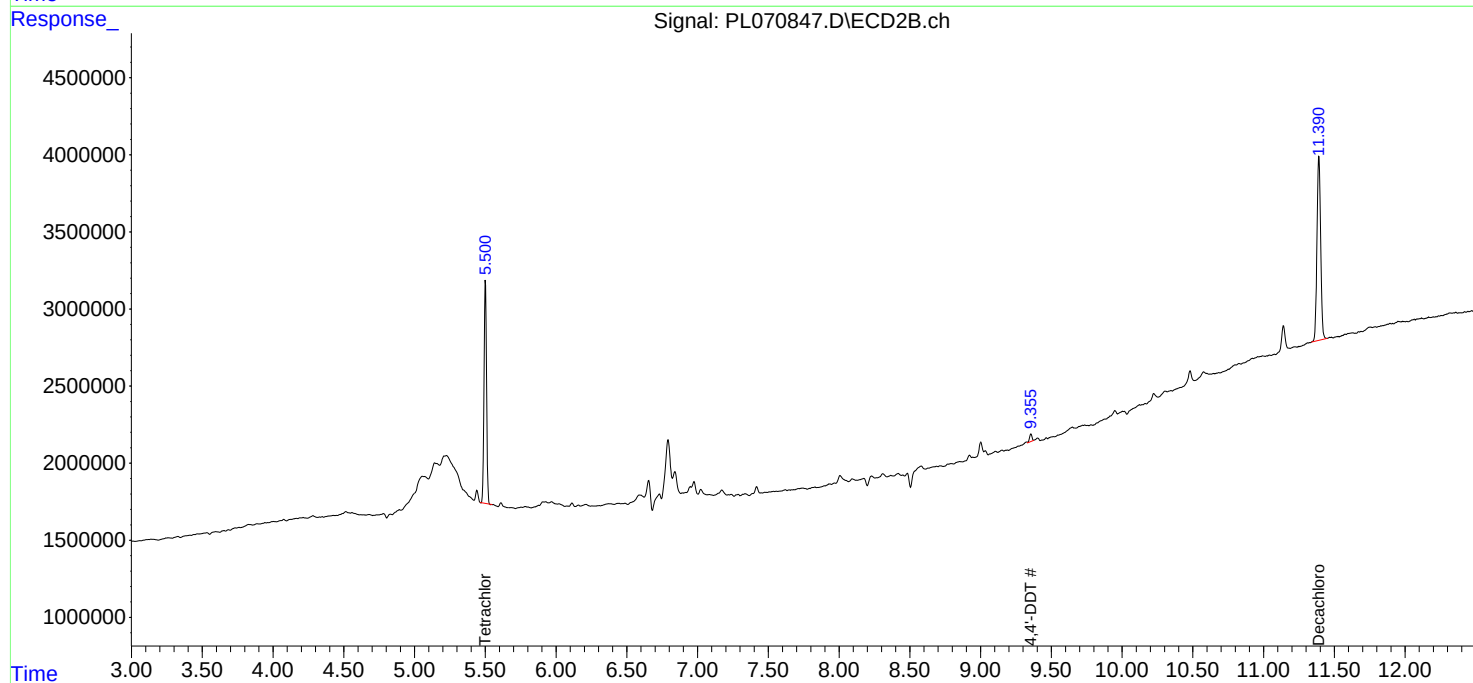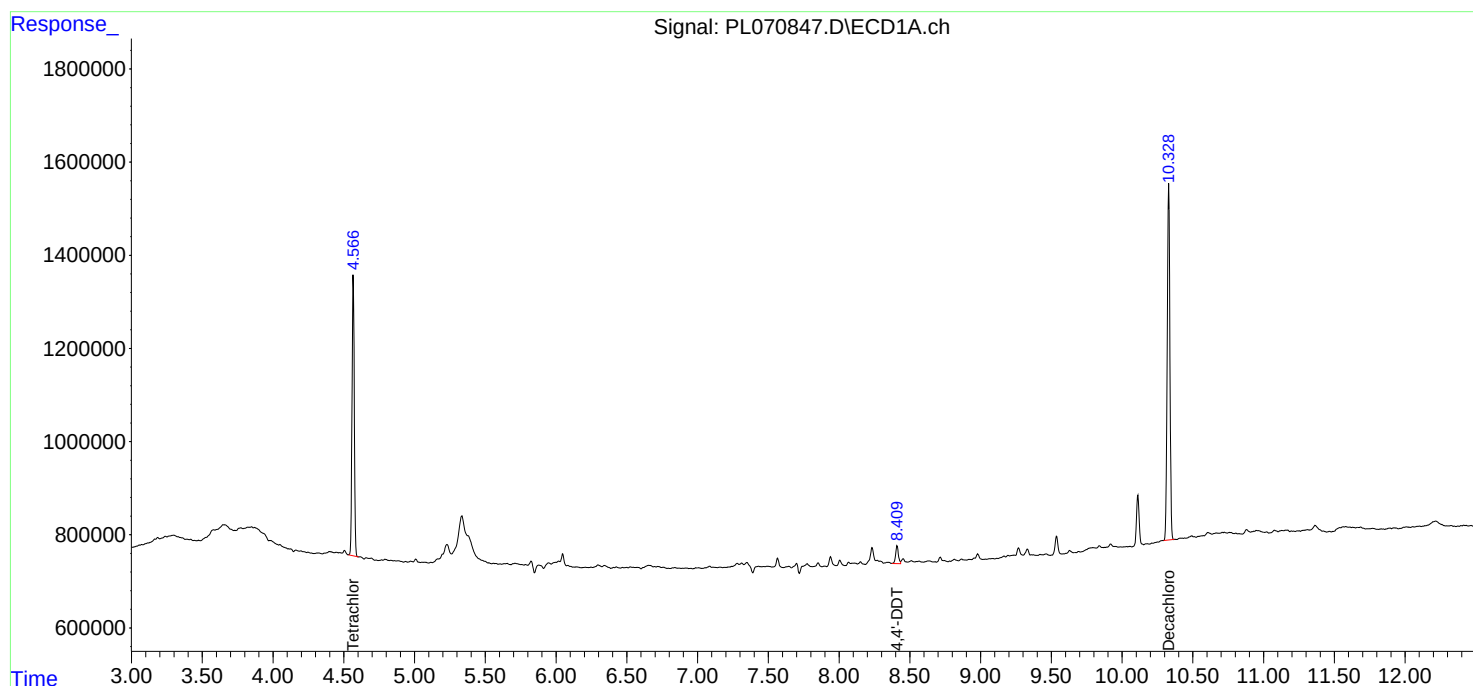

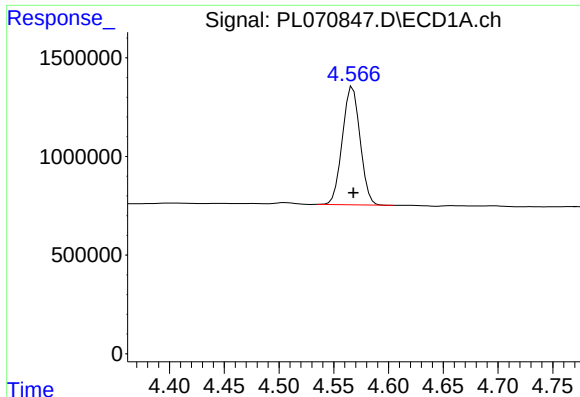


#1 Tetrachloro-m-xylene

R.T.: 4.567 min
Delta R.T.: 0.000 min
Response: 6749960
Conc: 13.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
VWE-B6-110521-10-20


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/09/2021
Supervised By :mohammad ahmed 11/09/2021

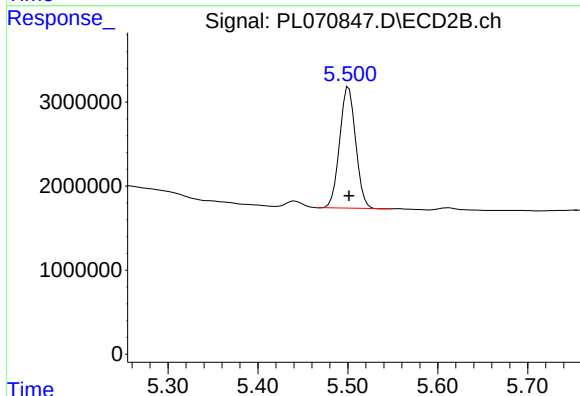


#1 Tetrachloro-m-xylene

R.T.: 5.501 min
Delta R.T.: 0.000 min
Response: 17781823
Conc: 14.10 ng/ml

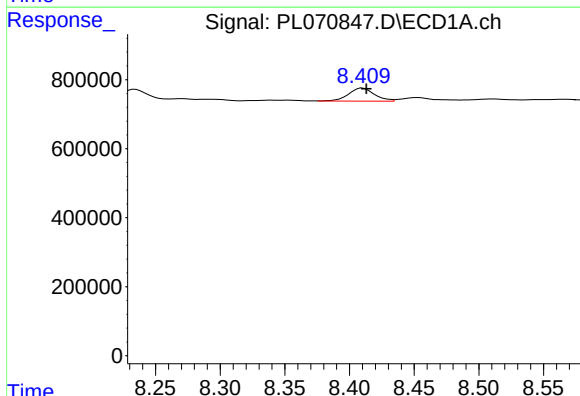


#17 4,4'-DDT

R.T.: 8.409 min
Delta R.T.: -0.004 min
Response: 522676
Conc: 0.95 ng/ml m

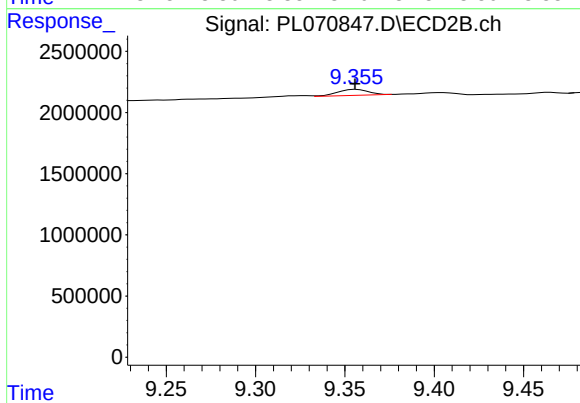

#17 4,4'-DDT

R.T.: 9.355 min
Delta R.T.: 0.000 min
Response: 602888
Conc: 0.48 ng/ml m

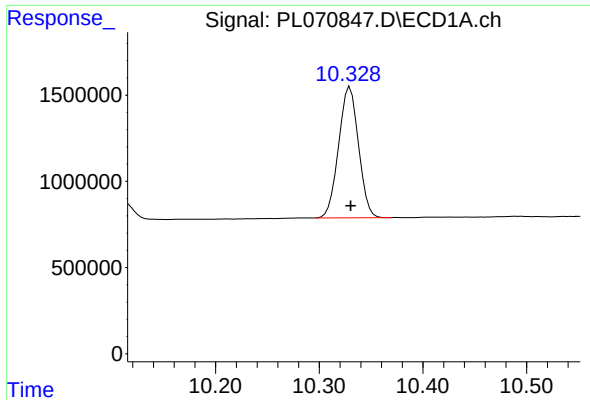


#28 Decachlorobiphenyl

R.T.: 10.330 min
Delta R.T.: 0.000 min
Response: 10121143
Conc: 14.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
VWE-B6-110521-10-20

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/09/2021
Supervised By :mohammad ahmed 11/09/2021

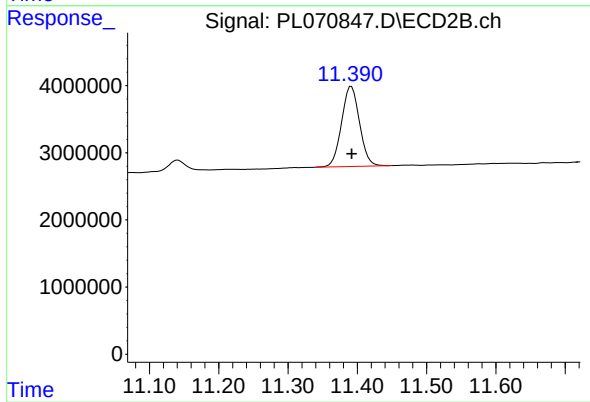

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: 0.000 min
Response: 21471886
Conc: 16.06 ng/ml