

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110822\
 Data File : PL078941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2022 00:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 02:21:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	2.568	39928257	51261856	20.938	20.078
28)	SA Decachlor...	8.767	7.634	30195485	41648403	20.072	21.988
Target Compounds							
3)	MA gamma-BHC...	4.136f	0.000	481394	0	0.180	N.D. #
6)	B beta-BHC	4.317	0.000	260695	0	0.226	N.D. #
8)	B Heptachlo...	5.462	4.498f	9904433	827398	4.665	0.275 #
9)	A Endosulfan I	5.862f	0.000	673618	0	0.316	N.D. #
10)	B gamma-Chl...	5.703	0.000	391879	0	0.174	N.D. #
13)	MA Dieldrin	0.000	5.093	0	2854978	N.D.	0.964 #
14)	MA Endrin	0.000	5.390f	0	3108024	N.D.	1.193 #
17)	MA 4,4'-DDT	6.822	0.000	609430	0	0.340	N.D. #
20)	A Methoxychlor	7.274f	0.000	9951	0	0.011	N.D. #
24)	Chlordane-2	0.000	4.122f	0	25748795	N.D.	241.940 #
25)	Chlordane-3	5.703	0.000	391879	0	1.173	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110822\
Data File : PL078941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2022 00:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 02:21:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

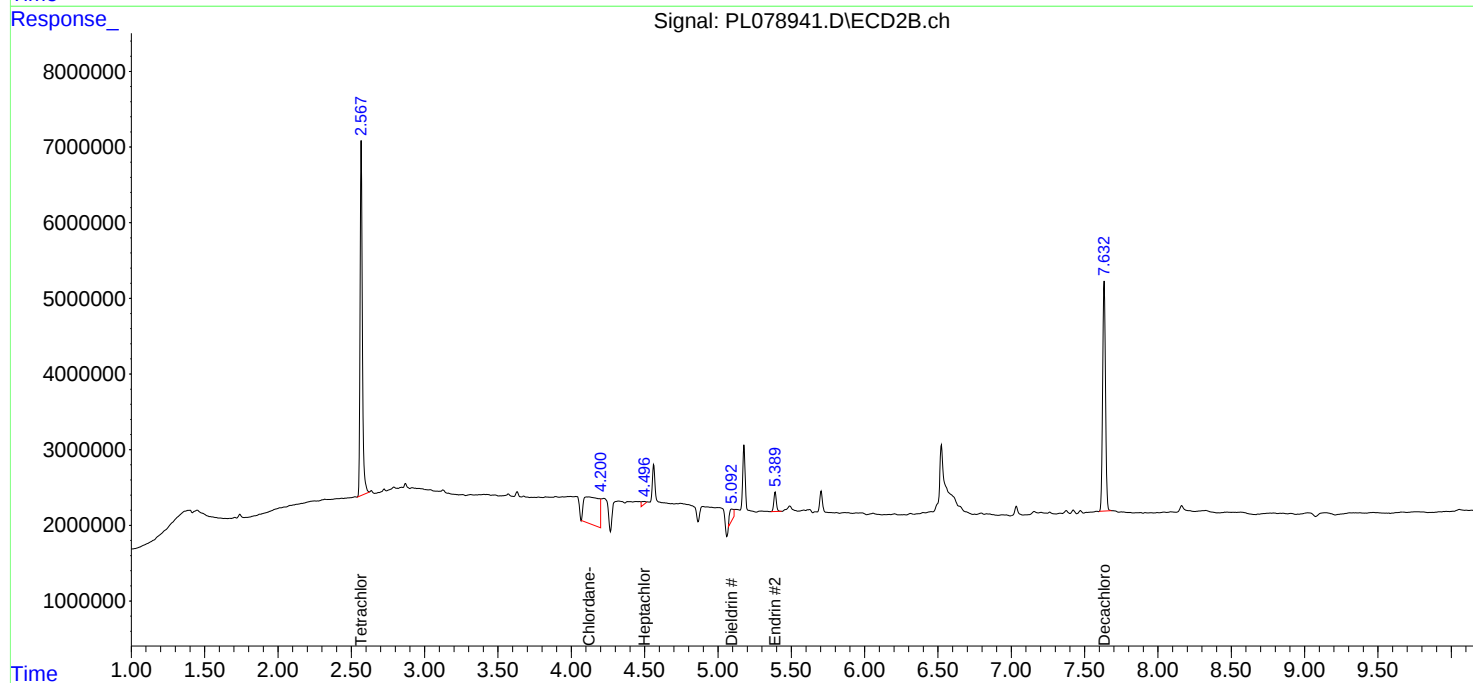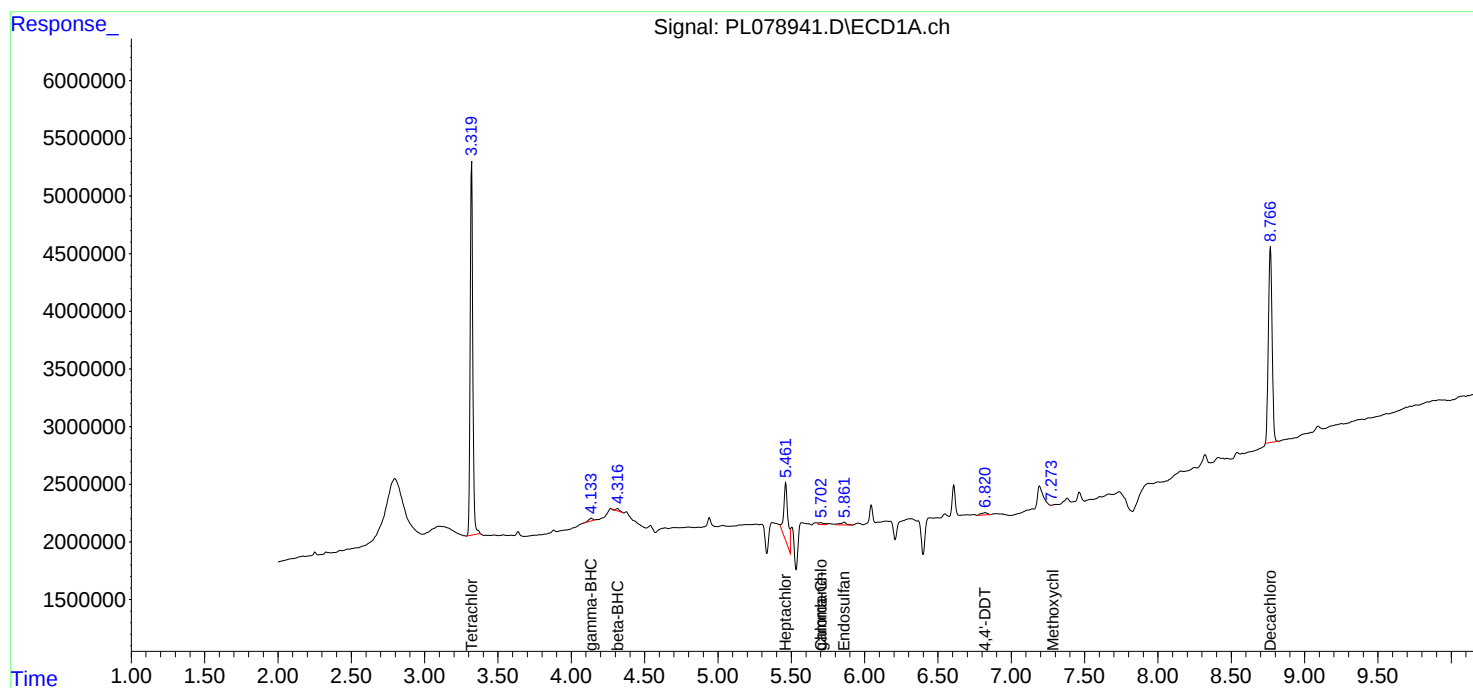


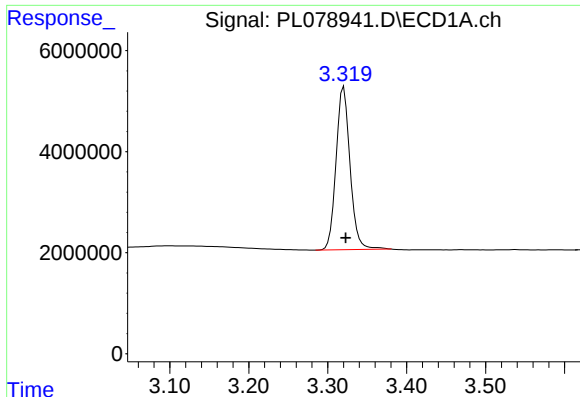

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: -0.003 min
Response: 39928257
Conc: 20.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

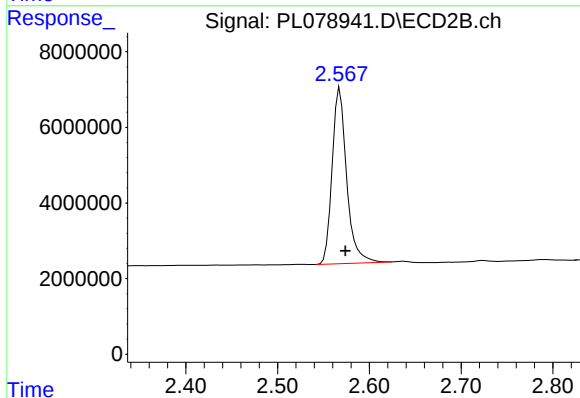


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.006 min
Response: 51261856
Conc: 20.08 ng/ml

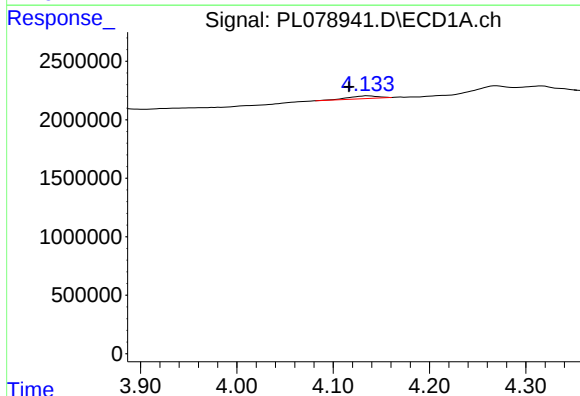


#3 gamma-BHC (Lindane)

R.T.: 4.136 min
Delta R.T.: 0.019 min
Response: 481394
Conc: 0.18 ng/ml

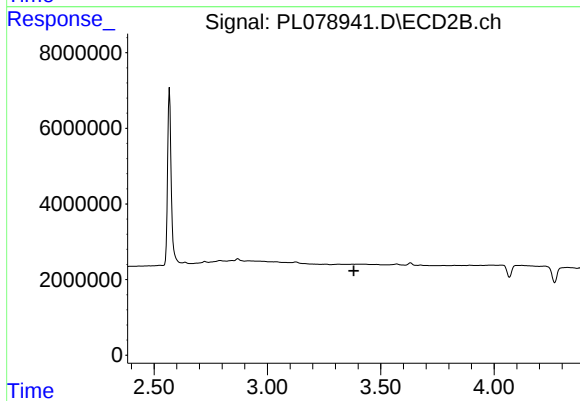

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.382 min
Response: 0
Conc: N.D.

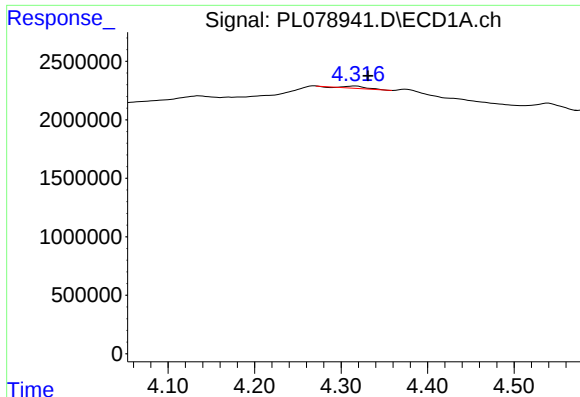

#6 beta-BHC


R.T.: 4.317 min
Delta R.T.: -0.015 min
Response: 260695
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

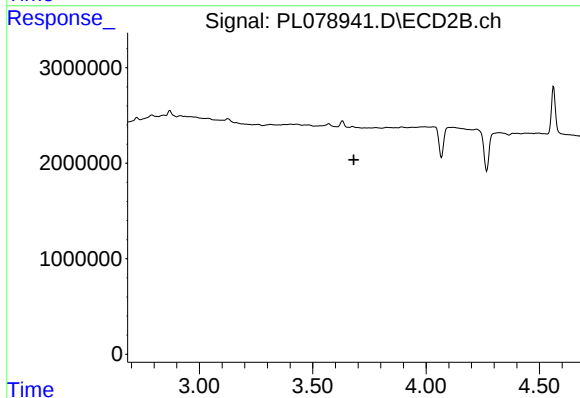


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 3.681 min
Response: 0
Conc: N.D.

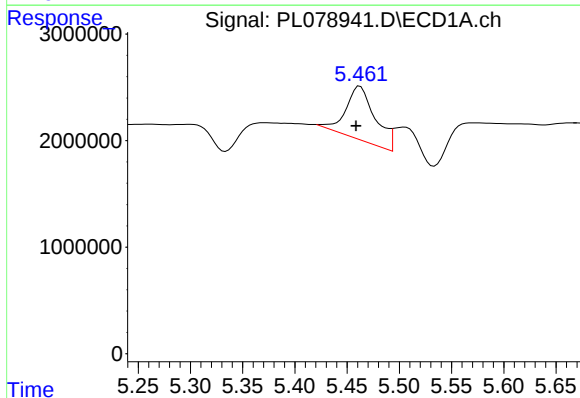


#8 Heptachlor epoxide

R.T.: 5.462 min
Delta R.T.: 0.004 min
Response: 9904433
Conc: 4.67 ng/ml

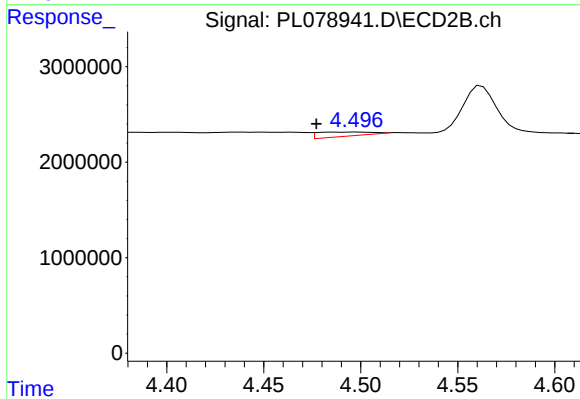

#8 Heptachlor epoxide


R.T.: 4.498 min
Delta R.T.: 0.021 min
Response: 827398
Conc: 0.27 ng/ml

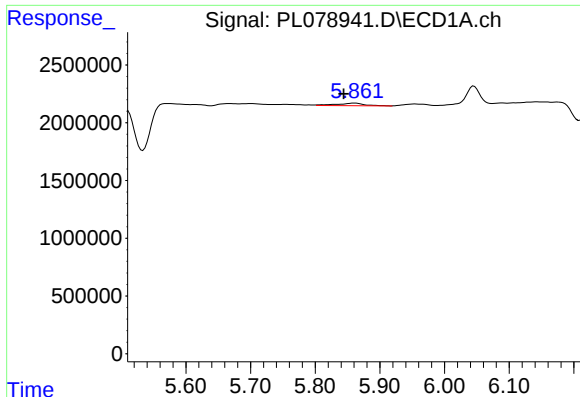

#9 Endosulfan I


R.T.: 5.862 min
Delta R.T.: 0.018 min
Response: 673618
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

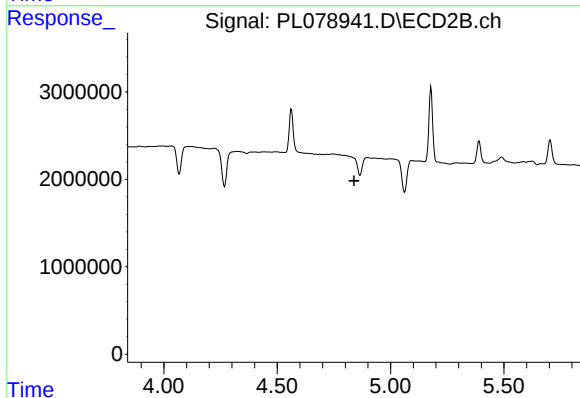


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 4.840 min
Response: 0
Conc: N.D.

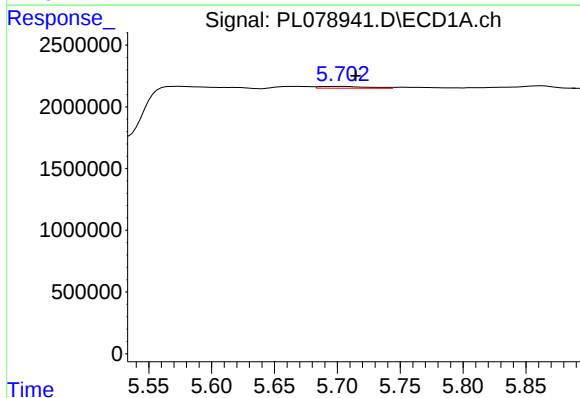


#10 gamma-Chlordane

R.T.: 5.703 min
Delta R.T.: -0.011 min
Response: 391879
Conc: 0.17 ng/ml

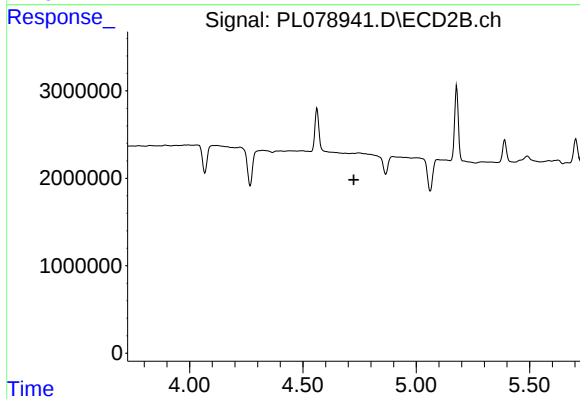

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.725 min
Response: 0
Conc: N.D.

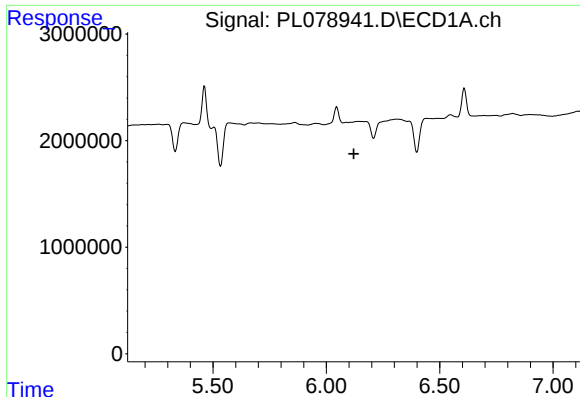

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

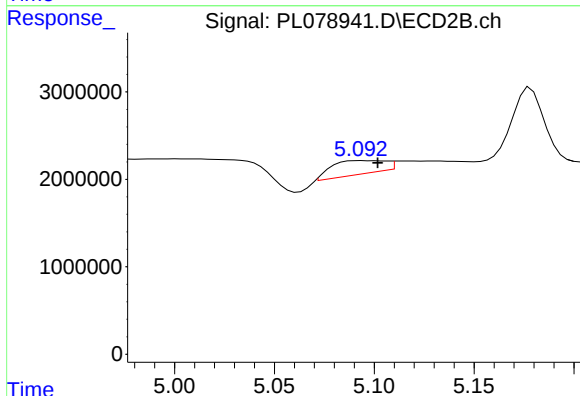


#13 Dieldrin

R.T.: 5.093 min
Delta R.T.: -0.008 min
Response: 2854978
Conc: 0.96 ng/ml

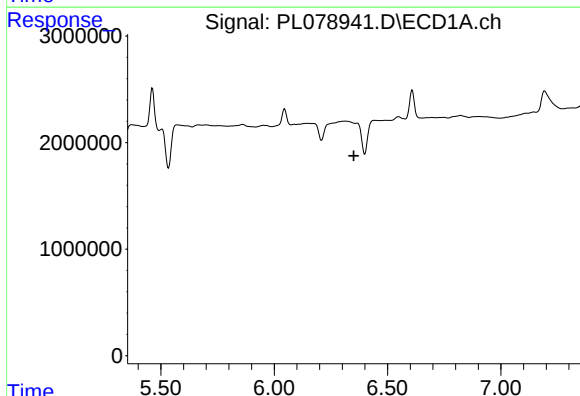


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.351 min
Response: 0
Conc: N.D.

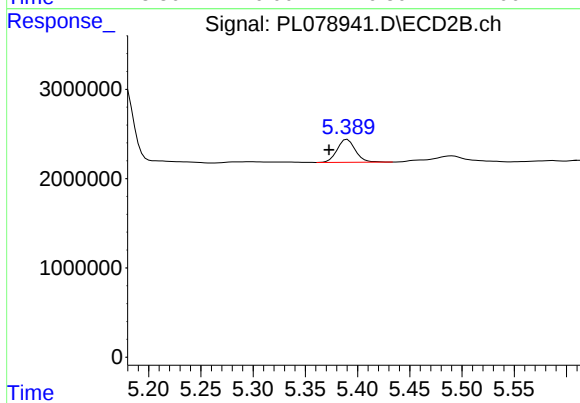

#14 Endrin


R.T.: 5.390 min
Delta R.T.: 0.018 min
Response: 3108024
Conc: 1.19 ng/ml

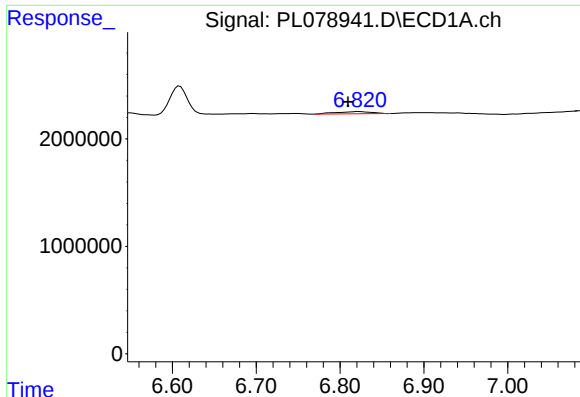

#17 4,4'-DDT


R.T.: 6.822 min
Delta R.T.: 0.012 min
Response: 609430
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

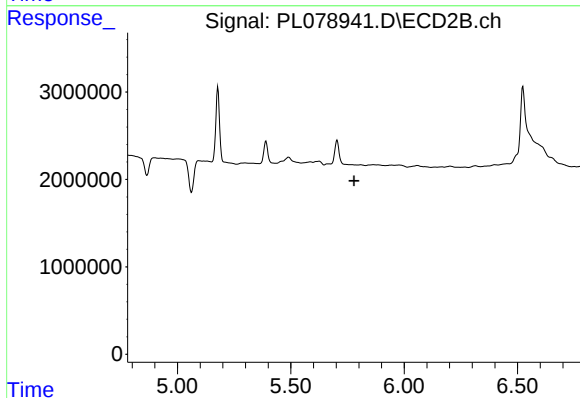


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 5.779 min
Response: 0
Conc: N.D.

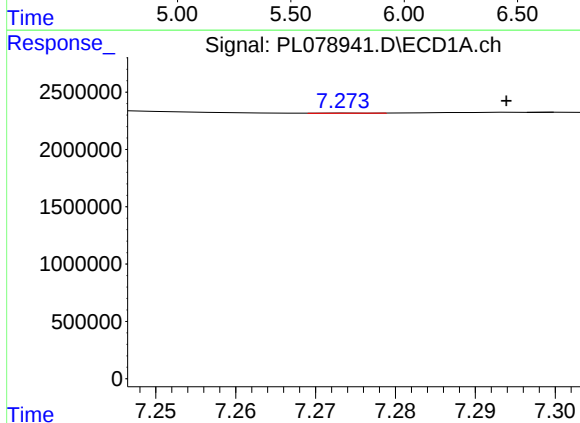


#20 Methoxychlor

R.T.: 7.274 min
Delta R.T.: -0.020 min
Response: 9951
Conc: 0.01 ng/ml

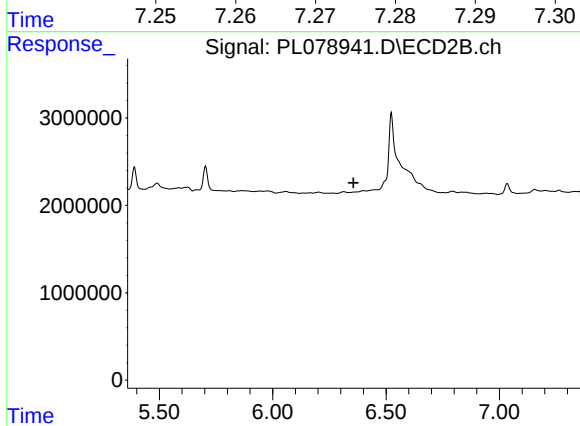

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.357 min
Response: 0
Conc: N.D.

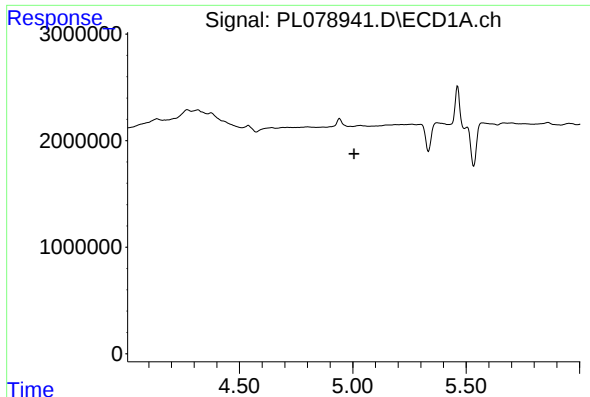

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

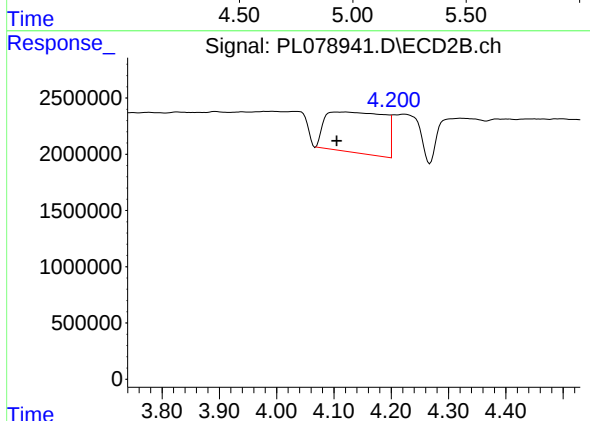


#24 Chlordane-2

R.T.: 4.122 min
Delta R.T.: 0.017 min
Response: 25748795
Conc: 241.94 ng/ml

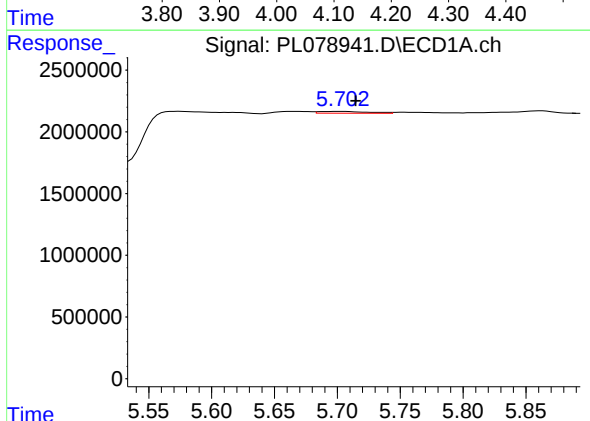


#25 Chlordane-3

R.T.: 5.703 min
Delta R.T.: -0.011 min
Response: 391879
Conc: 1.17 ng/ml

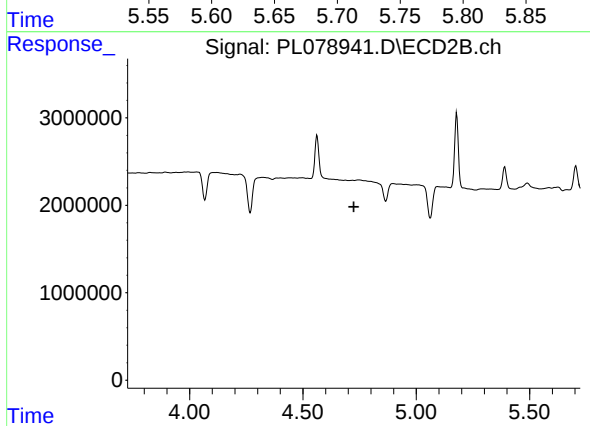

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 4.725 min
Response: 0
Conc: N.D.

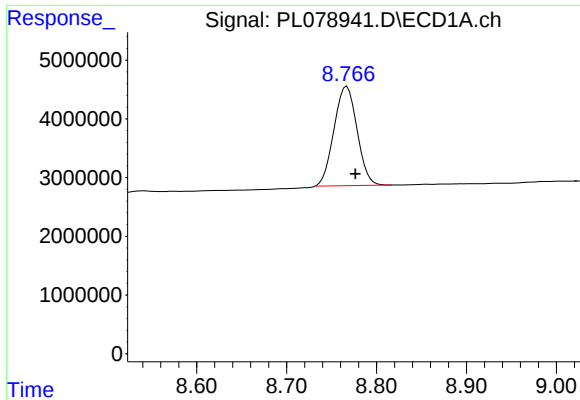

#28 Decachlorobiphenyl

R.T.: 8.767 min
Delta R.T.: -0.009 min
Response: 30195485
Conc: 20.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

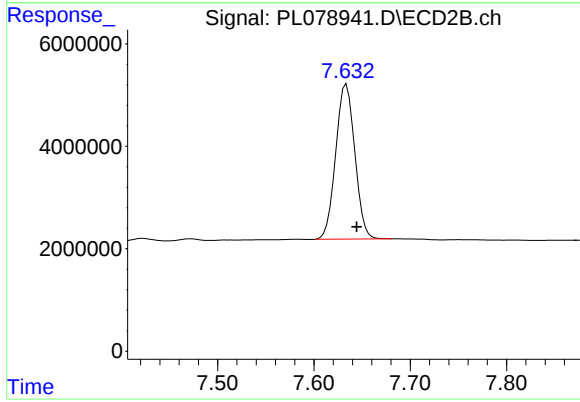

#28 Decachlorobiphenyl

R.T.: 7.634 min
Delta R.T.: -0.011 min
Response: 41648403
Conc: 21.99 ng/ml