

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110822\
 Data File : PL078906.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 12:12
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 21:07:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.326	2.567	95295400	146.0E6	49.971	57.195
28)	SA Decachlor...	8.774	7.637	73194762	99232526	48.655	52.390
Target Compounds							
23)	Chlordane-1	4.474	3.532	32874389	46384989	419.571	459.918
24)	Chlordane-2	5.007	4.099	40423888	47187913	488.543	443.386
25)	Chlordane-3	5.716	4.719	161.6E6	144.0E6	483.913	472.340
26)	Chlordane-4	5.794	4.779	204.5E6	153.9E6	498.159	471.015
27)	Chlordane-5	6.649	5.441	31267141	38954255	478.160	477.637



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110822\
Data File : PL078906.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 12:12
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 21:07:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

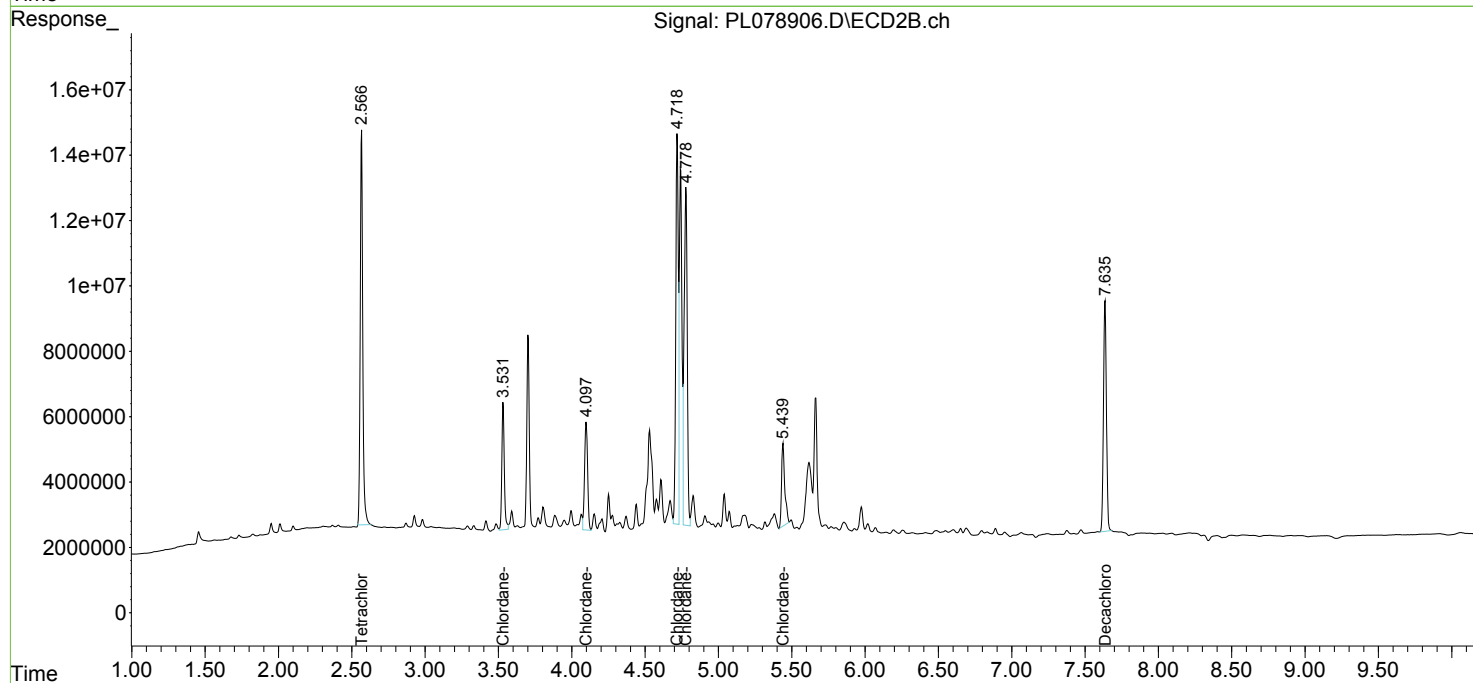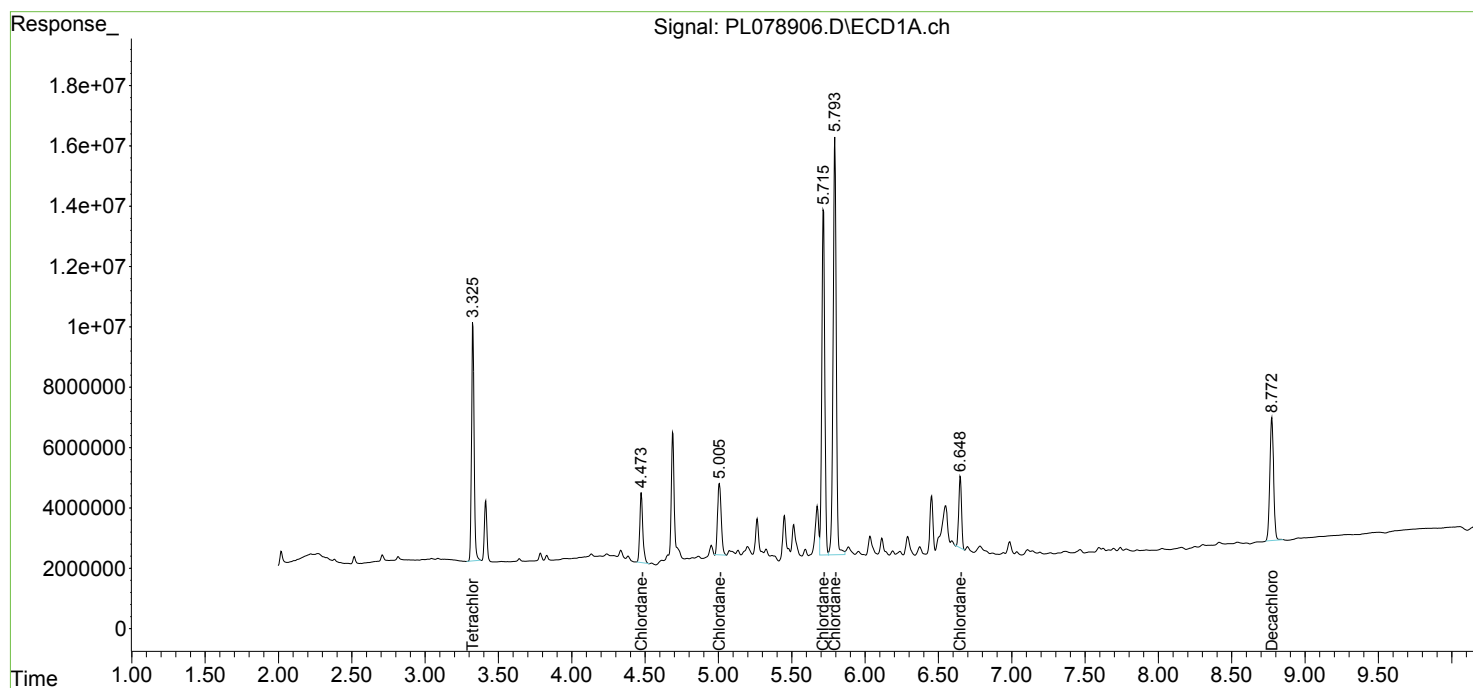


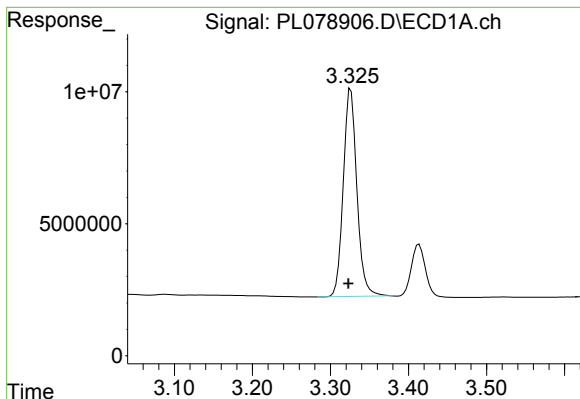

#1 Tetrachloro-m-xylene


R.T.: 3.326 min
Delta R.T.: 0.003 min
Response: 95295400
Conc: 49.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

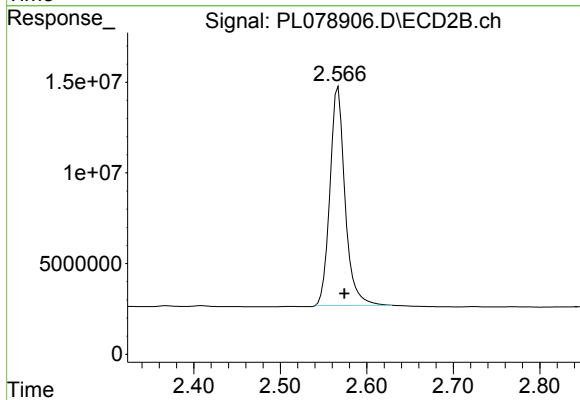


#1 Tetrachloro-m-xylene

R.T.: 2.567 min
Delta R.T.: -0.007 min
Response: 146029344
Conc: 57.19 ng/ml

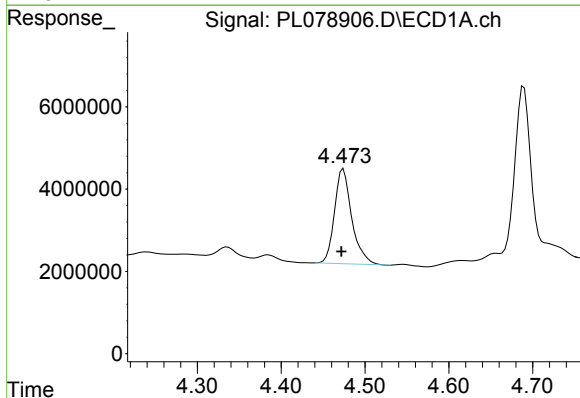


#23 Chlordane-1

R.T.: 4.474 min
Delta R.T.: 0.002 min
Response: 32874389
Conc: 419.57 ng/ml

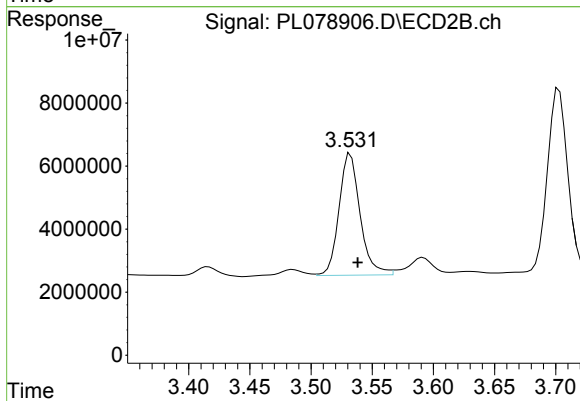

#23 Chlordane-1


R.T.: 3.532 min
Delta R.T.: -0.006 min
Response: 46384989
Conc: 459.92 ng/ml

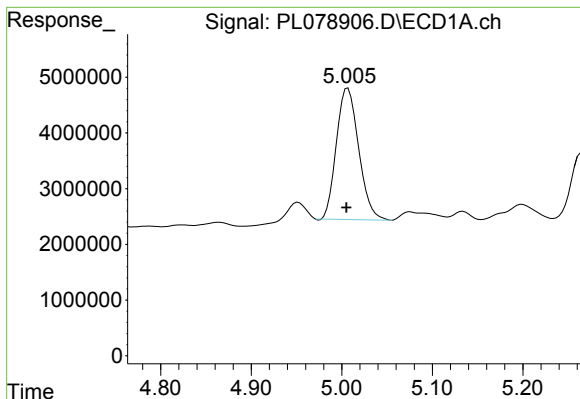

#24 Chlordane-2


R.T.: 5.007 min
Delta R.T.: 0.002 min
Response: 40423888
Conc: 488.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

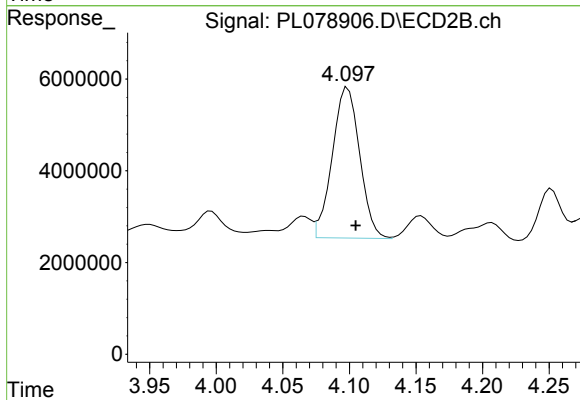


#24 Chlordane-2

R.T.: 4.099 min
Delta R.T.: -0.006 min
Response: 47187913
Conc: 443.39 ng/ml

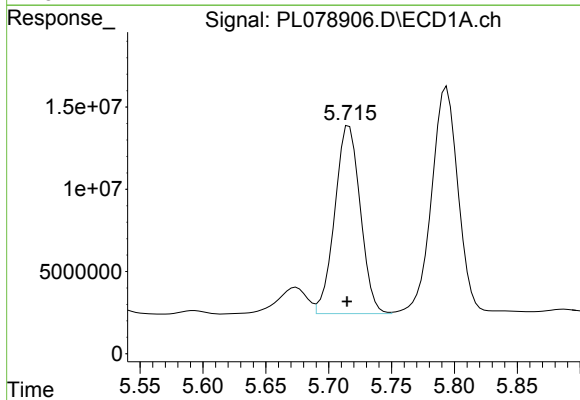


#25 Chlordane-3

R.T.: 5.716 min
Delta R.T.: 0.002 min
Response: 161648044
Conc: 483.91 ng/ml

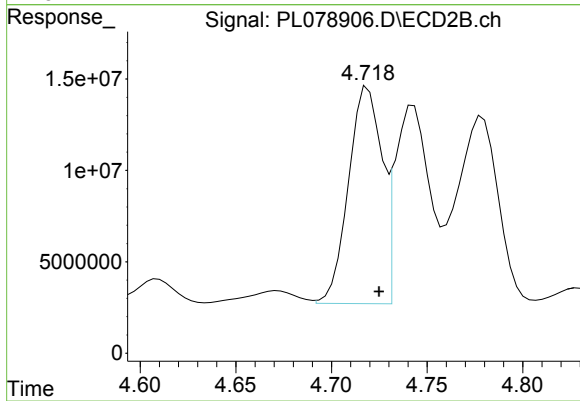

#25 Chlordane-3


R.T.: 4.719 min
Delta R.T.: -0.006 min
Response: 143962005
Conc: 472.34 ng/ml

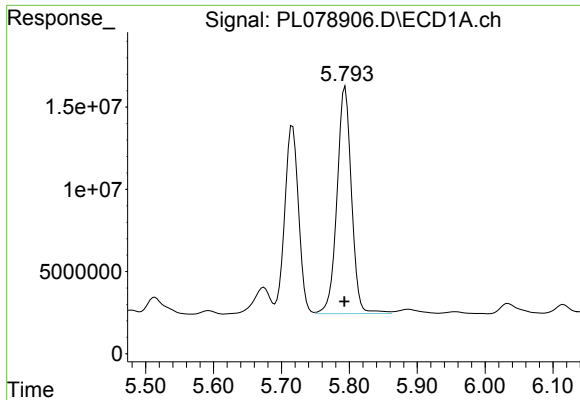

#26 Chlordane-4


R.T.: 5.794 min
Delta R.T.: 0.001 min
Response: 204513926
Conc: 498.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

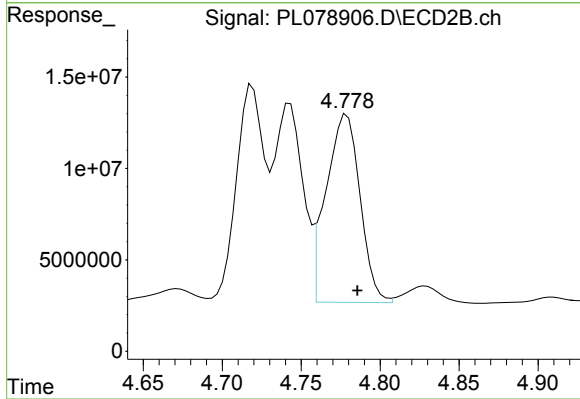


#26 Chlordane-4

R.T.: 4.779 min
Delta R.T.: -0.007 min
Response: 153910660
Conc: 471.02 ng/ml

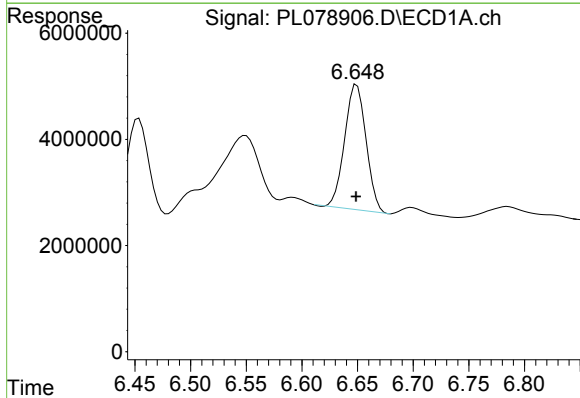


#27 Chlordane-5

R.T.: 6.649 min
Delta R.T.: 0.000 min
Response: 31267141
Conc: 478.16 ng/ml

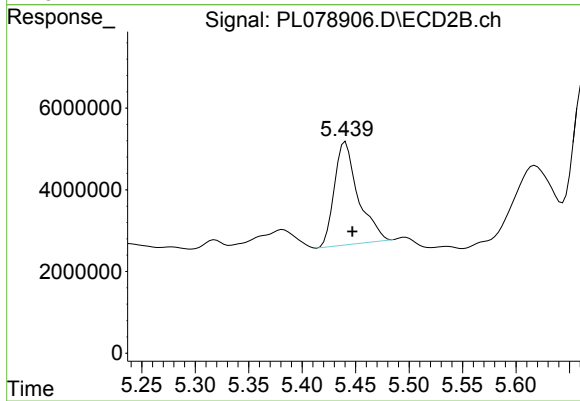

#27 Chlordane-5


R.T.: 5.441 min
Delta R.T.: -0.006 min
Response: 38954255
Conc: 477.64 ng/ml

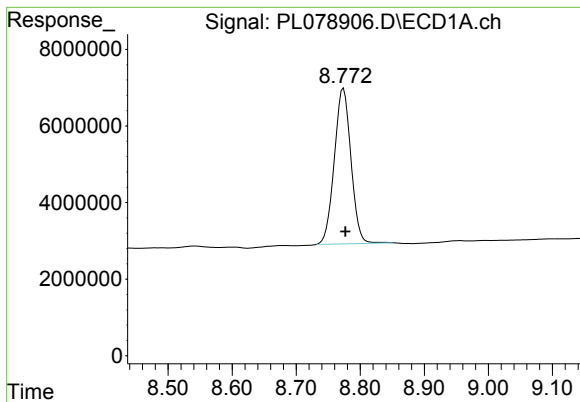

#28 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: -0.003 min
Response: 73194762
Conc: 48.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

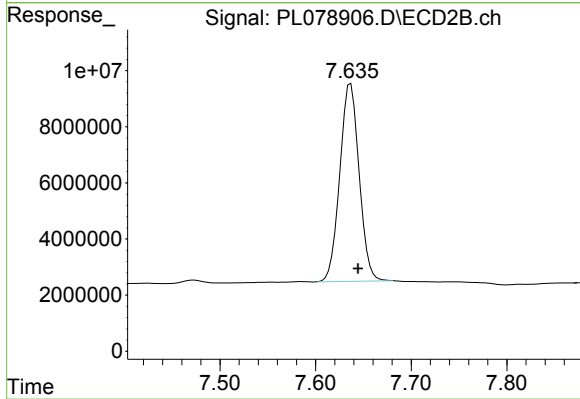

#28 Decachlorobiphenyl

R.T.: 7.637 min
Delta R.T.: -0.008 min
Response: 99232526
Conc: 52.39 ng/ml