

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110822\
 Data File : PL078909.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 13:48
 Operator : AR\AJ
 Sample : N5436-02RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 250FERRYBLVD-TFS-02RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 17:12:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	2.587	43607466	26048855	22.867	10.202 #
28)	SA Decachlor...	8.770	7.655	272.8E6	287.6E6	181.318	151.840
Target Compounds							
13)	MA Dieldrin	6.114	5.122f	159.4E6	79843777	73.927m	26.946m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110822\
Data File : PL078909.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 13:48
Operator : AR\AJ
Sample : N5436-02RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-02RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 17:12:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

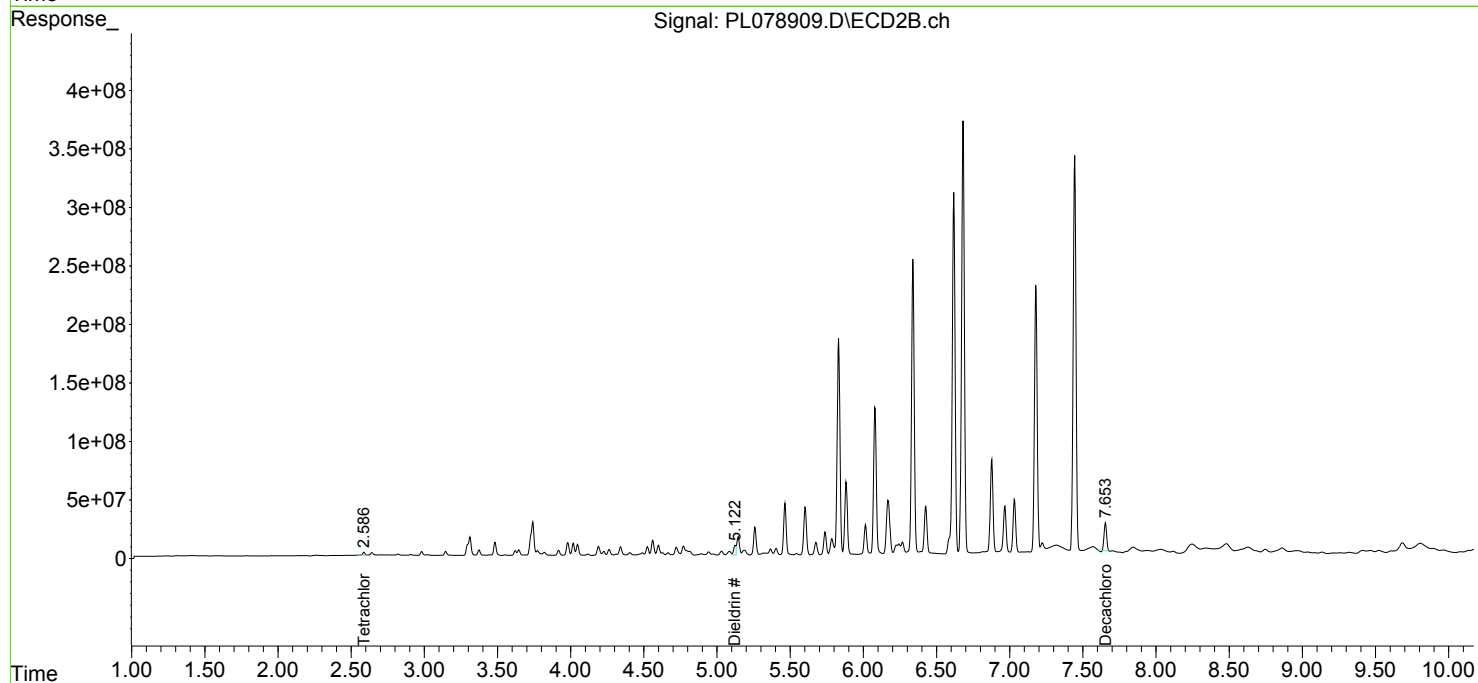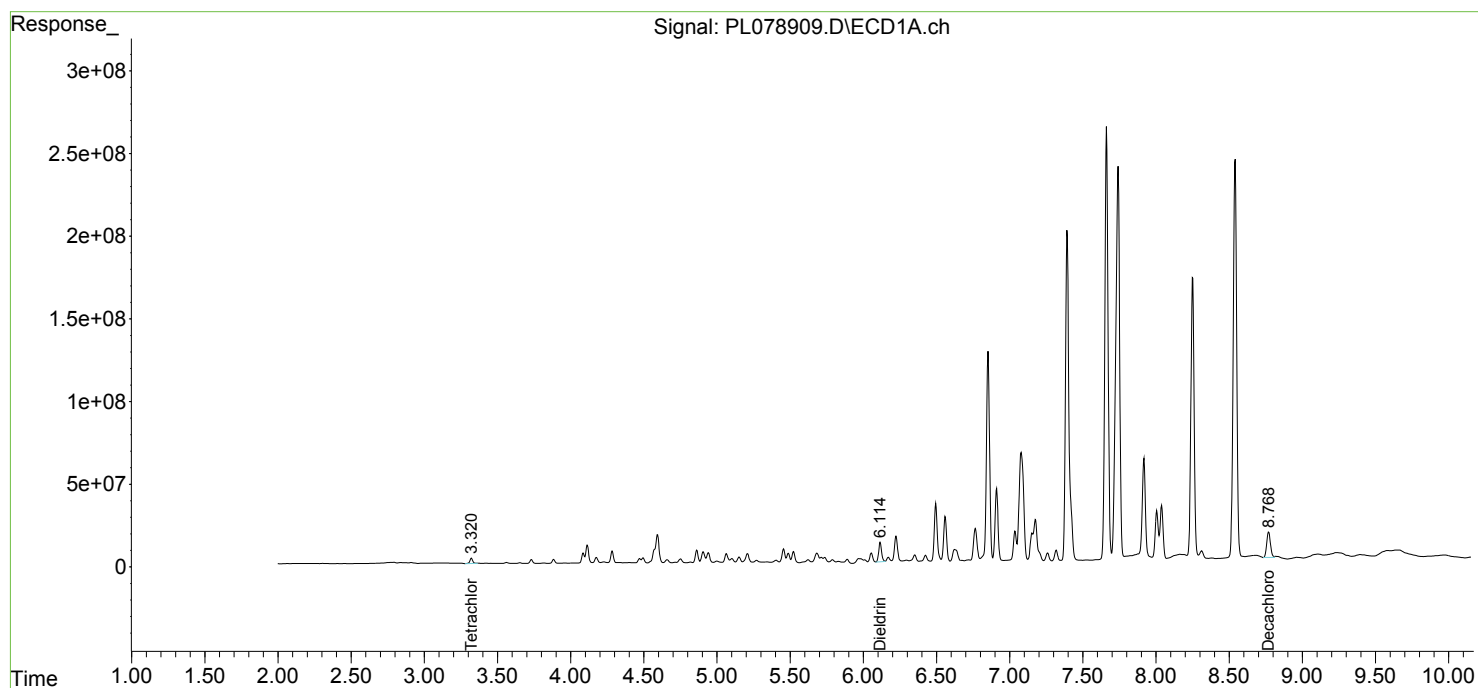


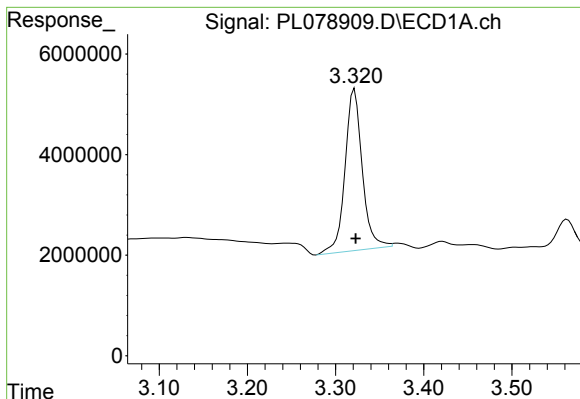

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: -0.002 min
Response: 43607466
Conc: 22.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-02RE

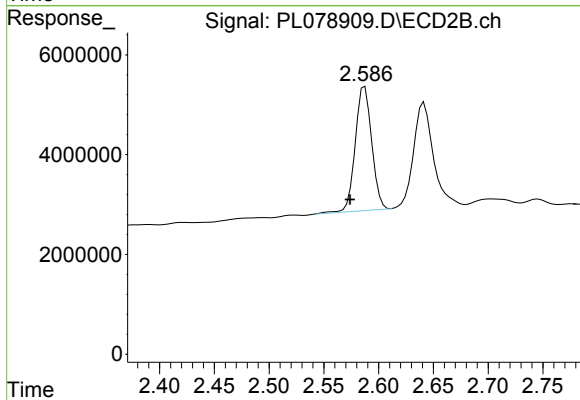


#1 Tetrachloro-m-xylene

R.T.: 2.587 min
Delta R.T.: 0.014 min
Response: 26048855
Conc: 10.20 ng/ml

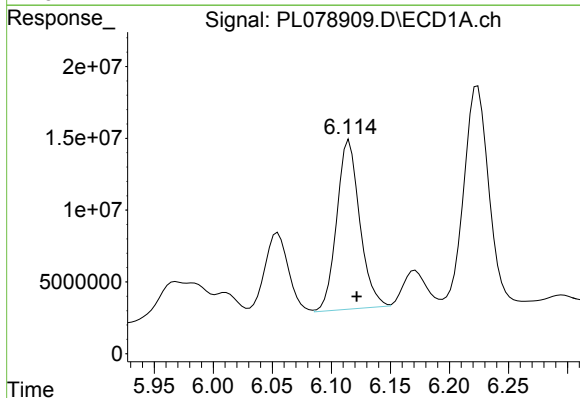


#13 Dieldrin

R.T.: 6.114 min
Delta R.T.: -0.008 min
Response: 159423938
Conc: 73.93 ng/ml m

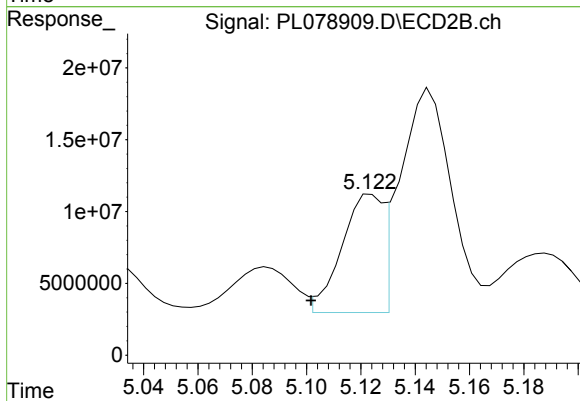

#13 Dieldrin


R.T.: 5.122 min
Delta R.T.: 0.021 min
Response: 79843777
Conc: 26.95 ng/ml m

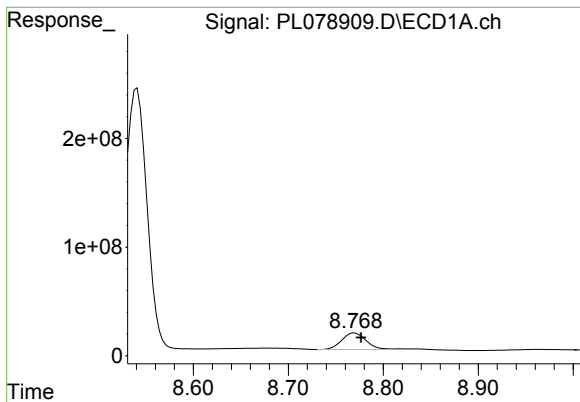

#28 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.007 min
Response: 272766740
Conc: 181.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-02RE

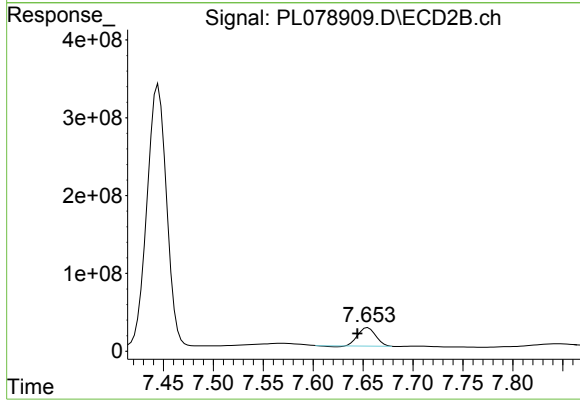

#28 Decachlorobiphenyl

R.T.: 7.655 min
Delta R.T.: 0.010 min
Response: 287600061
Conc: 151.84 ng/ml