

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110822\
 Data File : PL078913.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 14:44
 Operator : AR\AJ
 Sample : N5436-06RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 250FERRYBLVD-TFS-06RE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/10/2022
 Supervised By :Ankita Jodhani 11/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 17:25:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.322	2.568	44188883	24653755	23.172	9.656 #
2) SA Decachlor...	8.770	7.634	313.1E6	366.3E6	208.116	193.385
Target Compounds						
13) MA Dieldrin	6.115	5.102	167.2E6	125.4E6	77.514	42.312m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110822\
Data File : PL078913.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 14:44
Operator : AR\AJ
Sample : N5436-06RE
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-06RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/10/2022
Supervised By : Ankita Jodhani 11/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 17:25:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

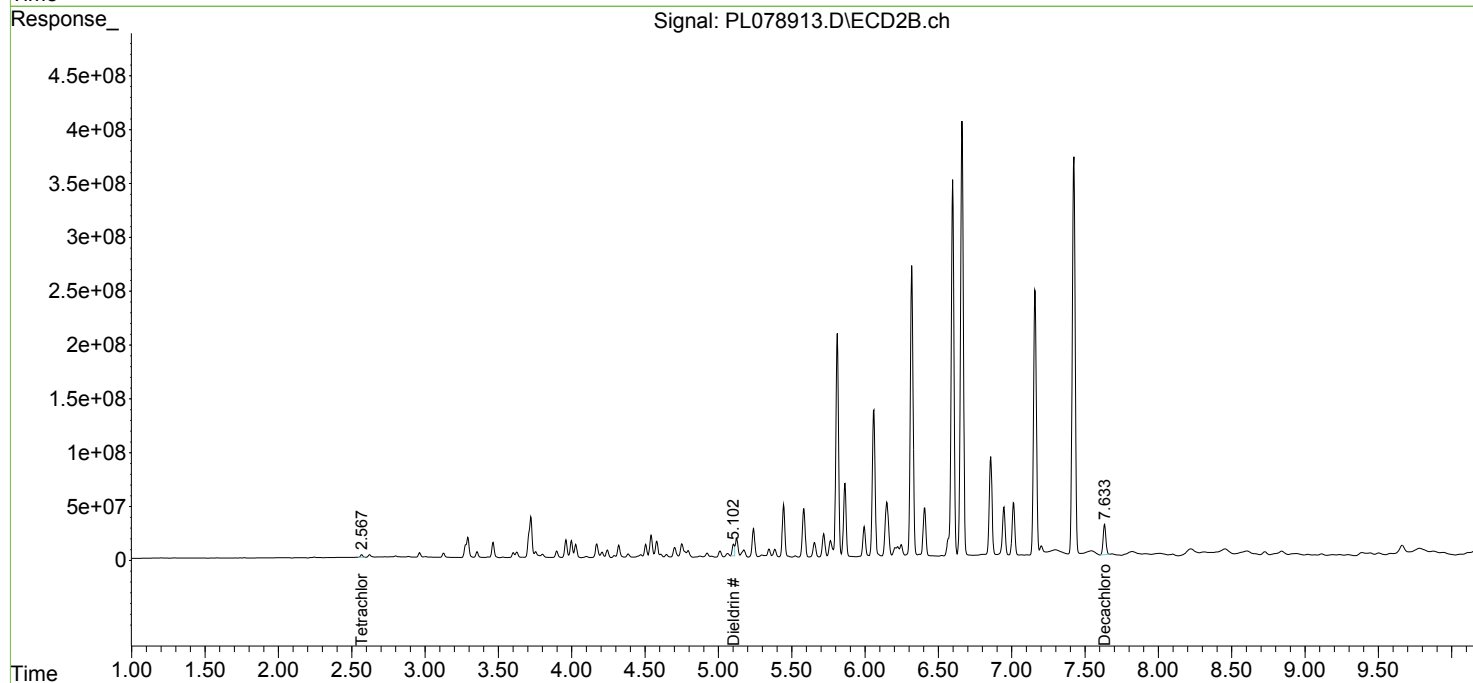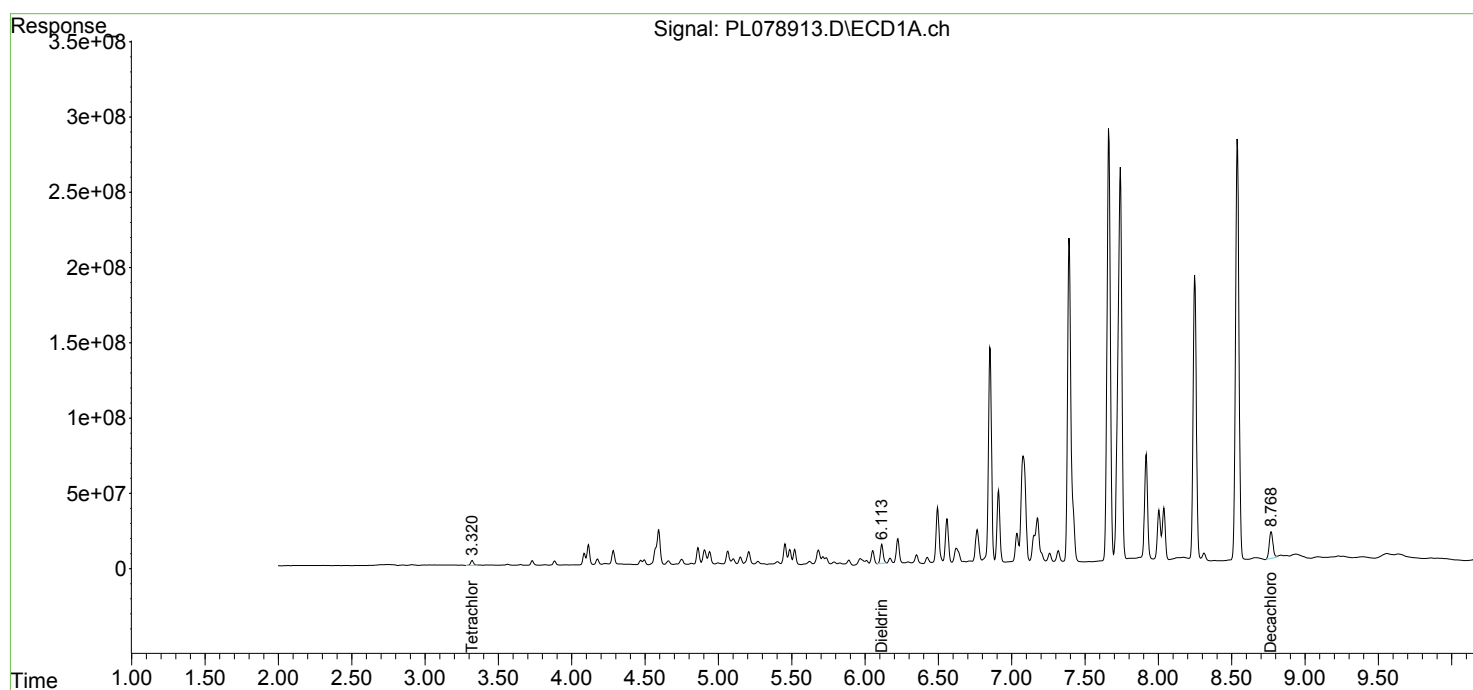

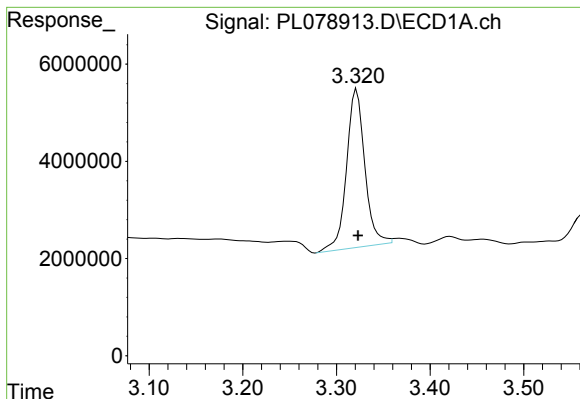


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: -0.001 min
Response: 44188883
Conc: 23.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-06RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/10/2022
Supervised By :Ankita Jodhani 11/10/2022

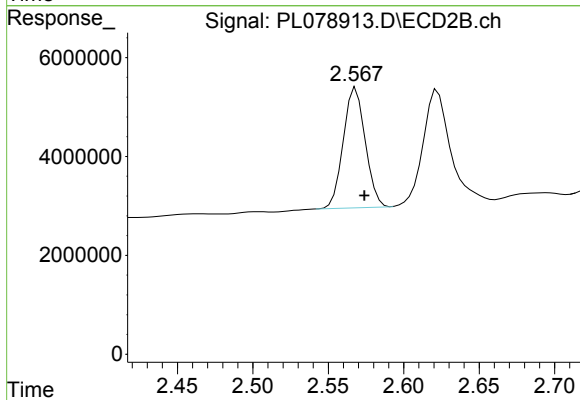


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.005 min
Response: 24653755
Conc: 9.66 ng/ml

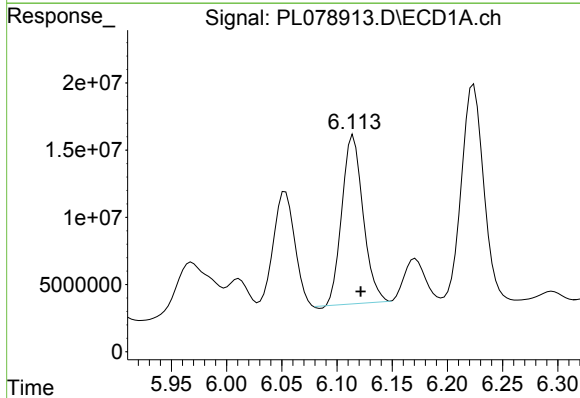


#13 Dieldrin

R.T.: 6.115 min
Delta R.T.: -0.007 min
Response: 167159999
Conc: 77.51 ng/ml

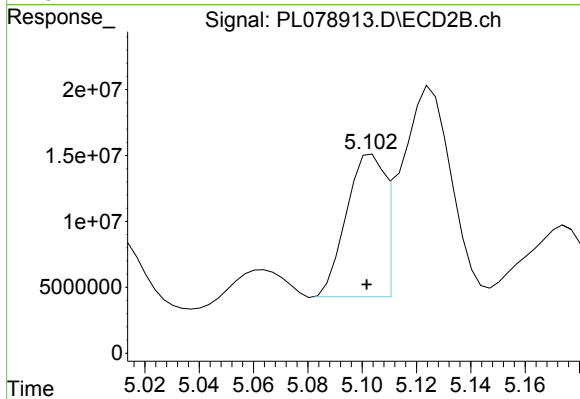

#13 Dieldrin

R.T.: 5.102 min
Delta R.T.: 0.000 min
Response: 125374658
Conc: 42.31 ng/ml m

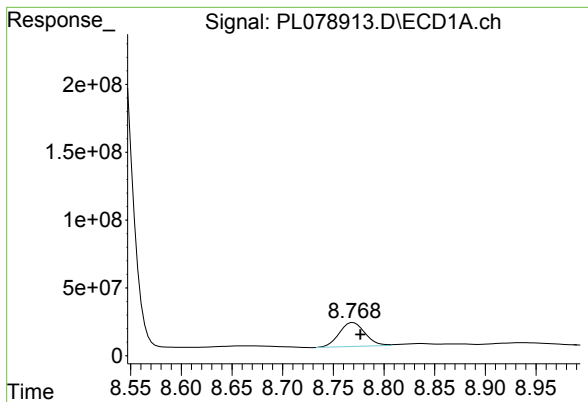


#28 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.007 min
Response: 313080778
Conc: 208.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-06RE

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/10/2022
Supervised By :Ankita Jodhani 11/10/2022

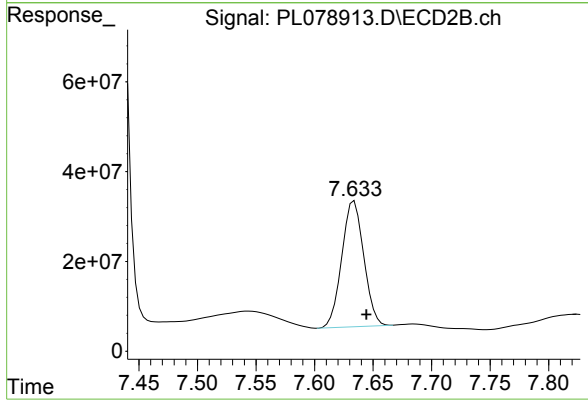

#28 Decachlorobiphenyl

R.T.: 7.634 min
Delta R.T.: -0.010 min
Response: 366291926
Conc: 193.39 ng/ml